

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035472.D
 Acq On : 06 Dec 2024 22:22
 Operator : RC/JU
 Sample : P5107-09
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	7	12	21	rBV	15296	21257	0.72%	0.083%
2	3.340	74	77	90	rBV	56590	93719	3.19%	0.366%
3	3.640	123	128	133	rBV3	4534	6302	0.21%	0.025%
4	4.069	197	201	205	rVB	8720	11256	0.38%	0.044%
5	4.516	273	277	281	rBV2	4158	6283	0.21%	0.025%
6	6.499	606	614	621	rVB	94329	142097	4.84%	0.555%
7	6.658	635	641	651	rVB	236340	351773	11.97%	1.374%
8	6.834	665	671	684	rVB	285383	434124	14.77%	1.696%
9	7.293	743	749	756	rBV	328457	501423	17.06%	1.959%
10	8.010	864	871	880	rBV	281226	423235	14.40%	1.653%
11	8.434	936	943	951	rBV	300571	454599	15.47%	1.776%
12	8.899	1015	1022	1028	rVB2	3849	7104	0.24%	0.028%
13	9.146	1057	1064	1073	rBV	268661	406092	13.82%	1.586%
14	9.675	1148	1154	1168	rBV	431711	711662	24.22%	2.780%
15	10.046	1210	1217	1224	rVB	480723	765991	26.07%	2.992%
16	10.193	1235	1242	1252	rBV	387439	618675	21.05%	2.417%
17	11.387	1438	1445	1449	rBV4	2440	4413	0.15%	0.017%
18	11.646	1483	1489	1494	rVB3	5286	9267	0.32%	0.036%
19	13.387	1778	1785	1798	rBV	983461	1327290	45.17%	5.185%
20	13.640	1821	1828	1841	rBV	1028270	1476337	50.24%	5.768%
21	13.957	1875	1882	1893	rBV	910319	1273652	43.34%	4.976%
22	14.192	1916	1922	1932	rBV	81860	148871	5.07%	0.582%
23	14.963	2047	2053	2061	rBV	1445728	2027484	69.00%	7.921%
24	15.098	2070	2076	2087	rBV	450578	581889	19.80%	2.273%
25	15.204	2090	2094	2099	rVB2	5645	7307	0.25%	0.029%
26	16.504	2312	2315	2322	rBV4	2696	3912	0.13%	0.015%
27	16.722	2346	2352	2363	rBV	1159011	1600675	54.47%	6.253%
28	16.822	2363	2369	2383	rVV2	1688640	2342444	79.71%	9.151%
29	17.051	2404	2408	2412	rVB	4125	5167	0.18%	0.020%
30	17.669	2508	2513	2518	rBV4	4182	5958	0.20%	0.023%
31	18.698	2682	2688	2693	rBV2	20687	27612	0.94%	0.108%
32	18.775	2697	2701	2706	rBV2	16551	23845	0.81%	0.093%
33	18.851	2710	2714	2727	rVB	42835	56287	1.92%	0.220%
34	18.980	2732	2736	2738	rVV5	4010	4188	0.14%	0.016%
35	19.145	2757	2764	2777	rBV	2132739	2873710	97.79%	11.227%
36	20.974	3069	3075	3085	rBV	1460573	1902515	64.74%	7.433%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035472.D
Acq On : 06 Dec 2024 22:22
Operator : RC/JU
Sample : P5107-09
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ86

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	22.957	3409	3412	3420	rVB5	23576	38302	1.30%	0.150%
38	23.468	3490	3499	3511	rBV	1314112	2938573	100.00%	11.480%
39	23.645	3521	3529	3539	rBV	875984	1961877	66.76%	7.664%




Sum of corrected areas: 25597167

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035472.D
Acq On : 06 Dec 2024 22:22
Operator : RC/JU
Sample : P5107-09
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

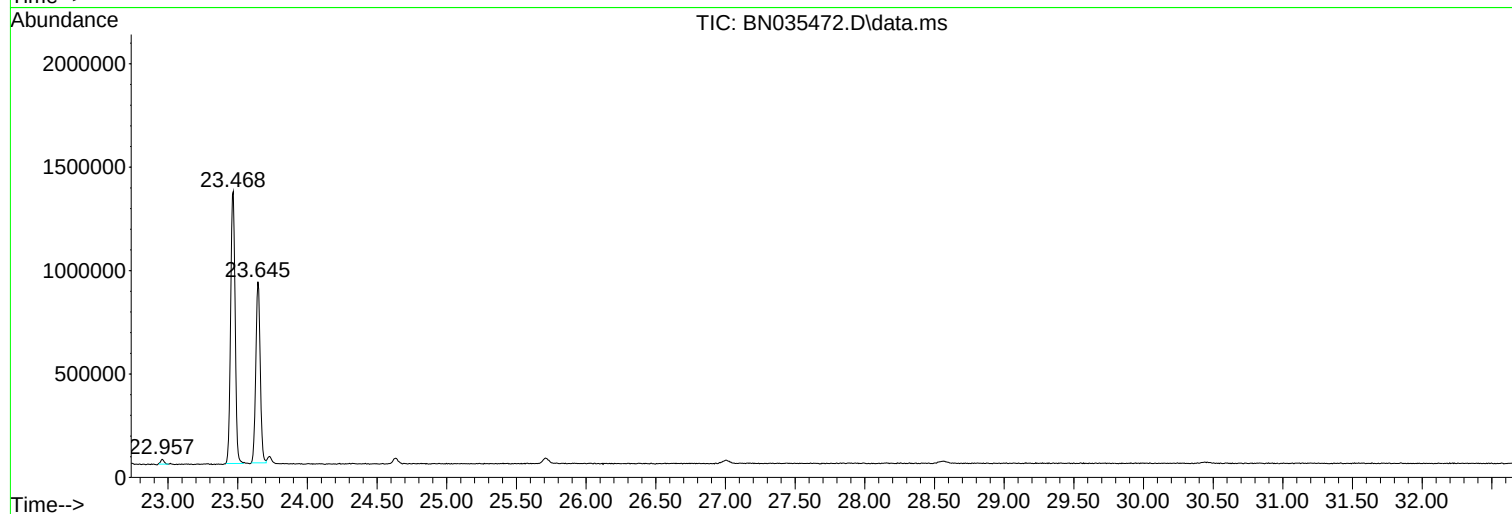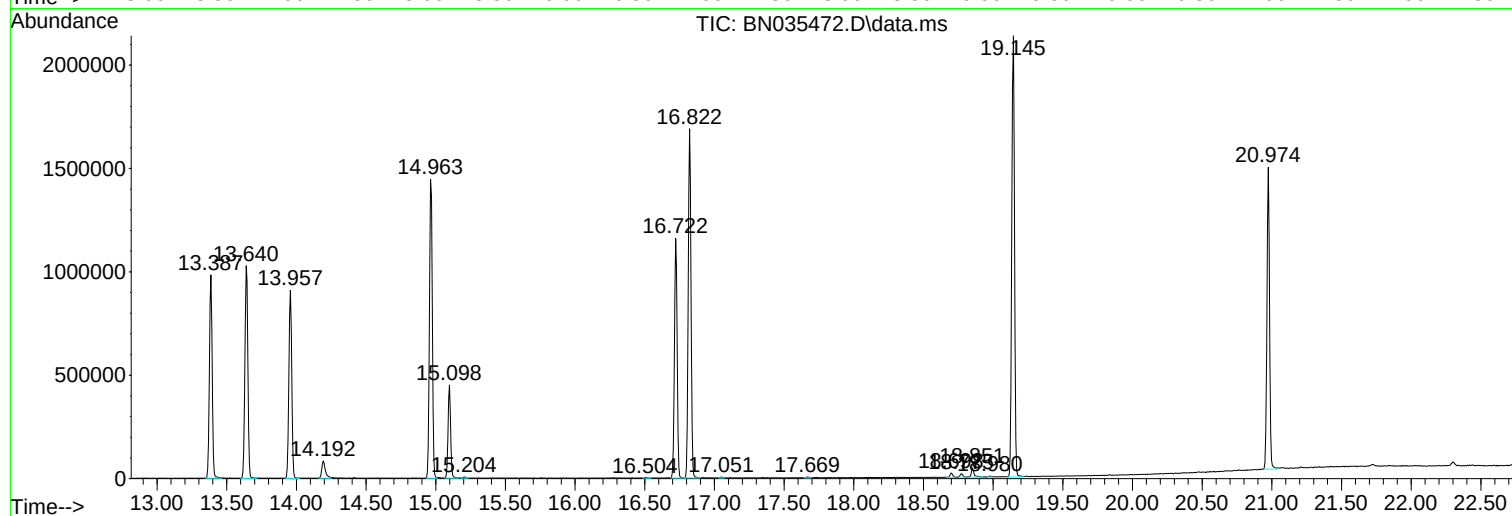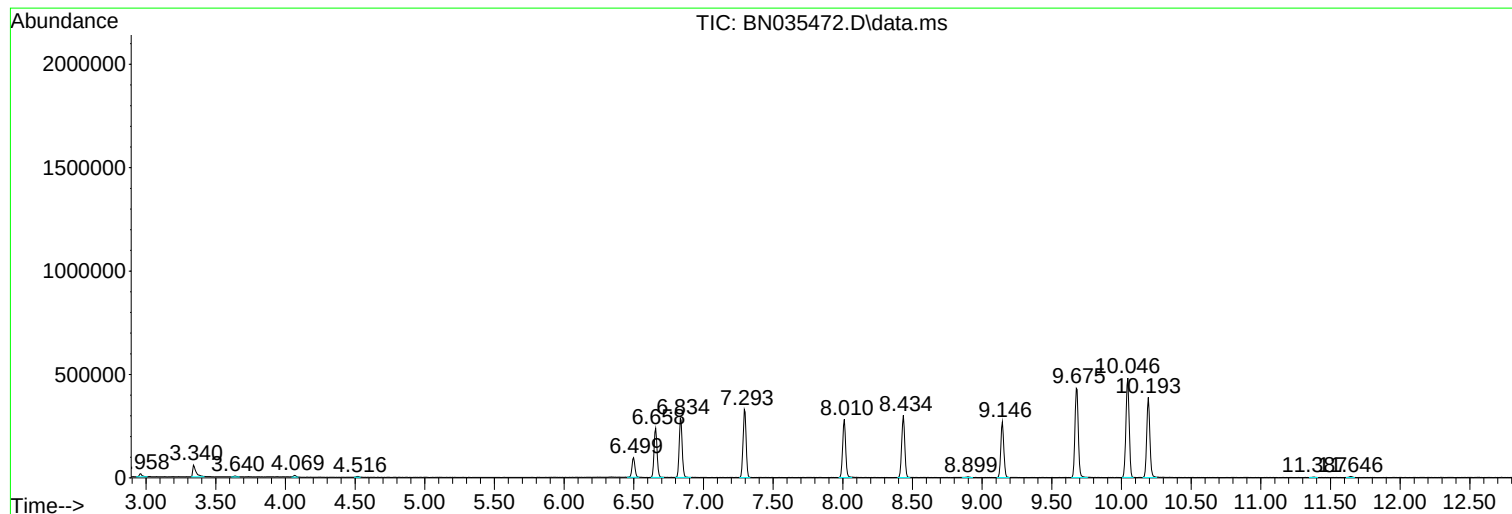

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035472.D
Acq On : 06 Dec 2024 22:22
Operator : RC/JU
Sample : P5107-09
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035472.D
Acq On : 06 Dec 2024 22:22
Operator : RC/JU
Sample : P5107-09
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc