

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035473.D
 Acq On : 06 Dec 2024 23:01
 Operator : RC/JU
 Sample : P5107-10
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	22	rVB	13729	18148	0.59%	0.071%
2	3.346	74	78	93	rBV	35032	62294	2.04%	0.244%
3	3.634	124	127	133	rVB2	3623	5253	0.17%	0.021%
4	4.069	197	201	208	rVB	8199	12293	0.40%	0.048%
5	4.516	273	277	283	rVB3	8310	10792	0.35%	0.042%
6	6.499	607	614	621	rBV	89399	133811	4.38%	0.524%
7	6.658	634	641	654	rVB	239456	355774	11.66%	1.393%
8	6.834	666	671	679	rBV	282948	425487	13.94%	1.666%
9	7.293	743	749	761	rVB	312933	477524	15.65%	1.870%
10	8.010	864	871	882	rBV	272980	404193	13.25%	1.583%
11	8.434	934	943	952	rBV	292309	451311	14.79%	1.767%
12	8.899	1018	1022	1028	rVB4	3990	6293	0.21%	0.025%
13	9.146	1057	1064	1071	rBV	265699	403780	13.23%	1.581%
14	9.675	1146	1154	1164	rBV	431702	703857	23.06%	2.756%
15	10.040	1207	1216	1224	rBV	441177	733789	24.05%	2.873%
16	10.193	1236	1242	1254	rBV	268429	432000	14.16%	1.692%
17	11.381	1440	1444	1449	rVB2	2467	3300	0.11%	0.013%
18	11.645	1484	1489	1495	rBV2	5251	8890	0.29%	0.035%
19	13.387	1778	1785	1799	rBV	991543	1352440	44.32%	5.296%
20	13.639	1822	1828	1844	rVB	1023600	1485551	48.68%	5.817%
21	13.957	1875	1882	1894	rBV	835211	1220995	40.01%	4.781%
22	14.192	1916	1922	1935	rBV	78842	141018	4.62%	0.552%
23	14.963	2046	2053	2060	rBV	1467382	2033259	66.63%	7.962%
24	15.016	2060	2062	2070	rVV5	4440	7318	0.24%	0.029%
25	15.098	2070	2076	2086	rVV	454848	584552	19.16%	2.289%
26	15.204	2090	2094	2099	rVB	4599	6648	0.22%	0.026%
27	15.345	2112	2118	2127	rBV	63314	83712	2.74%	0.328%
28	15.910	2208	2214	2220	rBV	17017	21918	0.72%	0.086%
29	16.504	2311	2315	2321	rVB3	2199	4111	0.13%	0.016%
30	16.722	2346	2352	2360	rBV	1135608	1530628	50.16%	5.994%
31	16.822	2363	2369	2381	rVV	1722664	2364853	77.49%	9.261%
32	17.351	2453	2459	2461	rBV3	2048	3538	0.12%	0.014%
33	17.669	2509	2513	2518	rBV2	17696	21070	0.69%	0.083%
34	17.945	2558	2560	2566	rBV5	3080	4685	0.15%	0.018%
35	18.116	2584	2589	2592	rVB5	1968	3135	0.10%	0.012%
36	18.304	2615	2621	2624	rBV6	2190	3933	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035473.D
 Acq On : 06 Dec 2024 23:01
 Operator : RC/JU
 Sample : P5107-10
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

37	18.504	2651	2655	2661	rVB3	9446	15066	0.49%	0.059%
38	18.698	2684	2688	2694	rBV2	20804	28232	0.93%	0.111%
39	18.775	2696	2701	2706	rBV	17801	25057	0.82%	0.098%
40	18.857	2710	2715	2726	rVV	103397	150596	4.93%	0.590%
41	18.980	2732	2736	2740	rBV4	13694	17364	0.57%	0.068%
42	19.145	2758	2764	2773	rBV	2163971	2869181	94.02%	11.236%
43	19.874	2884	2888	2891	rBV5	16794	18239	0.60%	0.071%
44	20.974	3069	3075	3084	rBV2	1474409	1908560	62.54%	7.474%
45	23.468	3490	3499	3515	rVB	1383183	3051650	100.00%	11.950%
46	23.645	3521	3529	3537	rBV	909335	1930477	63.26%	7.560%




Sum of corrected areas: 25536575

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035473.D
Acq On : 06 Dec 2024 23:01
Operator : RC/JU
Sample : P5107-10
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

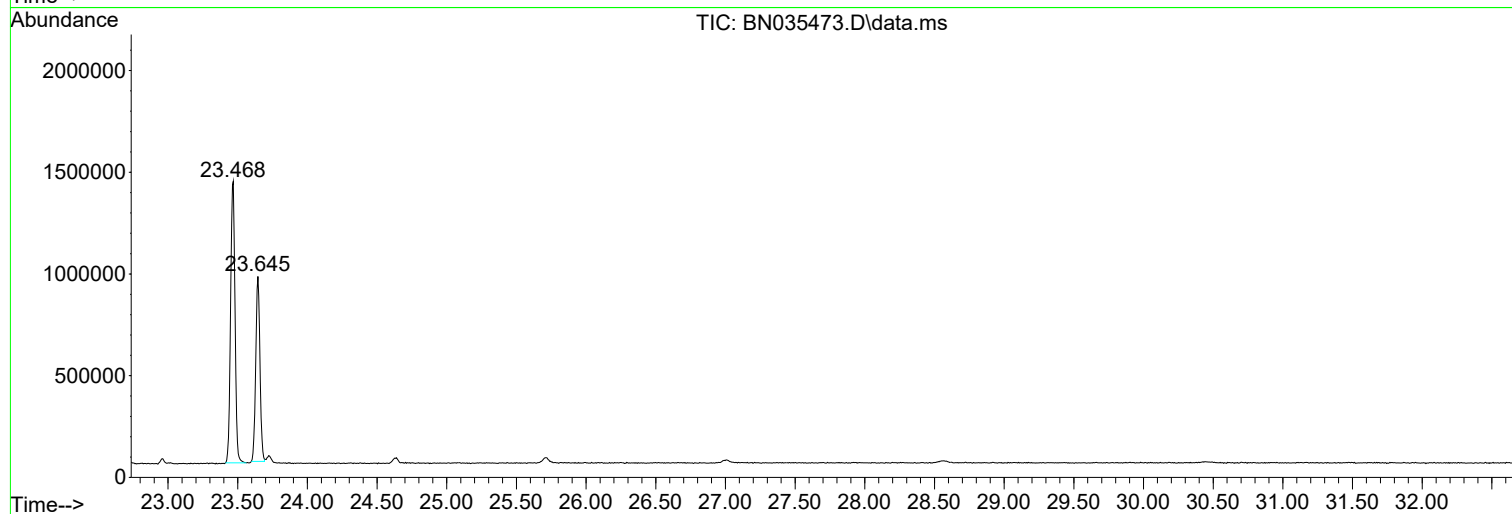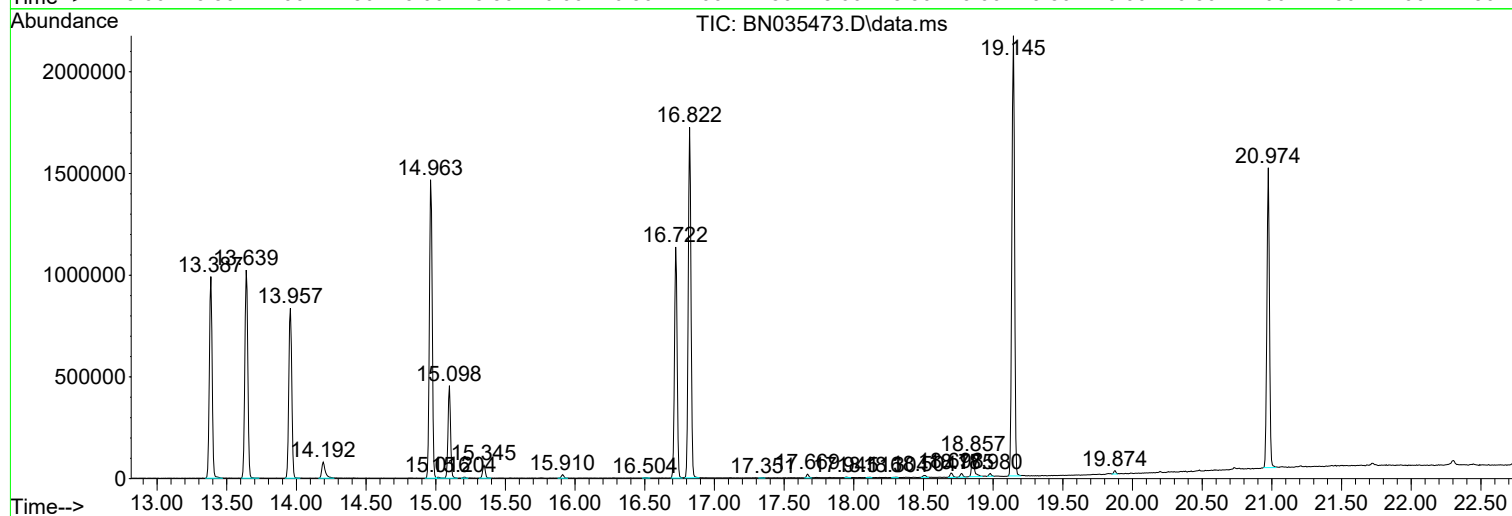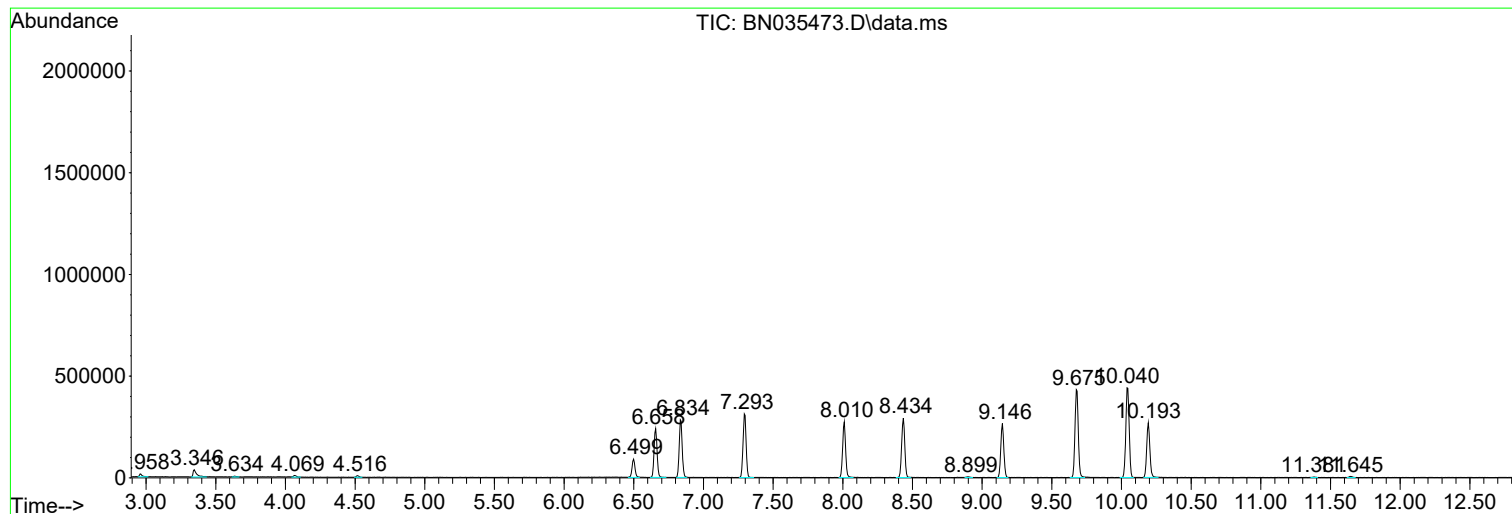

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035473.D
Acq On : 06 Dec 2024 23:01
Operator : RC/JU
Sample : P5107-10
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035473.D
Acq On : 06 Dec 2024 23:01
Operator : RC/JU
Sample : P5107-10
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc