

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035474.D
 Acq On : 06 Dec 2024 23:40
 Operator : RC/JU
 Sample : P5107-11
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035474.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.928	4	7	9	rBV	3803	4638	0.15%	0.017%
2	2.958	9	12	18	rVB	13416	16657	0.52%	0.063%
3	3.340	74	77	92	rBV	56846	96883	3.04%	0.364%
4	3.640	124	128	134	rVB2	3538	5180	0.16%	0.019%
5	4.070	197	201	207	rVB	9170	13342	0.42%	0.050%
6	4.517	271	277	283	rBV2	11391	16874	0.53%	0.063%
7	6.499	608	614	621	rVB	86053	128634	4.04%	0.483%
8	6.658	634	641	649	rBV	256762	380593	11.94%	1.430%
9	6.834	665	671	685	rVB	296364	452040	14.18%	1.699%
10	7.293	741	749	757	rBV	324120	496539	15.58%	1.866%
11	8.011	863	871	882	rBV	276152	418695	13.13%	1.574%
12	8.434	936	943	952	rBV	326643	497115	15.59%	1.868%
13	8.899	1018	1022	1028	rVB5	4412	7408	0.23%	0.028%
14	9.146	1057	1064	1073	rBV	294477	438591	13.76%	1.648%
15	9.675	1148	1154	1169	rBV	474277	759422	23.82%	2.854%
16	10.046	1208	1217	1227	rBV	474272	765481	24.01%	2.877%
17	10.193	1235	1242	1252	rBV	403238	665781	20.89%	2.502%
18	11.387	1437	1445	1448	rVB5	2915	5103	0.16%	0.019%
19	11.646	1483	1489	1494	rBV2	5723	9485	0.30%	0.036%
20	13.387	1779	1785	1804	rBV	1019801	1392803	43.69%	5.235%
21	13.640	1821	1828	1838	rBV	1083146	1585226	49.73%	5.958%
22	13.957	1875	1882	1891	rBV	896449	1285668	40.33%	4.832%
23	14.193	1917	1922	1933	rBV	67641	125796	3.95%	0.473%
24	14.963	2047	2053	2061	rBV	1483811	2106506	66.08%	7.917%
25	15.098	2070	2076	2087	rVB	460894	592999	18.60%	2.229%
26	15.204	2091	2094	2098	rBV2	6515	8170	0.26%	0.031%
27	16.281	2271	2277	2282	rBV5	2206	3579	0.11%	0.013%
28	16.504	2312	2315	2321	rBV2	2203	3660	0.11%	0.014%
29	16.722	2346	2352	2362	rBV	1174759	1611043	50.54%	6.055%
30	16.822	2362	2369	2381	rBV2	1730828	2404082	75.41%	9.036%
31	17.669	2510	2513	2517	rVB5	5740	6807	0.21%	0.026%
32	18.704	2684	2689	2694	rVB3	19547	28413	0.89%	0.107%
33	18.775	2695	2701	2705	rBV	17412	24549	0.77%	0.092%
34	18.851	2710	2714	2724	rBV	65954	93980	2.95%	0.353%
35	18.975	2732	2735	2738	rBV3	5614	7371	0.23%	0.028%
36	19.145	2757	2764	2776	rBV	2132686	2920685	91.62%	10.977%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035474.D
Acq On : 06 Dec 2024 23:40
Operator : RC/JU
Sample : P5107-11
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ88

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	19.392	2802	2806	2811	rBV8	5185	10188	0.32%	0.038%
38	19.445	2811	2815	2819	rVV	44620	51373	1.61%	0.193%
39	20.975	3069	3075	3085	rBV	1478089	1920340	60.24%	7.218%
40	23.463	3489	3498	3515	rBV	1452806	3187814	100.00%	11.981%
41	23.645	3521	3529	3538	rBV	929756	2057123	64.53%	7.732%




Sum of corrected areas: 26606636

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035474.D
Acq On : 06 Dec 2024 23:40
Operator : RC/JU
Sample : P5107-11
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

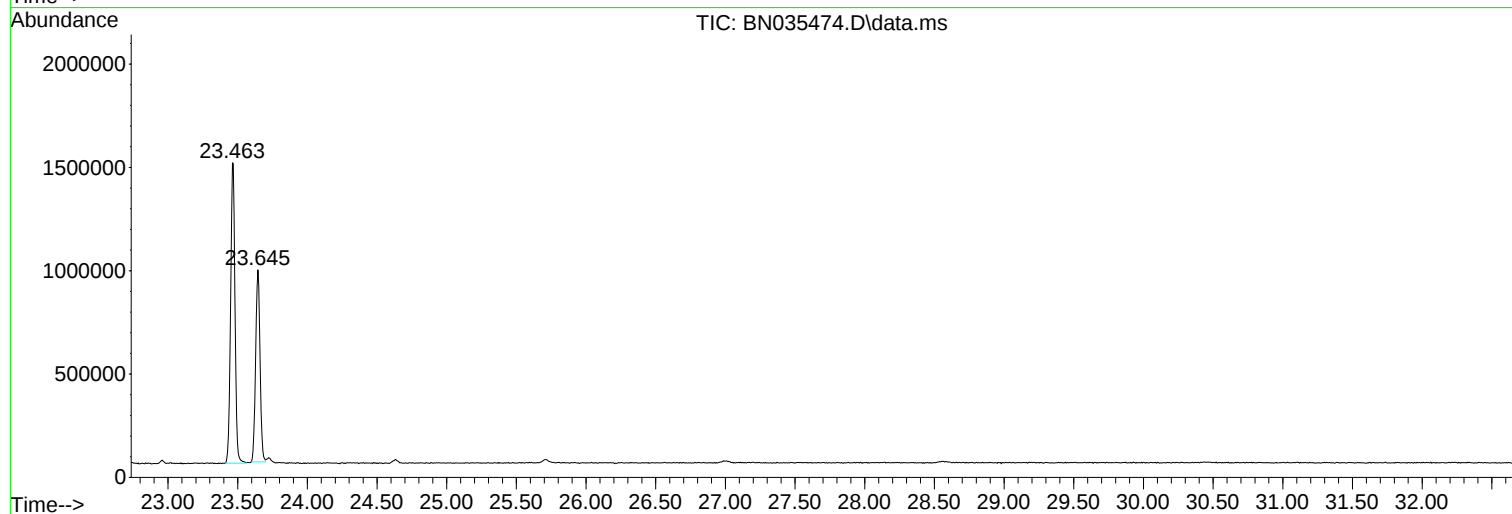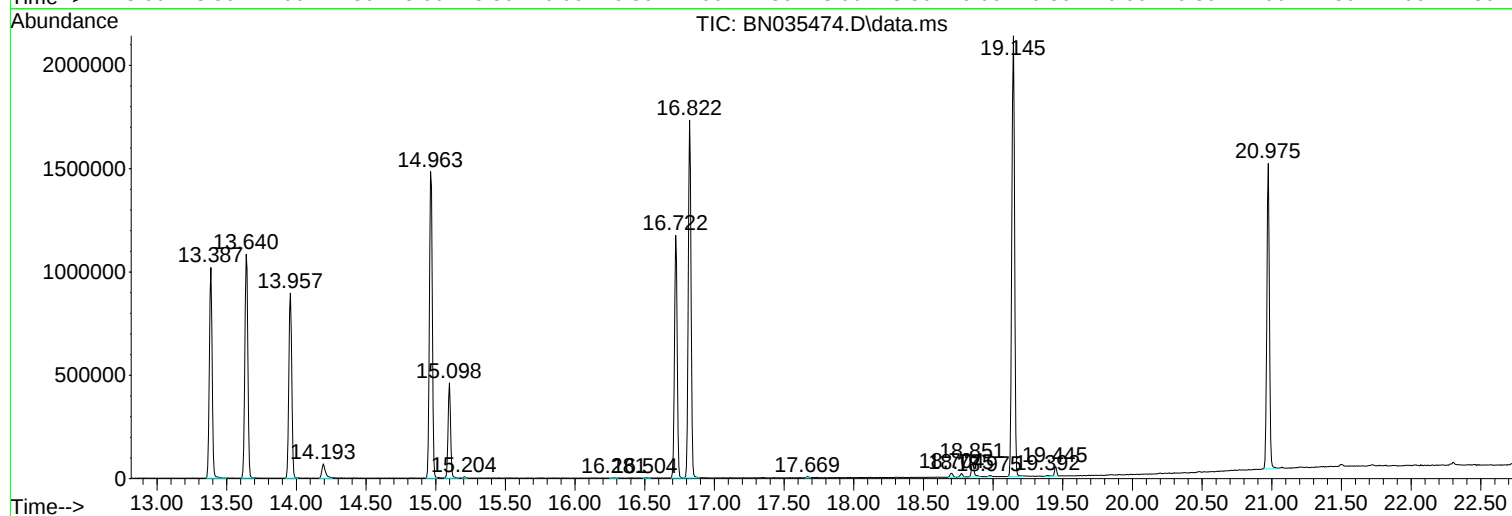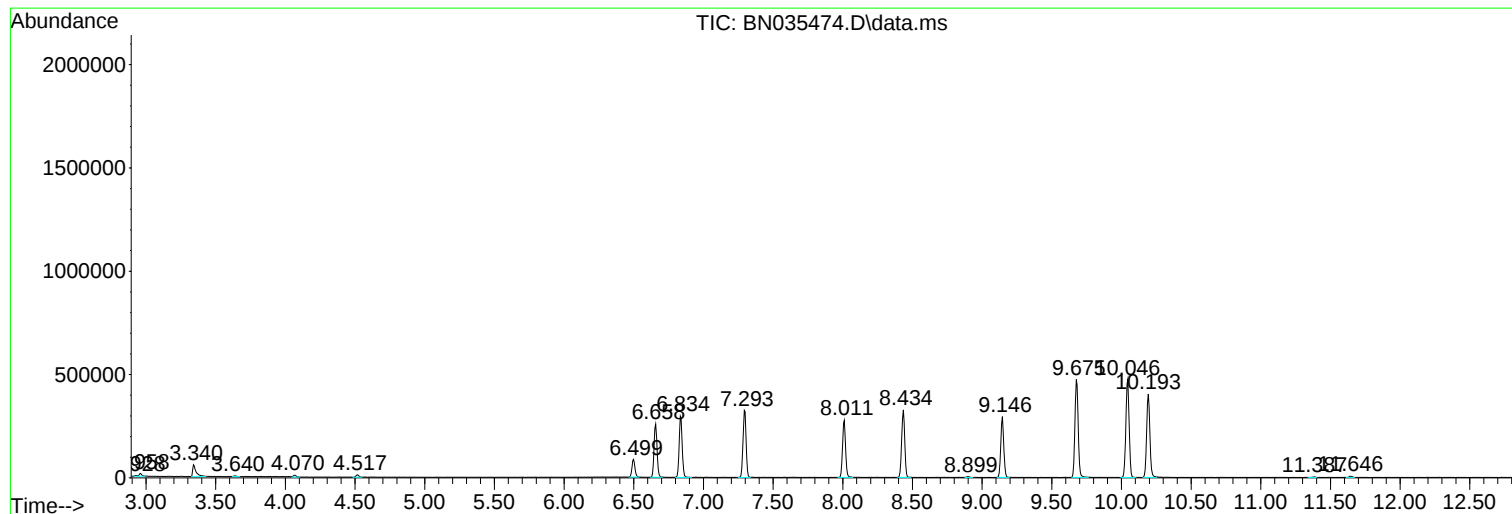

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035474.D
Acq On : 06 Dec 2024 23:40
Operator : RC/JU
Sample : P5107-11
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035474.D
Acq On : 06 Dec 2024 23:40
Operator : RC/JU
Sample : P5107-11
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc