

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035476.D
 Acq On : 07 Dec 2024 00:58
 Operator : RC/JU
 Sample : P5107-13
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	19	rVB	14237	18311	0.56%	0.068%
2	3.340	74	77	89	rBV	48607	81639	2.48%	0.302%
3	3.634	124	127	134	rVB	2919	4325	0.13%	0.016%
4	4.070	197	201	206	rVB	9282	13419	0.41%	0.050%
5	4.517	272	277	286	rVB2	6234	8985	0.27%	0.033%
6	6.499	608	614	626	rVB	91023	135934	4.12%	0.502%
7	6.658	634	641	651	rBV	265491	396856	12.03%	1.467%
8	6.834	665	671	684	rBV	308592	470791	14.27%	1.740%
9	7.293	743	749	756	rBV	320868	486585	14.75%	1.798%
10	8.011	864	871	881	rBV	279404	426024	12.92%	1.574%
11	8.434	935	943	950	rBV	337142	508936	15.43%	1.881%
12	8.899	1017	1022	1027	rVB2	4037	5458	0.17%	0.020%
13	9.146	1058	1064	1073	rBV	295800	454772	13.79%	1.681%
14	9.675	1146	1154	1169	rBV	494521	795793	24.13%	2.941%
15	10.046	1209	1217	1226	rBV	470989	751796	22.79%	2.778%
16	10.193	1235	1242	1251	rBV	406208	647307	19.63%	2.392%
17	11.381	1438	1444	1448	rVB4	2742	4284	0.13%	0.016%
18	11.640	1484	1488	1496	rVB2	6071	10316	0.31%	0.038%
19	13.387	1778	1785	1801	rBV	1066387	1473111	44.66%	5.444%
20	13.640	1822	1828	1844	rVB2	1102129	1612134	48.88%	5.958%
21	13.957	1875	1882	1891	rBV	858317	1229842	37.29%	4.545%
22	14.193	1915	1922	1931	rBV	70478	130698	3.96%	0.483%
23	14.963	2047	2053	2061	rBV	1582570	2200150	66.70%	8.131%
24	15.016	2061	2062	2068	rVV3	3649	4226	0.13%	0.016%
25	15.098	2068	2076	2088	rVV	495905	630549	19.12%	2.330%
26	15.204	2091	2094	2098	rVB2	5915	6780	0.21%	0.025%
27	16.722	2346	2352	2363	rBV	1140381	1543049	46.78%	5.702%
28	16.822	2363	2369	2378	rBV2	1856550	2527548	76.63%	9.341%
29	17.669	2509	2513	2516	rBV4	7036	8043	0.24%	0.030%
30	18.698	2684	2688	2693	rVB2	21012	27782	0.84%	0.103%
31	18.775	2696	2701	2708	rBV	18388	24837	0.75%	0.092%
32	18.851	2710	2714	2726	rVB2	64623	88249	2.68%	0.326%
33	18.975	2731	2735	2741	rVB5	7505	10546	0.32%	0.039%
34	19.145	2758	2764	2772	rBV	2331509	3098206	93.93%	11.449%
35	20.975	3069	3075	3085	rBV	1388815	1870044	56.70%	6.911%
36	22.027	3250	3254	3258	rVB2	47708	66910	2.03%	0.247%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035476.D
Acq On : 07 Dec 2024 00:58
Operator : RC/JU
Sample : P5107-13
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ90

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	23.469	3489	3499	3514	rBV	1455395	3298378	100.00%	12.189%
38	23.645	3520	3529	3538	rBV	894203	1987470	60.26%	7.345%




Sum of corrected areas: 27060083

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035476.D
Acq On : 07 Dec 2024 00:58
Operator : RC/JU
Sample : P5107-13
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

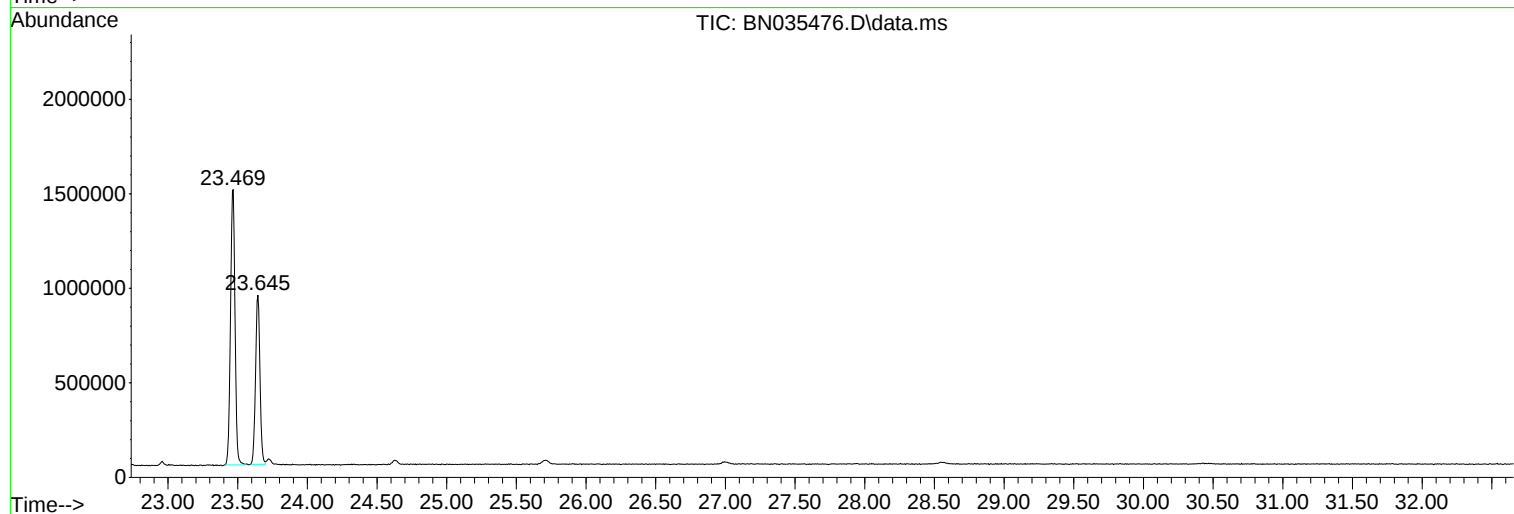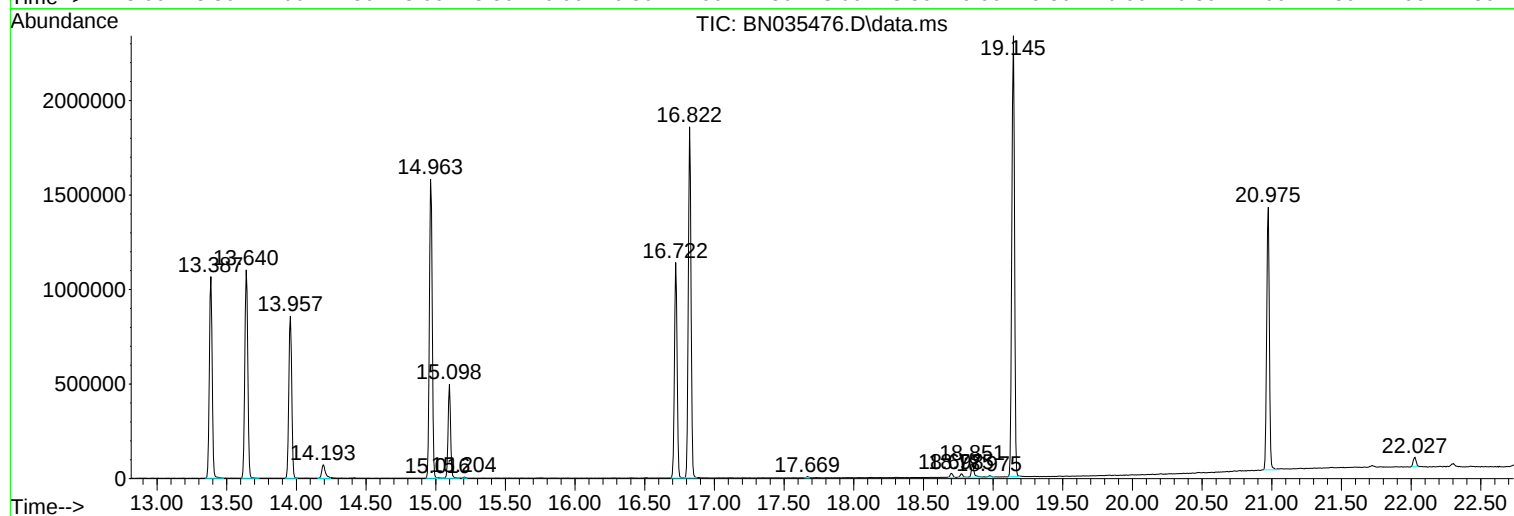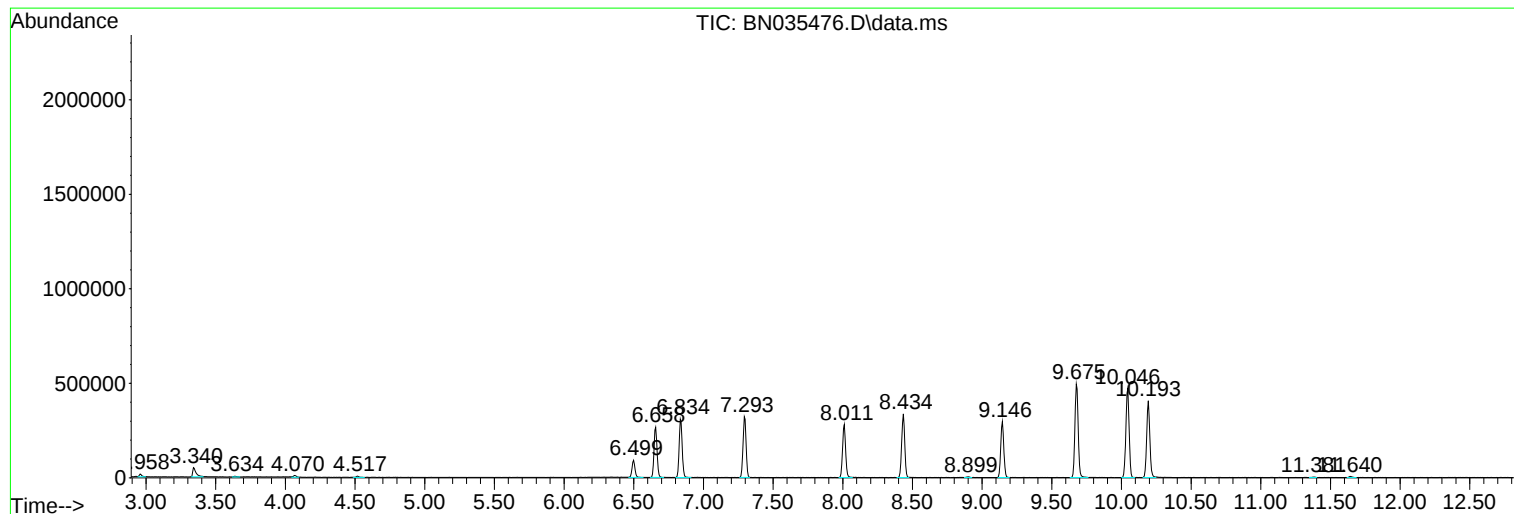

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035476.D
Acq On : 07 Dec 2024 00:58
Operator : RC/JU
Sample : P5107-13
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035476.D
Acq On : 07 Dec 2024 00:58
Operator : RC/JU
Sample : P5107-13
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ90

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc