

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035477.D
 Acq On : 07 Dec 2024 01:37
 Operator : RC/JU
 Sample : P5107-14
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	19	rVB	12382	14864	0.48%	0.058%
2	3.346	74	78	87	rBV	41344	69226	2.22%	0.268%
3	3.634	124	127	132	rVB	3748	4298	0.14%	0.017%
4	4.070	197	201	206	rVB	9056	13116	0.42%	0.051%
5	4.517	274	277	285	rVB3	3326	5014	0.16%	0.019%
6	6.499	608	614	623	rVB	86621	131988	4.23%	0.512%
7	6.658	634	641	650	rBV	252577	382038	12.24%	1.481%
8	6.834	665	671	682	rVB	305362	457665	14.66%	1.774%
9	7.293	743	749	758	rVB	324082	482256	15.45%	1.869%
10	8.011	864	871	882	rBV	265882	412399	13.21%	1.599%
11	8.434	936	943	951	rBV	324247	488849	15.66%	1.895%
12	8.899	1017	1022	1026	rVB3	4499	6883	0.22%	0.027%
13	9.146	1057	1064	1072	rBV	287515	436668	13.99%	1.693%
14	9.675	1147	1154	1168	rBV	474794	765991	24.53%	2.969%
15	10.040	1208	1216	1224	rBV	444494	740086	23.70%	2.869%
16	10.193	1234	1242	1254	rBV	373313	605192	19.38%	2.346%
17	11.381	1438	1444	1450	rVB5	2593	4284	0.14%	0.017%
18	11.646	1482	1489	1496	rBV	7120	10834	0.35%	0.042%
19	13.387	1777	1785	1799	rBV	994499	1368092	43.82%	5.303%
20	13.640	1821	1828	1838	rBV	1054198	1555616	49.82%	6.030%
21	13.957	1875	1882	1889	rBV	874508	1229905	39.39%	4.768%
22	14.016	1890	1892	1896	rVB2	5272	5919	0.19%	0.023%
23	14.193	1917	1922	1934	rBV	65436	126279	4.04%	0.490%
24	14.410	1957	1959	1965	rVB4	3314	4400	0.14%	0.017%
25	14.963	2047	2053	2060	rBV	1499254	2060111	65.98%	7.986%
26	15.098	2070	2076	2090	rVV	432613	565772	18.12%	2.193%
27	15.204	2090	2094	2098	rVB2	5814	7466	0.24%	0.029%
28	16.275	2271	2276	2285	rBV7	2131	4790	0.15%	0.019%
29	16.722	2346	2352	2363	rBV	1139350	1536997	49.23%	5.958%
30	16.822	2363	2369	2382	rVB	1700764	2326315	74.51%	9.018%
31	17.669	2509	2513	2516	rBV	10402	11996	0.38%	0.047%
32	18.698	2684	2688	2693	rBV2	19830	25686	0.82%	0.100%
33	18.775	2696	2701	2707	rBV	19525	23432	0.75%	0.091%
34	18.851	2710	2714	2724	rVV	56666	74695	2.39%	0.290%
35	18.975	2732	2735	2740	rBV6	11365	15963	0.51%	0.062%
36	19.145	2757	2764	2772	rBV	2151275	2885376	92.41%	11.185%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035477.D
Acq On : 07 Dec 2024 01:37
Operator : RC/JU
Sample : P5107-14
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ91

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	20.975	3069	3075	3085	rBV	1433116	1840736	58.96%	7.136%
38	23.469	3490	3499	3512	rBV	1421302	3122270	100.00%	12.103%
39	23.645	3521	3529	3539	rBV	907980	1973132	63.20%	7.649%




Sum of corrected areas: 25796599

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035477.D
Acq On : 07 Dec 2024 01:37
Operator : RC/JU
Sample : P5107-14
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

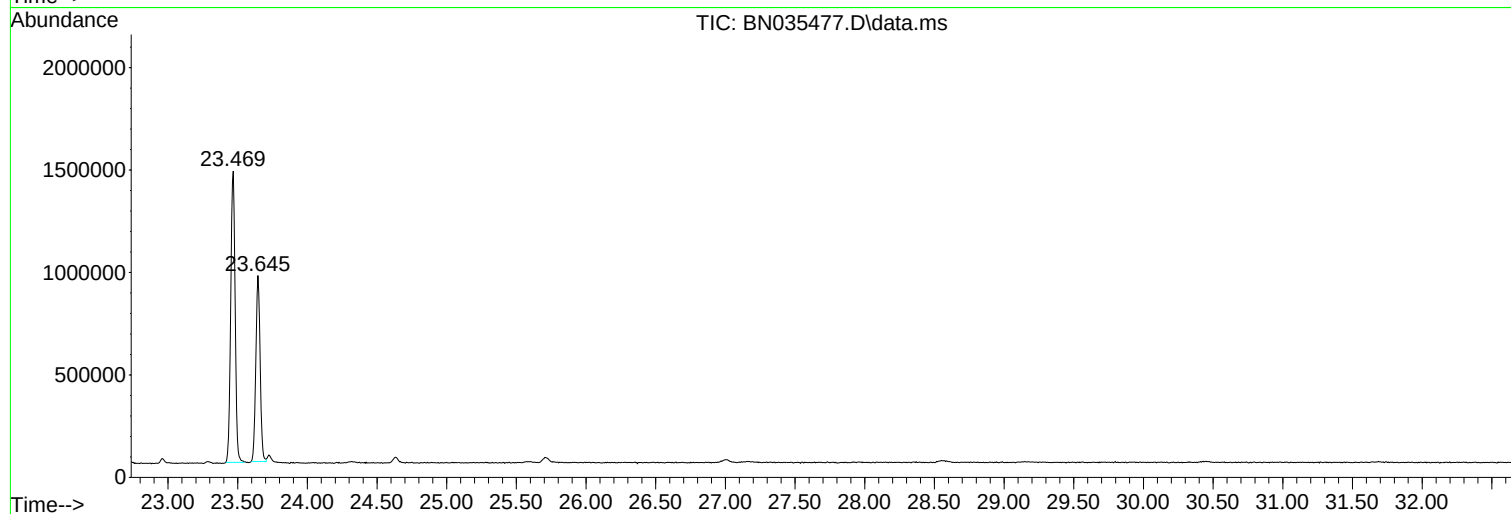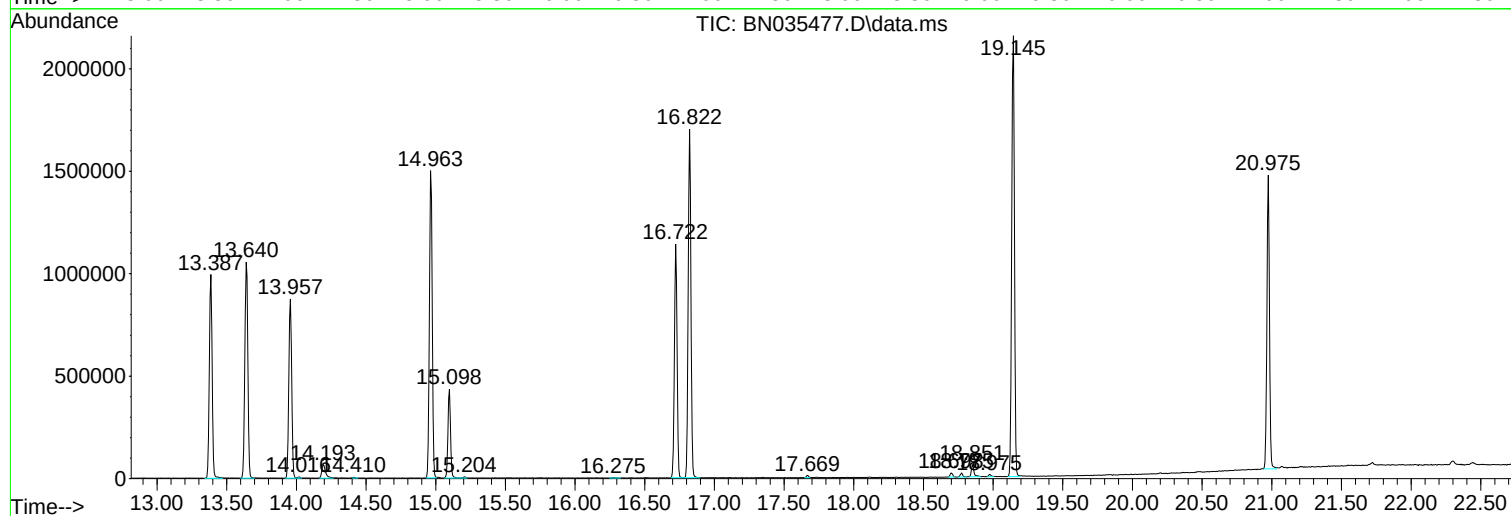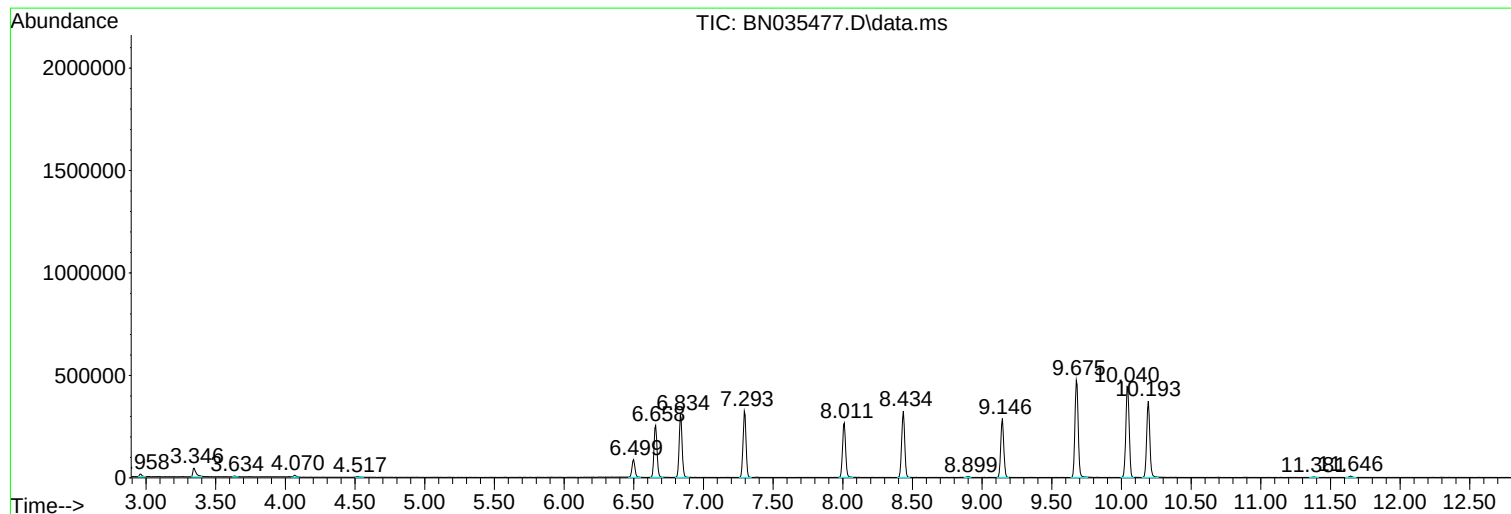

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035477.D
Acq On : 07 Dec 2024 01:37
Operator : RC/JU
Sample : P5107-14
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035477.D
Acq On : 07 Dec 2024 01:37
Operator : RC/JU
Sample : P5107-14
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc