

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035484.D
 Acq On : 07 Dec 2024 10:31
 Operator : RC/JU
 Sample : PB165451BL
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK451

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.952	8	11	18	rBV	22942	29693	1.00%	0.097%
2	3.346	75	78	98	rBV	137943	349114	11.70%	1.146%
3	3.628	123	126	133	rVB2	6806	9651	0.32%	0.032%
4	4.064	199	200	208	rVB3	3333	5270	0.18%	0.017%
5	4.828	327	330	337	rBV5	2214	4246	0.14%	0.014%
6	5.416	428	430	436	rVB6	2749	3220	0.11%	0.011%
7	6.493	607	613	626	rVB	458651	695313	23.31%	2.282%
8	6.646	633	639	651	rVB	307150	453816	15.21%	1.489%
9	6.828	661	670	681	rVB	466105	707278	23.71%	2.321%
10	7.287	740	748	755	rBV	408585	616264	20.66%	2.022%
11	8.005	863	870	884	rBV	583744	897169	30.07%	2.944%
12	8.428	935	942	950	rBV	362115	565140	18.94%	1.855%
13	9.140	1056	1063	1071	rVB	327581	499460	16.74%	1.639%
14	9.675	1147	1154	1167	rBV	594169	983123	32.96%	3.226%
15	10.034	1209	1215	1226	rBV	527372	873262	29.27%	2.866%
16	10.187	1234	1241	1258	rBV	357446	696934	23.36%	2.287%
17	11.504	1456	1465	1472	rBV2	10820	21436	0.72%	0.070%
18	11.640	1482	1488	1493	rBV2	8077	13136	0.44%	0.043%
19	13.381	1778	1784	1795	rBV	1030628	1453645	48.73%	4.771%
20	13.640	1821	1828	1838	rBV	1113989	1661212	55.69%	5.452%
21	13.951	1875	1881	1888	rBV	977216	1433531	48.05%	4.705%
22	14.192	1915	1922	1941	rBV	355655	663261	22.23%	2.177%
23	14.816	2023	2028	2034	rBV6	2240	5086	0.17%	0.017%
24	14.963	2046	2053	2067	rBV	1555465	2201628	73.80%	7.225%
25	15.092	2070	2075	2086	rVV	420369	567176	19.01%	1.861%
26	15.204	2090	2094	2100	rVB3	6328	8502	0.28%	0.028%
27	15.463	2133	2138	2142	rBV5	2747	5634	0.19%	0.018%
28	16.104	2244	2247	2252	rBV3	2058	3235	0.11%	0.011%
29	16.269	2269	2275	2282	rBV3	15700	24297	0.81%	0.080%
30	16.510	2311	2316	2322	rVB4	2816	4328	0.15%	0.014%
31	16.657	2338	2341	2345	rBV2	3816	3965	0.13%	0.013%
32	16.722	2345	2352	2362	rVV	1411270	1912090	64.10%	6.275%
33	16.822	2362	2369	2380	rVV	1836119	2466053	82.66%	8.093%
34	17.345	2454	2458	2463	rBV2	12380	16732	0.56%	0.055%
35	17.669	2510	2513	2516	rBV5	2222	3128	0.10%	0.010%
36	17.698	2516	2518	2523	rVV5	2192	3449	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035484.D
Acq On : 07 Dec 2024 10:31
Operator : RC/JU
Sample : PB165451BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK451

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	18.304	2617	2621	2630	rVB3	10699	14845	0.50%	0.049%
38	18.633	2672	2677	2680	rBV3	3667	4623	0.15%	0.015%
39	18.698	2684	2688	2693	rVB2	20778	27287	0.91%	0.090%
40	18.775	2696	2701	2705	rBV	20322	27590	0.92%	0.091%
41	19.063	2747	2750	2754	rVB5	3088	3787	0.13%	0.012%
42	19.145	2757	2764	2774	rBV	2144604	2975663	99.75%	9.765%
43	19.839	2879	2882	2888	rVB2	13969	16646	0.56%	0.055%
44	20.474	2987	2990	2994	rBV2	16661	20966	0.70%	0.069%
45	20.980	3070	3076	3086	rBV	1634038	2274564	76.25%	7.465%
46	21.074	3090	3092	3095	rVB2	14307	16689	0.56%	0.055%
47	23.468	3490	3499	3518	rVB	1317541	2983207	100.00%	9.790%
48	23.651	3522	3530	3540	rBV2	1034387	2245015	75.26%	7.368%




Sum of corrected areas: 30471359

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035484.D
Acq On : 07 Dec 2024 10:31
Operator : RC/JU
Sample : PB165451BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK451

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

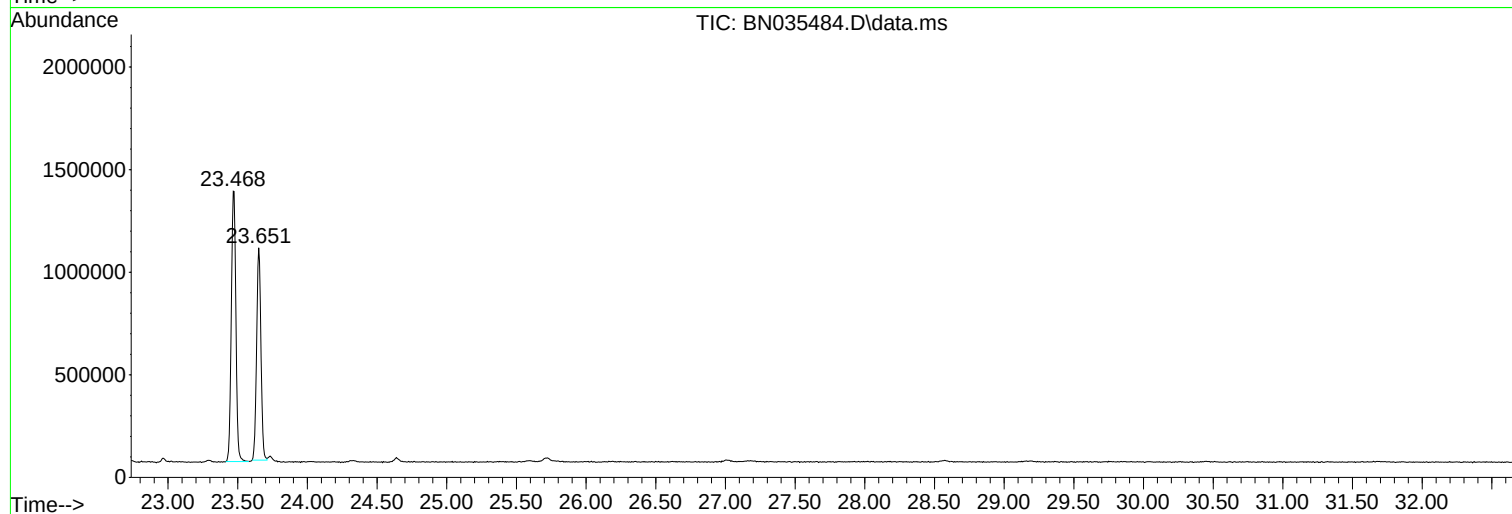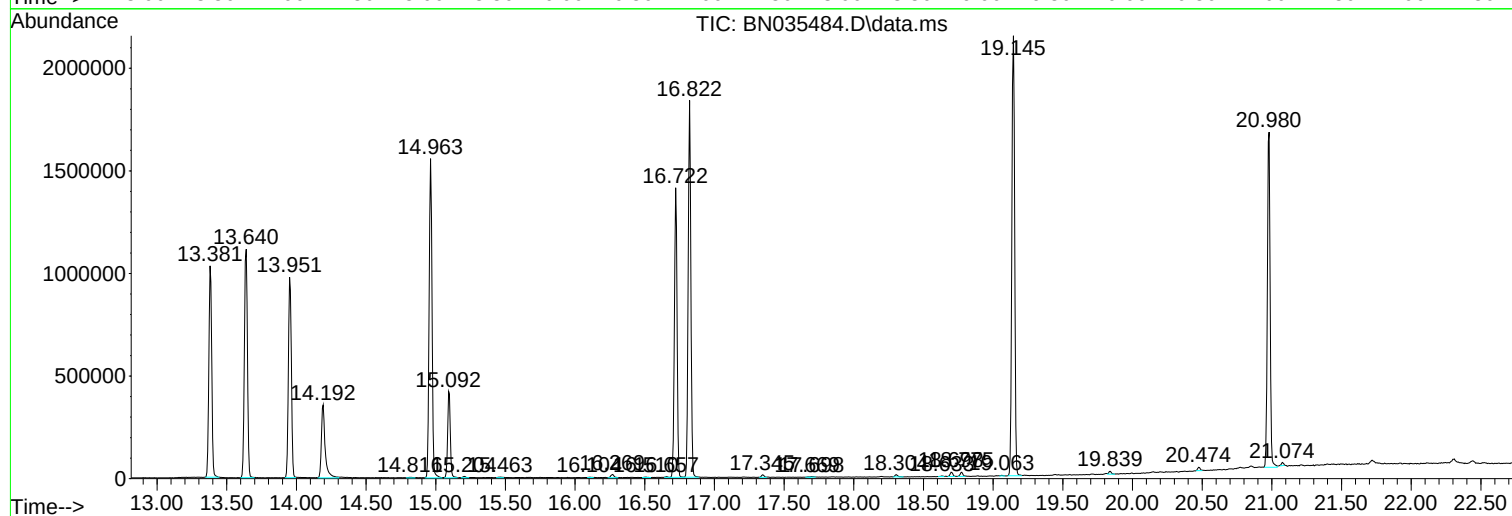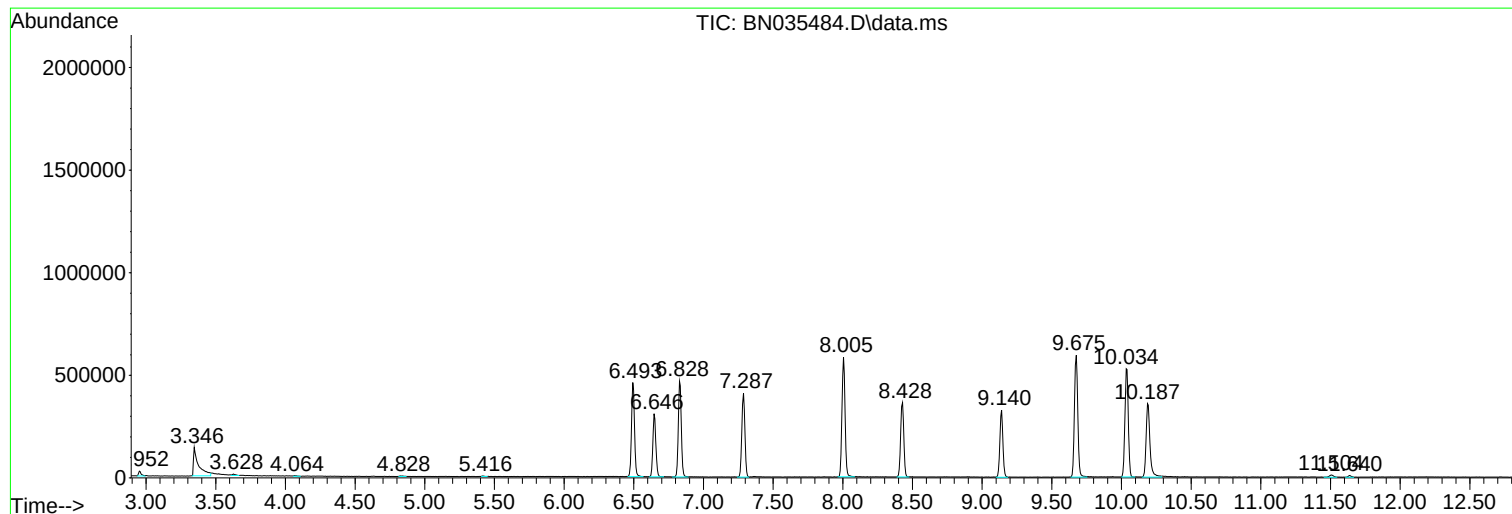

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035484.D
Acq On : 07 Dec 2024 10:31
Operator : RC/JU
Sample : PB165451BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK451

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035484.D
Acq On : 07 Dec 2024 10:31
Operator : RC/JU
Sample : PB165451BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK451

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc