

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035486.D
 Acq On : 07 Dec 2024 12:27
 Operator : RC/JU
 Sample : PB165451BL
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK451

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	8	12	19	rBV	21882	29668	0.97%	0.101%
2	3.334	72	76	96	rBV	269068	429046	14.00%	1.459%
3	3.640	124	128	133	rBV3	3372	5676	0.19%	0.019%
4	6.499	608	614	623	rVB	395629	593051	19.35%	2.016%
5	6.657	635	641	651	rVB	316990	472162	15.41%	1.605%
6	6.834	664	671	682	rBV	418866	630117	20.56%	2.142%
7	7.293	742	749	760	rBV	326379	492374	16.07%	1.674%
8	8.010	863	871	882	rBV	532946	823602	26.87%	2.800%
9	8.434	936	943	952	rBV	403505	611081	19.94%	2.077%
10	9.146	1057	1064	1071	rBV	357441	552040	18.01%	1.877%
11	9.675	1148	1154	1162	rBV	586590	935139	30.51%	3.179%
12	10.040	1209	1216	1224	rBV	474114	767696	25.05%	2.610%
13	10.193	1235	1242	1256	rBV	561930	924882	30.18%	3.144%
14	11.645	1484	1489	1495	rBV	8389	14078	0.46%	0.048%
15	13.387	1778	1785	1798	rBV	1149388	1595987	52.08%	5.425%
16	13.639	1820	1828	1840	rBV	1277763	1828382	59.66%	6.215%
17	13.957	1875	1882	1894	rBV	816765	1187935	38.76%	4.038%
18	14.186	1915	1921	1940	rBV	407340	677373	22.10%	2.303%
19	14.963	2046	2053	2065	rBV	1620347	2261472	73.79%	7.688%
20	15.098	2070	2076	2085	rBV	483187	627137	20.46%	2.132%
21	15.204	2091	2094	2100	rVB2	6464	8009	0.26%	0.027%
22	16.722	2346	2352	2363	rBV	1135085	1527265	49.83%	5.192%
23	16.822	2363	2369	2381	rVV2	1845765	2571382	83.90%	8.741%
24	18.698	2684	2688	2693	rBV	20281	26056	0.85%	0.089%
25	18.774	2696	2701	2706	rBV	19210	24378	0.80%	0.083%
26	19.145	2758	2764	2775	rBV	2327843	3064703	100.00%	10.418%
27	20.974	3070	3075	3087	rBV	1316210	1755973	57.30%	5.969%
28	22.298	3297	3300	3306	rVB6	22518	35951	1.17%	0.122%
29	22.962	3409	3413	3418	rVB2	26927	42299	1.38%	0.144%
30	23.468	3490	3499	3514	rBV	1410787	3047158	99.43%	10.359%
31	23.645	3521	3529	3538	rBV	785242	1764743	57.58%	5.999%
32	23.727	3540	3543	3556	rVB3	44427	90053	2.94%	0.306%




Sum of corrected areas: 29416868

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035486.D
Acq On : 07 Dec 2024 12:27
Operator : RC/JU
Sample : PB165451BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK451

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

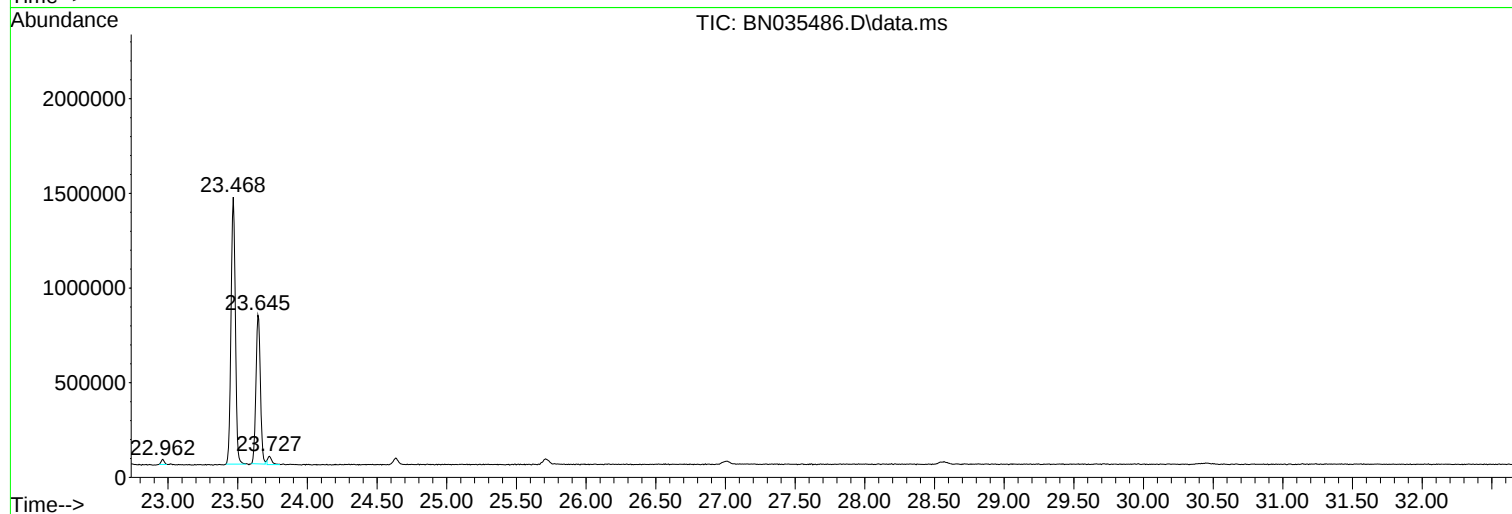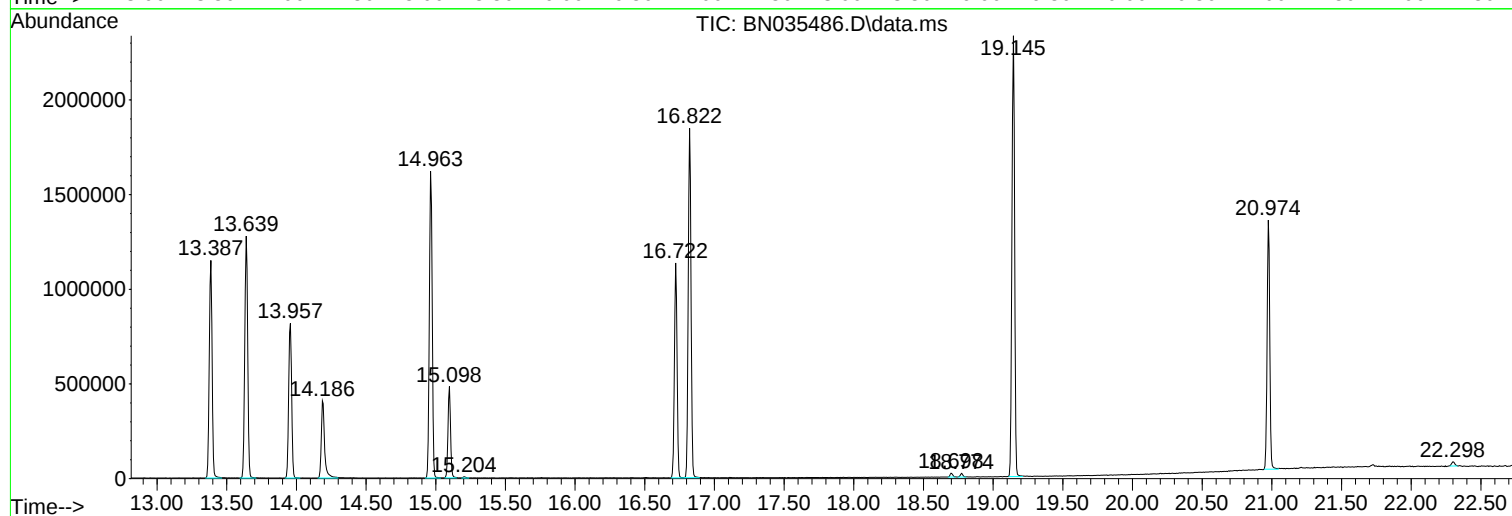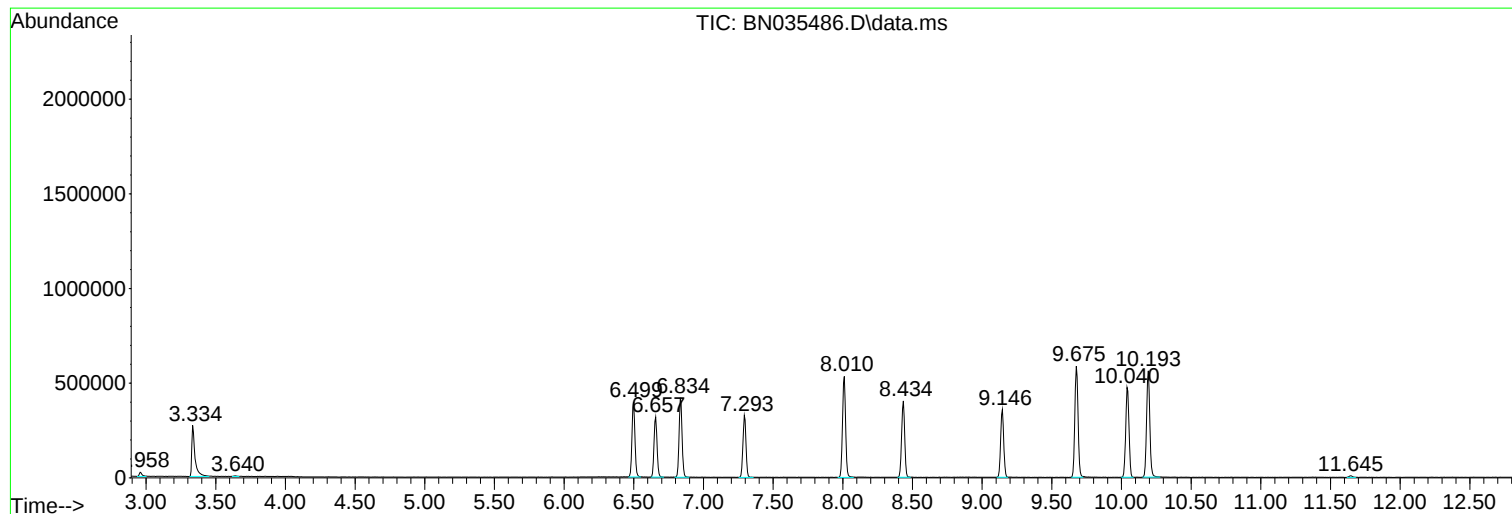

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035486.D
Acq On : 07 Dec 2024 12:27
Operator : RC/JU
Sample : PB165451BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK451

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035486.D
Acq On : 07 Dec 2024 12:27
Operator : RC/JU
Sample : PB165451BL
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK451

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc