

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035487.D
 Acq On : 07 Dec 2024 13:06
 Operator : RC/JU
 Sample : PB165449BL
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK449

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	19	rBV	18105	23762	0.80%	0.091%
2	3.334	72	76	95	rBV	230835	373028	12.55%	1.436%
3	6.499	607	614	624	rVB	339763	514983	17.32%	1.982%
4	6.658	635	641	650	rVB	265595	401948	13.52%	1.547%
5	6.834	665	671	682	rBV	356550	540622	18.18%	2.081%
6	7.293	743	749	757	rVB	266199	401600	13.51%	1.546%
7	8.010	864	871	879	rBV	454946	706083	23.75%	2.718%
8	8.434	936	943	951	rBV	341767	524058	17.63%	2.017%
9	9.146	1057	1064	1072	rBV	305073	467536	15.72%	1.800%
10	9.675	1147	1154	1165	rBV	494407	797603	26.83%	3.070%
11	10.040	1209	1216	1225	rBV	381299	614468	20.67%	2.365%
12	10.193	1235	1242	1258	rBV	468848	778694	26.19%	2.997%
13	11.646	1482	1489	1496	rBV2	6678	11546	0.39%	0.044%
14	13.387	1778	1785	1797	rBV	969398	1386110	46.62%	5.335%
15	13.640	1821	1828	1840	rBV	1128534	1597469	53.73%	6.149%
16	13.957	1875	1882	1893	rBV	689250	1014105	34.11%	3.903%
17	14.187	1915	1921	1942	rBV	361778	600931	20.21%	2.313%
18	14.963	2046	2053	2066	rBV	1435131	2031269	68.32%	7.818%
19	15.098	2070	2076	2090	rVV	412621	551712	18.56%	2.123%
20	15.204	2090	2094	2101	rVB4	6278	9451	0.32%	0.036%
21	16.510	2310	2316	2320	rBV4	2088	3667	0.12%	0.014%
22	16.722	2346	2352	2362	rBV	942275	1283125	43.15%	4.939%
23	16.822	2362	2369	2385	rVB	1700884	2301452	77.40%	8.858%
24	18.698	2684	2688	2695	rBV	20116	26825	0.90%	0.103%
25	18.775	2697	2701	2705	rVB	15367	20065	0.67%	0.077%
26	19.145	2757	2764	2779	rBV	2077959	2803463	94.29%	10.790%
27	20.974	3070	3075	3084	rBV2	1213844	1581059	53.17%	6.085%
28	23.468	3490	3499	3512	rBV	1352811	2973339	100.00%	11.444%
29	23.645	3521	3529	3538	rBV	747329	1641322	55.20%	6.317%




Sum of corrected areas: 25981295

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035487.D
Acq On : 07 Dec 2024 13:06
Operator : RC/JU
Sample : PB165449BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

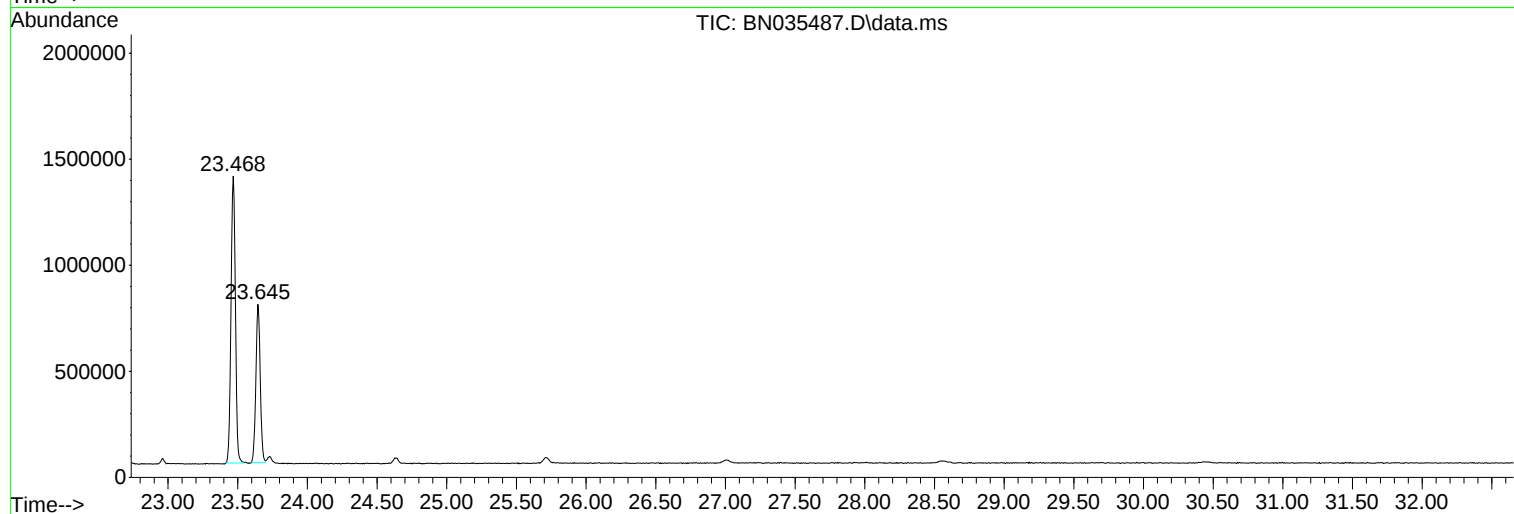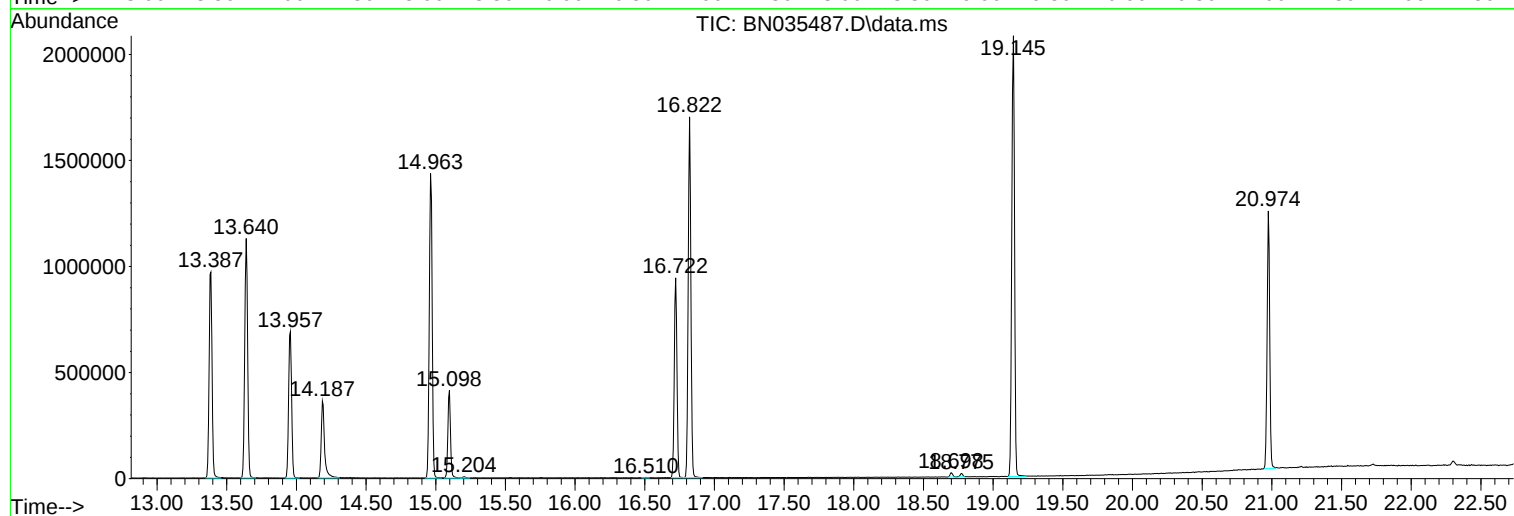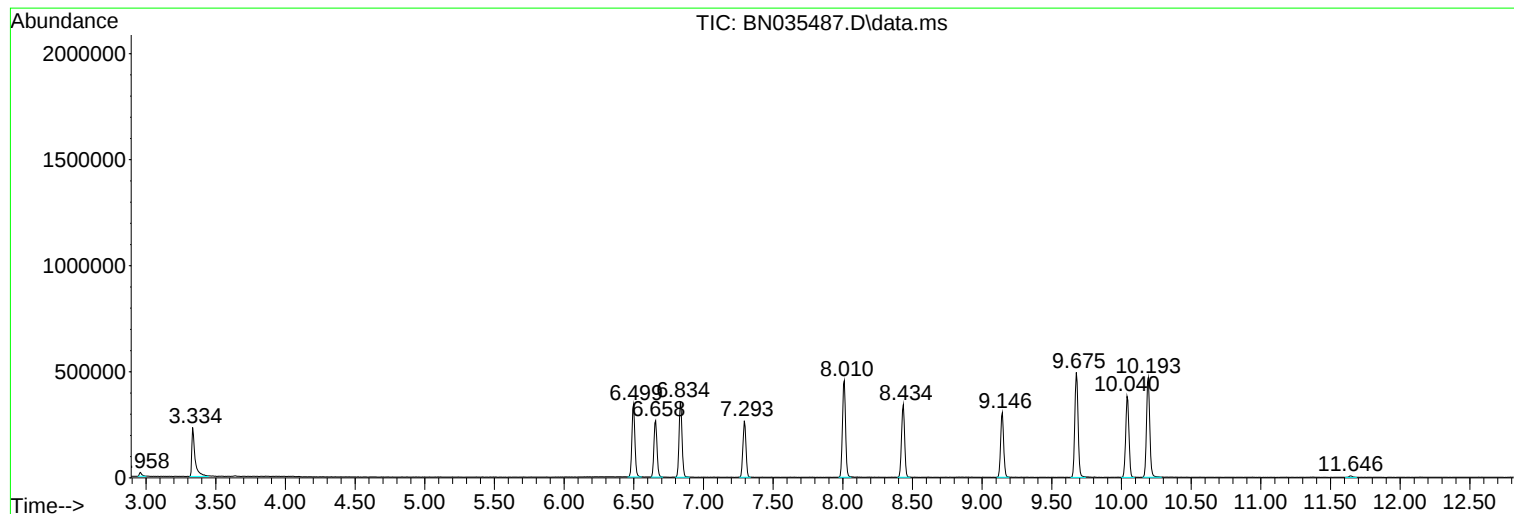

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035487.D
Acq On : 07 Dec 2024 13:06
Operator : RC/JU
Sample : PB165449BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035487.D
Acq On : 07 Dec 2024 13:06
Operator : RC/JU
Sample : PB165449BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc