

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035488.D
 Acq On : 07 Dec 2024 13:45
 Operator : RC/JU
 Sample : P5114-04
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1PK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	10	13	19	rVB	17310	22955	0.54%	0.067%
2	3.346	74	78	88	rBV	51798	88236	2.07%	0.257%
3	3.634	125	127	133	rVB2	6645	8756	0.21%	0.025%
4	3.987	182	187	191	rBV4	8420	11851	0.28%	0.034%
5	4.516	272	277	281	rBV2	13529	18495	0.43%	0.054%
6	6.499	608	614	621	rVB	110207	169077	3.97%	0.492%
7	6.658	634	641	648	rBV	345746	528098	12.41%	1.537%
8	6.834	664	671	685	rVB	416088	637819	14.99%	1.856%
9	7.005	697	700	705	rBV6	3492	5498	0.13%	0.016%
10	7.293	740	749	759	rBV	427320	644021	15.14%	1.874%
11	8.010	864	871	884	rBV	355701	559212	13.14%	1.627%
12	8.434	935	943	956	rVB	453033	695114	16.34%	2.023%
13	8.616	970	974	981	rVB3	11966	16592	0.39%	0.048%
14	8.899	1018	1022	1026	rVB2	4450	5348	0.13%	0.016%
15	9.146	1057	1064	1076	rBV	403223	622477	14.63%	1.812%
16	9.410	1105	1109	1116	rBV4	4444	8872	0.21%	0.026%
17	9.675	1147	1154	1166	rBV	655541	1044073	24.54%	3.039%
18	10.040	1207	1216	1223	rBV	598633	974568	22.91%	2.836%
19	10.193	1234	1242	1255	rBV	441328	738868	17.37%	2.150%
20	10.881	1353	1359	1364	rBV2	16618	28119	0.66%	0.082%
21	11.646	1484	1489	1493	rVB2	8118	12684	0.30%	0.037%
22	13.387	1778	1785	1797	rBV	1264857	1731190	40.69%	5.038%
23	13.640	1821	1828	1836	rBV	1350336	2005609	47.14%	5.837%
24	13.957	1872	1882	1893	rBV	1081685	1570294	36.91%	4.570%
25	14.192	1916	1922	1933	rBV	100916	179714	4.22%	0.523%
26	14.410	1956	1959	1964	rVB4	8508	11185	0.26%	0.033%
27	14.963	2047	2053	2065	rVB	1868139	2603970	61.20%	7.578%
28	15.098	2070	2076	2085	rBV	615822	795383	18.69%	2.315%
29	15.204	2090	2094	2098	rVB2	6418	9075	0.21%	0.026%
30	16.504	2310	2315	2319	rBV3	2671	4375	0.10%	0.013%
31	16.722	2345	2352	2360	rBV	1454921	1972599	46.36%	5.741%
32	16.822	2362	2369	2382	rBV	2205765	3040182	71.46%	8.848%
33	17.669	2508	2513	2519	rBV	18966	24323	0.57%	0.071%
34	18.698	2684	2688	2694	rBV2	28091	39249	0.92%	0.114%
35	18.775	2696	2701	2707	rVB	24904	33714	0.79%	0.098%
36	18.975	2732	2735	2741	rVB4	13537	15292	0.36%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035488.D
Acq On : 07 Dec 2024 13:45
Operator : RC/JU
Sample : P5114-04
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PK0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Title : SVOA CALIBRATION

37	19.145	2758	2764	2775	rBV	2718015	3746667	88.06%	10.904%
38	19.986	2904	2907	2910	rBV5	5428	7372	0.17%	0.021%
39	20.080	2919	2923	2930	rBV	64976	91872	2.16%	0.267%
40	20.198	2941	2943	2947	rVB5	5367	4260	0.10%	0.012%
41	20.974	3069	3075	3088	rBV2	1887829	2525620	59.36%	7.350%
42	22.298	3298	3300	3305	rVB3	21812	27649	0.65%	0.080%
43	22.963	3408	3413	3419	rVB4	29816	55246	1.30%	0.161%
44	23.468	3490	3499	3517	rVB	1890944	4254594	100.00%	12.382%
45	23.651	3521	3530	3538	rBV	1245901	2770819	65.13%	8.064%




Sum of corrected areas: 34360986

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035488.D
Acq On : 07 Dec 2024 13:45
Operator : RC/JU
Sample : P5114-04
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PK0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

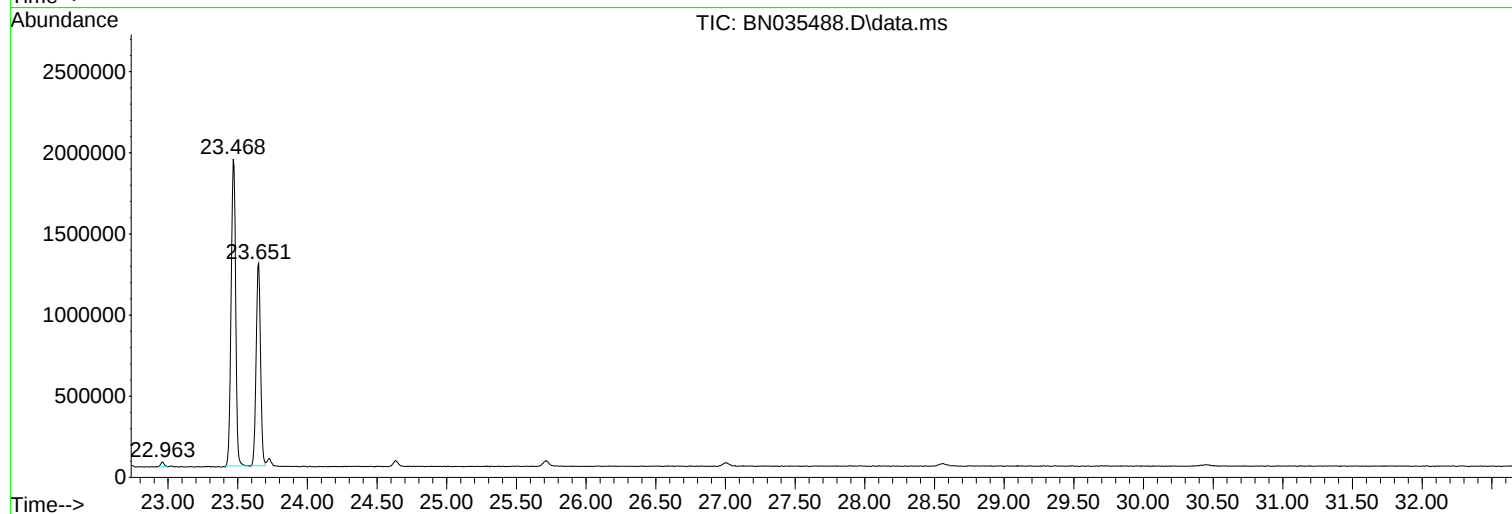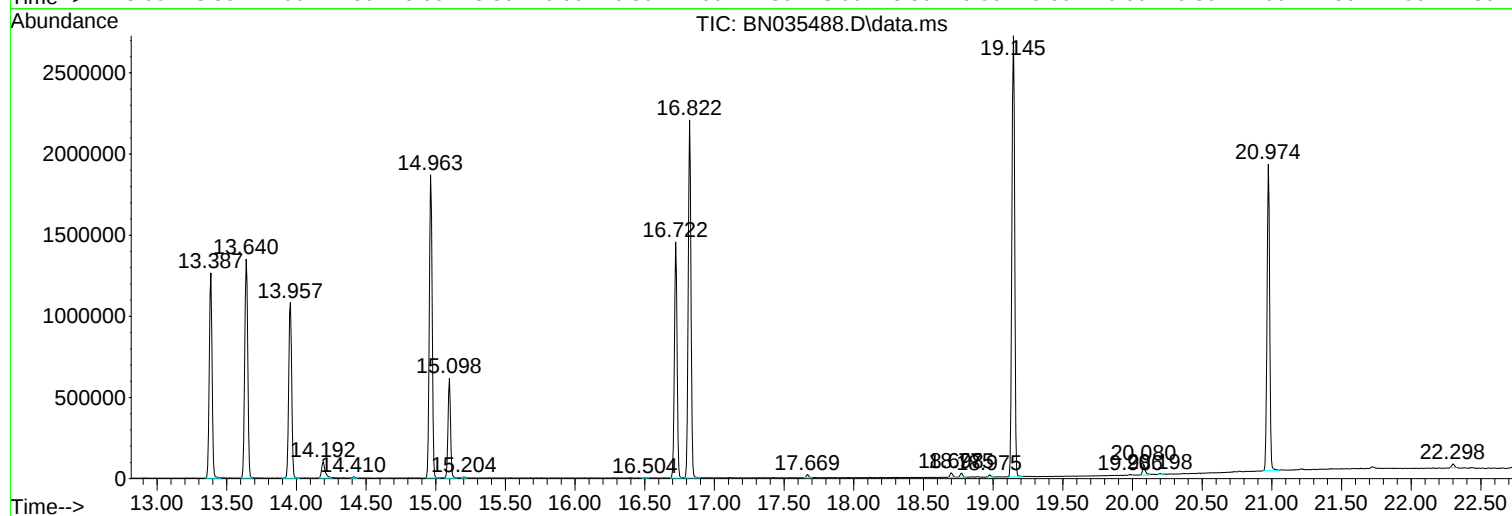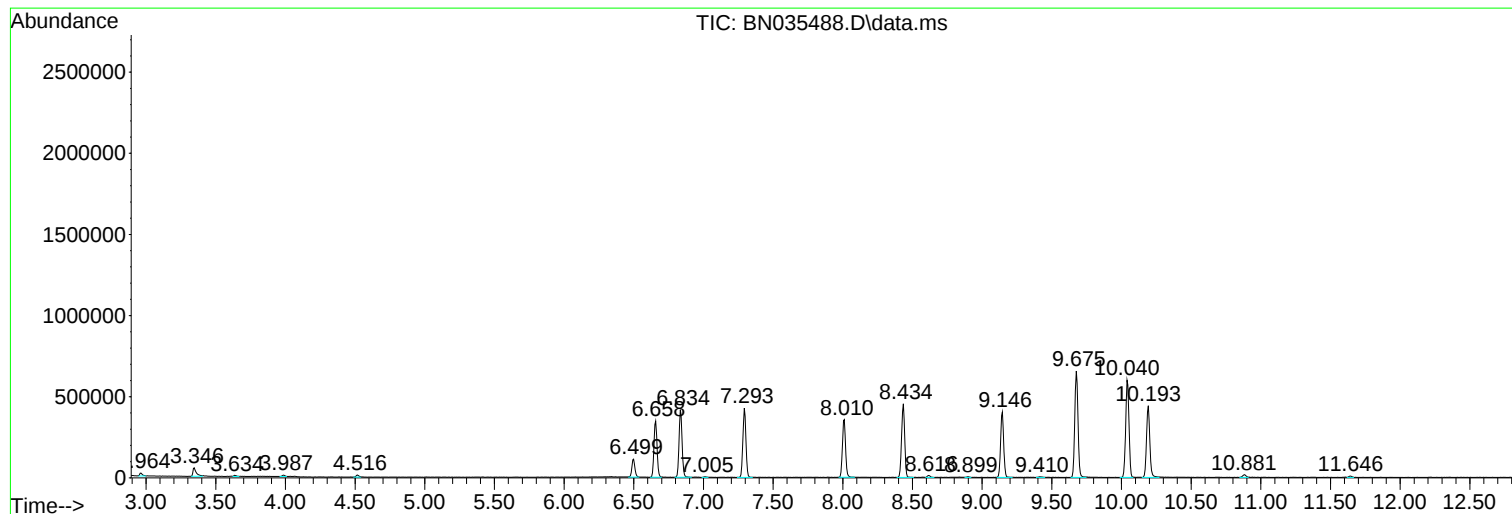

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035488.D
Acq On : 07 Dec 2024 13:45
Operator : RC/JU
Sample : P5114-04
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PK0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035488.D
Acq On : 07 Dec 2024 13:45
Operator : RC/JU
Sample : P5114-04
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PK0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------