

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035492.D
 Acq On : 07 Dec 2024 16:21
 Operator : RC/JU
 Sample : P5107-19
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	9	12	21	rVB	15697	21830	0.61%	0.078%
2	3.346	74	78	92	rBV	34742	57471	1.61%	0.205%
3	3.634	124	127	133	rVB2	3810	5225	0.15%	0.019%
4	4.069	196	201	208	rVB	11301	17215	0.48%	0.061%
5	4.516	272	277	283	rBV2	8960	13084	0.37%	0.047%
6	6.499	608	614	625	rVB	103424	160117	4.50%	0.570%
7	6.658	635	641	650	rBV	281789	427837	12.02%	1.523%
8	6.834	665	671	683	rVB	339931	512391	14.40%	1.824%
9	7.293	743	749	759	rVB	293889	437601	12.29%	1.558%
10	8.010	864	871	882	rBV	316462	477878	13.43%	1.702%
11	8.434	934	943	953	rBV	366388	556064	15.62%	1.980%
12	8.899	1015	1022	1027	rVB3	4623	7439	0.21%	0.026%
13	9.146	1057	1064	1076	rVB	324618	497403	13.97%	1.771%
14	9.675	1147	1154	1169	rBV	522738	843955	23.71%	3.005%
15	10.046	1210	1217	1226	rVB	409420	675235	18.97%	2.404%
16	10.193	1235	1242	1253	rBV	355128	590604	16.59%	2.103%
17	11.387	1439	1445	1449	rVB3	4166	5541	0.16%	0.020%
18	11.646	1484	1489	1494	rVB	6072	10084	0.28%	0.036%
19	13.387	1778	1785	1798	rBV	1111914	1532904	43.07%	5.458%
20	13.640	1822	1828	1840	rBV	1174413	1711394	48.08%	6.094%
21	13.957	1875	1882	1889	rBV	777777	1110986	31.21%	3.956%
22	14.192	1916	1922	1937	rBV	88277	161038	4.52%	0.573%
23	14.410	1952	1959	1964	rVB5	4253	6585	0.19%	0.023%
24	14.822	2024	2029	2035	rBV	5965	7750	0.22%	0.028%
25	14.963	2047	2053	2060	rBV	1627290	2231815	62.70%	7.947%
26	15.098	2070	2076	2086	rVV	528765	667353	18.75%	2.376%
27	15.204	2090	2094	2100	rVB3	6047	8386	0.24%	0.030%
28	15.739	2180	2185	2194	rVB2	9423	14919	0.42%	0.053%
29	16.533	2313	2320	2325	rBV2	23624	34004	0.96%	0.121%
30	16.586	2325	2329	2335	rVV3	6394	10739	0.30%	0.038%
31	16.722	2346	2352	2359	rBV	1053021	1396359	39.23%	4.972%
32	16.822	2362	2369	2384	rVV	1961229	2675533	75.17%	9.527%
33	16.963	2388	2393	2397	rBV5	6791	10807	0.30%	0.038%
34	17.192	2429	2432	2438	rVB5	3830	6158	0.17%	0.022%
35	17.275	2441	2446	2452	rBV2	35208	43474	1.22%	0.155%
36	17.451	2469	2476	2480	rVB	11088	14917	0.42%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035492.D
 Acq On : 07 Dec 2024 16:21
 Operator : RC/JU
 Sample : P5107-19
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHJ98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

37	17.669	2509	2513	2519	rBV2	31903	42248	1.19%	0.150%
38	17.780	2529	2532	2539	rBV8	2614	6415	0.18%	0.023%
39	17.975	2560	2565	2570	rBV	37371	44306	1.24%	0.158%
40	18.080	2579	2583	2587	rBV7	2310	4207	0.12%	0.015%
41	18.122	2587	2590	2593	rVB3	4257	5589	0.16%	0.020%
42	18.445	2642	2645	2649	rBV4	3999	4402	0.12%	0.016%
43	18.622	2668	2675	2683	rBV4	33622	84425	2.37%	0.301%
44	18.698	2684	2688	2694	rVB	28131	38478	1.08%	0.137%
45	18.775	2697	2701	2705	rBV	28229	36441	1.02%	0.130%
46	18.822	2705	2709	2712	rBV	52260	67600	1.90%	0.241%
47	18.857	2712	2715	2726	rVB2	81083	124071	3.49%	0.442%
48	18.980	2732	2736	2740	rBV	19452	26732	0.75%	0.095%
49	19.145	2757	2764	2773	rBV2	2457213	3322253	93.34%	11.829%
50	19.216	2773	2776	2780	rVB	23695	25764	0.72%	0.092%
51	19.763	2865	2869	2874	rBV3	13511	18509	0.52%	0.066%
52	20.216	2944	2946	2950	rVV3	8267	8581	0.24%	0.031%
53	20.263	2952	2954	2958	rVB4	9413	10905	0.31%	0.039%
54	20.974	3070	3075	3084	rBV	1376424	1743435	48.98%	6.208%
55	21.892	3227	3231	3237	rVB	96880	127529	3.58%	0.454%
56	23.468	3490	3499	3517	rBV	1627048	3559421	100.00%	12.674%
57	23.645	3521	3529	3539	rBV2	804203	1821627	51.18%	6.486%




Sum of corrected areas: 28085033

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035492.D
Acq On : 07 Dec 2024 16:21
Operator : RC/JU
Sample : P5107-19
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

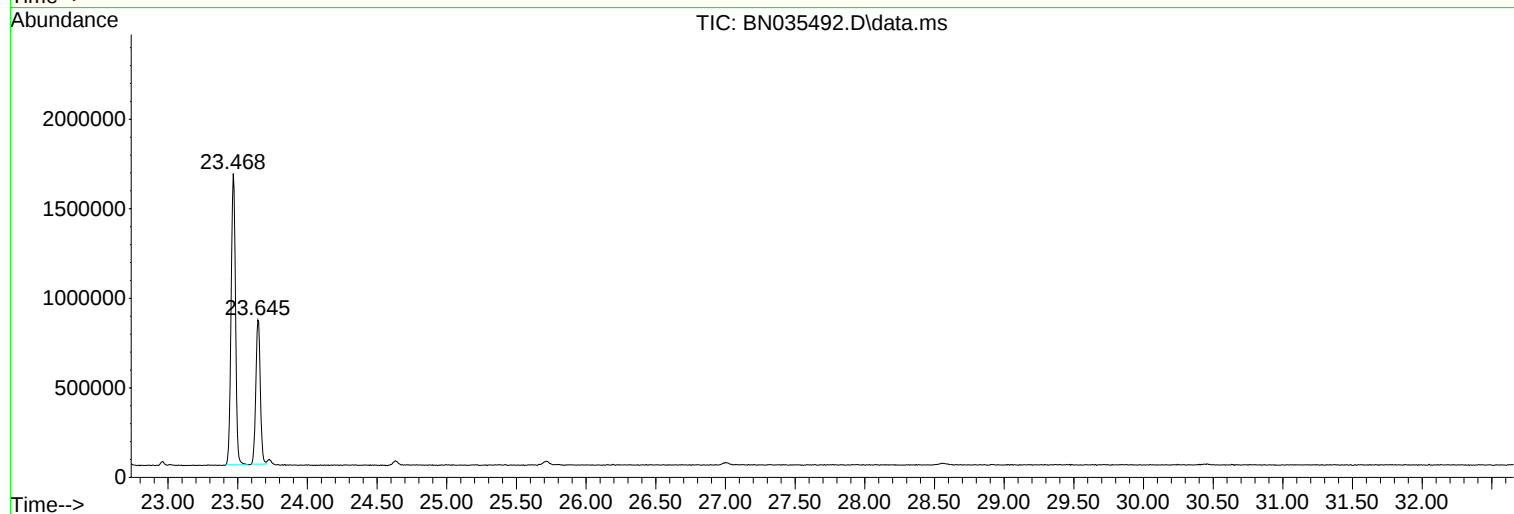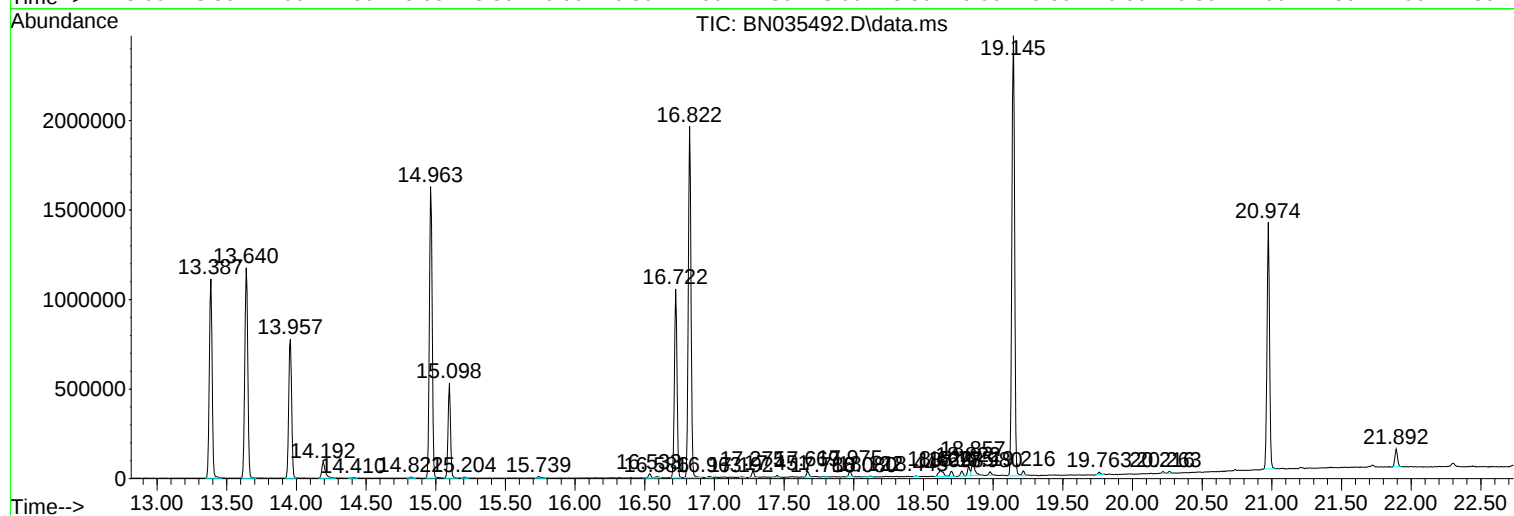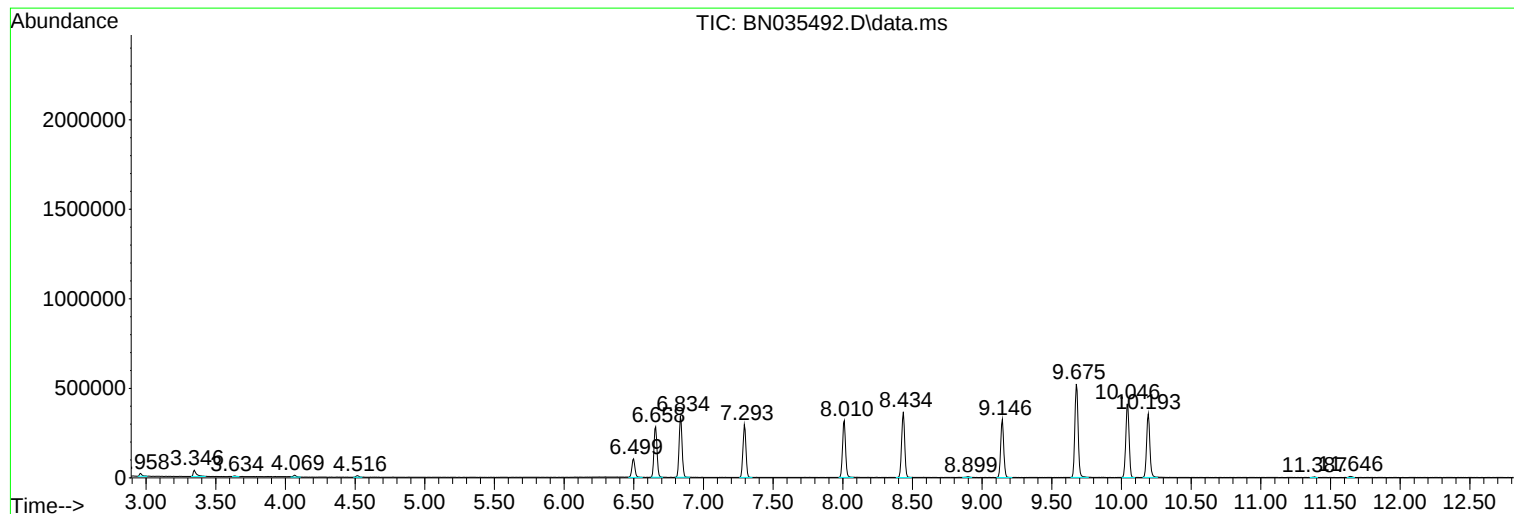

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035492.D
Acq On : 07 Dec 2024 16:21
Operator : RC/JU
Sample : P5107-19
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035492.D
Acq On : 07 Dec 2024 16:21
Operator : RC/JU
Sample : P5107-19
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHJ98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc