

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035495.D
 Acq On : 07 Dec 2024 18:18
 Operator : RC/JU
 Sample : P5114-03
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1PJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN035495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	8	12	21	rVB	14925	19722	0.57%	0.070%
2	3.340	74	77	92	rBV	58963	97604	2.84%	0.345%
3	3.634	124	127	132	rVB2	3880	5711	0.17%	0.020%
4	3.981	182	186	191	rVB6	6858	9864	0.29%	0.035%
5	4.069	197	201	206	rVB	10903	15293	0.44%	0.054%
6	4.517	273	277	283	rVB2	6525	8259	0.24%	0.029%
7	6.499	608	614	620	rBV	89826	134390	3.90%	0.476%
8	6.652	634	640	650	rBV	277125	423640	12.31%	1.499%
9	6.834	664	671	683	rBV	341431	507930	14.76%	1.797%
10	7.010	698	701	704	rVB3	3891	4372	0.13%	0.015%
11	7.293	742	749	756	rBV	297974	443375	12.88%	1.569%
12	8.010	864	871	880	rBV	272866	418230	12.15%	1.480%
13	8.434	936	943	955	rBV	358198	555258	16.13%	1.965%
14	8.616	970	974	979	rVB3	10459	14084	0.41%	0.050%
15	8.899	1015	1022	1027	rVB2	5481	7706	0.22%	0.027%
16	9.146	1057	1064	1072	rBV	322543	498222	14.47%	1.763%
17	9.675	1148	1154	1166	rBV	534545	859566	24.97%	3.042%
18	10.040	1209	1216	1225	rBV	428043	690114	20.05%	2.442%
19	10.193	1235	1242	1257	rBV	396542	667967	19.41%	2.364%
20	10.881	1353	1359	1364	rBV5	6534	10158	0.30%	0.036%
21	11.381	1440	1444	1449	rBV2	3142	5137	0.15%	0.018%
22	11.646	1484	1489	1494	rBV	6942	11632	0.34%	0.041%
23	13.387	1778	1785	1799	rBV	1200285	1627929	47.30%	5.760%
24	13.640	1821	1828	1841	rBV	1269686	1807016	52.50%	6.394%
25	13.957	1875	1882	1893	rBV	791524	1146626	33.31%	4.057%
26	14.192	1913	1922	1936	rBV	84724	152670	4.44%	0.540%
27	14.410	1957	1959	1964	rVB5	4390	5233	0.15%	0.019%
28	14.963	2047	2053	2060	rBV	1699952	2421150	70.34%	8.567%
29	15.016	2060	2062	2070	rVV5	3906	5484	0.16%	0.019%
30	15.098	2070	2076	2086	rVV	563258	714046	20.75%	2.527%
31	15.204	2090	2094	2098	rVB3	7636	9278	0.27%	0.033%
32	15.345	2113	2118	2123	rBV	33269	42336	1.23%	0.150%
33	16.292	2272	2279	2285	rBV5	3618	7654	0.22%	0.027%
34	16.722	2346	2352	2363	rBV	1064505	1425869	41.43%	5.045%
35	16.822	2363	2369	2383	rVB	1993976	2748738	79.86%	9.726%
36	17.669	2508	2513	2520	rBV2	30233	39206	1.14%	0.139%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
 Data File : BN035495.D
 Acq On : 07 Dec 2024 18:18
 Operator : RC/JU
 Sample : P5114-03
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1PJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
 Title : SVOA CALIBRATION

37	17.945	2555	2560	2566	rBV6	3425	5298	0.15%	0.019%
38	18.116	2585	2589	2593	rVB7	4588	6808	0.20%	0.024%
39	18.504	2652	2655	2660	rVB5	3031	3796	0.11%	0.013%
40	18.698	2684	2688	2696	rBV	25338	33591	0.98%	0.119%
41	18.775	2696	2701	2704	rBV	24002	30132	0.88%	0.107%
42	18.851	2711	2714	2725	rVB9	8830	16117	0.47%	0.057%
43	18.975	2731	2735	2740	rBV4	11713	15501	0.45%	0.055%
44	19.145	2757	2764	2776	rBV	2499632	3332361	96.82%	11.791%
45	19.980	2904	2906	2911	rBV4	3904	4768	0.14%	0.017%
46	20.080	2919	2923	2928	rBV	61370	77303	2.25%	0.274%
47	20.727	3029	3033	3037	rBV6	19283	34529	1.00%	0.122%
48	20.974	3069	3075	3087	rBV	1303980	1681770	48.86%	5.951%
49	22.298	3297	3300	3308	rVB5	28630	48635	1.41%	0.172%
50	22.957	3408	3412	3419	rVB3	33228	57087	1.66%	0.202%
51	23.468	3489	3499	3516	rBV	1564340	3441975	100.00%	12.179%
52	23.645	3520	3529	3538	rVV	784939	1735072	50.41%	6.140%
53	23.727	3539	3543	3551	rVB3	48335	95346	2.77%	0.337%
54	24.627	3692	3696	3703	rVB4	37097	79224	2.30%	0.280%




Sum of corrected areas: 28260782

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035495.D
Acq On : 07 Dec 2024 18:18
Operator : RC/JU
Sample : P5114-03
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

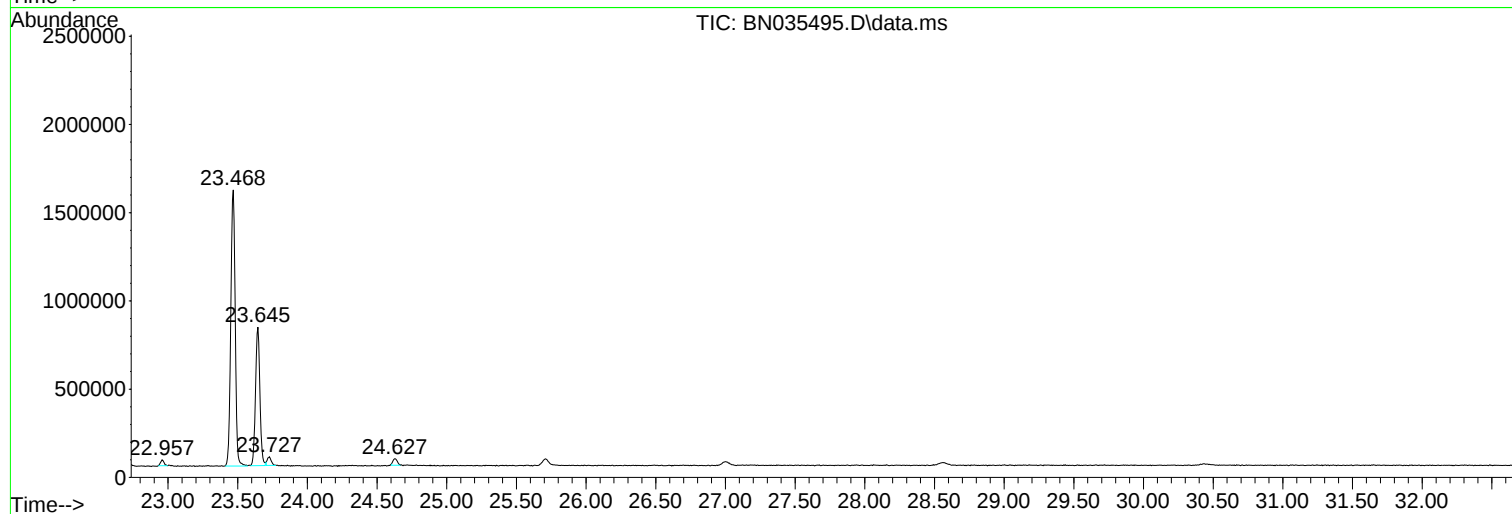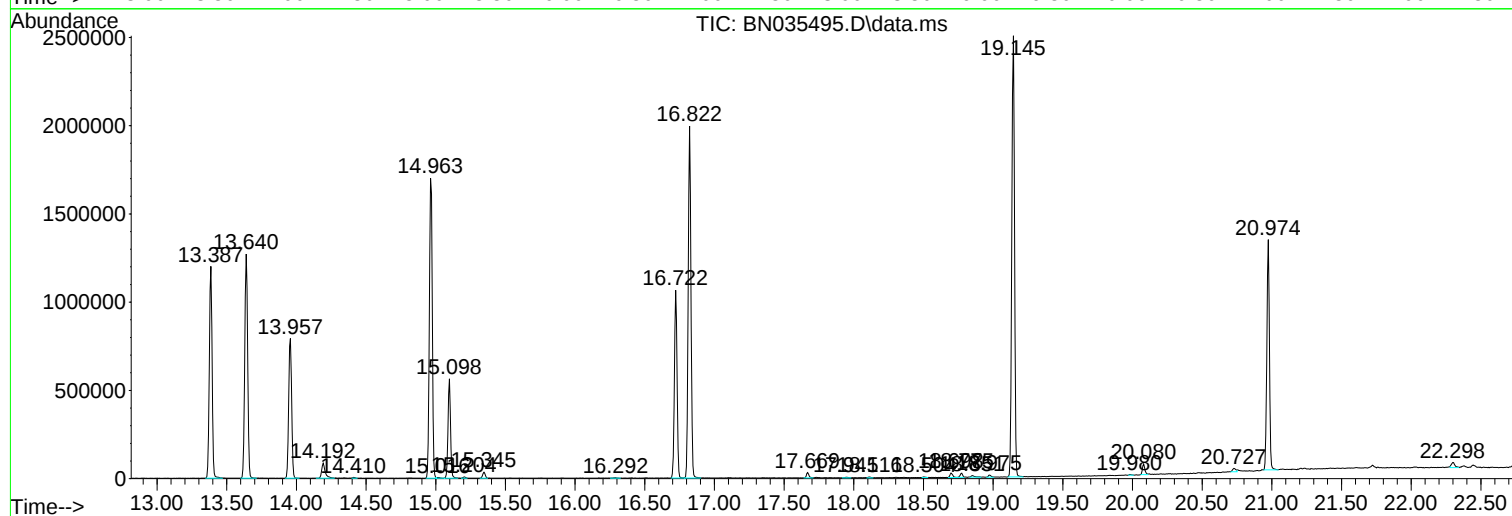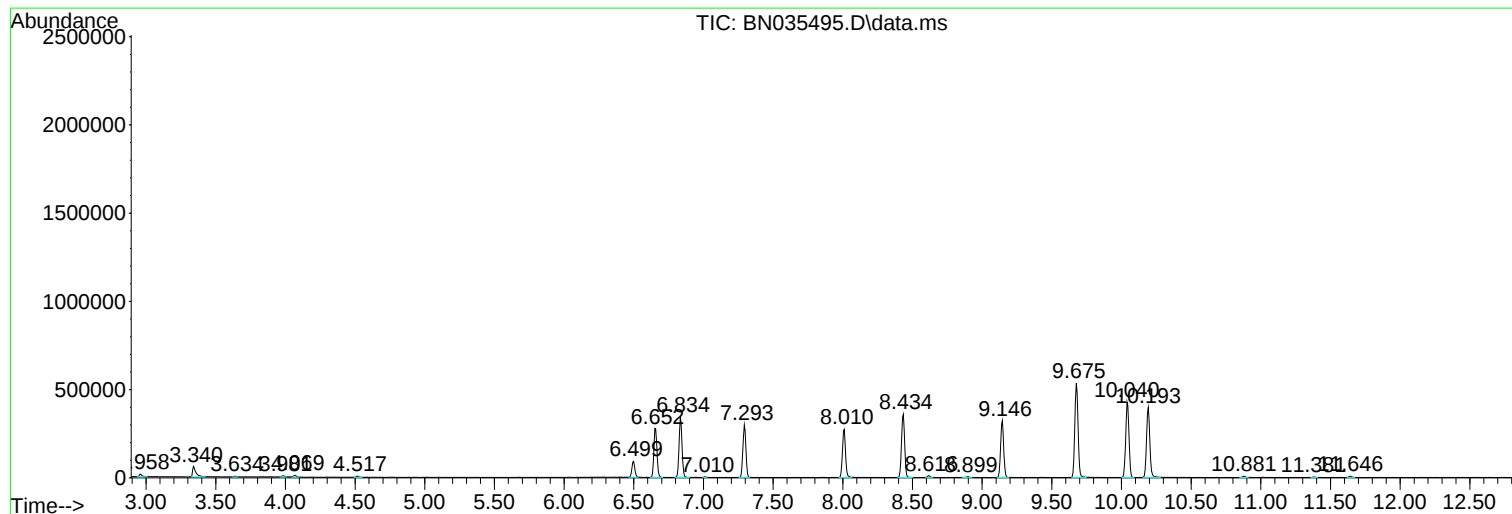

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035495.D
Acq On : 07 Dec 2024 18:18
Operator : RC/JU
Sample : P5114-03
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120624\
Data File : BN035495.D
Acq On : 07 Dec 2024 18:18
Operator : RC/JU
Sample : P5114-03
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1PJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN120224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------