

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003761.D
 Acq On : 07 Dec 2018 11:55
 Operator : JU/SJ
 Sample : PB115374BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK74

Quant Time: Dec 07 12:30:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 11:14:57 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4023	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	16650	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	9132	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1195264	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	17359	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	7036	0.28	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.68	128	1053	0.023	ng/ul#	82
23) Benzo(a)pyrene	23.56	252	4754	0.076	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003761.D
Acq On : 07 Dec 2018 11:55
Operator : JU/SJ
Sample : PB115374BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK74

Quant Time: Dec 07 12:30:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 11:14:57 2018
Response via : Initial Calibration

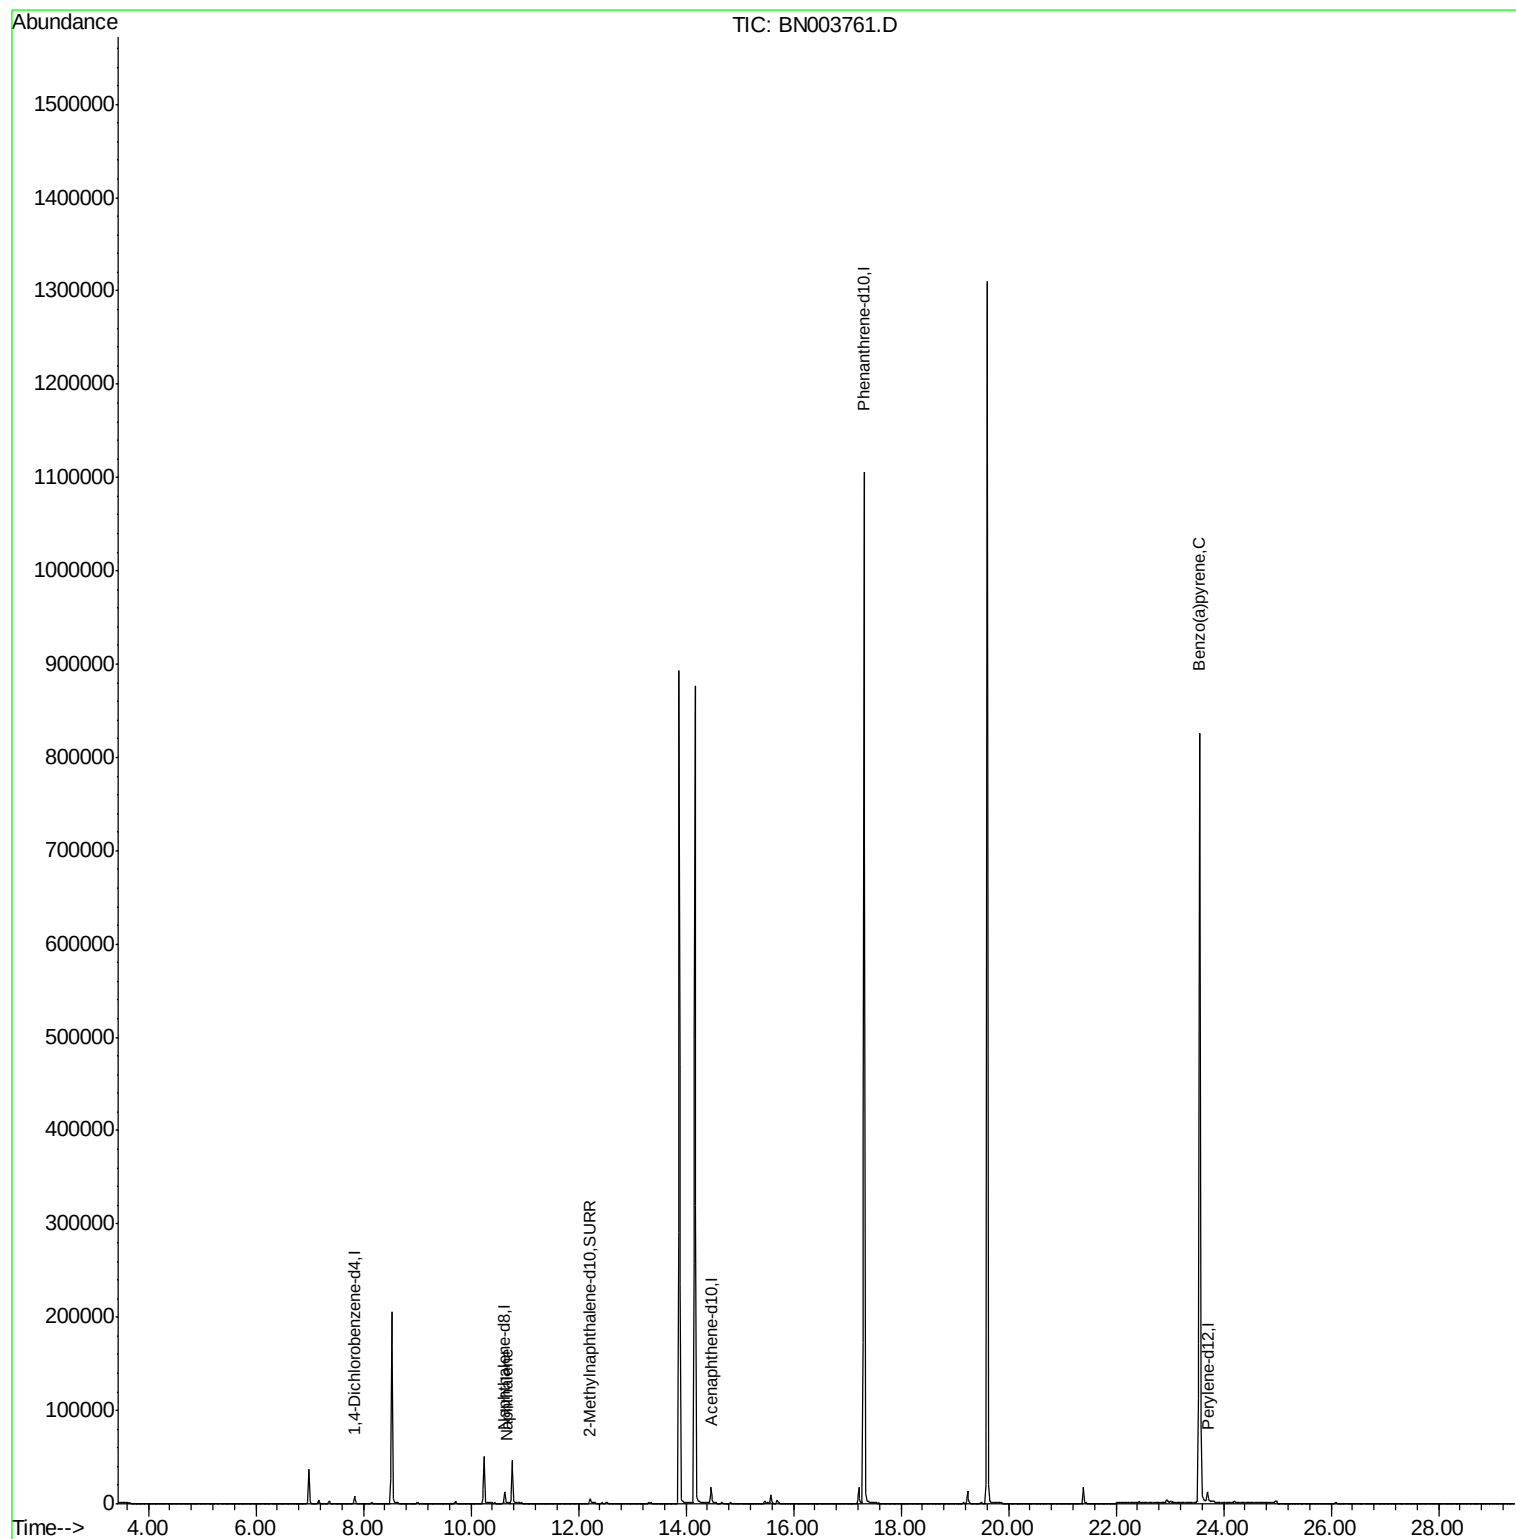

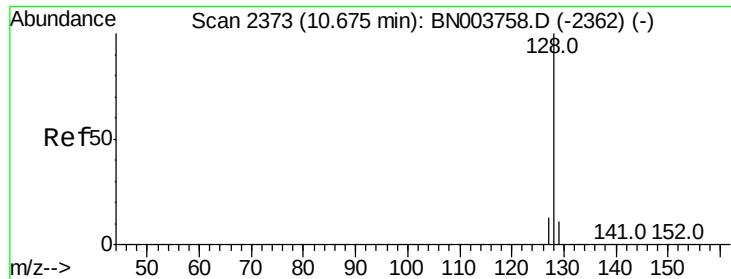

#3

Naphthalene

Concen: 0.023 ng/ul

RT: 10.68 min Scan# 2374

Delta R.T. 0.00 min

Lab File: BN003761.D

Acq: 07 Dec 2018 11:55

Instrument :

BNA_N

ClientSampleId :

SBLK74


Tot Ion:128 Resp: 1053

Ion Ratio Lower Upper

128 100

129 19.7 9.0 13.6#




127 18.7 10.5 15.7#

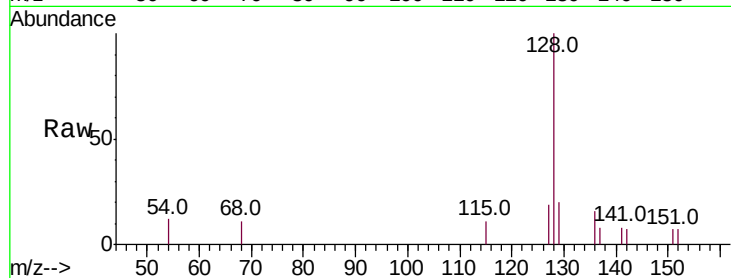

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

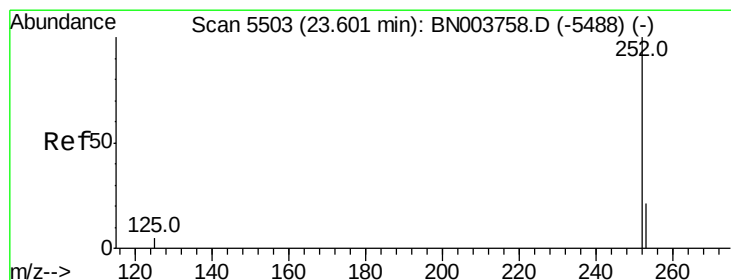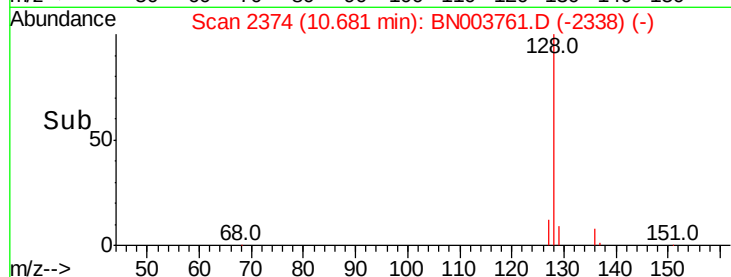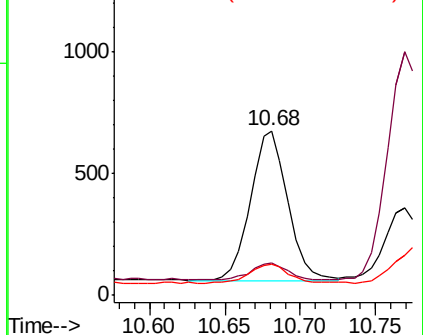

#23

Benzo(a)pyrene

Concen: 0.076 ng/ul

RT: 23.56 min Scan# 5487

Delta R.T. -0.05 min

Lab File: BN003761.D

Acq: 07 Dec 2018 11:55


Tgt Ion:252 Resp: 4754

Ion Ratio Lower Upper

252 100

253 39.5 19.0 28.4#

125 29.7 10.2 15.4#

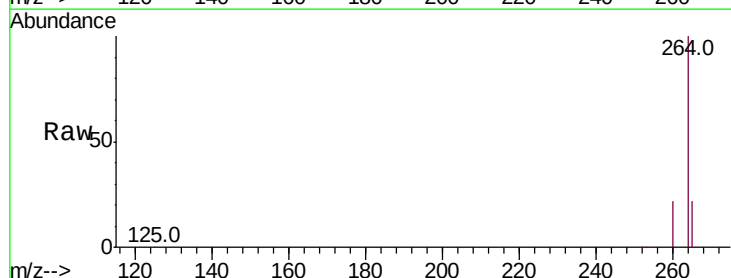

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

