

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003764.D
 Acq On : 07 Dec 2018 13:48
 Operator : JU/SJ
 Sample : J6228-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E78

Quant Time: Dec 07 15:50:06 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:33:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5160	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	21431	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12099	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1748849	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.70	264	20471	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	9994	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
21) Benzo(b)fluoranthene	23.01	252	2789	0.033	ng/ul#	28
22) Benzo(k)fluoranthene	23.01	252	2789	0.034	ng/ul#	28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003764.D
Acq On : 07 Dec 2018 13:48
Operator : JU/SJ
Sample : J6228-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E78

Quant Time: Dec 07 15:50:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

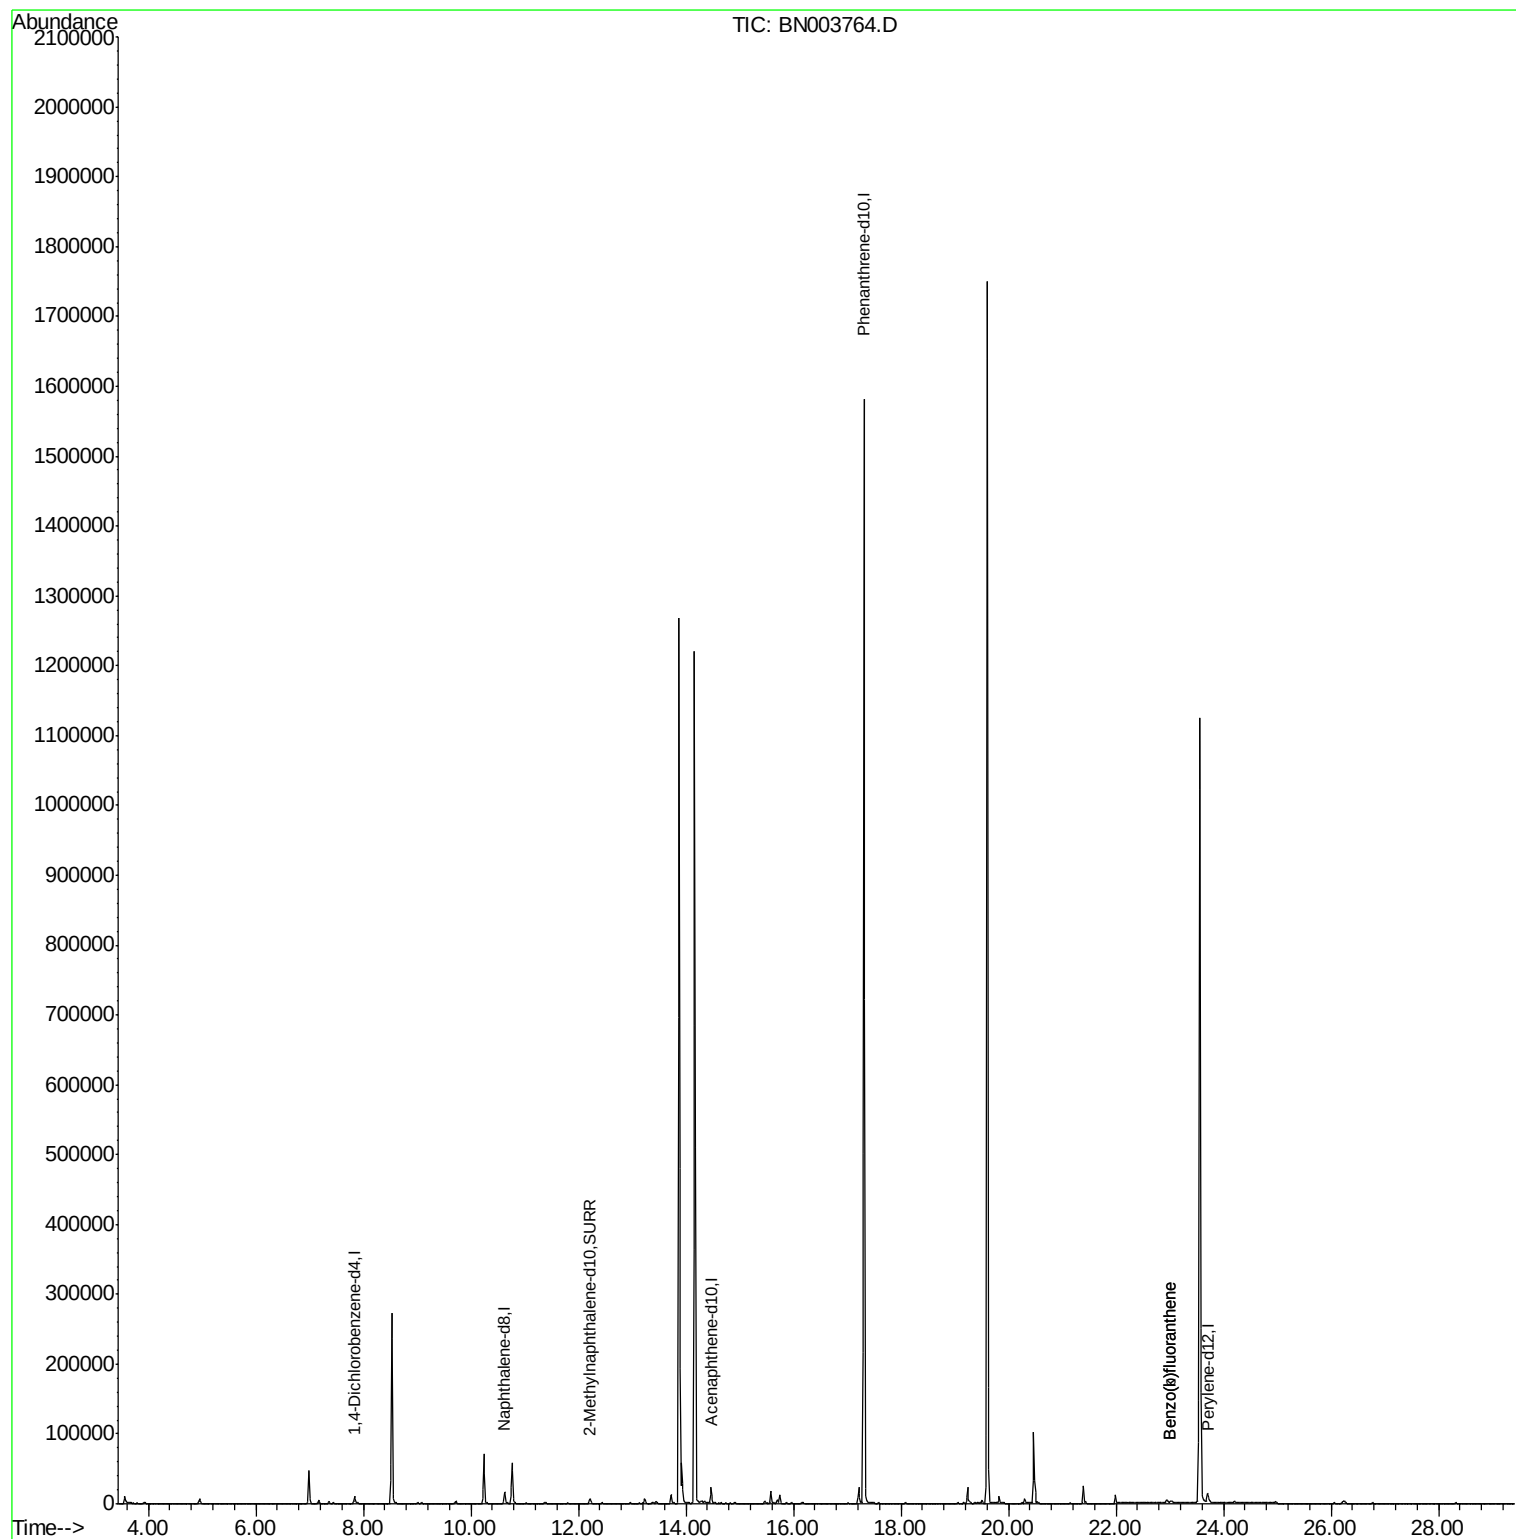

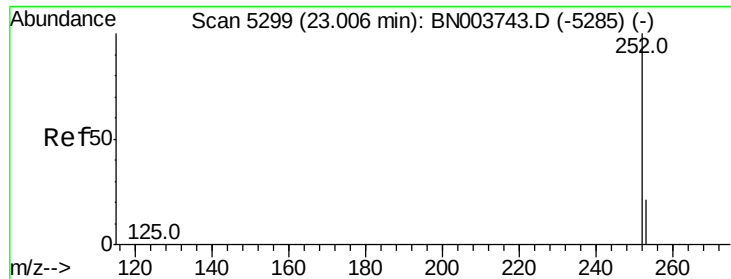

#21

Benzo(b)fluoranthene

Concen: 0.033 ng/ul

RT: 23.01 min Scan# 5299

Delta R.T. 0.00 min

Lab File: BN003764.D

Acq: 07 Dec 2018 13:48

Instrument :

BNA_N

ClientSampleId :

F9E78





Tot Ion:252 Resp: 2789

Ion Ratio Lower Upper

252 100

253 59.3 0.0 46.0#

125 36.5 0.0 22.4#

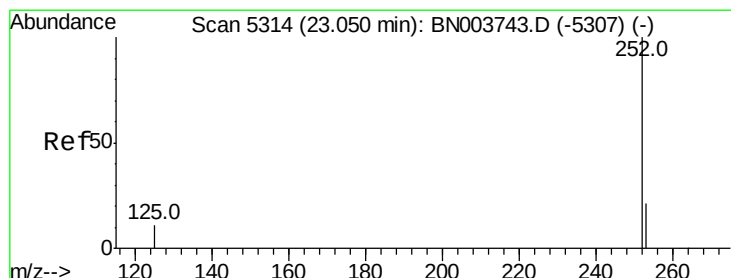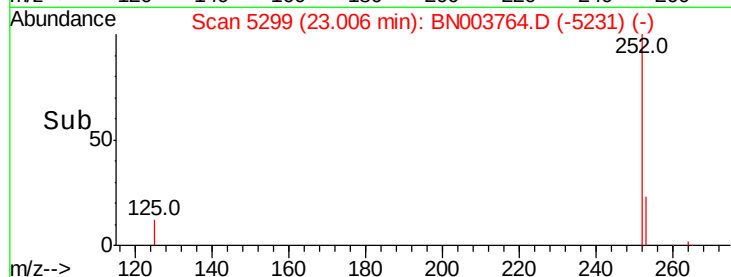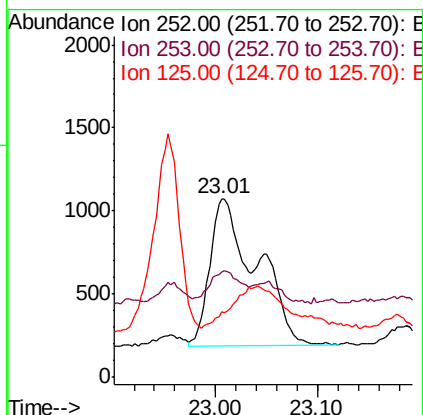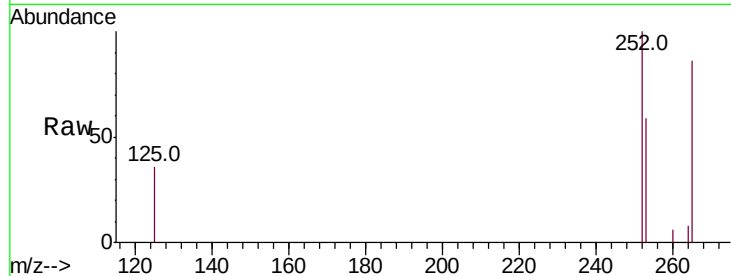

#22

Benzo(k)fluoranthene

Concen: 0.034 ng/ul

RT: 23.01 min Scan# 5299

Delta R.T. -0.04 min

Lab File: BN003764.D

Acq: 07 Dec 2018 13:48

Tgt Ion:252 Resp: 2789

Ion Ratio Lower Upper

252 100

253 59.3 18.5 27.7#

125 36.5 9.0 13.6#

