

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003768.D
 Acq On : 07 Dec 2018 16:08
 Operator : JU/SJ
 Sample : J6228-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E91

Quant Time: Dec 07 16:43:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:51:04 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4821	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	20125	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11181	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1462742	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.71	264	19891	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	8362	0.27	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.56	252	4931	0.069	ng/ul#	Ovalue 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003768.D
Acq On : 07 Dec 2018 16:08
Operator : JU/SJ
Sample : J6228-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E91

Quant Time: Dec 07 16:43:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:51:04 2018
Response via : Initial Calibration

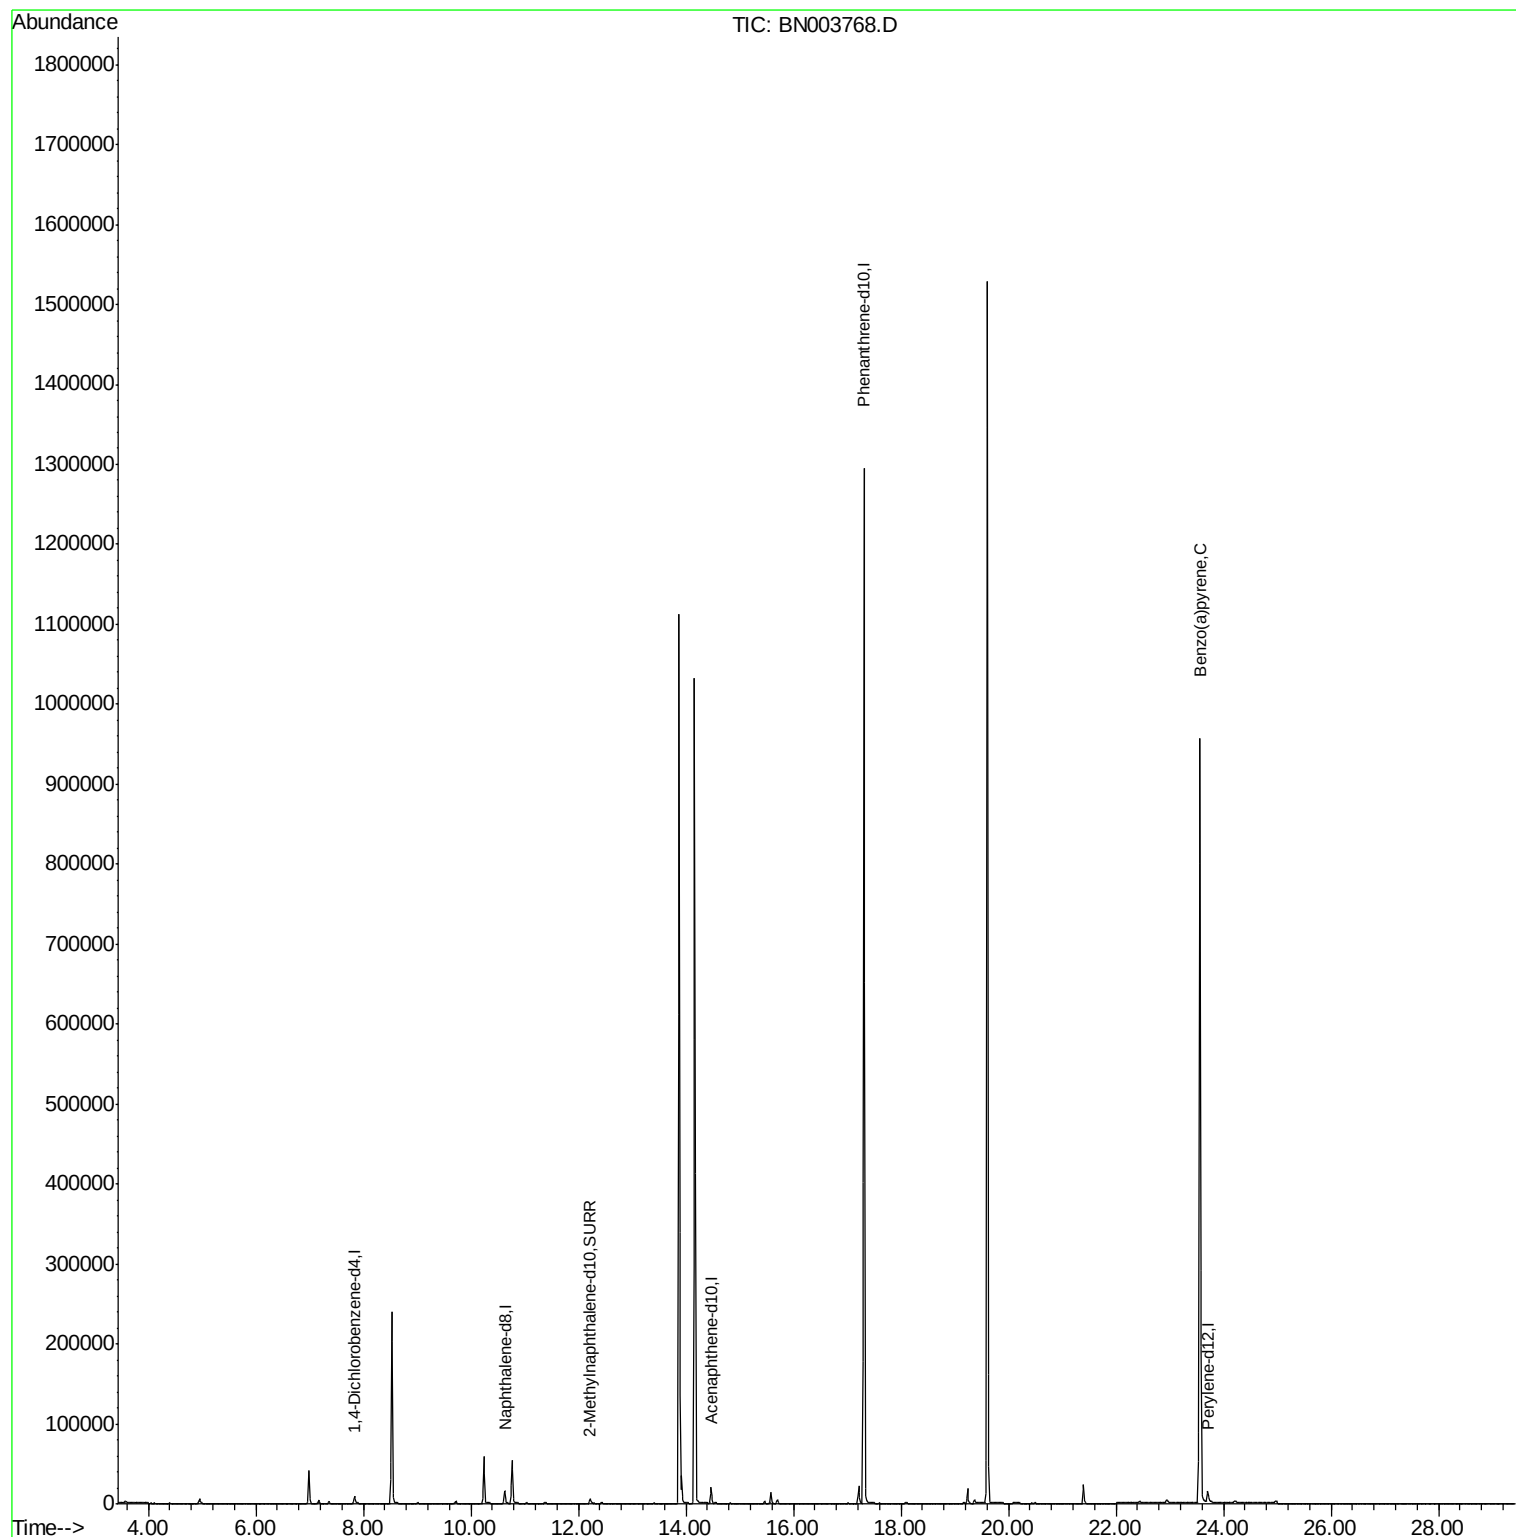

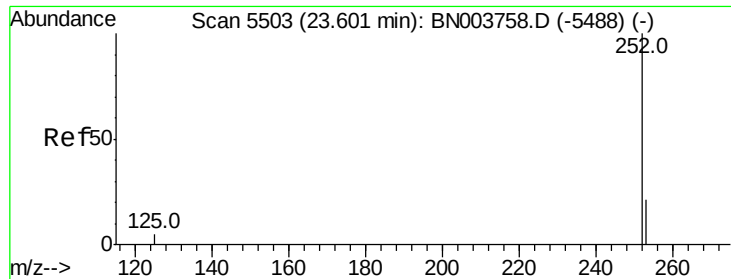

#23

Benzo(a)pyrene

Concen: 0.069 ng/ul

RT: 23.56 min Scan# 5489

Delta R.T. -0.04 min

Lab File: BN003768.D

Acq: 07 Dec 2018 16:08

Instrument :

BNA_N

ClientSampleId :

F9E91


Tot Ion: 252 Resp: 4931

Ion Ratio Lower Upper

252 100

253 40.9 19.0 28.4#

125 32.3 10.2 15.4#

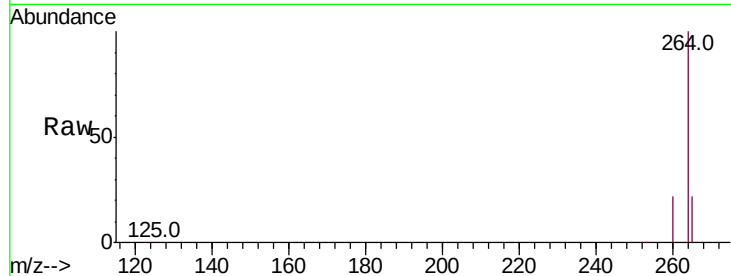

Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

