

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003759.D
 Acq On : 07 Dec 2018 10:45
 Operator : JU/SJ
 Sample : J6077-05DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9Y38DL

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:13 AM

Quant Time: Dec 07 11:17:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 04:08:50 2018
 Response via : Initial Calibration

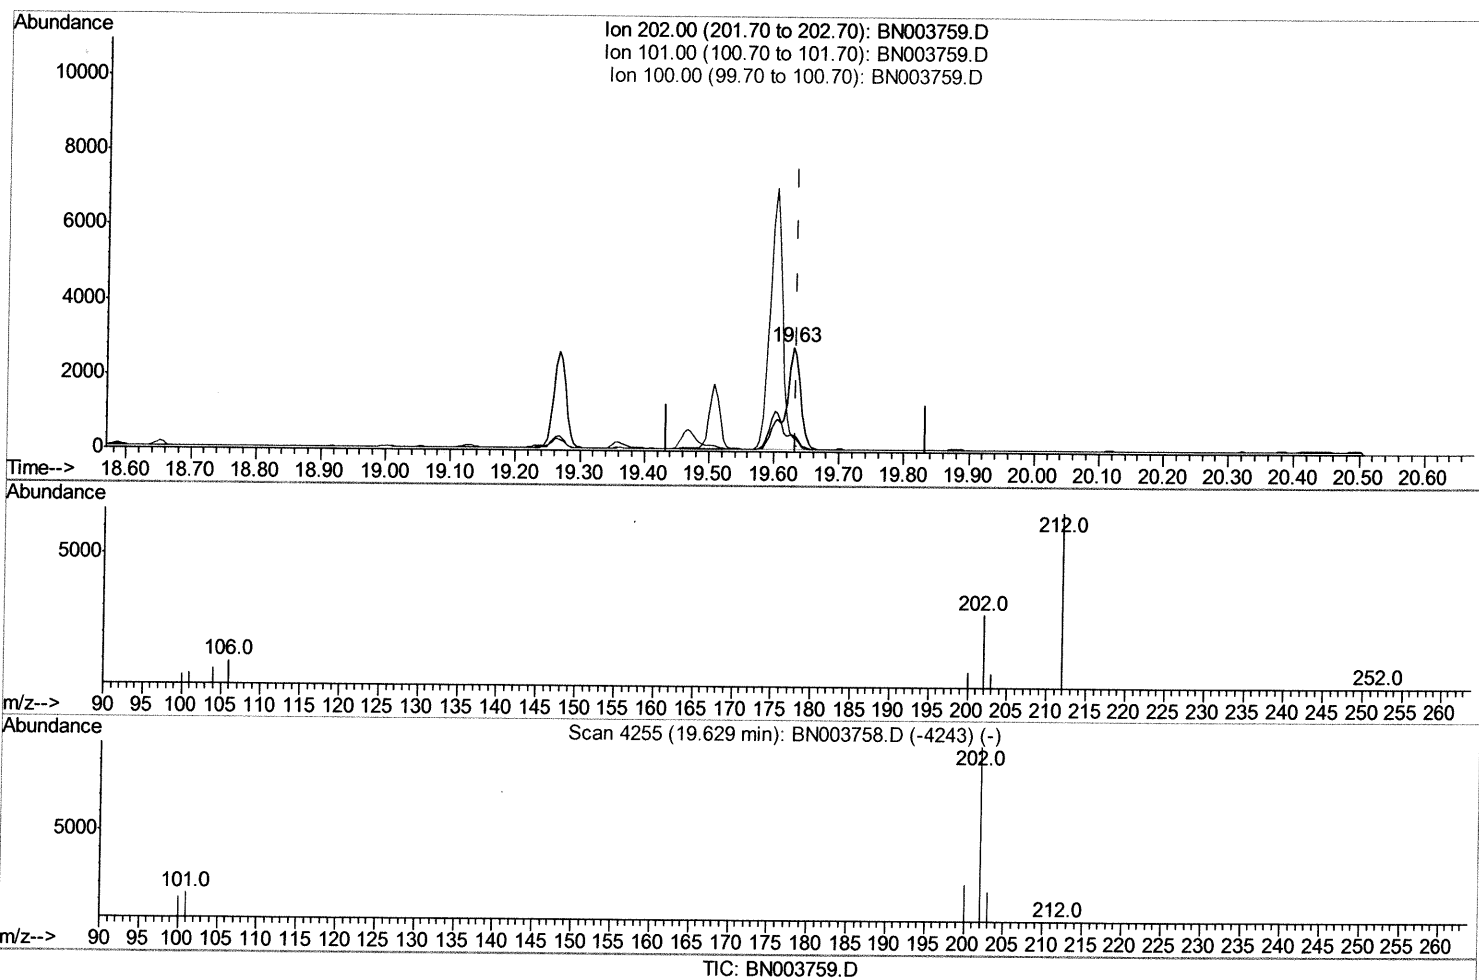

(17) Pyrene

19.629min (-0.005) 0.05ng/ul

response 4493

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	16.10#
100.00	10.60	14.35#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003759.D
Acq On : 07 Dec 2018 10:45
Operator : JU/SJ
Sample : J6077-05DL 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y38DL

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:13 AM

Quant Time: Dec 07 11:17:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

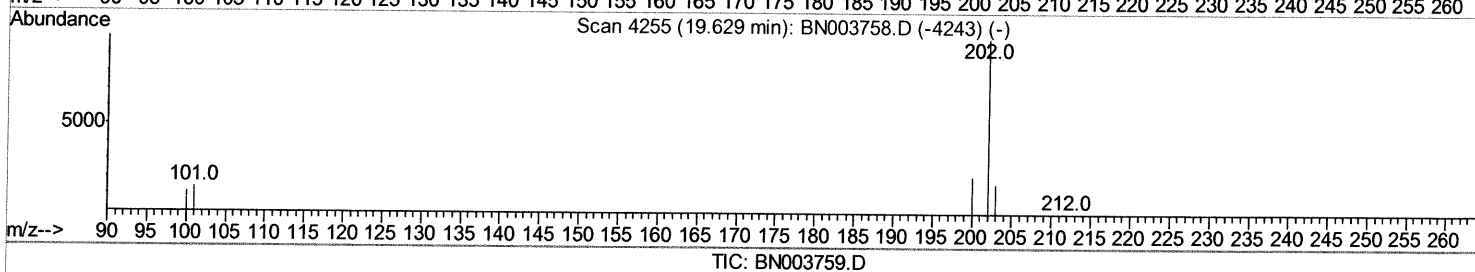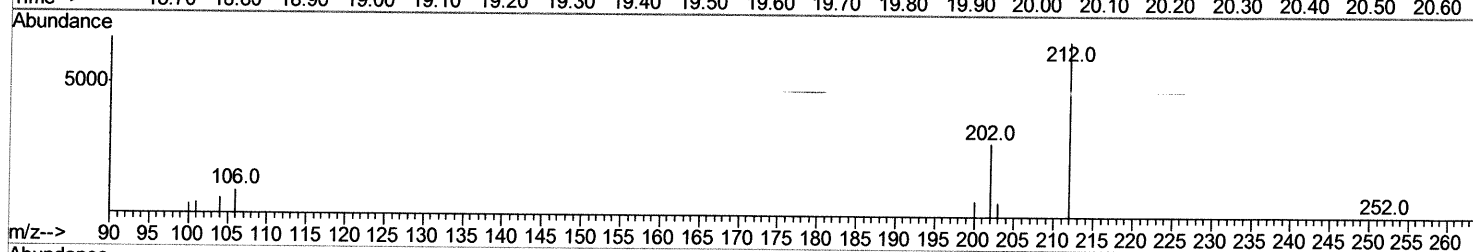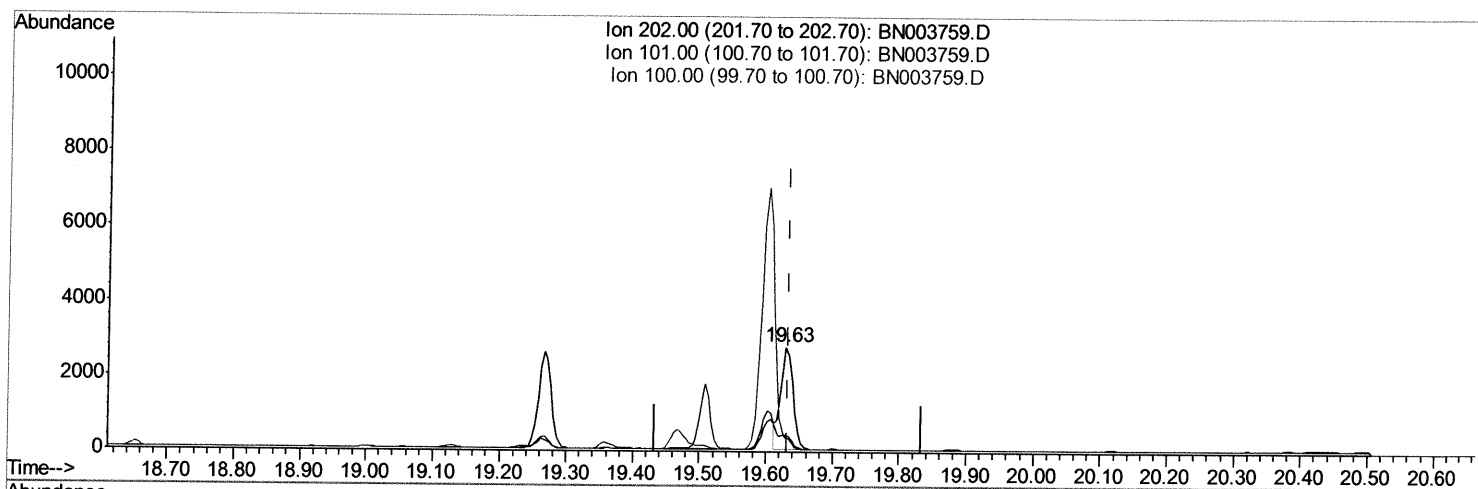

(17) Pyrene

19.629min (-0.005) 0.04ng/ul m

response 3561

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	16.10#
100.00	10.60	14.35#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003759.D
 Acq On : 07 Dec 2018 10:45
 Operator : JU/SJ
 Sample : J6077-05DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9Y38DL

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:13 AM

Quant Time: Dec 07 11:25:06 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 04:08:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5664	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	23808	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12963	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	28477	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	24125	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	22253	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	3317	0.09	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	7169	0.09	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.68	128	42831	0.640	ng/ul	97
5) 2-Methylnaphthalene	12.29	142	40380	0.865	ng/ul	100
8) Acenaphthene	14.53	153	1193	0.023	ng/ul	97
9) Fluorene	15.52	166	1360	0.023	ng/ul#	97
12) Phenanthrene	17.25	178	10147	0.109	ng/ul	98
17) Pyrene	19.63	202	3561m	0.041	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

12/11/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003759.D
Acq On : 07 Dec 2018 10:45
Operator : JU/SJ
Sample : J6077-05DL 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9Y38DL

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:13 AM

Quant Time: Dec 07 11:25:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

