

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003760.D
 Acq On : 07 Dec 2018 11:20
 Operator : JU/SJ
 Sample : J6077-06DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9Y41DL

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:14 AM

Quant Time: Dec 07 11:56:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 11:14:57 2018
 Response via : Initial Calibration

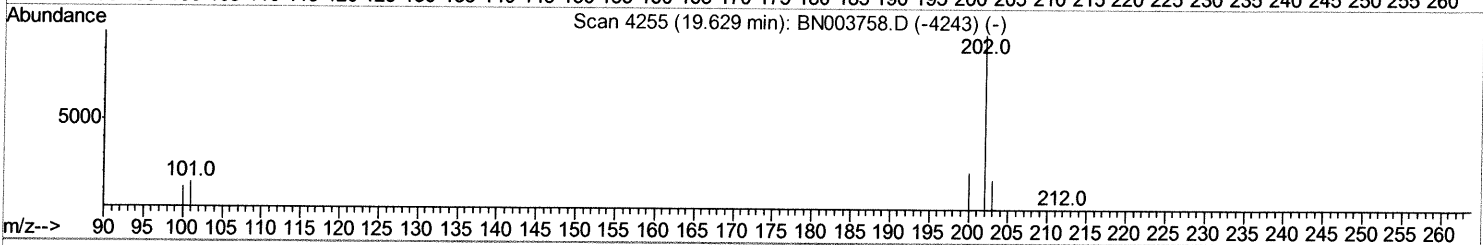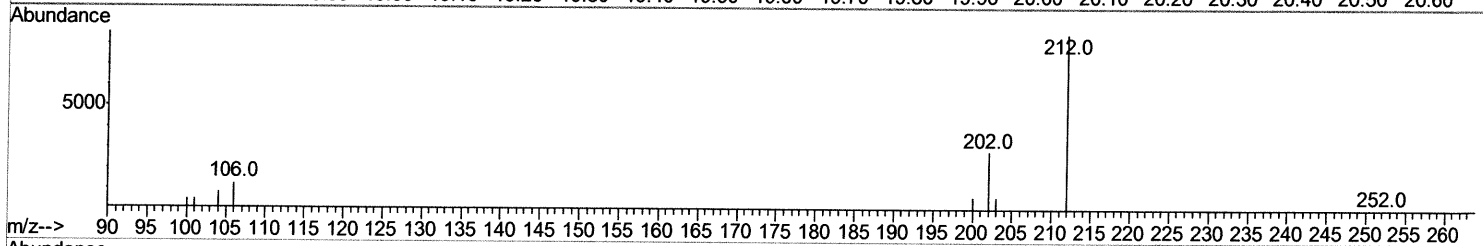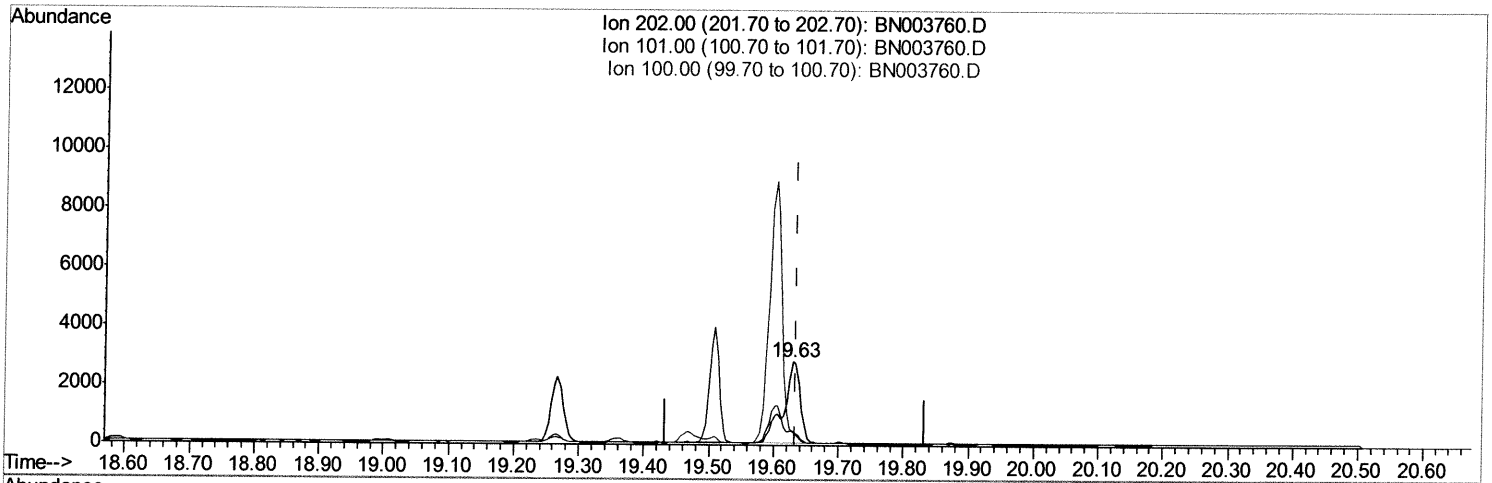

TIC: BN003760.D

(17) Pyrene

19.629min (-0.005) 0.05ng/ul

response 5020

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	17.42#
100.00	10.60	15.95#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003760.D
 Acq On : 07 Dec 2018 11:20
 Operator : JU/SJ
 Sample : J6077-06DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9Y41DL

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:14 AM

Quant Time: Dec 07 11:56:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 11:14:57 2018
 Response via : Initial Calibration

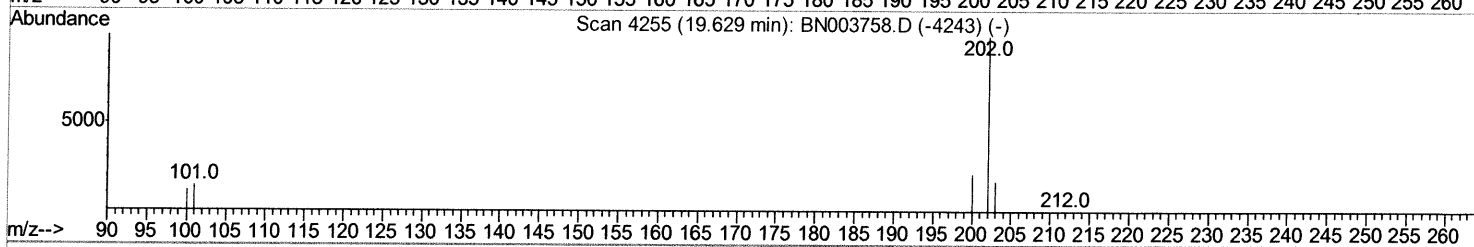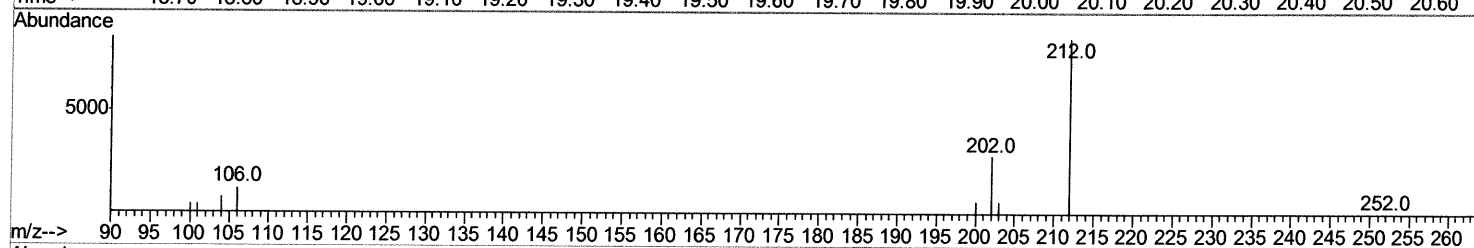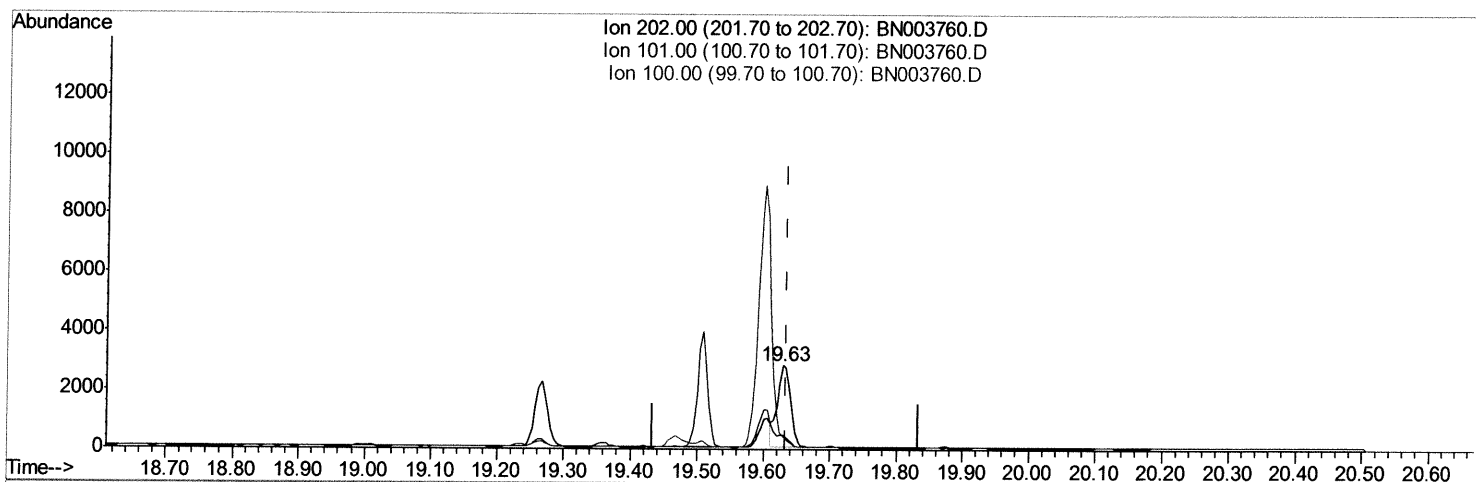

TIC: BN003760.D

(17) Pyrene

19.629min (-0.005) 0.04ng/ul m

response 3853

Ion Exp% Act%

202.00 100 100

101.00 12.90 17.42#

100.00 10.60 15.95#

0.00 0.00 0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003760.D
 Acq On : 07 Dec 2018 11:20
 Operator : JU/SJ
 Sample : J6077-06DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9Y41DL

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:14 AM

Quant Time: Dec 07 11:58:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 11:14:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	6365	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	26809	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	14854	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	33067	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	28017	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	26614	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	4242	0.10	ng/ul	0.00
14) Fluoranthene-d10	19.23	212	9237	0.10	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.68	128	71667	0.952	ng/ul	98
5) 2-Methylnaphthalene	12.29	142	72362	1.376	ng/ul	100
8) Acenaphthene	14.53	153	2198	0.038	ng/ul	96
9) Fluorene	15.52	166	2597	0.038	ng/ul#	96
12) Phenanthrene	17.25	178	15623	0.144	ng/ul	98
15) Fluoranthene	19.27	202	2913	0.023	ng/ul	90
17) Pyrene	19.63	202	3853m	0.038	ng/ul	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003760.D
Acq On : 07 Dec 2018 11:20
Operator : JU/SJ
Sample : J6077-06DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y41DL

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:14 AM

Quant Time: Dec 07 11:58:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 11:14:57 2018
Response via : Initial Calibration

