

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003763.D
 Acq On : 07 Dec 2018 13:12
 Operator : JU/SJ
 Sample : J6228-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E77

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:17 AM

Quant Time: Dec 07 15:50:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:33:20 2018
 Response via : Initial Calibration

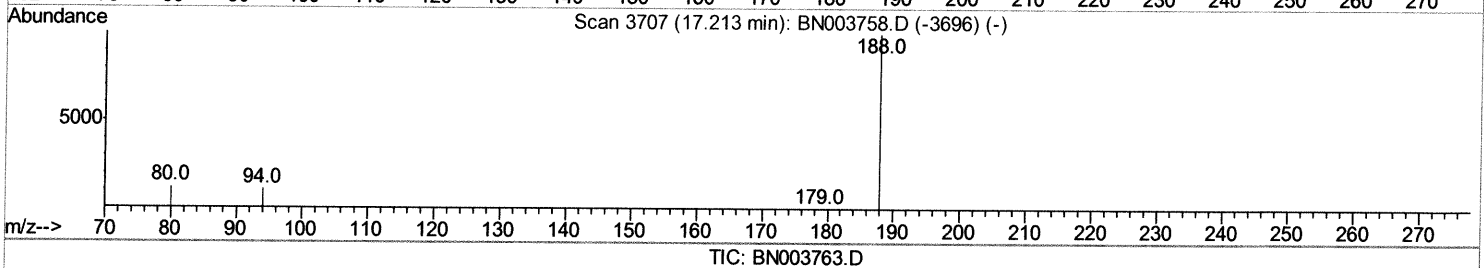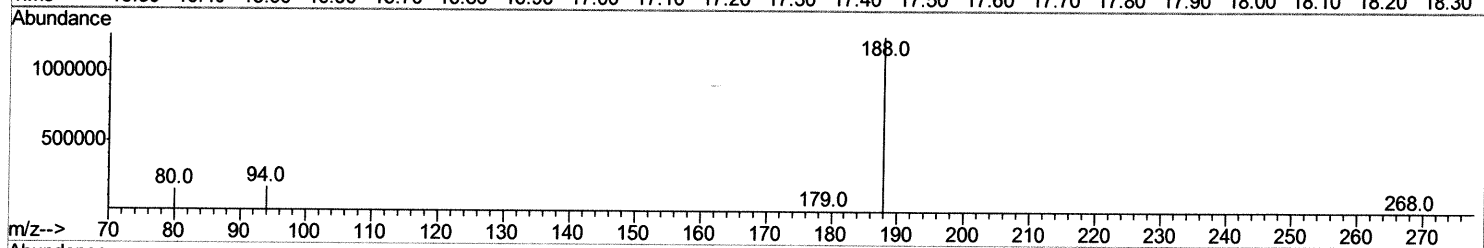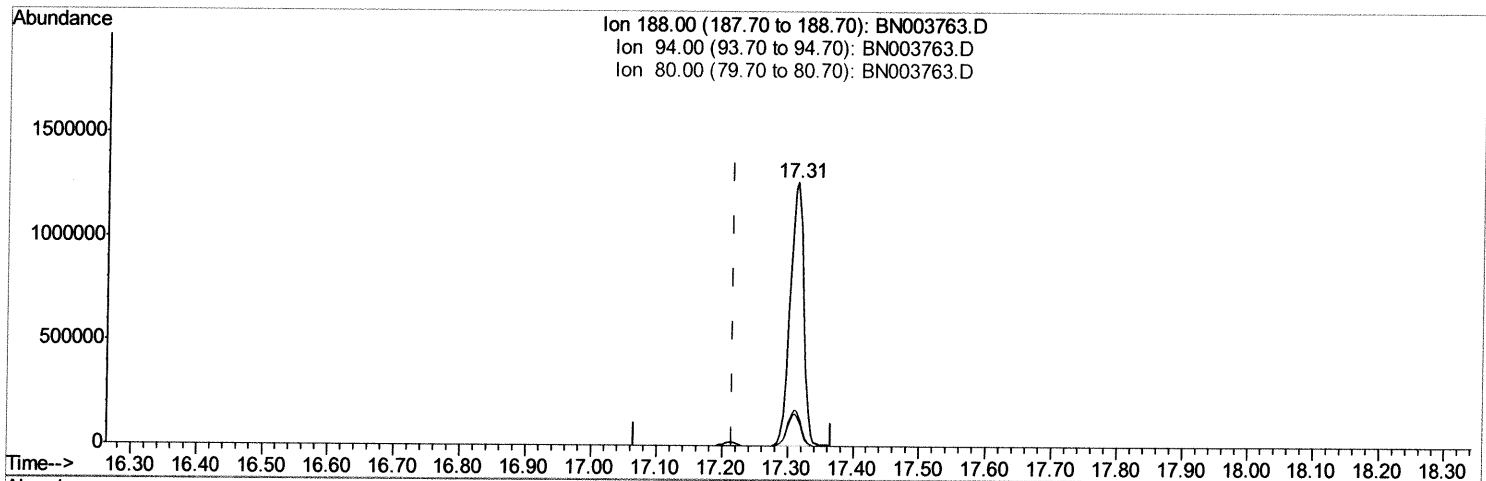

(10) Phenanthrene-d10 (I)
 17.314min (+0.097) 0.40ng/ul
 response 1791879

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.98#
80.00	11.60	11.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003763.D
Acq On : 07 Dec 2018 13:12
Operator : JU/SJ
Sample : J6228-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E77

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:17 AM

Quant Time: Dec 07 15:50:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

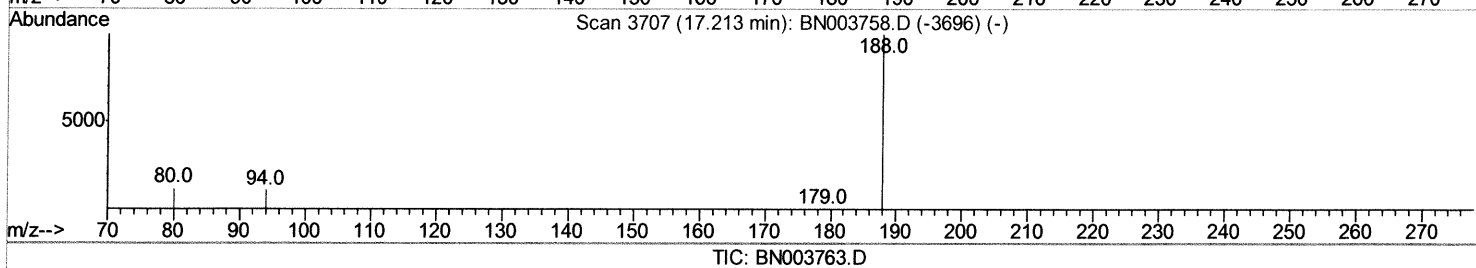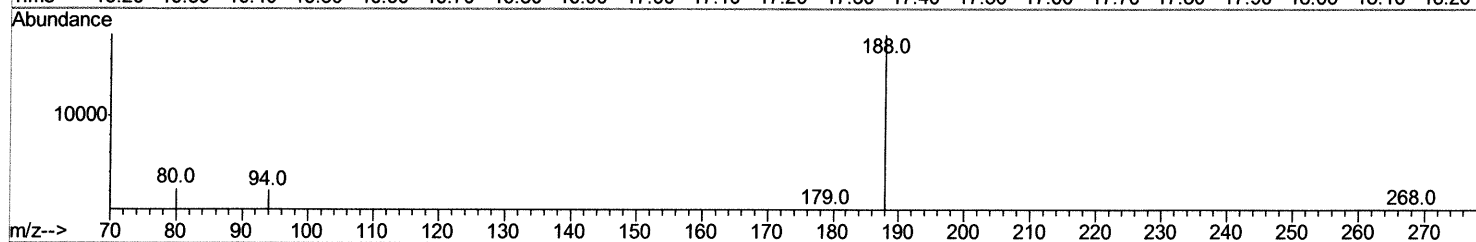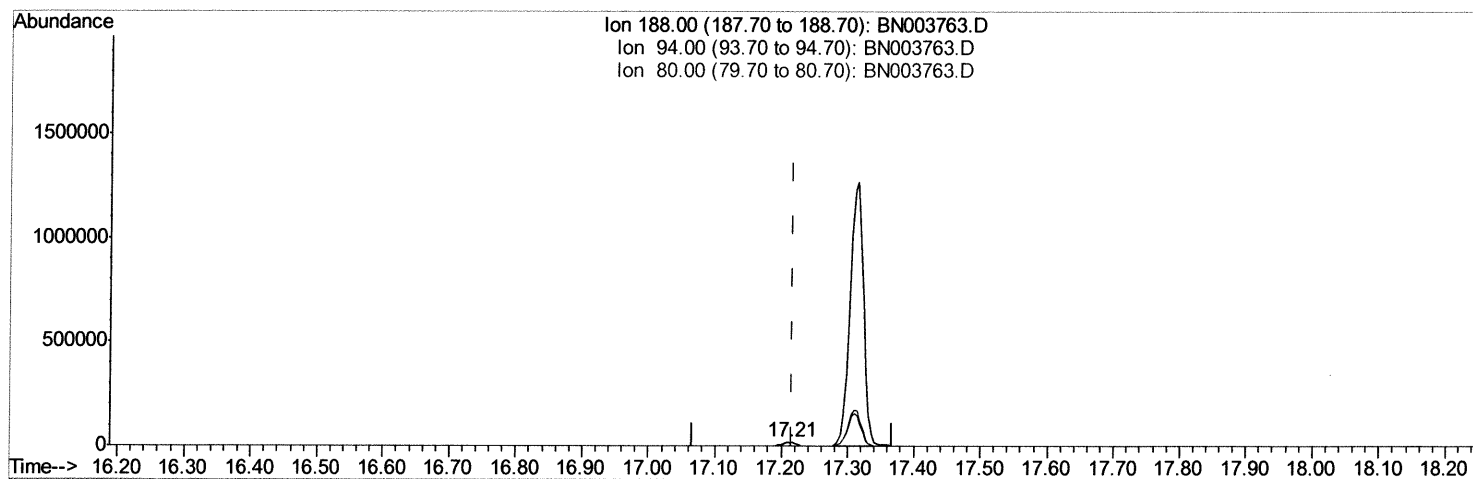

(10) Phenanthrene-d10 (I)

17.213min (-0.004) 0.40ng/ul m

MS
12/11/18

response 25411

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.09
80.00	11.60	12.13
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003763.D
Acq On : 07 Dec 2018 13:12
Operator : JU/SJ
Sample : J6228-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E77

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:17 AM

Quant Time: Dec 07 16:03:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

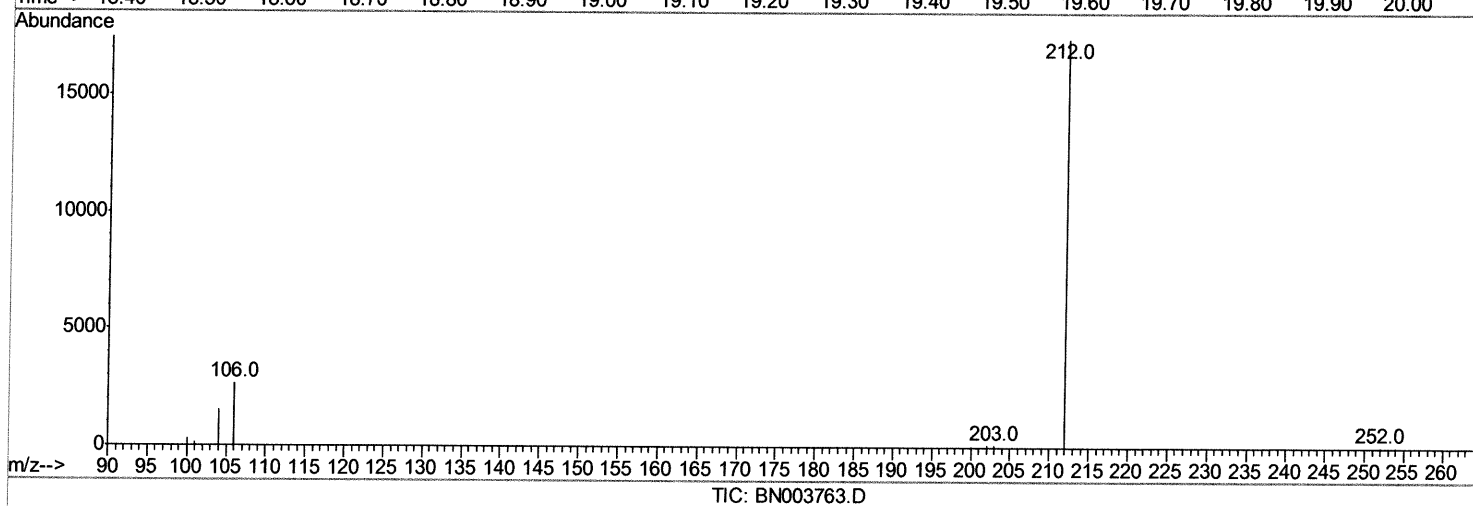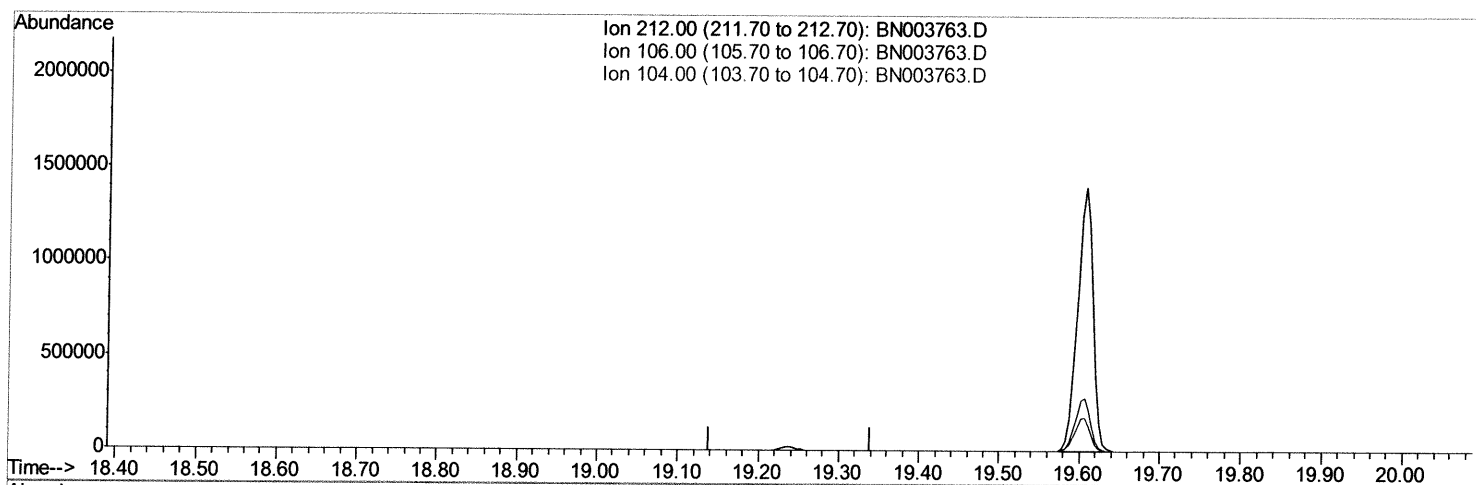

(14) Fluoranthene-d10 (SURR)

19.239min (-19.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003763.D
Acq On : 07 Dec 2018 13:12
Operator : JU/SJ
Sample : J6228-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E77

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:17 AM

Quant Time: Dec 07 16:03:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

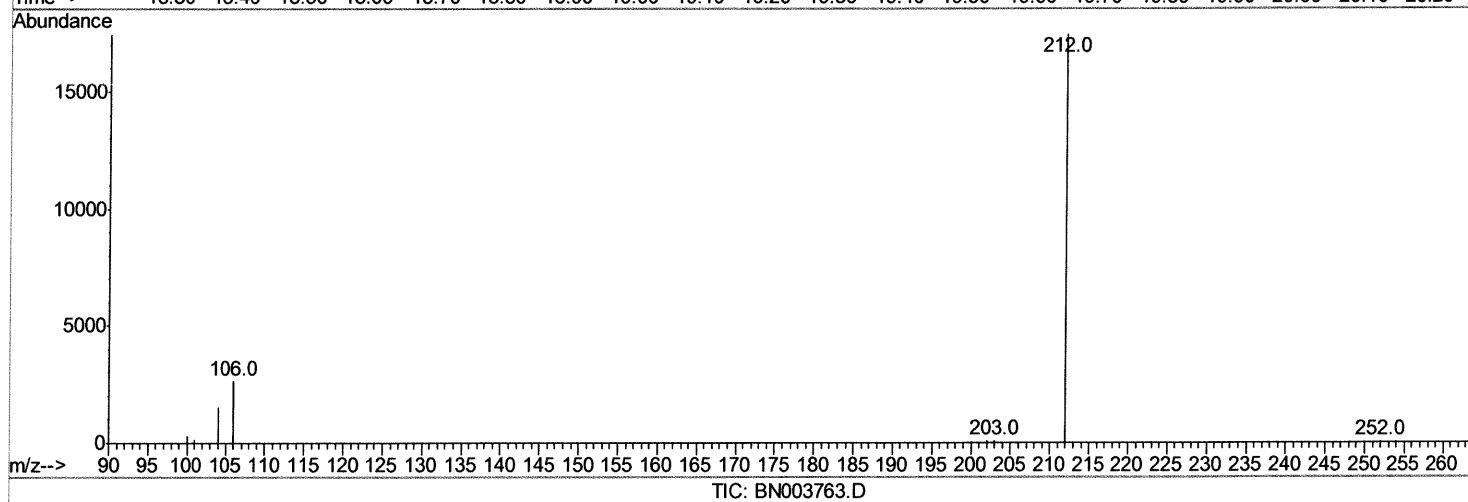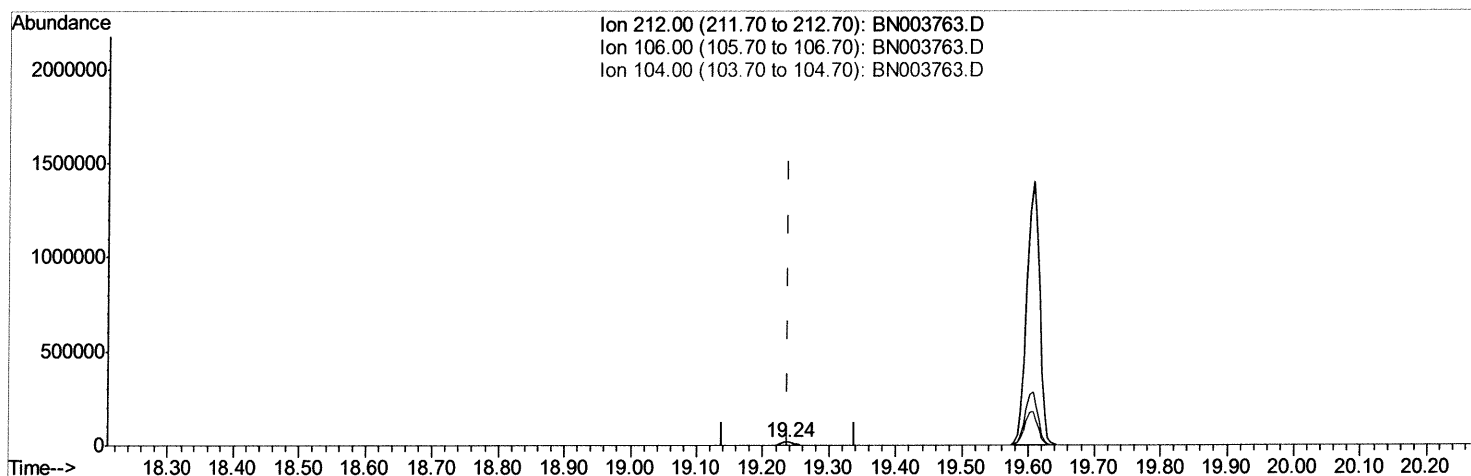

(14) Fluoranthene-d10 (SURR)

19.239min (+0.000) 0.32ng/ul m

response 23816

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003763.D
 Acq On : 07 Dec 2018 13:12
 Operator : JU/SJ
 Sample : J6228-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E77

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:17 AM

Quant Time: Dec 07 16:04:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:33:20 2018
 Response via : Initial Calibration

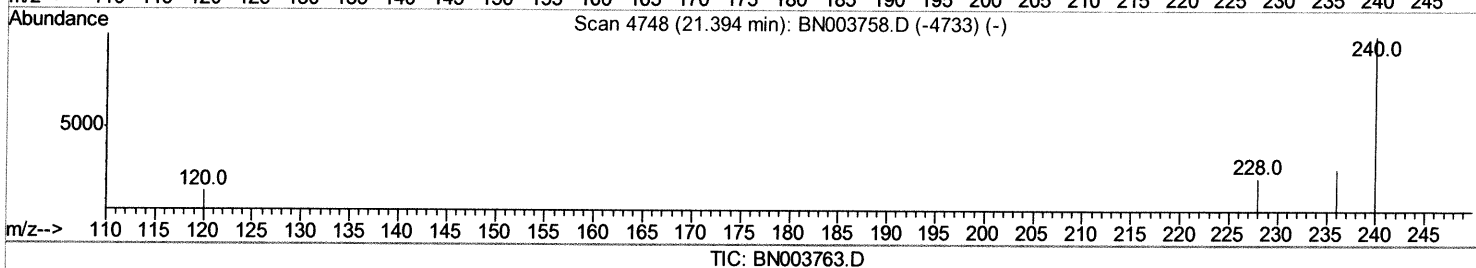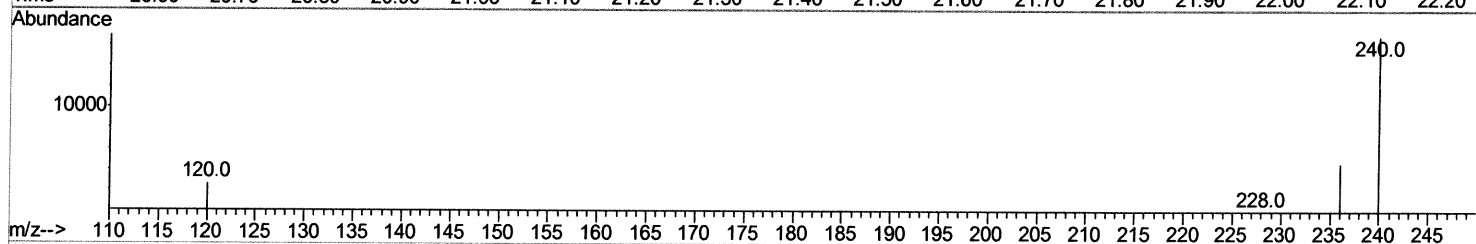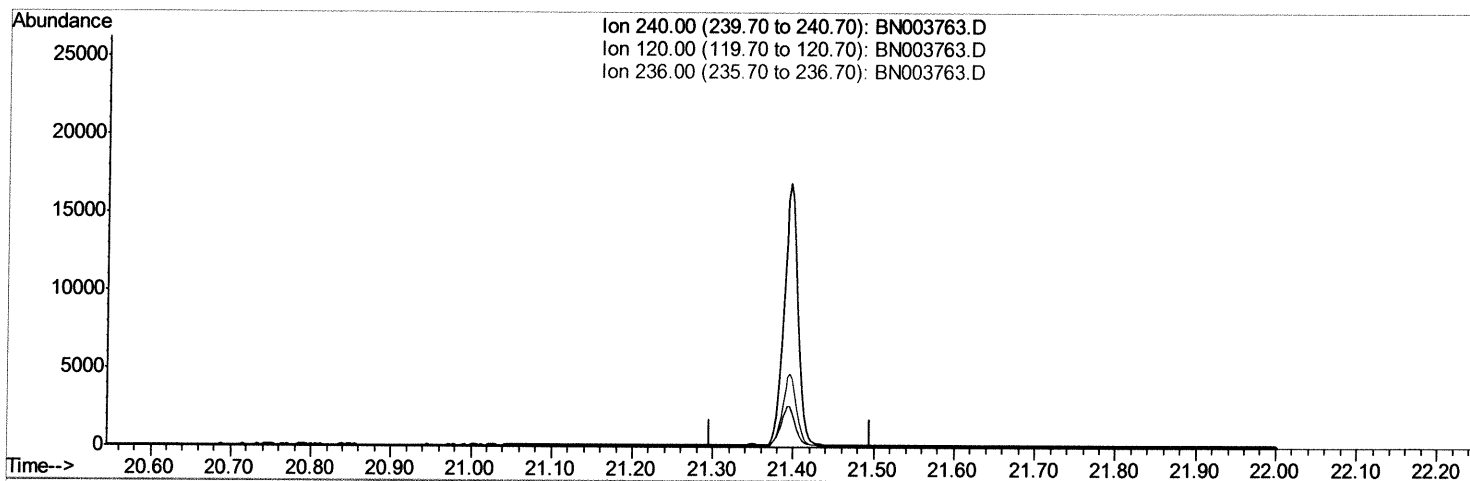

(16) Chrysene-d12 (I)

21.395min (-21.395) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003763.D
 Acq On : 07 Dec 2018 13:12
 Operator : JU/SJ
 Sample : J6228-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 F9E77

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:17 AM

Quant Time: Dec 07 16:04:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:33:20 2018
 Response via : Initial Calibration

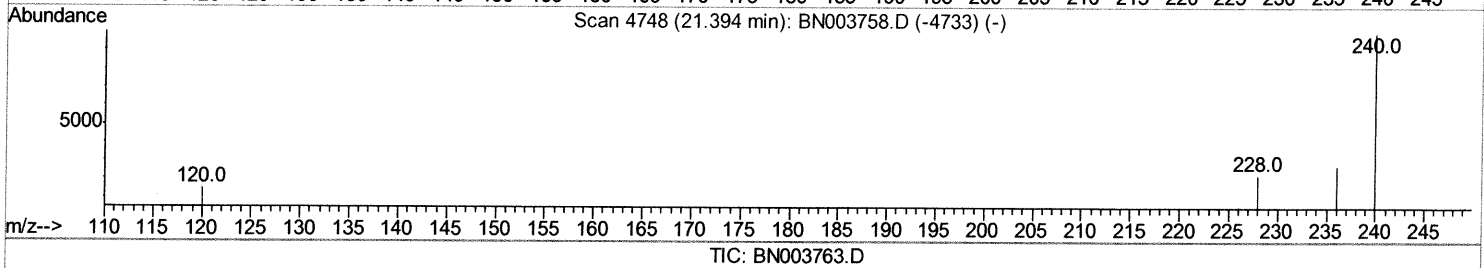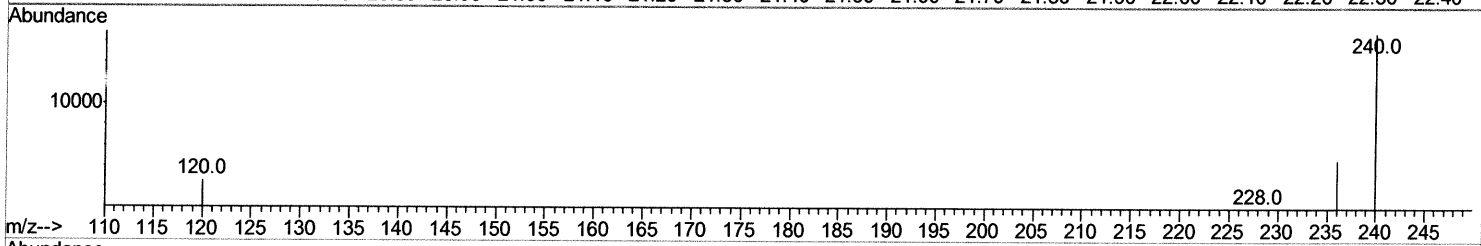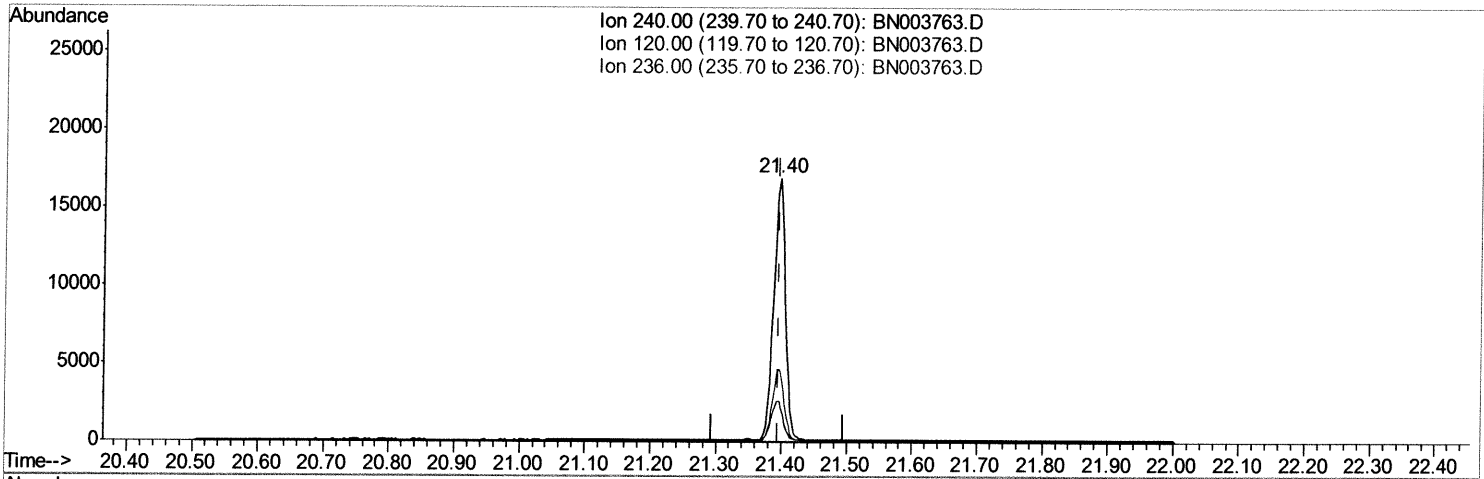

(16) Chrysene-d12 (I)

21.396min (+0.000) 0.40ng/ul m

response 21084

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	15.57
236.00	27.60	27.94
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003763.D
Acq On : 07 Dec 2018 13:12
Operator : JU/SJ
Sample : J6228-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E77

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:17 AM

Quant Time: Dec 07 16:05:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5117	0.40	nq/ul	0.00
2) Naphthalene-d8	10.63	136	21316	0.40	nq/ul	0.00
6) Acenaphthene-d10	14.47	164	11900	0.40	nq/ul	0.00
10) Phenanthrene-d10	17.21	188	25411m	0.40	nq/ul	0.00
16) Chrysene-d12	21.40	240	21084m	0.40	nq/ul	0.00
20) Perylene-d12	23.70	264	20663	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.22	152	10363	0.32	nq/ul	0.00
14) Fluoranthene-d10	19.24	212	23816m	0.32	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003763.D
Acq On : 07 Dec 2018 13:12
Operator : JU/SJ
Sample : J6228-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E77

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:17 AM

Quant Time: Dec 07 16:05:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

