

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003765.D
Acq On : 07 Dec 2018 14:23
Operator : JU/SJ
Sample : J6228-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E88

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:19 AM

Quant Time: Dec 07 15:50:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

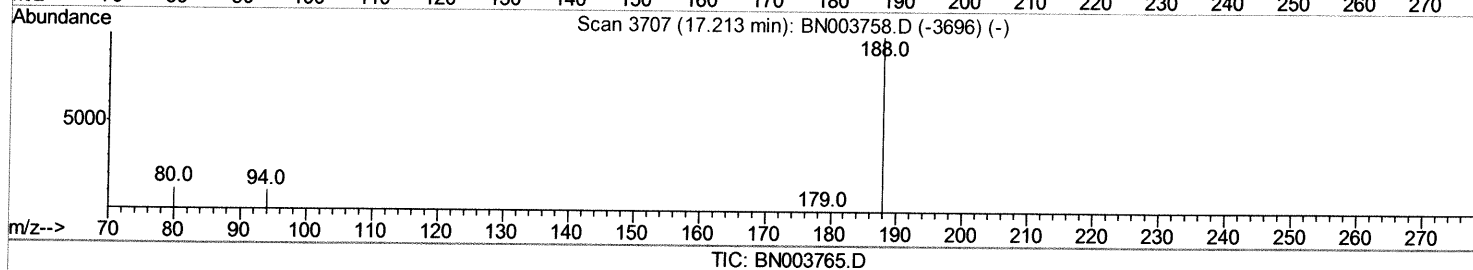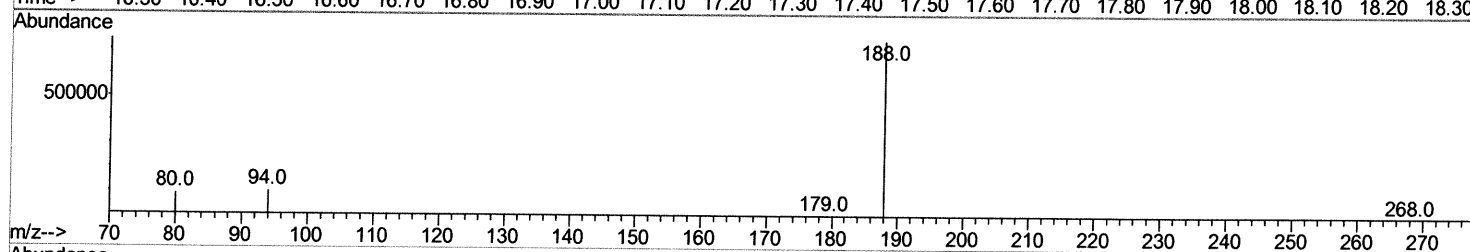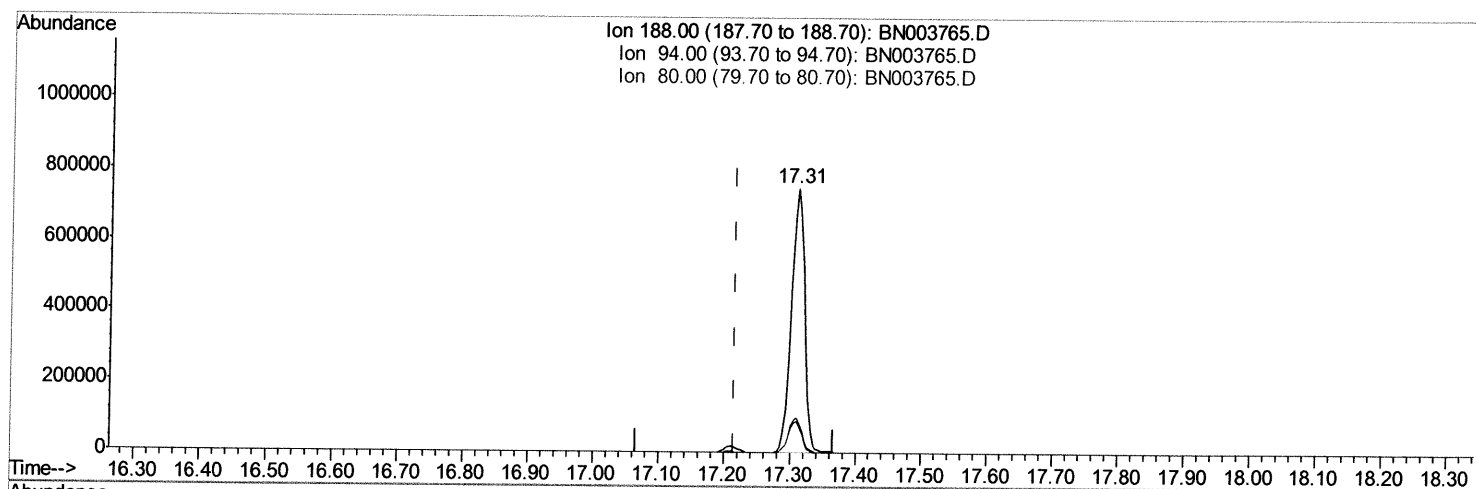

(10) Phenanthrene-d10 (I)

17.310min (+0.093) 0.40ng/ul

response 1042727

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.11#
80.00	11.60	11.76
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003765.D
Acq On : 07 Dec 2018 14:23
Operator : JU/SJ
Sample : J6228-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E88

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:19 AM

Quant Time: Dec 07 15:50:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

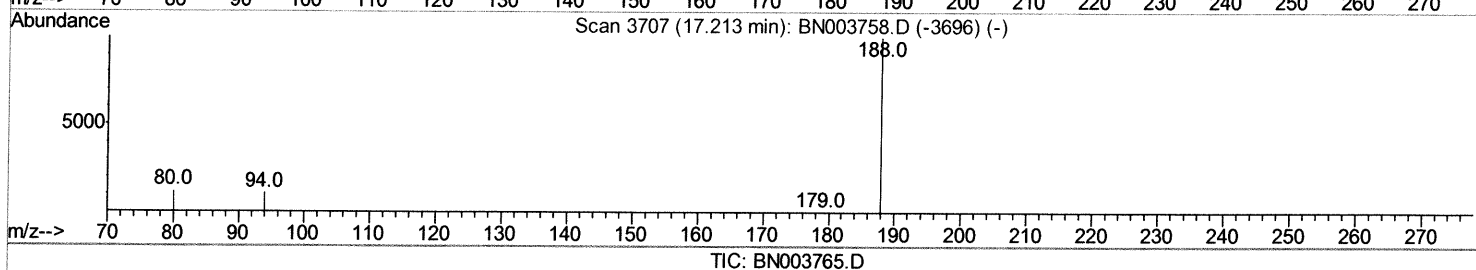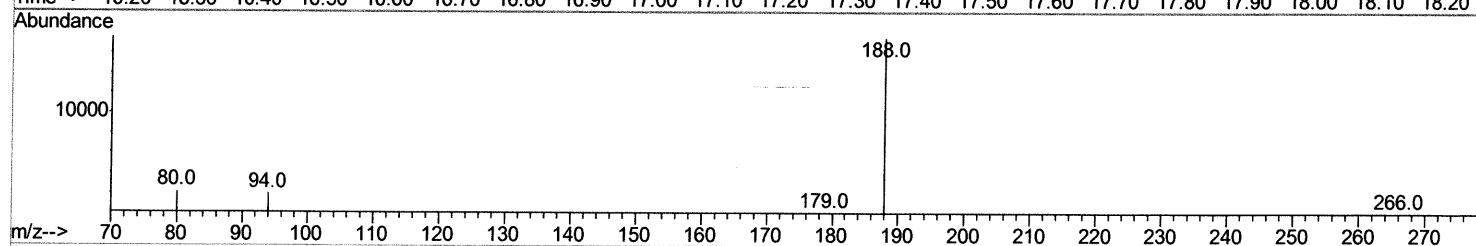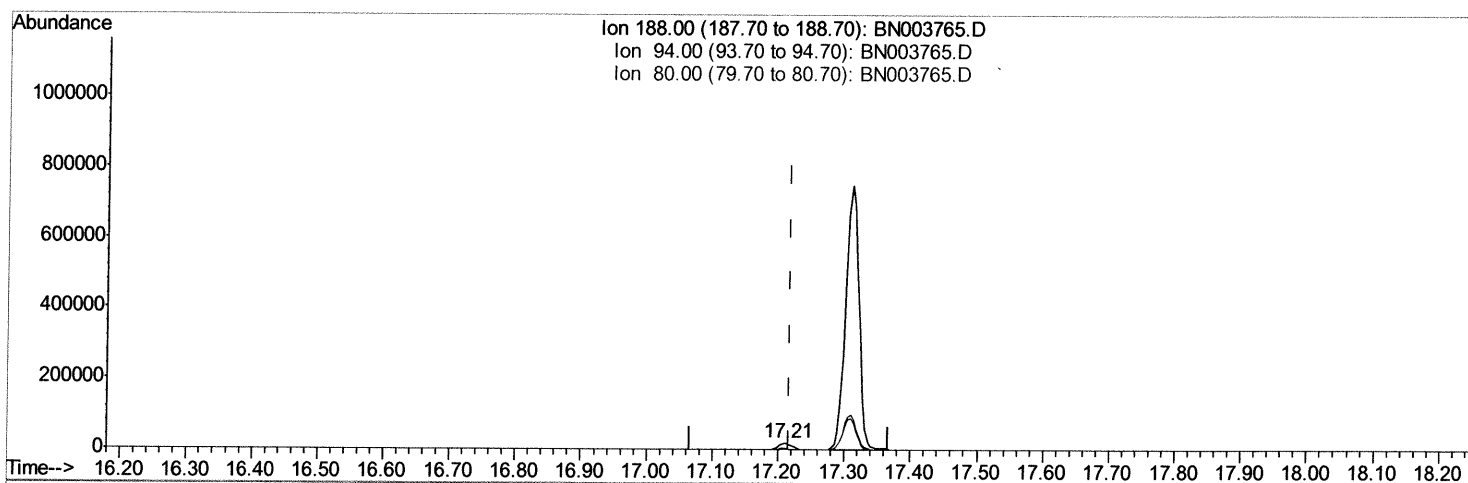

(10) Phenanthrene-d10 (I)

17.213min (-0.004) 0.40ng/ul m

response 24527

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.05
80.00	11.60	11.90
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003765.D
 Acq On : 07 Dec 2018 14:23
 Operator : JU/SJ
 Sample : J6228-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E88

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:19 AM

Quant Time: Dec 07 16:12:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:33:20 2018
 Response via : Initial Calibration

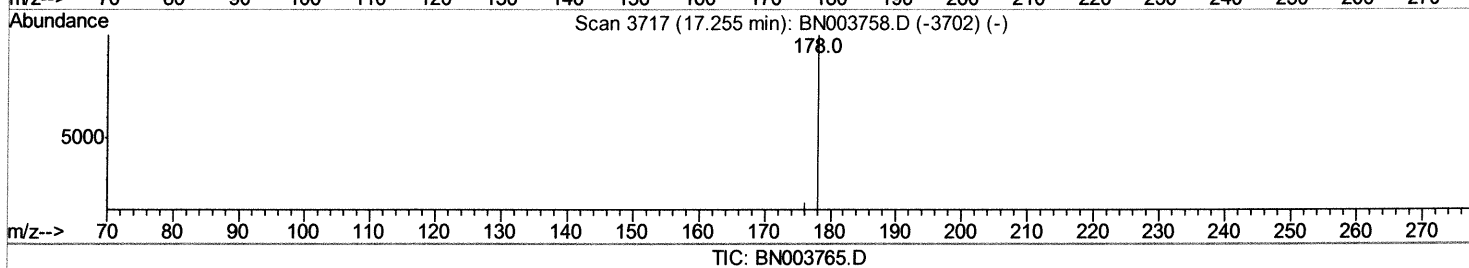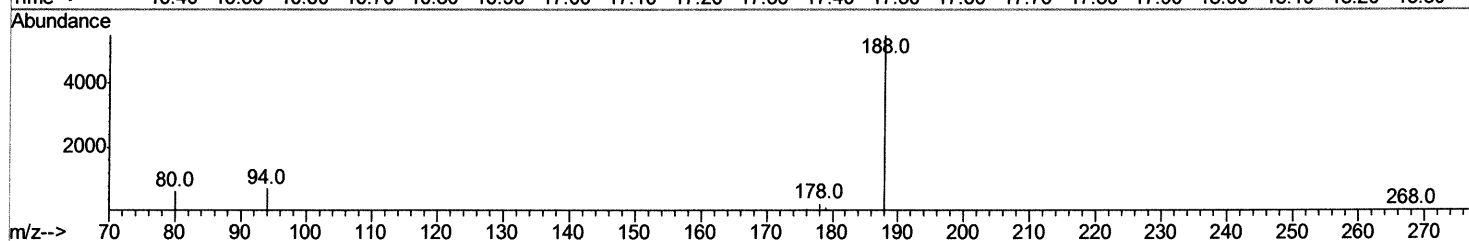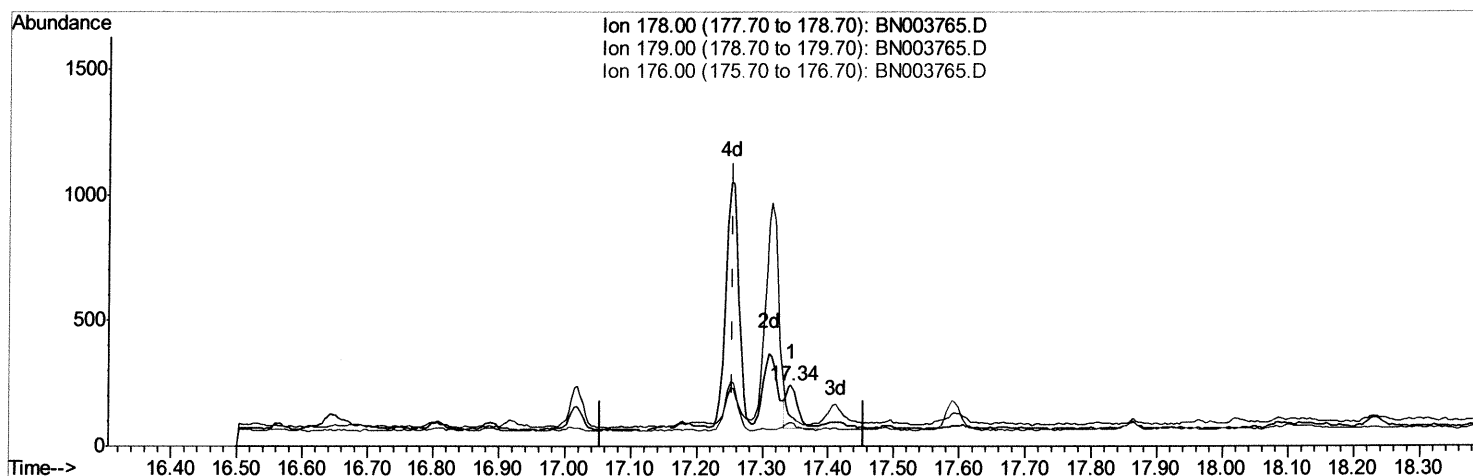

(12) Phenanthrene

17.344min (+0.089) 0.00ng/ul

response 222

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	49.38#
176.00	18.70	39.09#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003765.D
Acq On : 07 Dec 2018 14:23
Operator : JU/SJ
Sample : J6228-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E88

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:19 AM

Quant Time: Dec 07 16:12:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

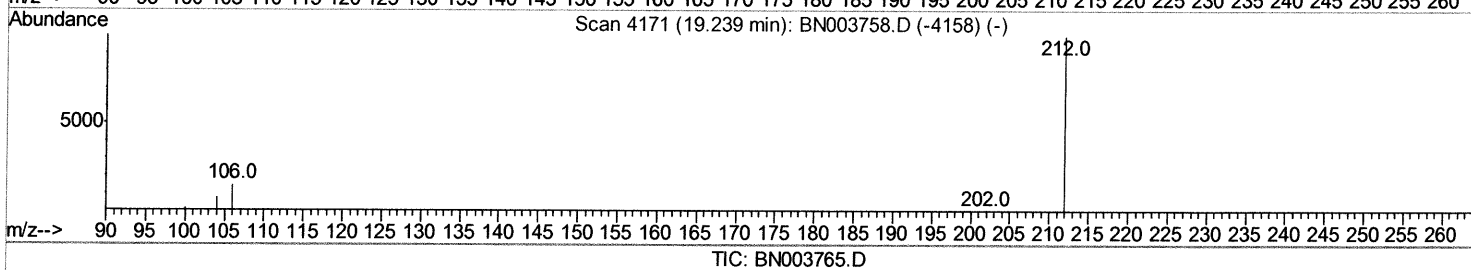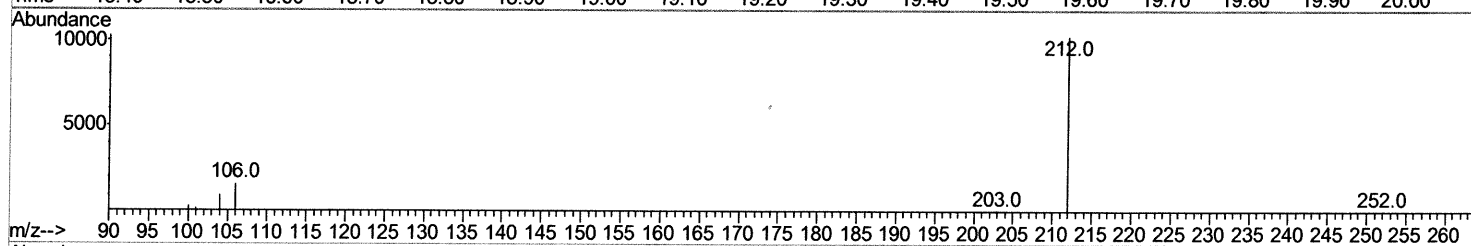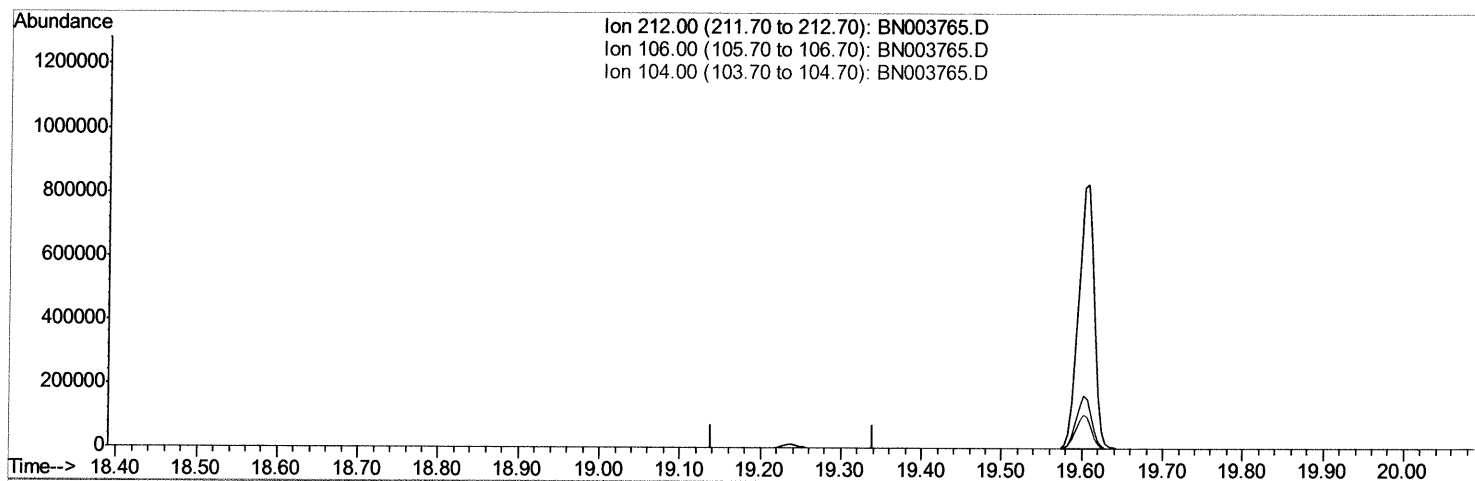

(14) Fluoranthene-d10 (SURR)

19.239min (-19.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003765.D
Acq On : 07 Dec 2018 14:23
Operator : JU/SJ
Sample : J6228-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E88

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:19 AM

Quant Time: Dec 07 16:12:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

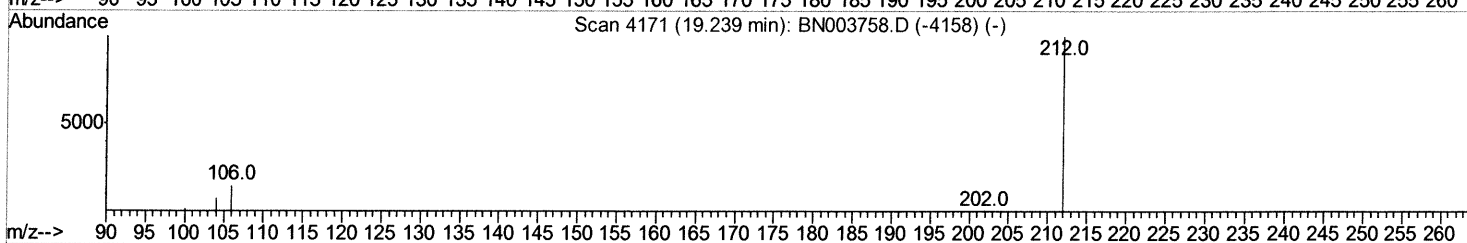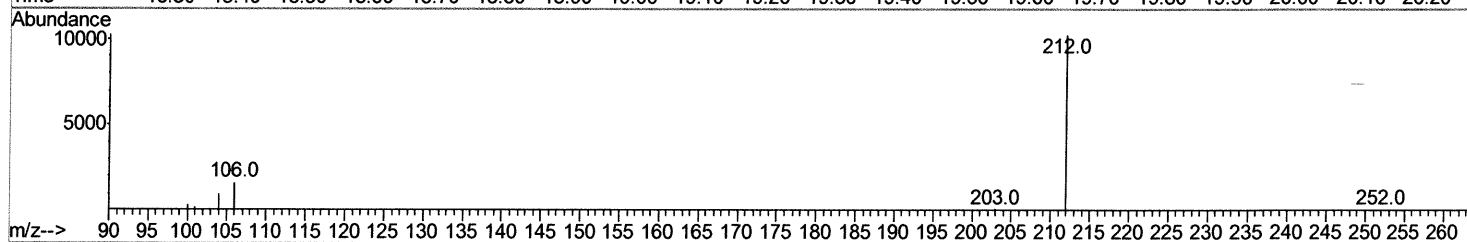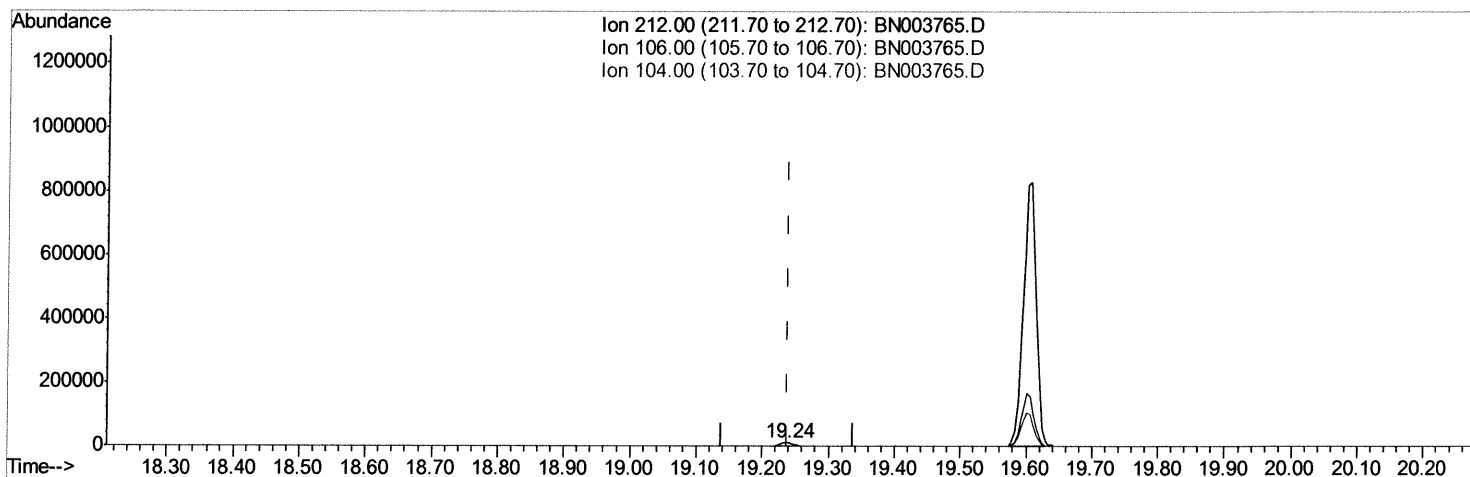

TIC: BN003765.D

(14) Fluoranthene-d10 (SURR)

19.239min (+0.000) 0.20ng/ul m

response 14101

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003765.D
Acq On : 07 Dec 2018 14:23
Operator : JU/SJ
Sample : J6228-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E88

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:19 AM

Quant Time: Dec 07 16:12:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

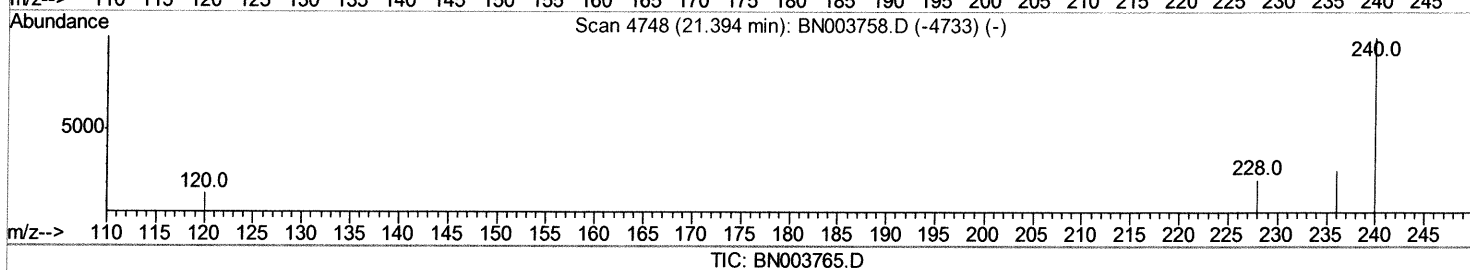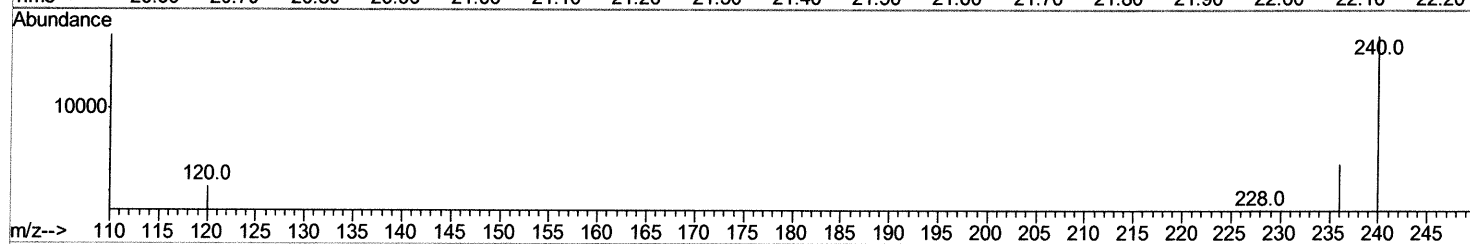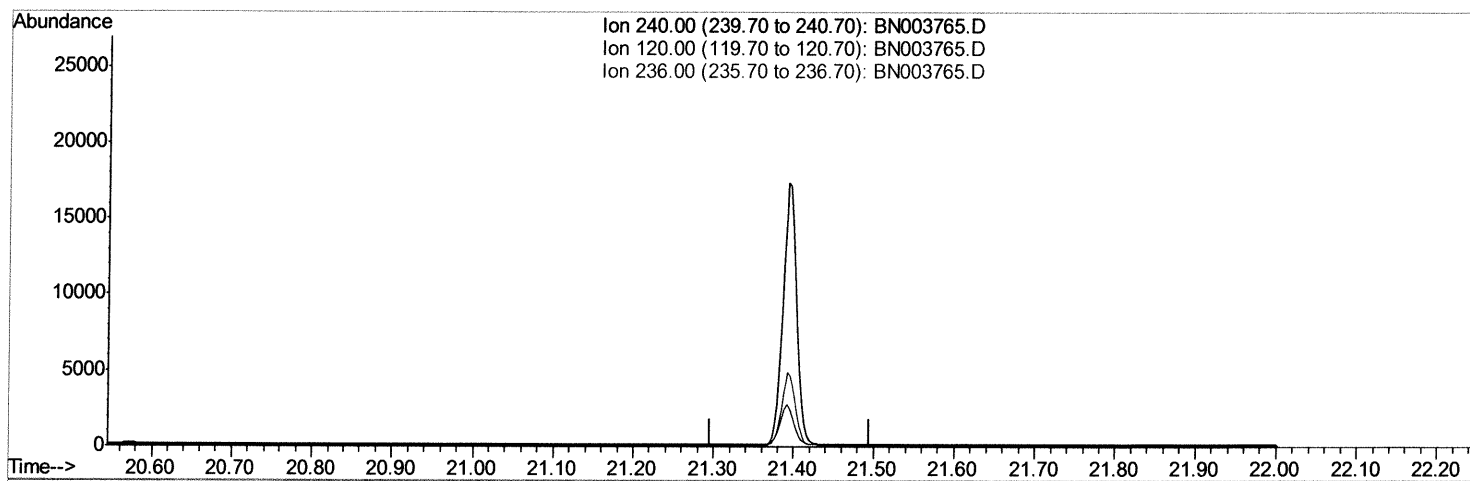

(16) Chrysene-d12 (I)

21.395min (-21.395) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003765.D
Acq On : 07 Dec 2018 14:23
Operator : JU/SJ
Sample : J6228-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E88

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:19 AM

Quant Time: Dec 07 16:12:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

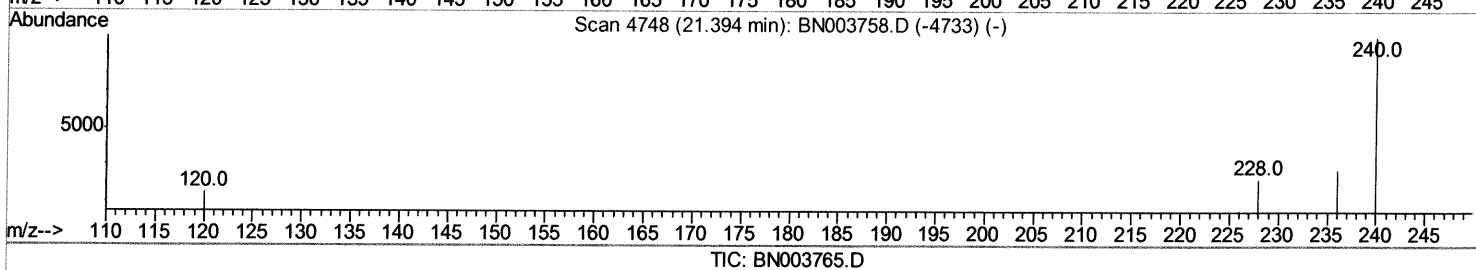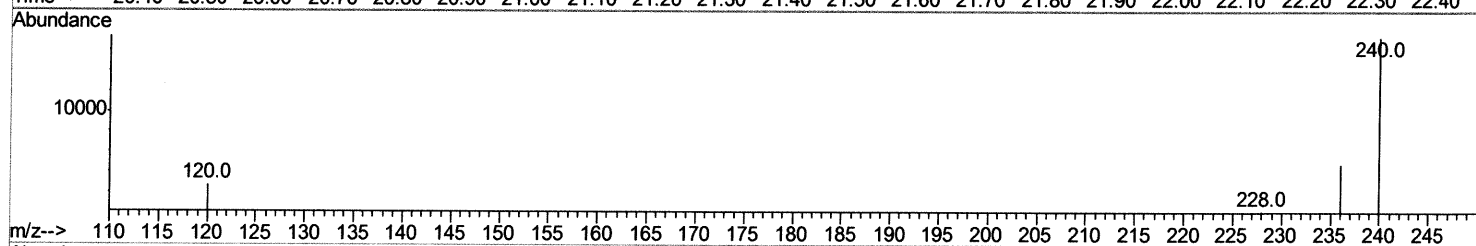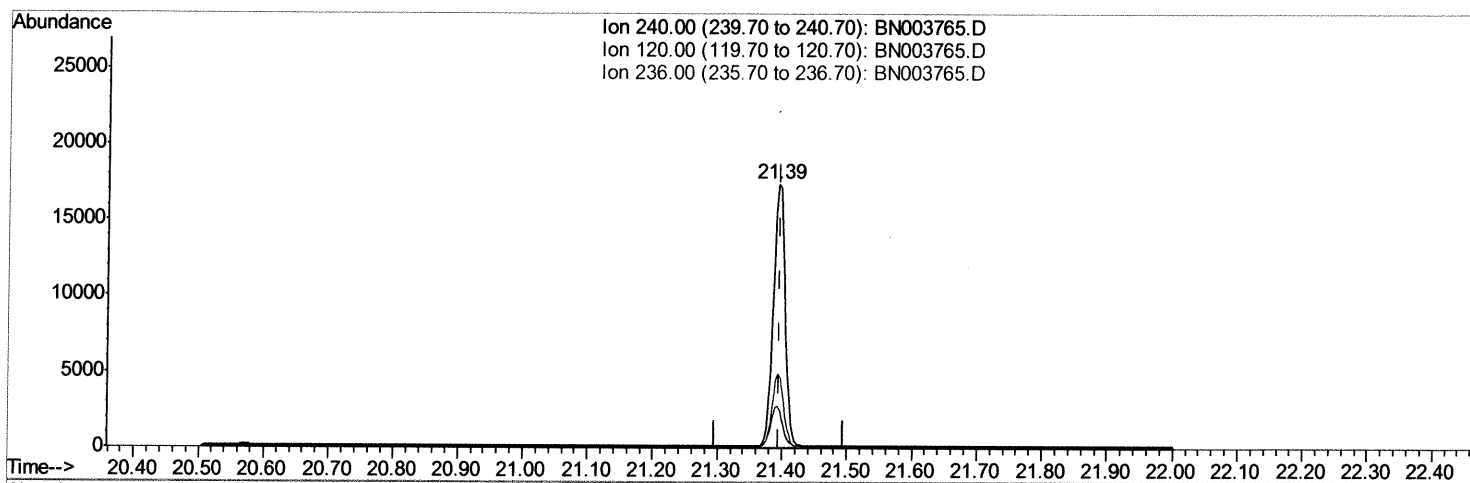

(16) Chrysene-d12 (I)

21.393min (-0.003) 0.40ng/ul m

response 21717

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	15.91
236.00	27.60	28.15
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003765.D
Acq On : 07 Dec 2018 14:23
Operator : JU/SJ
Sample : J6228-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E88

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:19 AM

Quant Time: Dec 07 16:14:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4814	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	20238	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11015	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	24527m	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	21717m	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	20619	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.22	152	5974	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	14101m	0.20	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003765.D
Acq On : 07 Dec 2018 14:23
Operator : JU/SJ
Sample : J6228-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E88

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:19 AM

Quant Time: Dec 07 16:14:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:33:20 2018
Response via : Initial Calibration

