

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003768.D
 Acq On : 07 Dec 2018 16:08
 Operator : JU/SJ
 Sample : J6228-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E91

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:20 AM

Quant Time: Dec 07 16:43:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:51:04 2018
 Response via : Initial Calibration

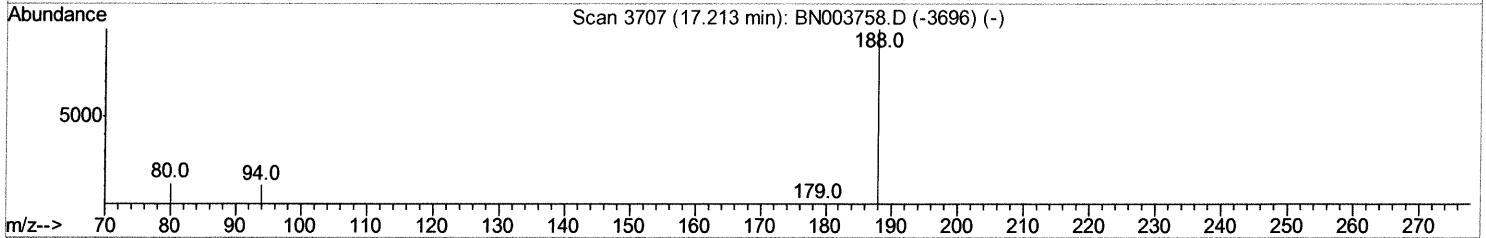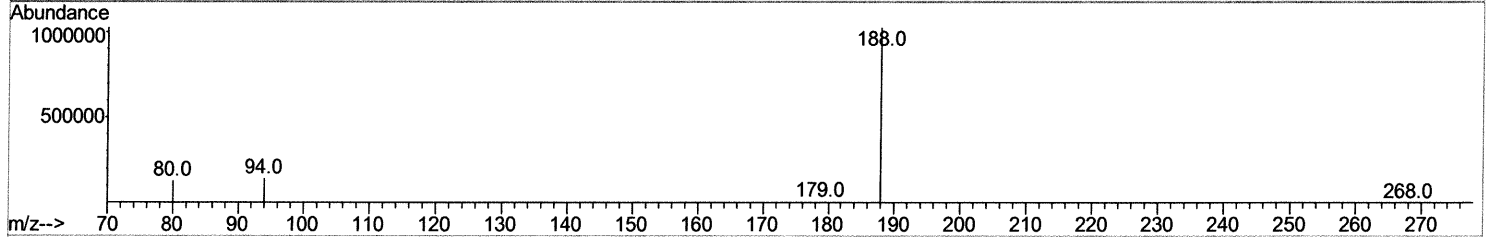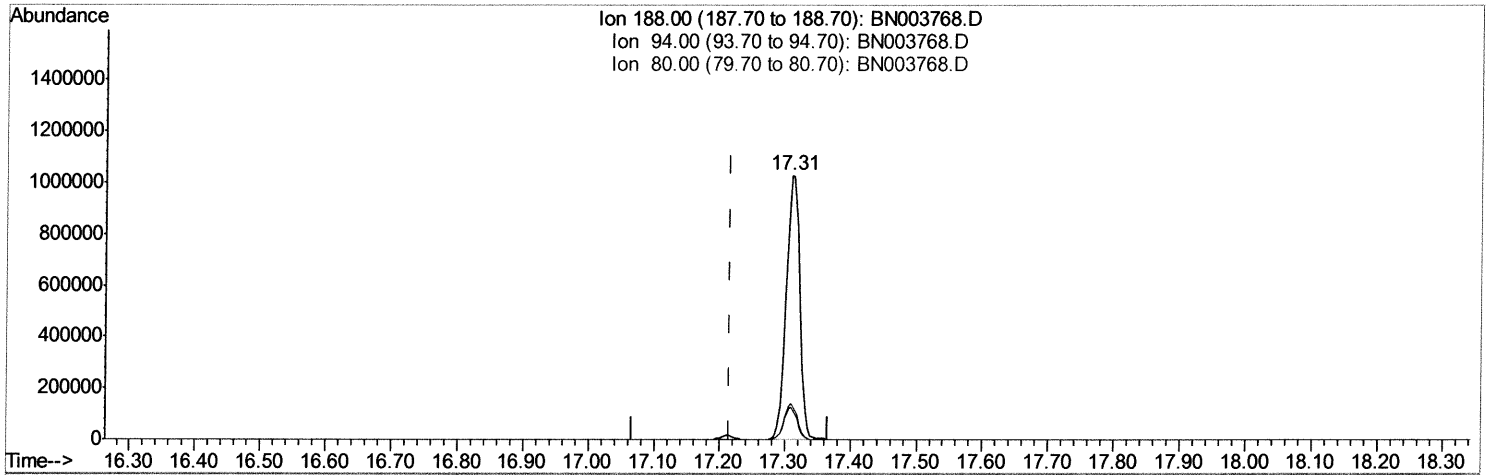

TIC: BN003768.D

(10) Phenanthrene-d10 (I)
 17.310min (+0.093) 0.40ng/ul
 response 1462742

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.53#
80.00	11.60	12.28
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003768.D
 Acq On : 07 Dec 2018 16:08
 Operator : JU/SJ
 Sample : J6228-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E91

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:20 AM

Quant Time: Dec 07 16:43:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:51:04 2018
 Response via : Initial Calibration

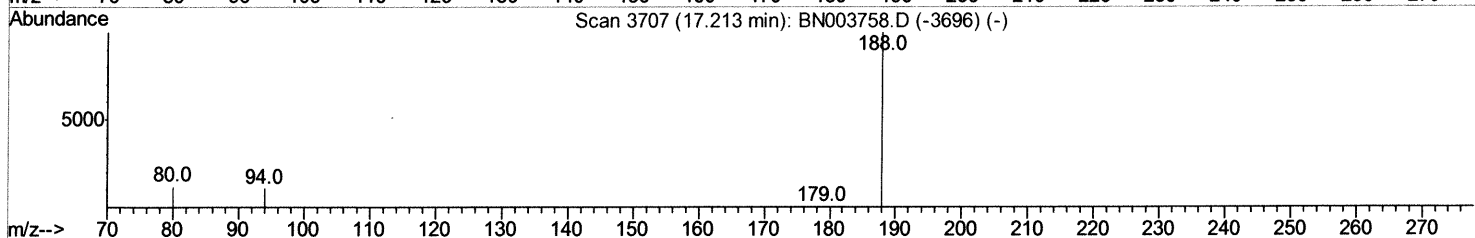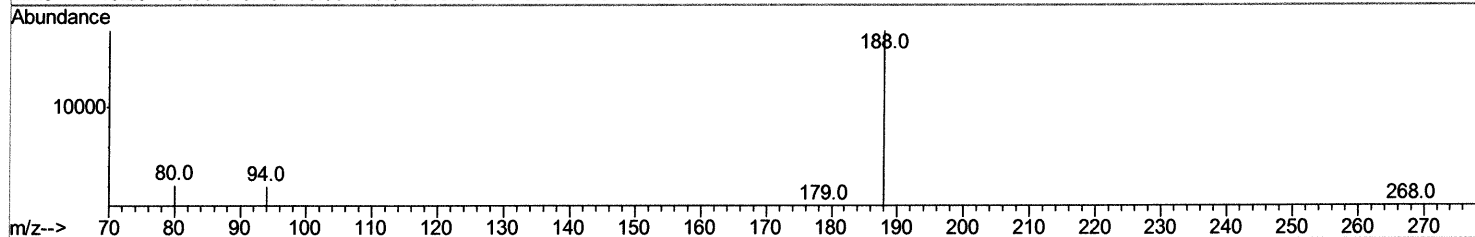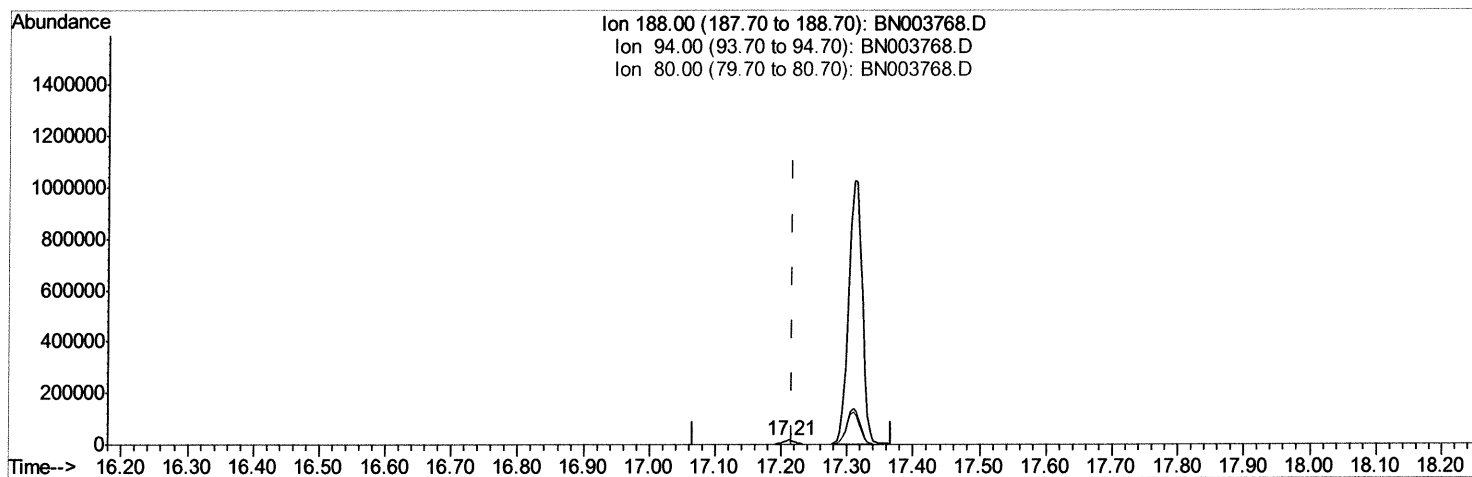

TIC: BN003768.D

(10) Phenanthrene-d10 (I)

17.213min (-0.004) 0.40ng/ul m

response 24417

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.29
80.00	11.60	12.09
0.00	0.00	0.00

MA
 12/11/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003768.D
 Acq On : 07 Dec 2018 16:08
 Operator : JU/SJ
 Sample : J6228-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E91

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:20 AM

Quant Time: Dec 07 16:47:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:51:04 2018
 Response via : Initial Calibration

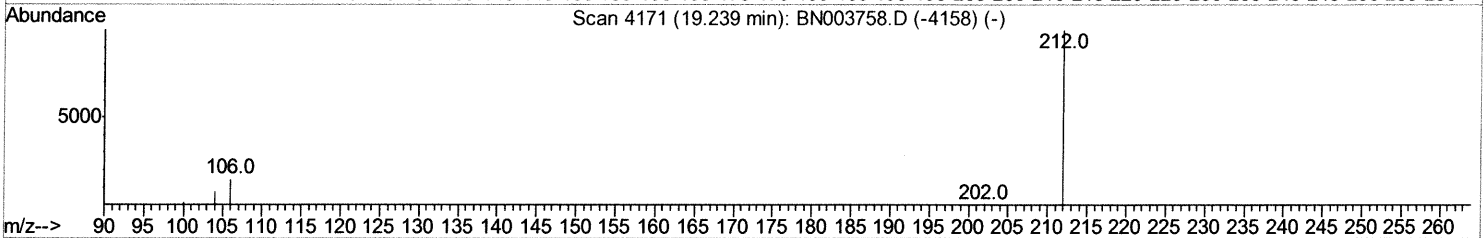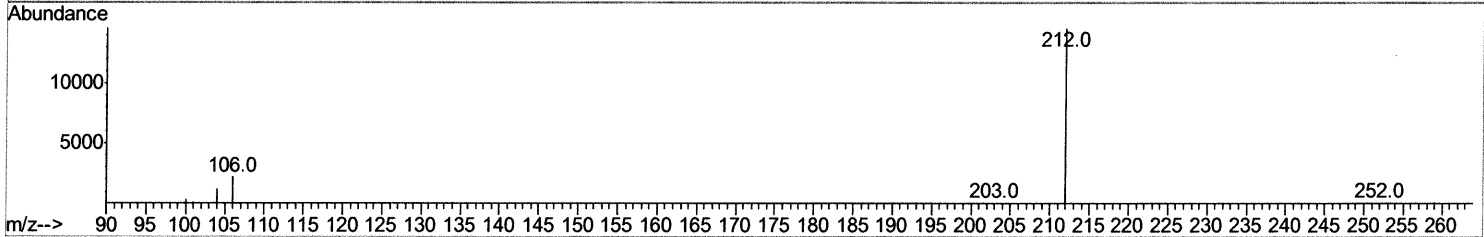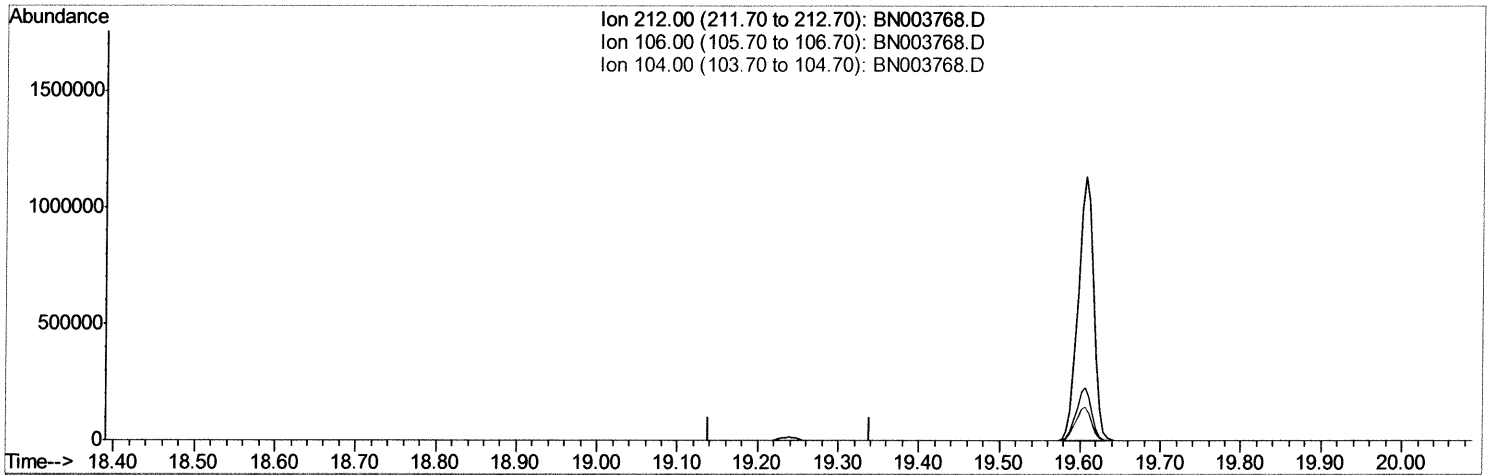

TIC: BN003768.D

(14) Fluoranthene-d10 (SURR)

19.239min (-19.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003768.D
 Acq On : 07 Dec 2018 16:08
 Operator : JU/SJ
 Sample : J6228-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E91

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:20 AM

Quant Time: Dec 07 16:47:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:51:04 2018
 Response via : Initial Calibration

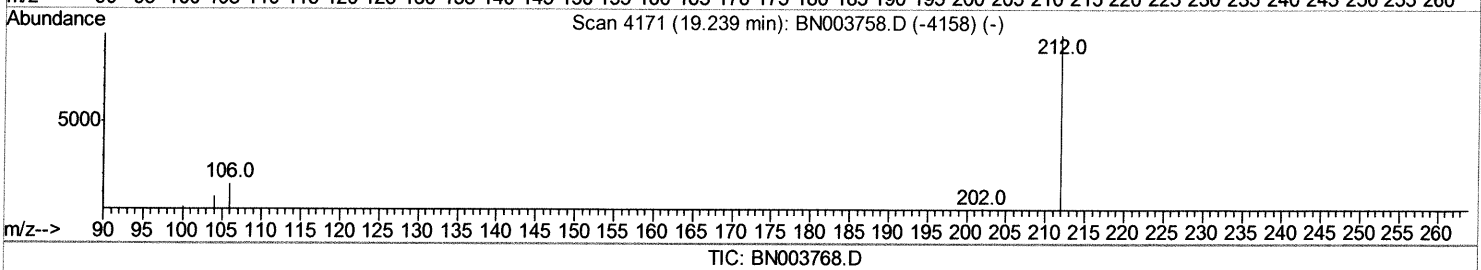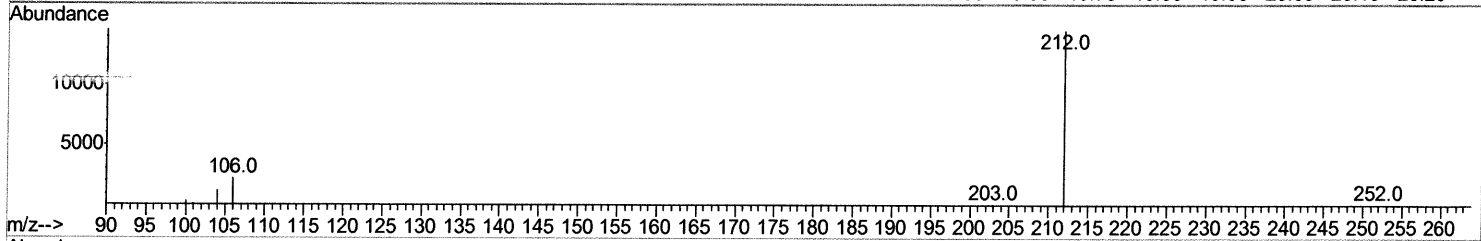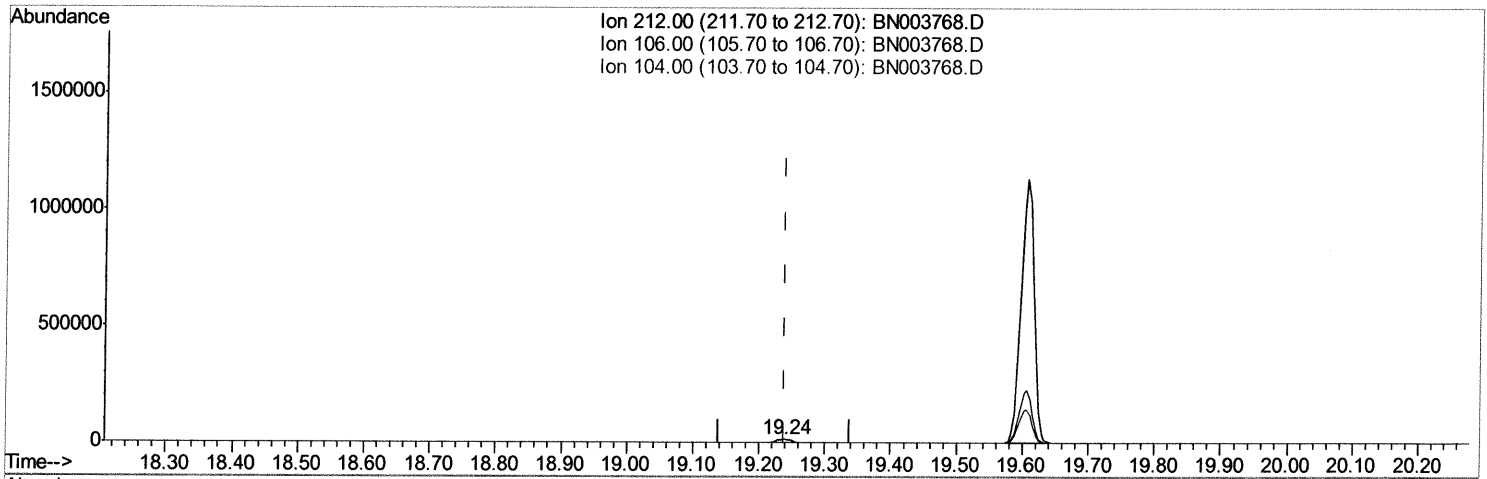

(14) Fluoranthene-d10 (SURR)

19.239min (-0.000) 0.27ng/ul m/s 12/11/18

response 19605

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003768.D
Acq On : 07 Dec 2018 16:08
Operator : JU/SJ
Sample : J6228-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E91

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:20 AM

Quant Time: Dec 07 16:47:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:51:04 2018
Response via : Initial Calibration

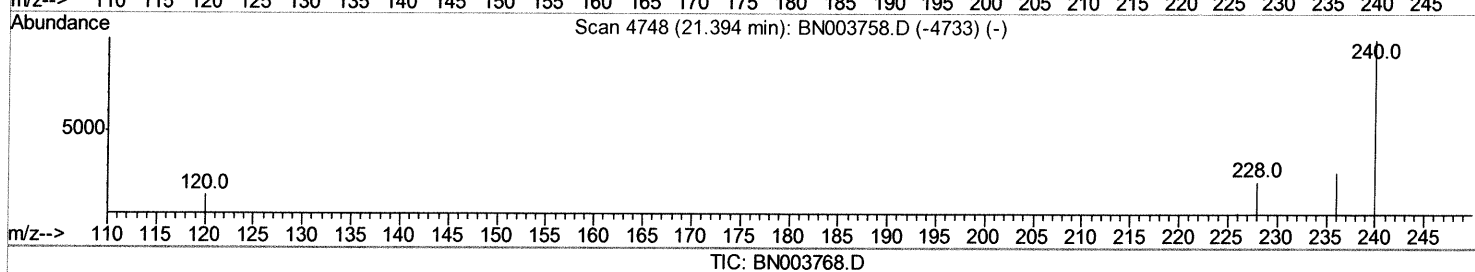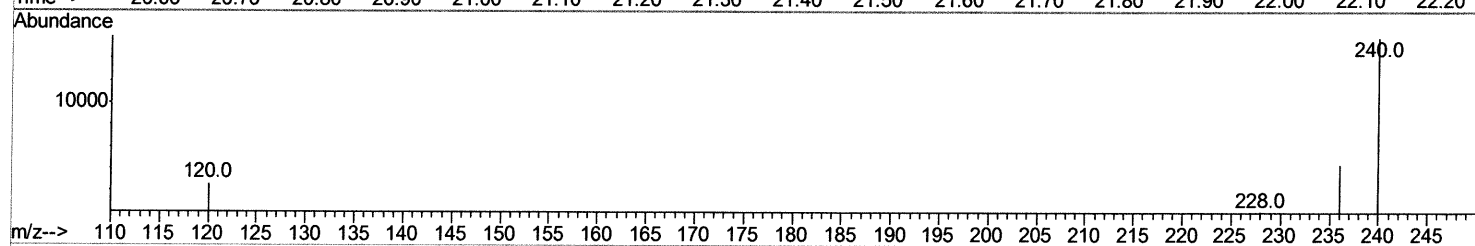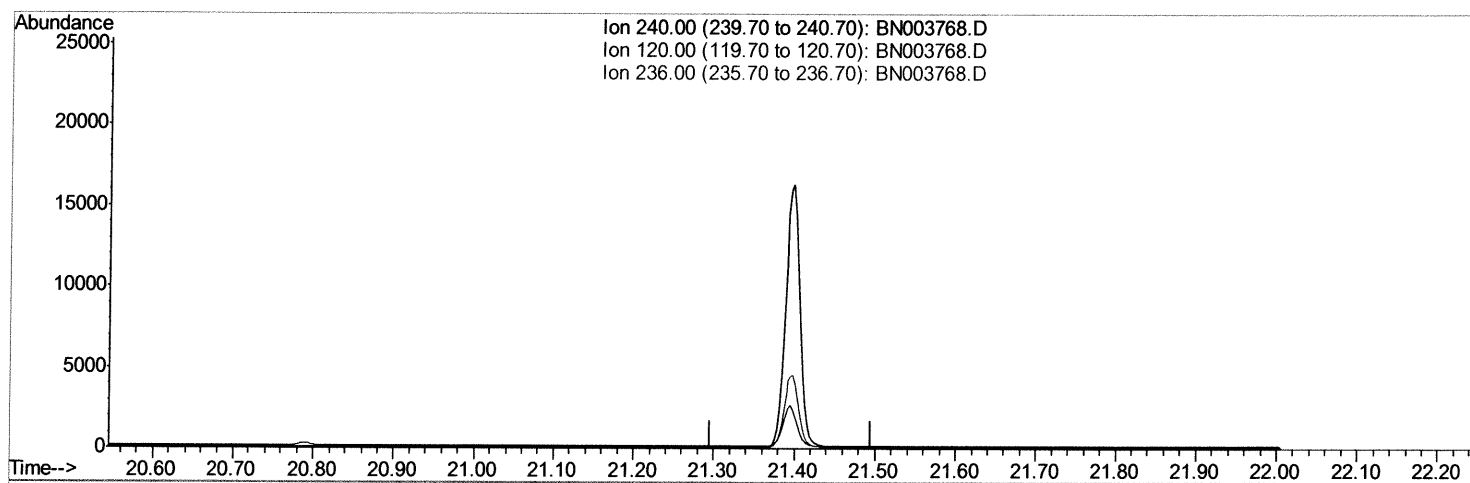

(16) Chrysene-d12 (I)

21.395min (-21.395) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003768.D
 Acq On : 07 Dec 2018 16:08
 Operator : JU/SJ
 Sample : J6228-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E91

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:20 AM

Quant Time: Dec 07 16:47:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 15:51:04 2018
 Response via : Initial Calibration

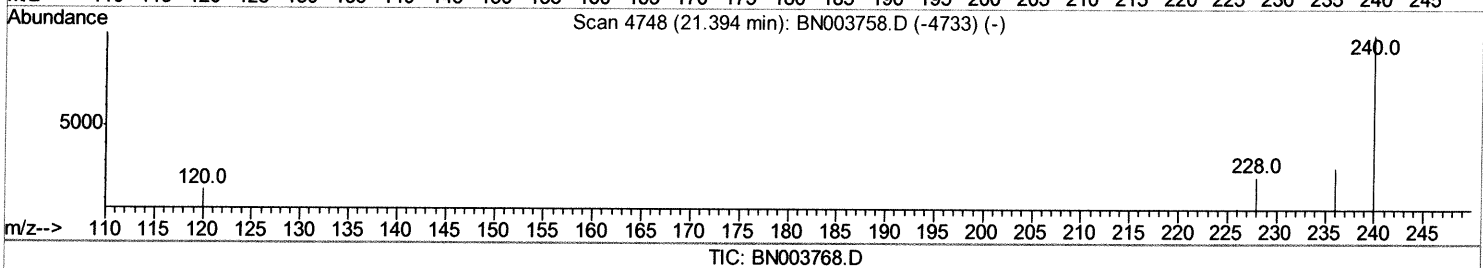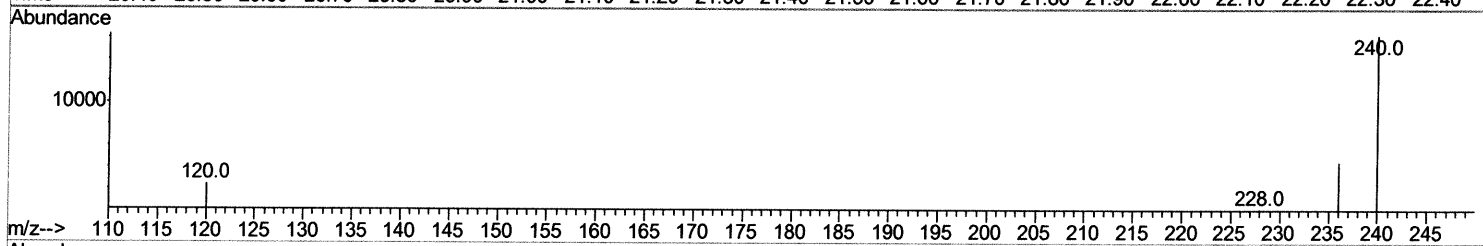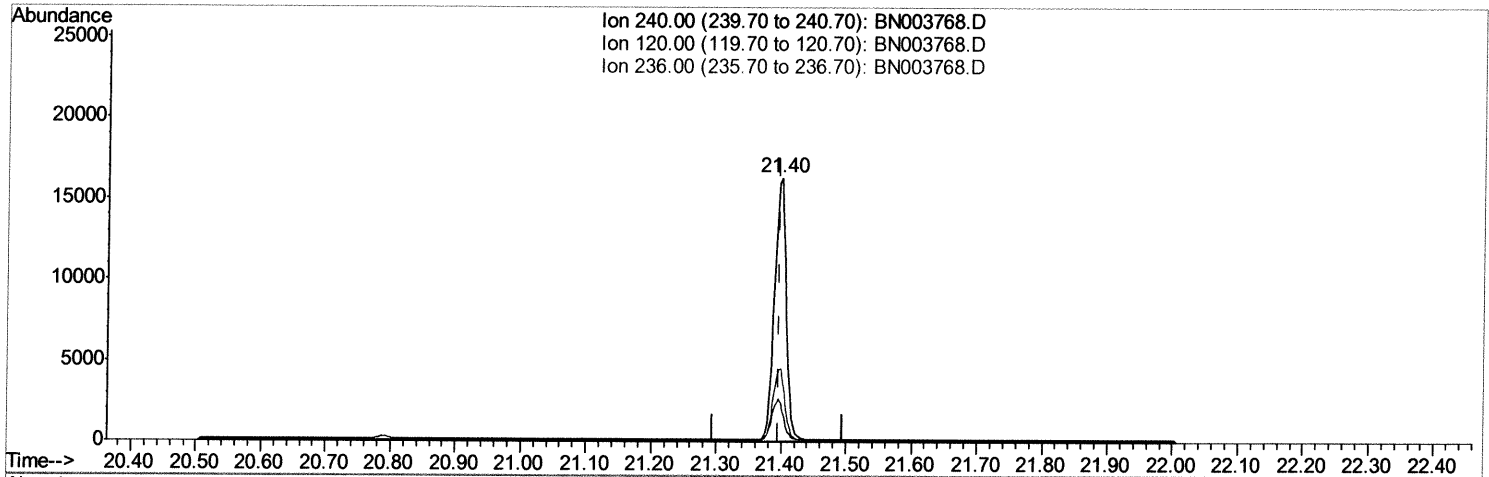

(16) Chrysene-d12 (I)

21.398min (+0.003) 0.40ng/ul m

response 20696

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	14.76
236.00	27.60	27.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003768.D
Acq On : 07 Dec 2018 16:08
Operator : JU/SJ
Sample : J6228-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E91

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:20 AM

Quant Time: Dec 07 16:48:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:51:04 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4821	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	20125	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11181	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	24417m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	20696m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	19891	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.21	152	8362	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	19605m	0.27	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003768.D
Acq On : 07 Dec 2018 16:08
Operator : JU/SJ
Sample : J6228-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E91

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:20 AM

Quant Time: Dec 07 16:48:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 15:51:04 2018
Response via : Initial Calibration

