

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003770.D
Acq On : 07 Dec 2018 17:18
Operator : JU/SJ
Sample : J6228-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E85

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:22 AM

Quant Time: Dec 08 00:46:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

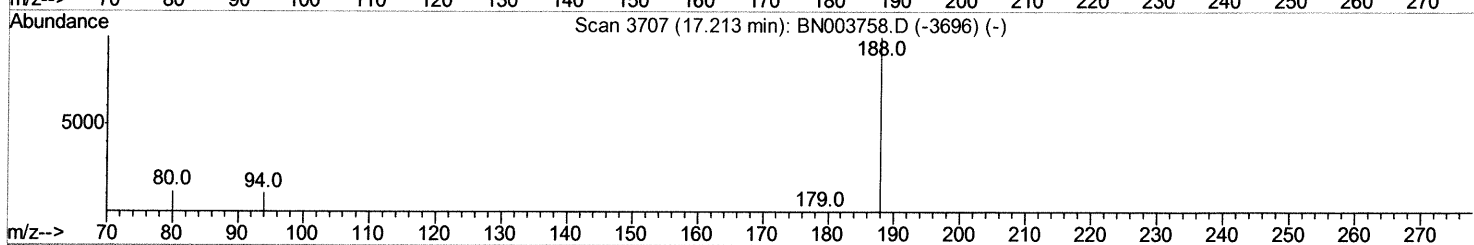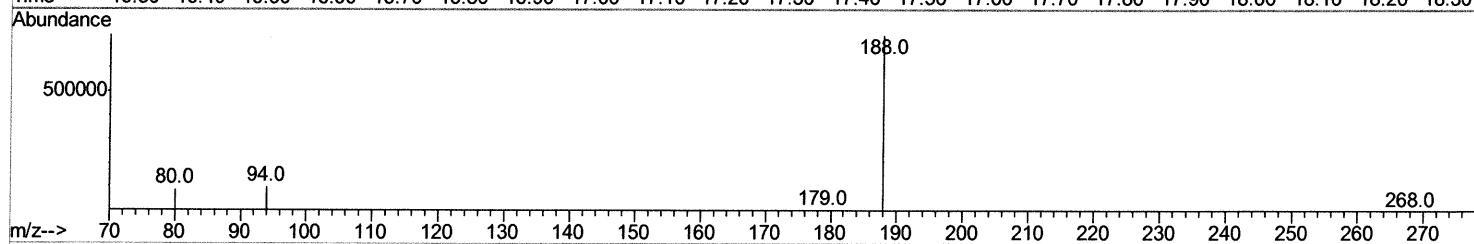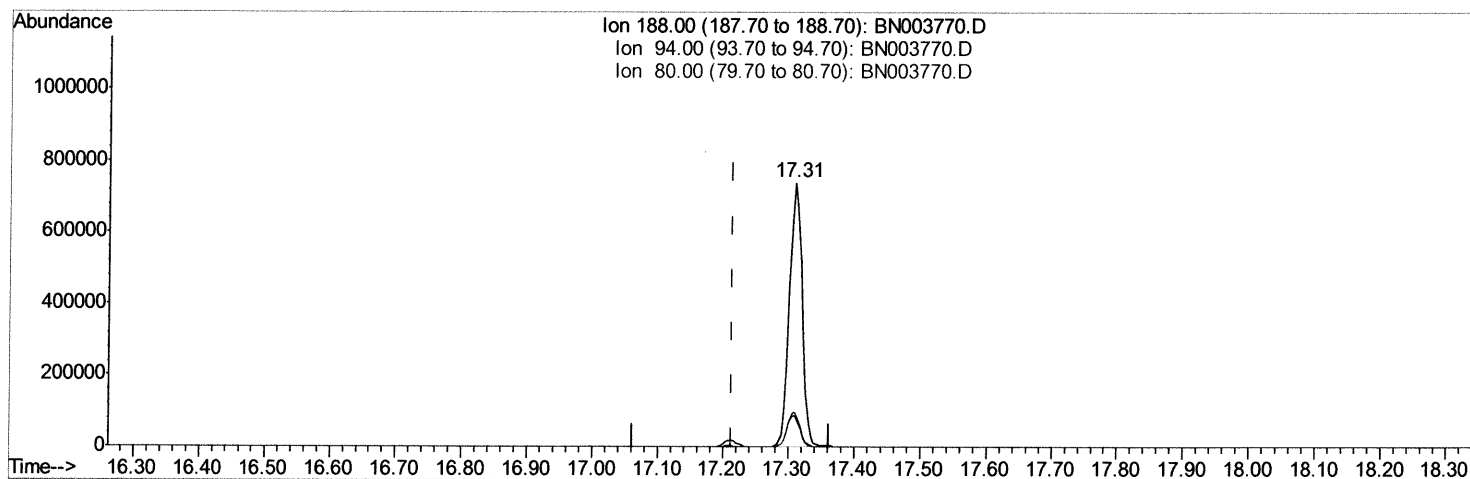

TIC: BN003770.D

(10) Phenanthrene-d10 (I)

17.309min (+0.097) 0.40ng/ul

response 1001306

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.07#
80.00	11.60	11.72
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003770.D
 Acq On : 07 Dec 2018 17:18
 Operator : JU/SJ
 Sample : J6228-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E85

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:22 AM

Quant Time: Dec 08 00:46:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

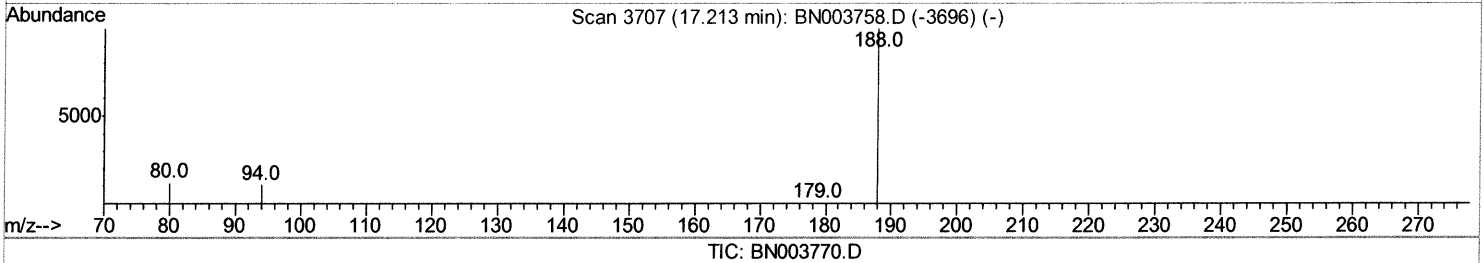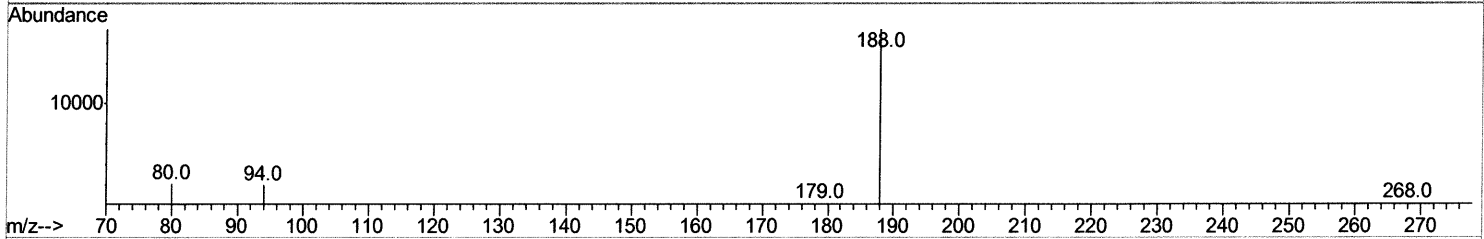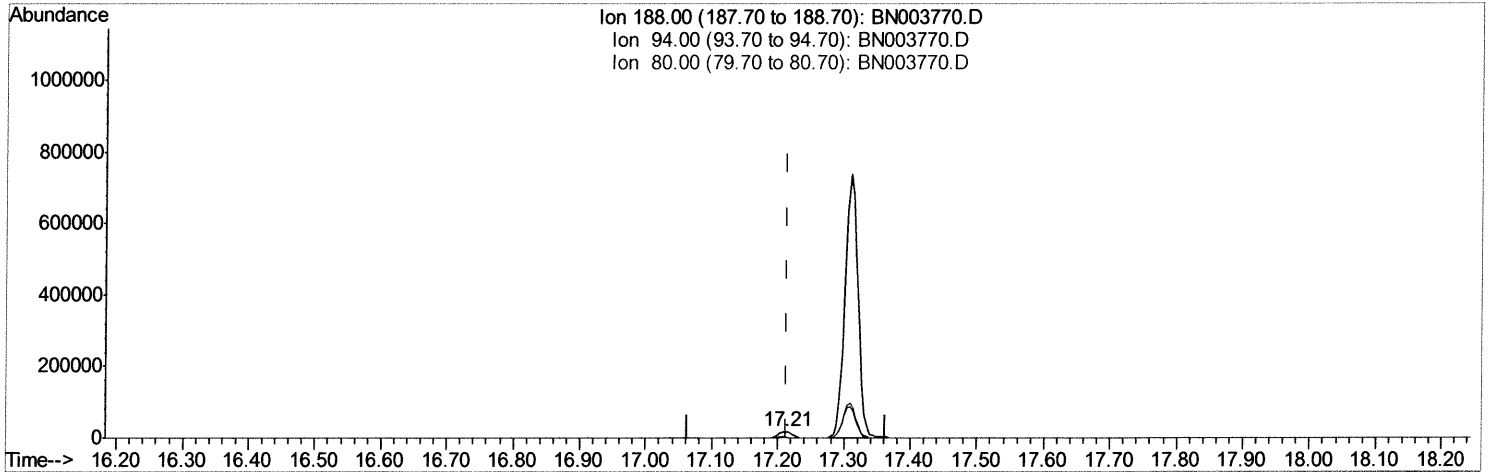

(10) Phenanthrene-d10 (I)

17.212min (-0.000) 0.40ng/ul m

response 24215

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.97
80.00	11.60	11.85
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003770.D
 Acq On : 07 Dec 2018 17:18
 Operator : JU/SJ
 Sample : J6228-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E85

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:22 AM

Quant Time: Dec 08 00:47:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

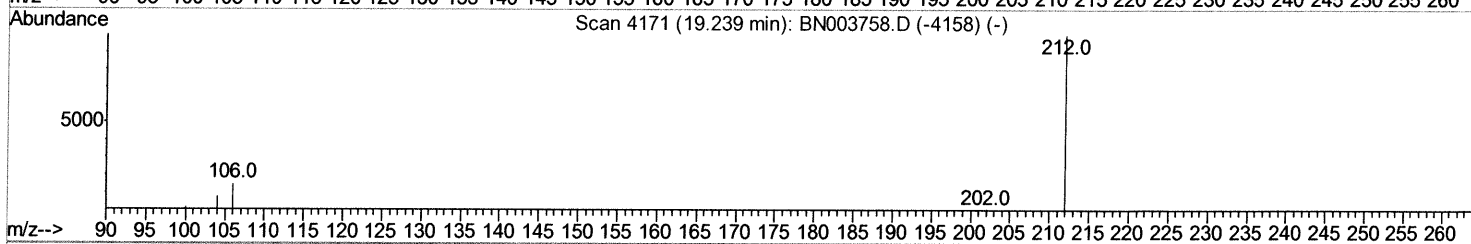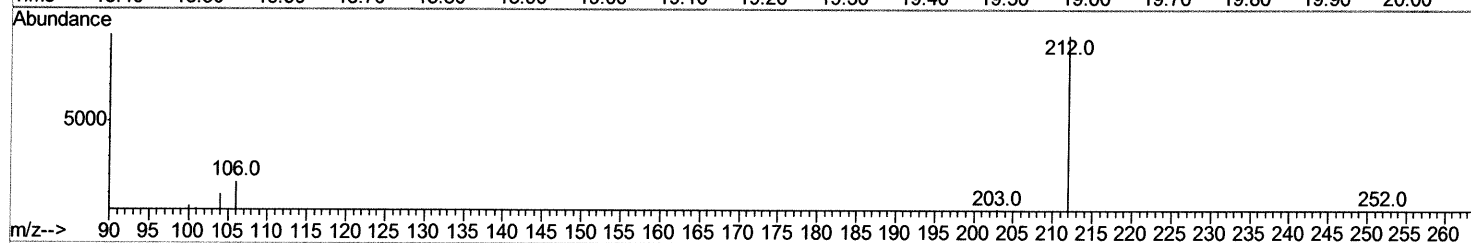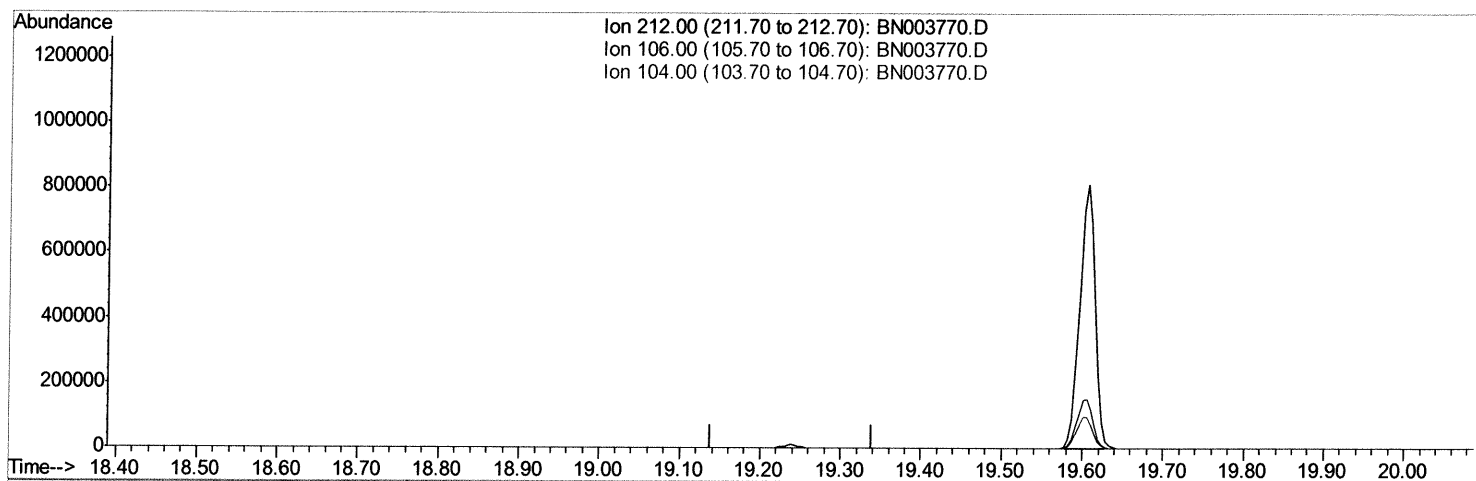

TIC: BN003770.D

(14) Fluoranthene-d10 (SURR)

19.239min (-19.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003770.D
 Acq On : 07 Dec 2018 17:18
 Operator : JU/SJ
 Sample : J6228-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E85

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:22 AM

Quant Time: Dec 08 00:47:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

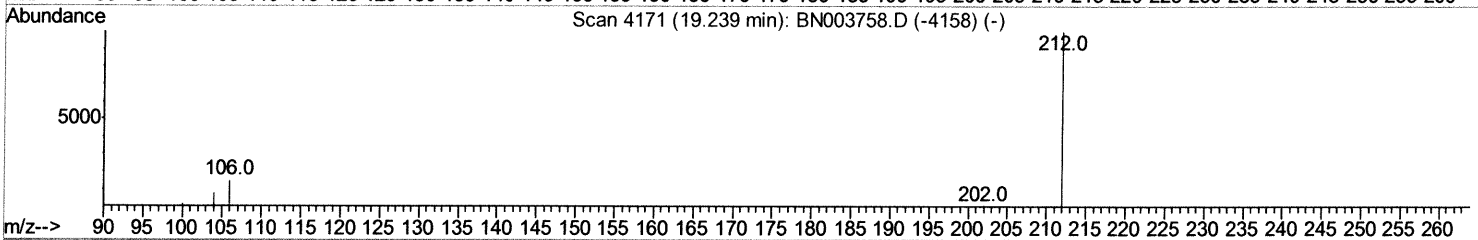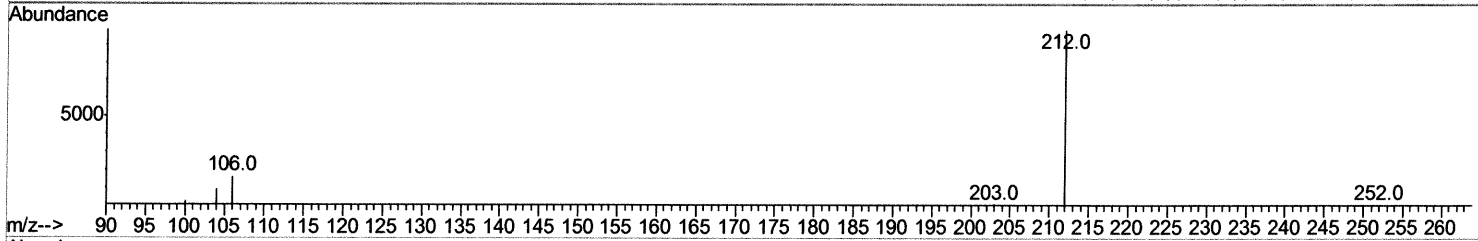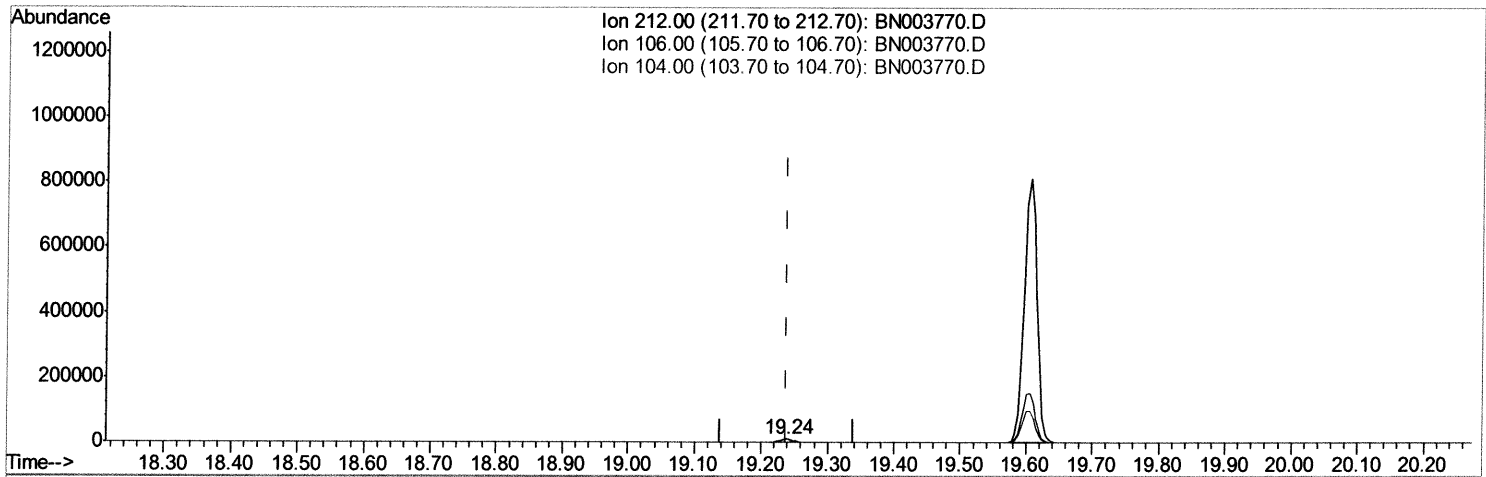

TIC: BN003770.D

(14) Fluoranthene-d10 (SURR)

19.238min (-0.000) 0.19ng/ul m

response 13645

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

MA
 12/11/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003770.D
Acq On : 07 Dec 2018 17:18
Operator : JU/SJ
Sample : J6228-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E85

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:22 AM

Quant Time: Dec 08 00:47:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

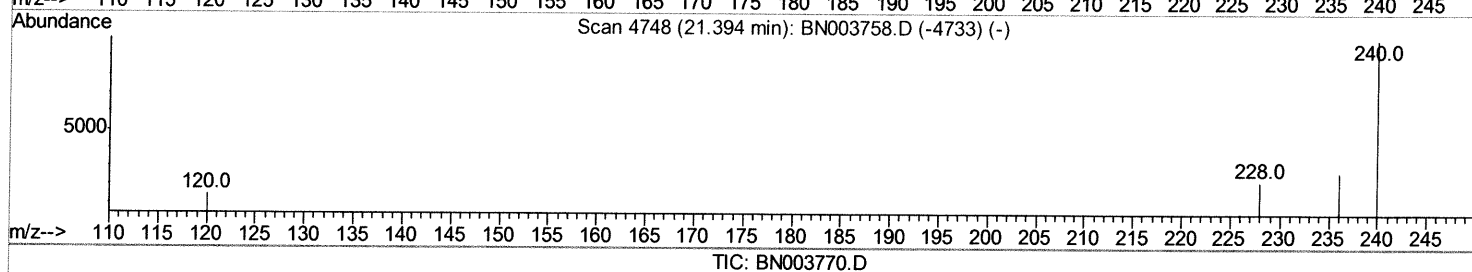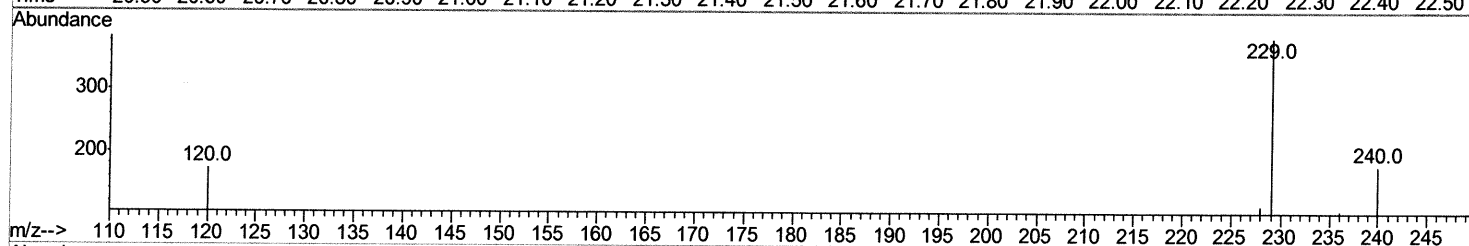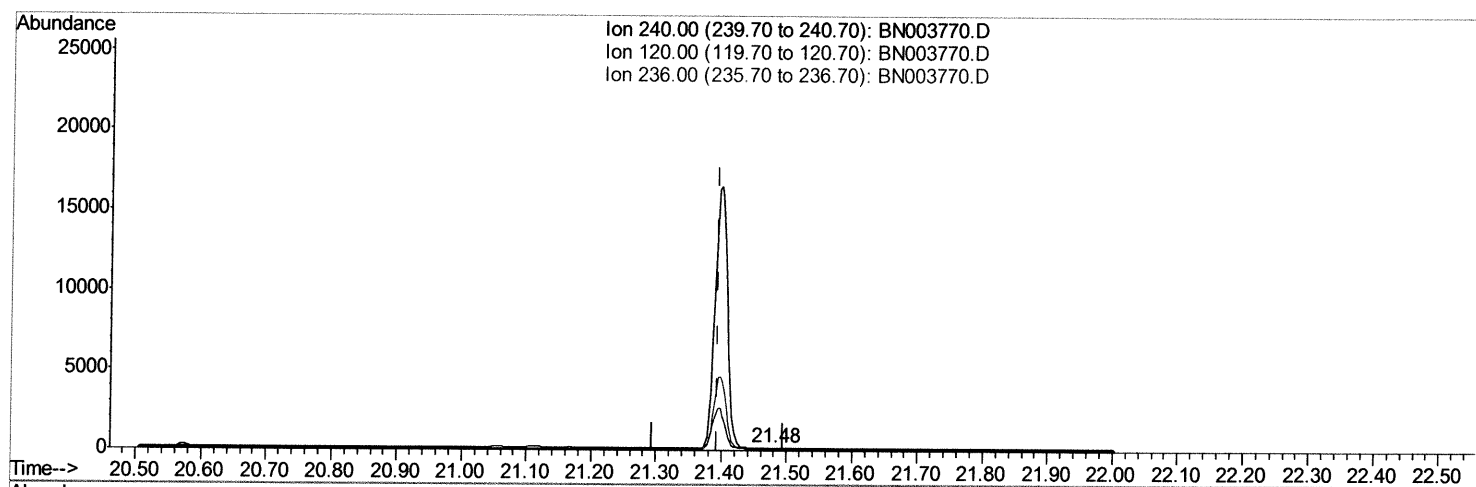

TIC: BN003770.D

(16) Chrysene-d12 (I)

21.480min (+0.086) 0.40ng/ul

response 171

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	96.65#
236.00	27.60	59.22#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003770.D
 Acq On : 07 Dec 2018 17:18
 Operator : JU/SJ
 Sample : J6228-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E85

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:22 AM

Quant Time: Dec 08 00:47:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

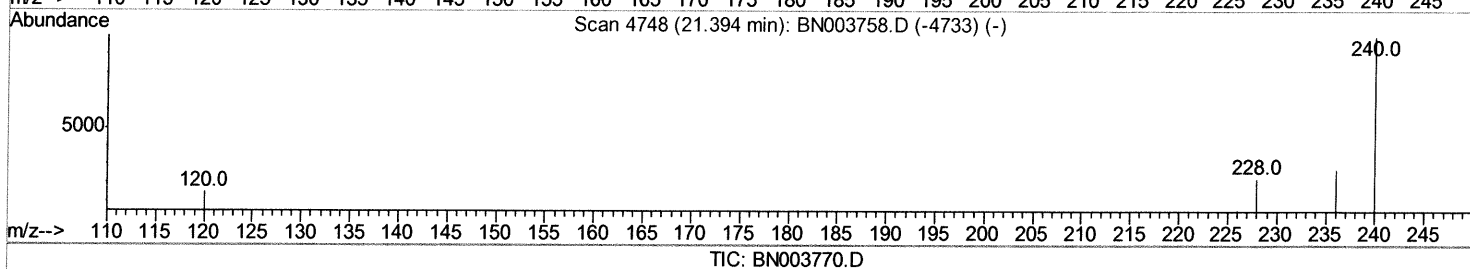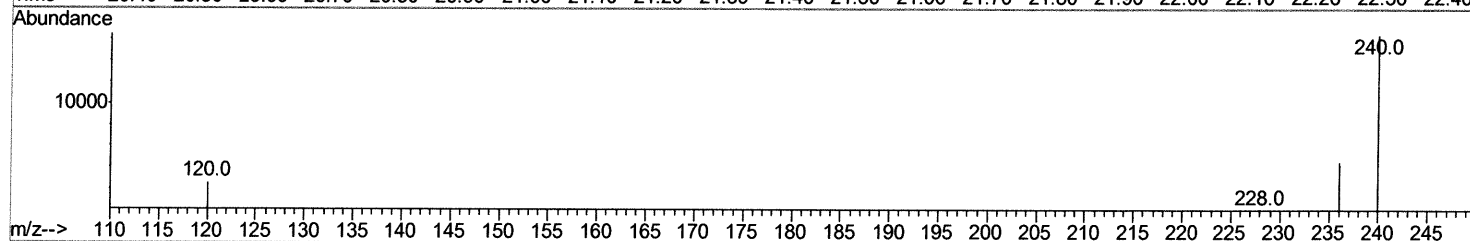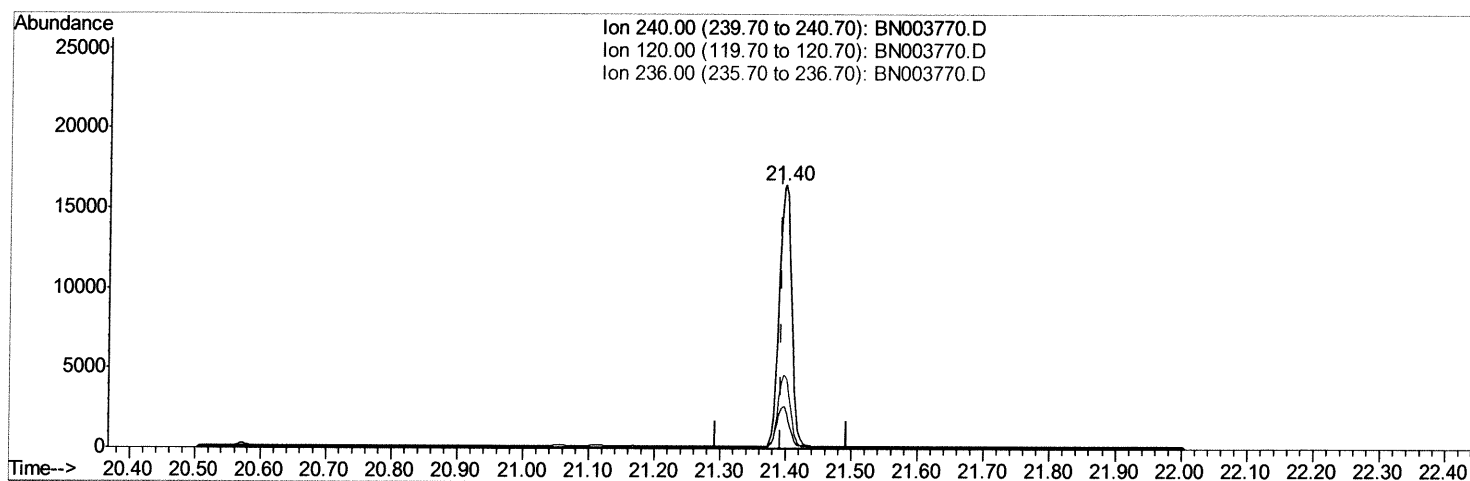

(16) Chrysene-d12 (I)

21.398min (+0.004) 0.40ng/ul m

response 21649

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	15.81
236.00	27.60	27.92
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003770.D
Acq On : 07 Dec 2018 17:18
Operator : JU/SJ
Sample : J6228-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E85

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:22 AM

Quant Time: Dec 08 00:47:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

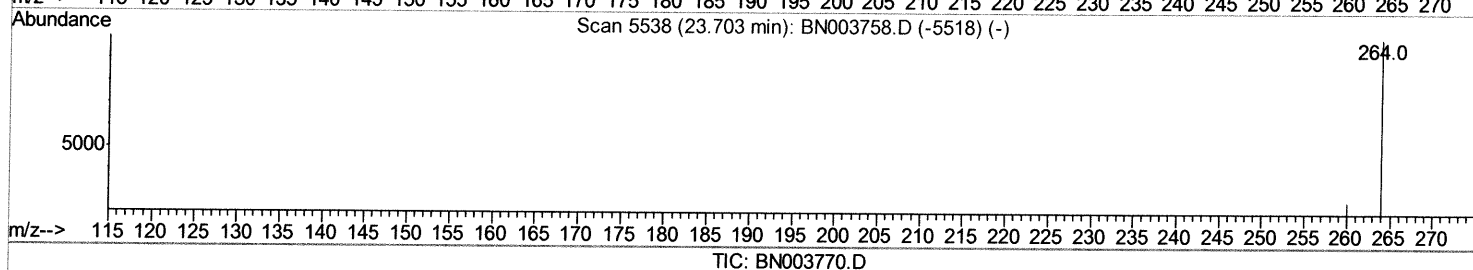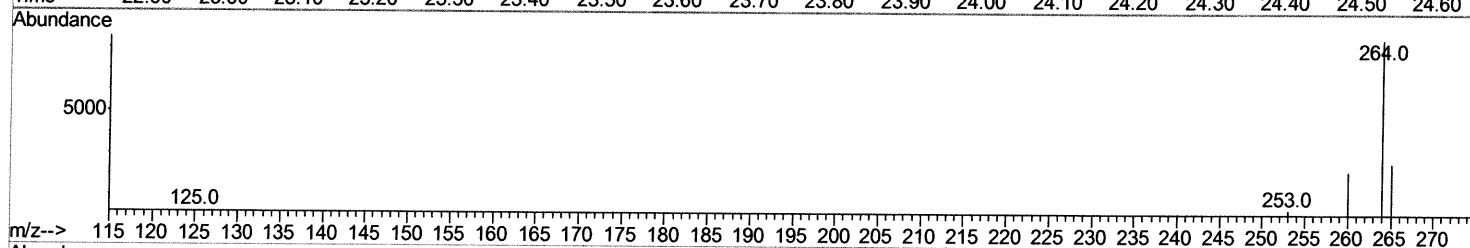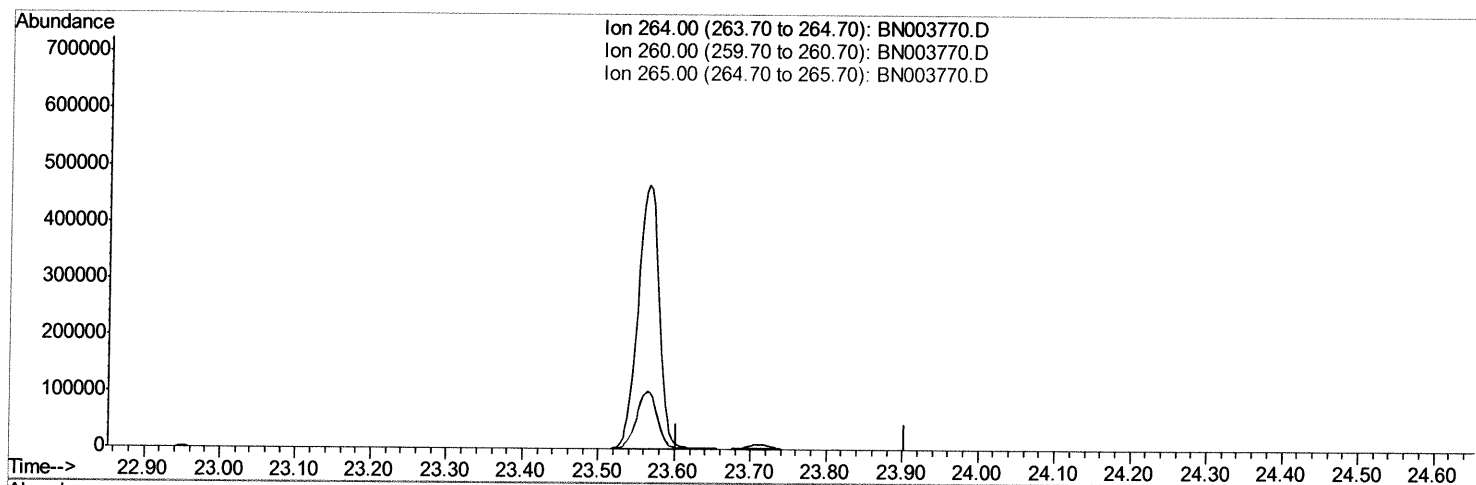

(20) Perylene-d12 (I)

23.703min (-23.703) 0.00ng/ul

response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	26.20	0.00#
265.00	33.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003770.D
 Acq On : 07 Dec 2018 17:18
 Operator : JU/SJ
 Sample : J6228-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 F9E85

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:22 AM

Quant Time: Dec 08 00:47:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

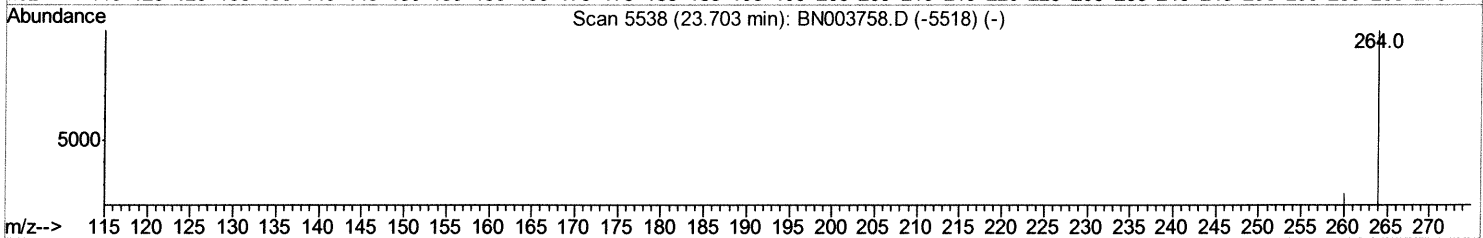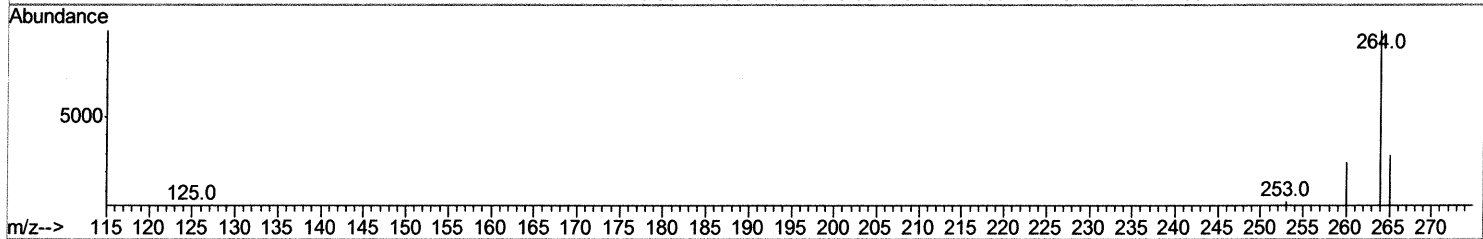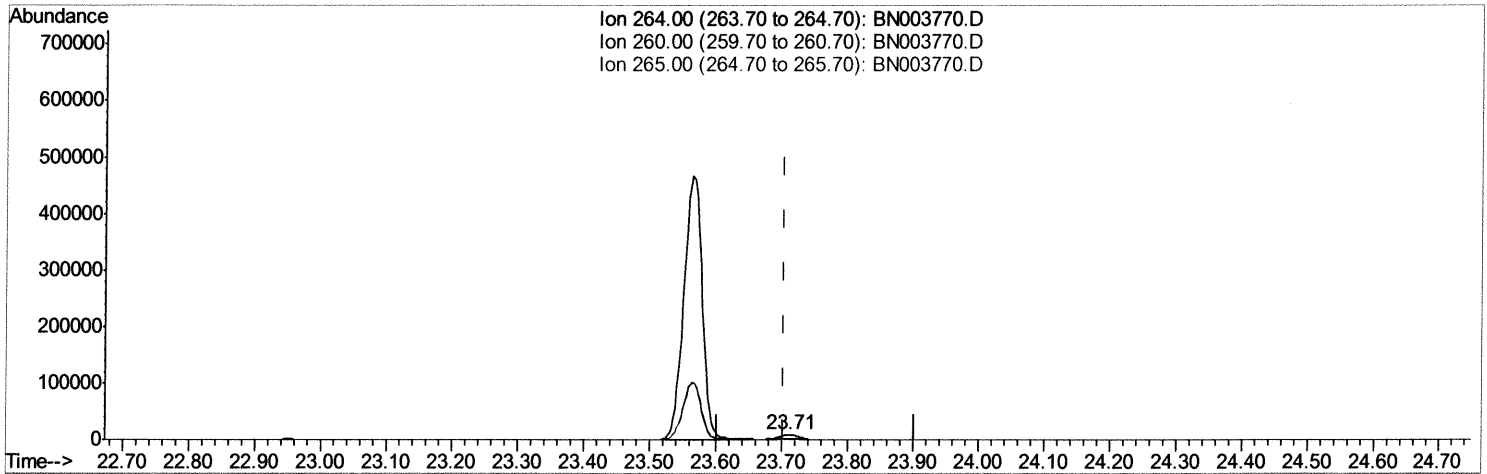

TIC: BN003770.D

(20) Perylene-d12 (I)

23.710min (+0.007) 0.40ng/ul m

response 17016

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.26
265.00	33.50	30.36
0.00	0.00	0.00

WA 12/11/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003770.D
Acq On : 07 Dec 2018 17:18
Operator : JU/SJ
Sample : J6228-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E85

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:22 AM

Quant Time: Dec 08 00:48:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4757	0.40	nq/ul	0.00
2) Naphthalene-d8	10.63	136	19848	0.40	nq/ul	0.00
6) Acenaphthene-d10	14.47	164	10875	0.40	nq/ul	0.00
10) Phenanthrene-d10	17.21	188	24215m	0.40	nq/ul	0.00
16) Chrysene-d12	21.40	240	21649m	0.40	nq/ul	0.00
20) Perylene-d12	23.71	264	17016m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.22	152	5657	0.19	nq/ul	0.00
14) Fluoranthene-d10	19.24	212	13645m	0.19	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003770.D
Acq On : 07 Dec 2018 17:18
Operator : JU/SJ
Sample : J6228-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E85

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:22 AM

Quant Time: Dec 08 00:48:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

