

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003771.D
Acq On : 07 Dec 2018 17:54
Operator : JU/SJ
Sample : J6228-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E53

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:37:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

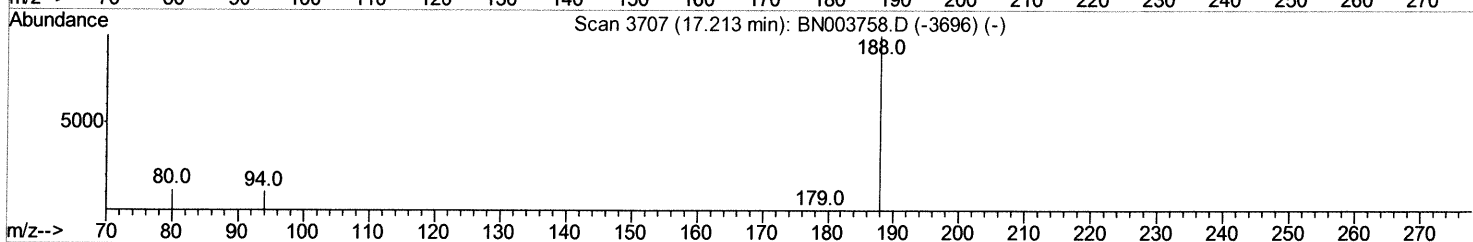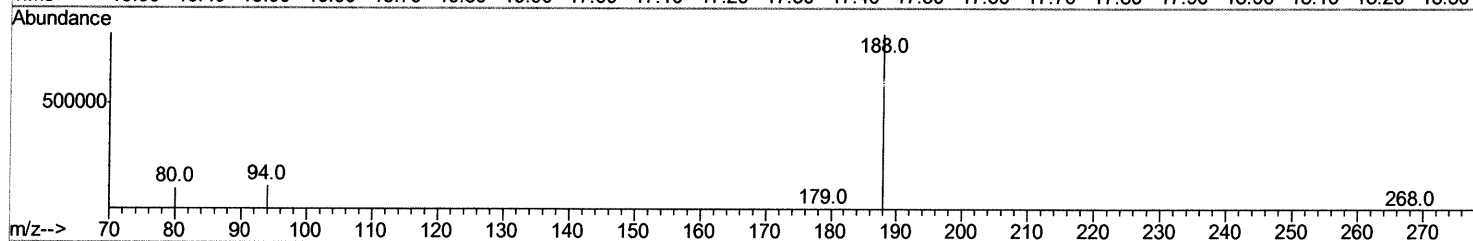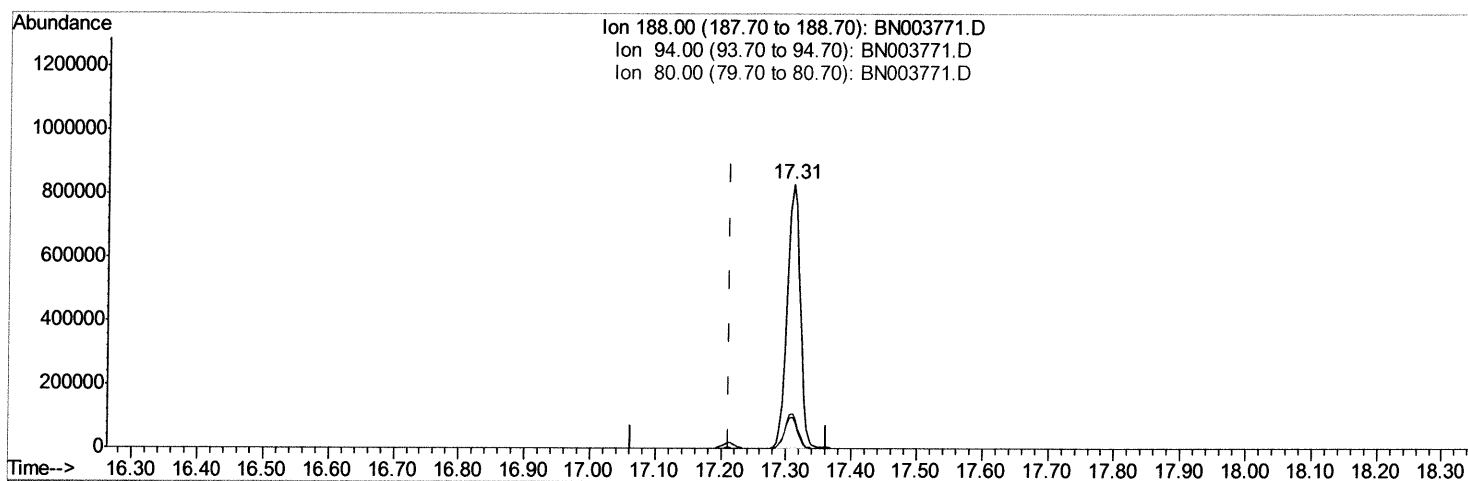

TIC: BN003771.D

(10) Phenanthrene-d10 (I)

17.310min (+0.097) 0.40ng/ul

response 1146854

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.13#
80.00	11.60	11.75
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:37:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

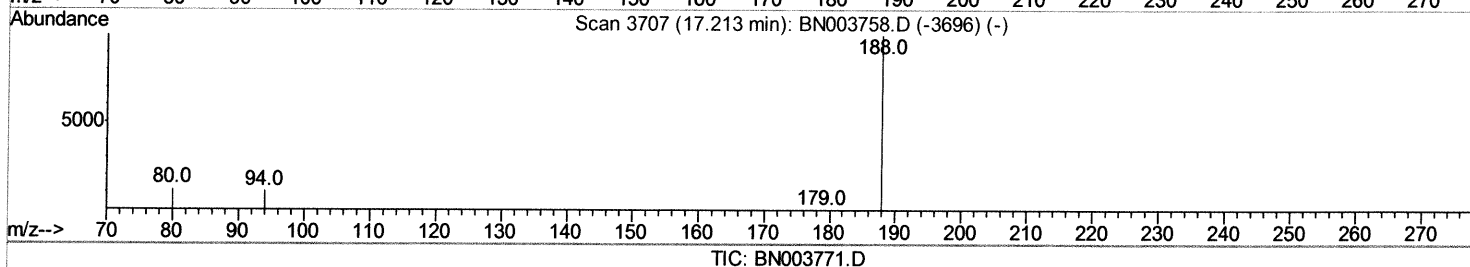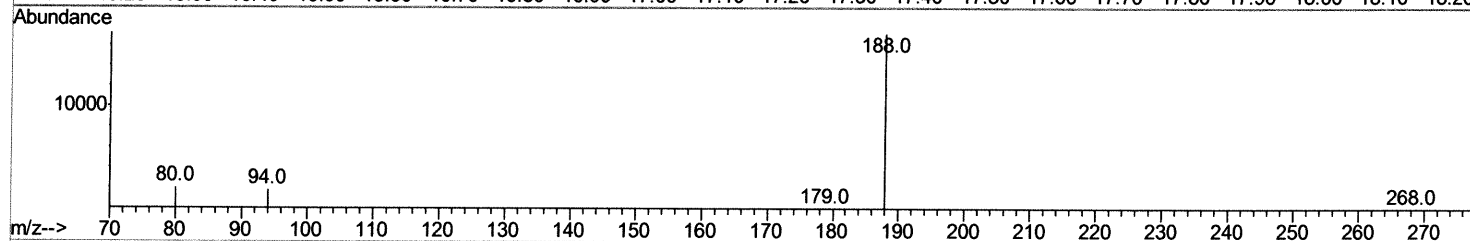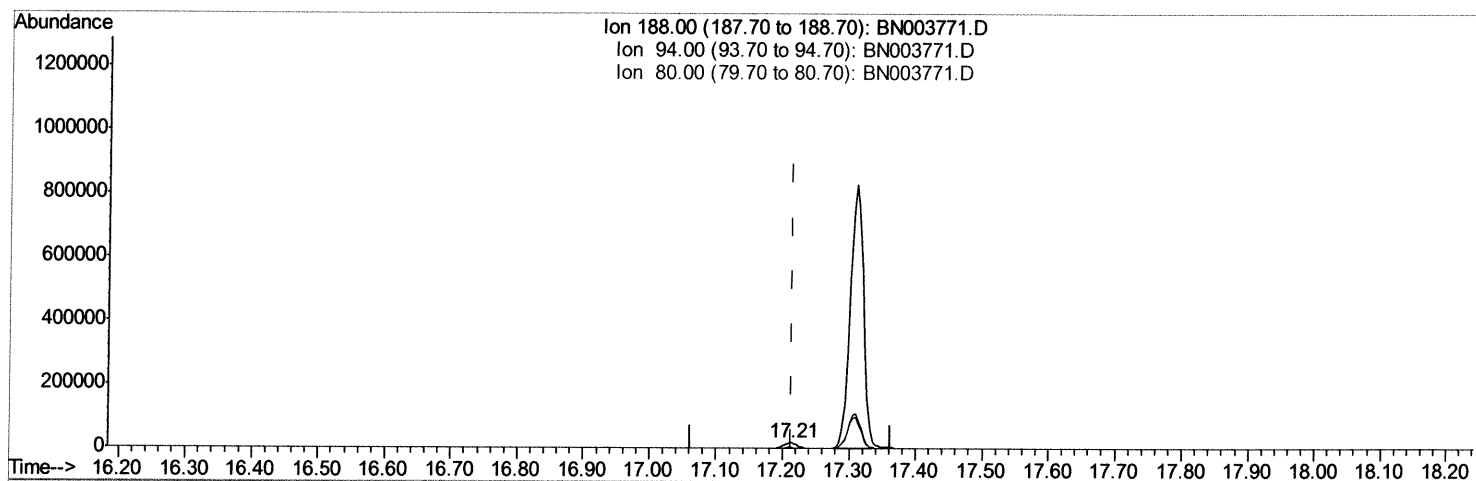

(10) Phenanthrene-d10 (I)

17.213min (-0.000) 0.40ng/ul m

response 23915

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.86
80.00	11.60	11.88
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:49:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

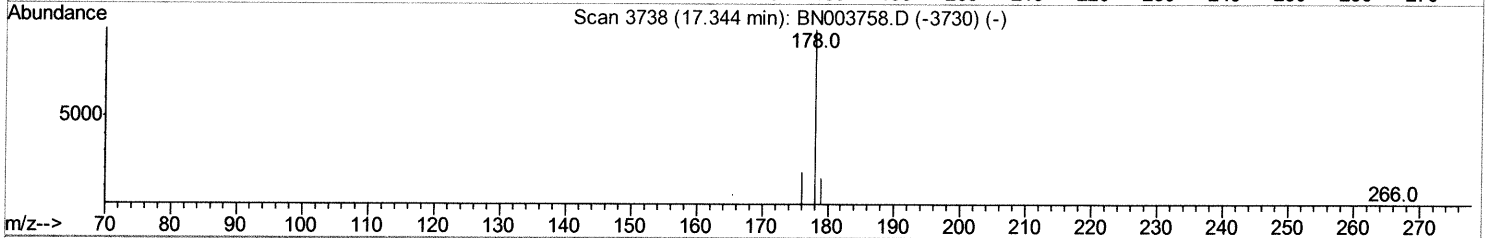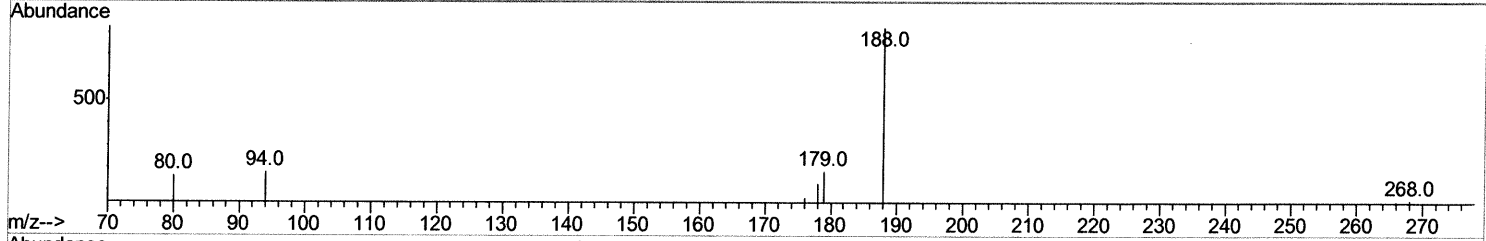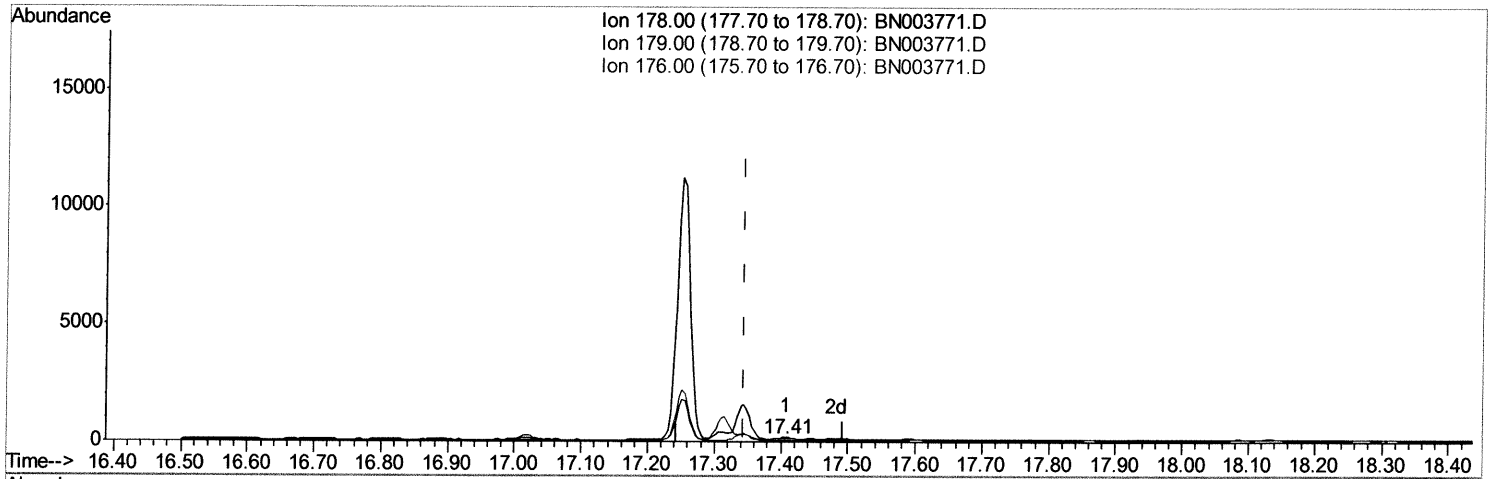

TIC: BN003771.D

(13) Anthracene

17.407min (+0.063) 0.00ng/ul

response 60

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	142.42#
176.00	18.50	52.27#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:49:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

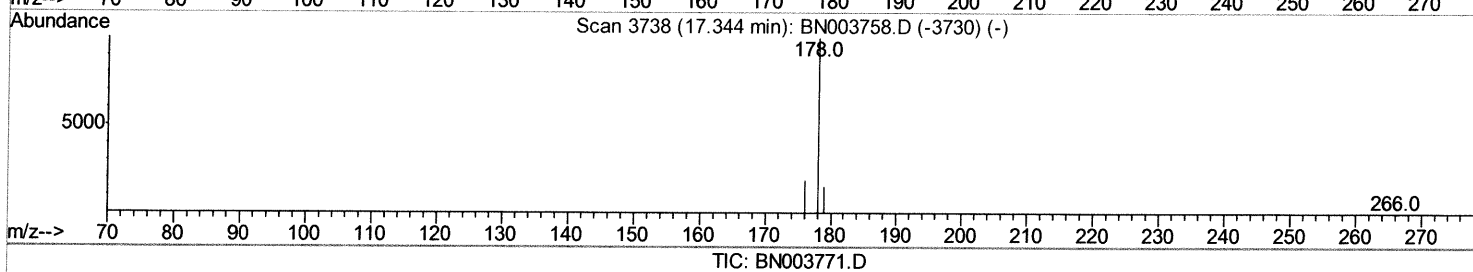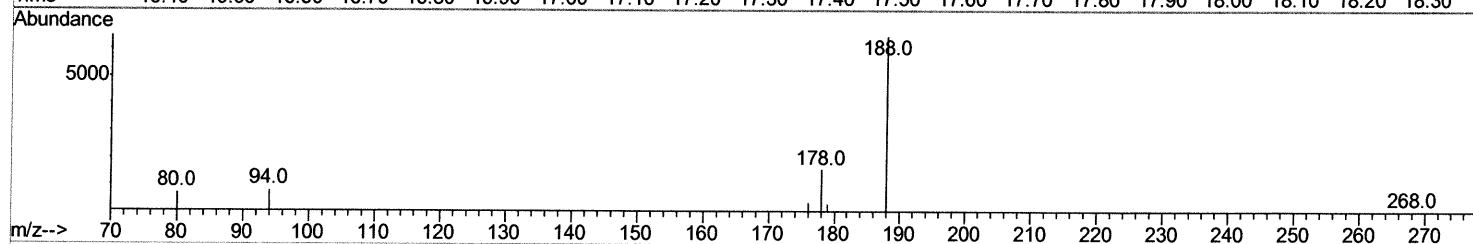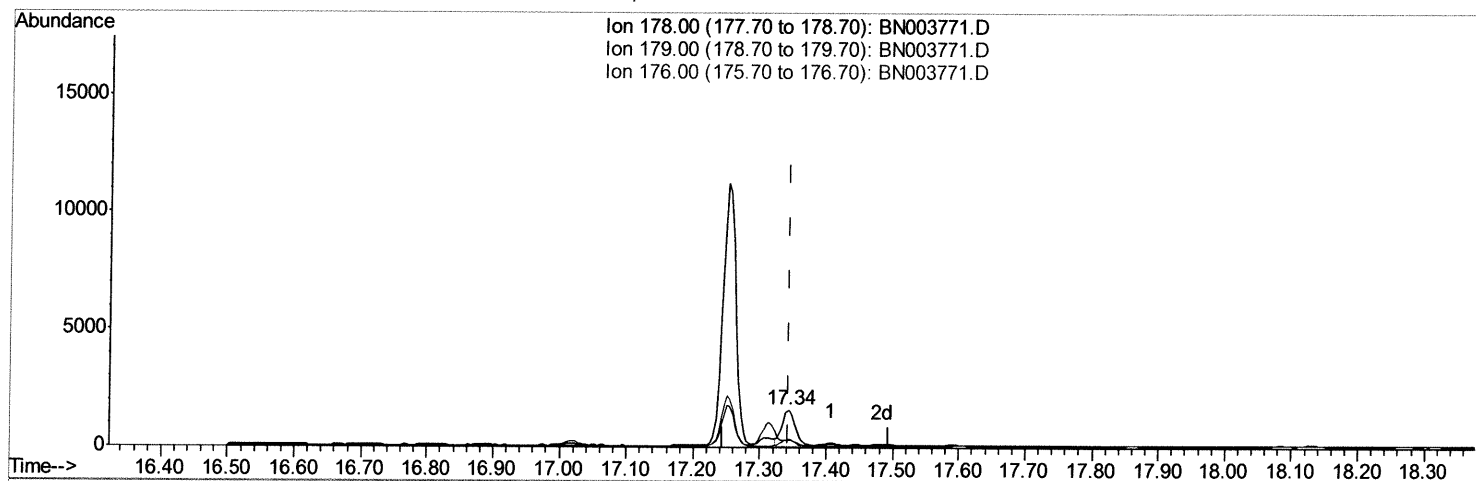

(13) Anthracene

17.344min (-0.000) 0.03ng/ul m

response 2229

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	20.93#
176.00	18.50	21.50
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:49:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

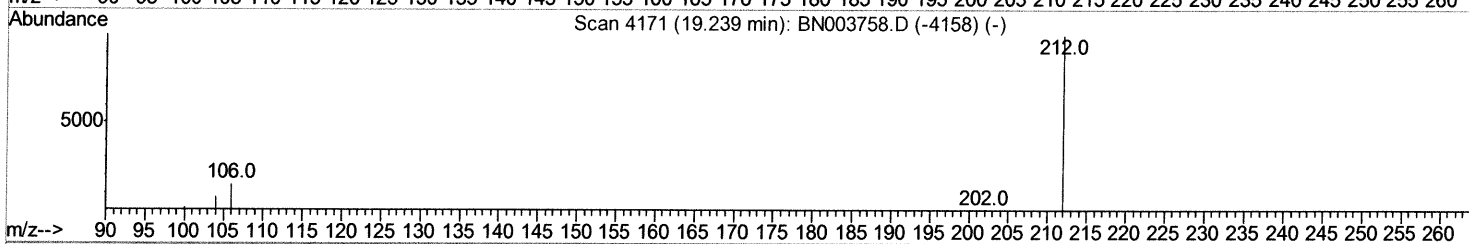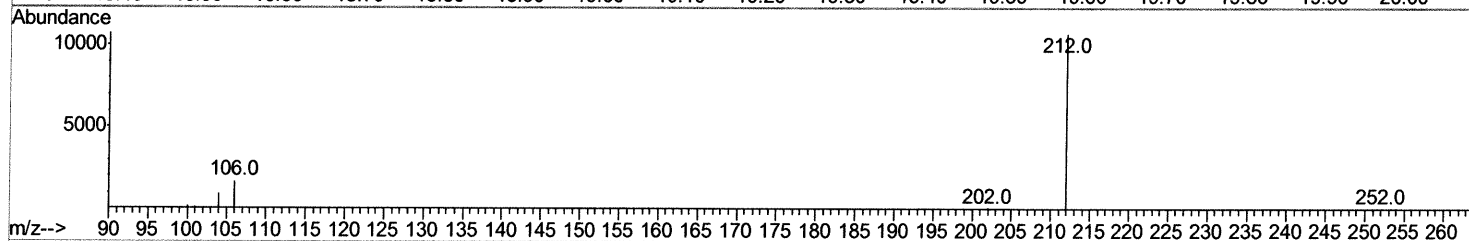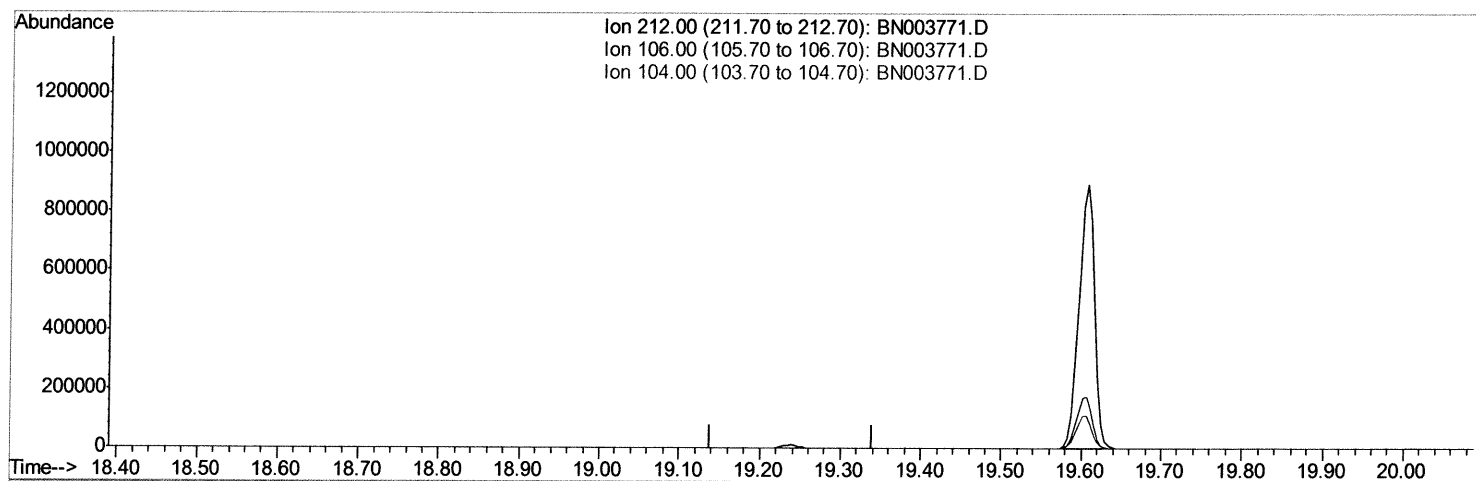

TIC: BN003771.D

(14) Fluoranthene-d10 (SURR)

19.239min (-19.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003771.D
Acq On : 07 Dec 2018 17:54
Operator : JU/SJ
Sample : J6228-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E53

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:49:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

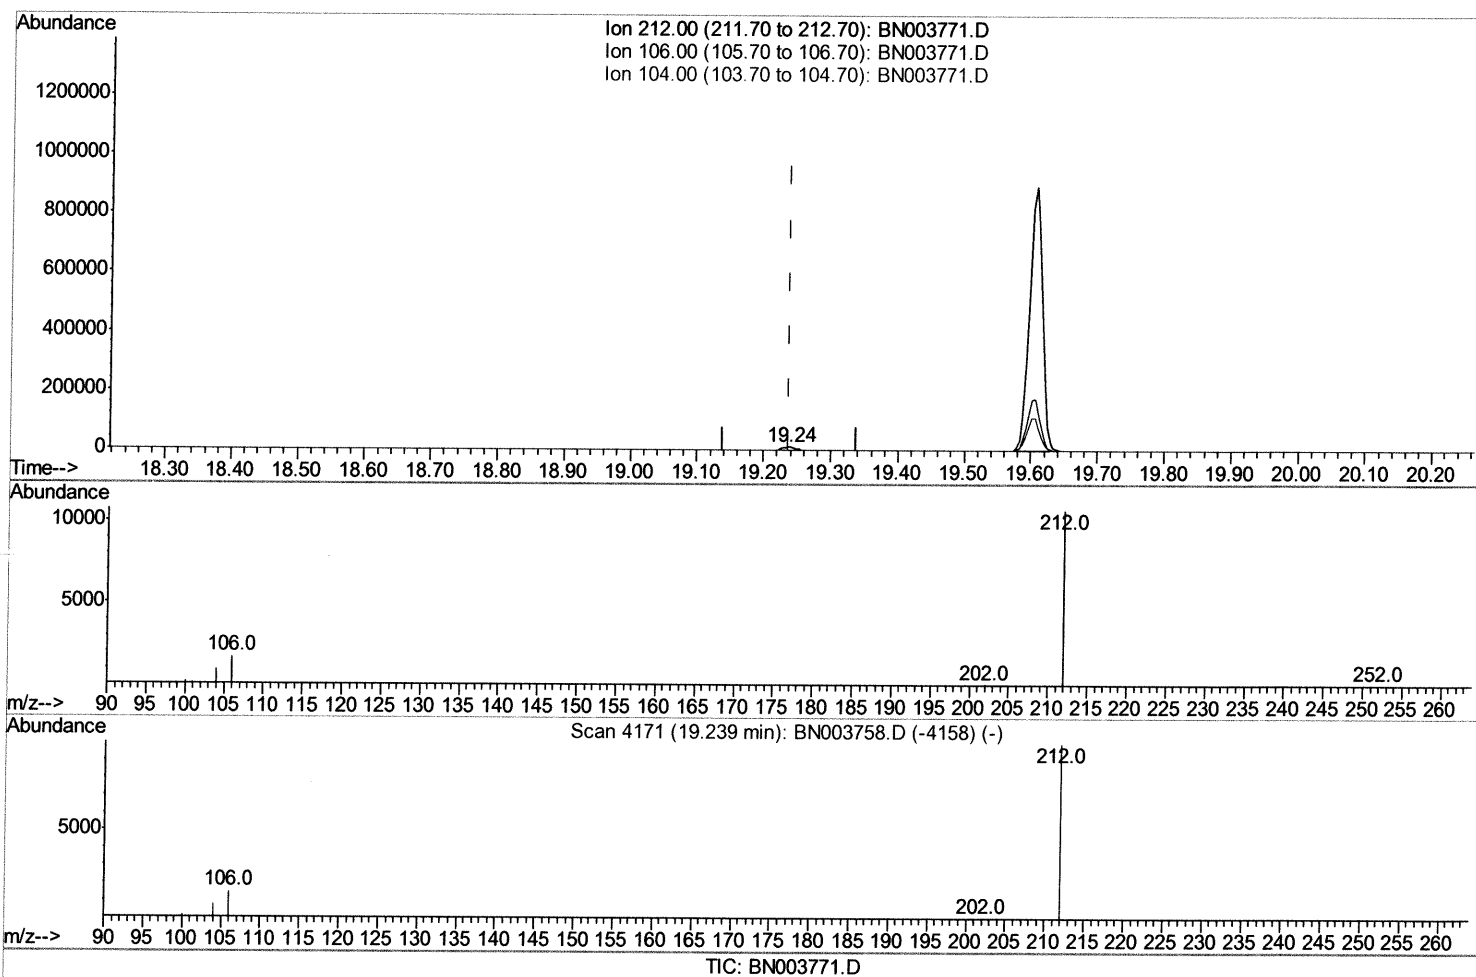

(14) Fluoranthene-d10 (SURR)

19.239min (-0.000) 0.21ng/ul m

response 14370

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:49:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

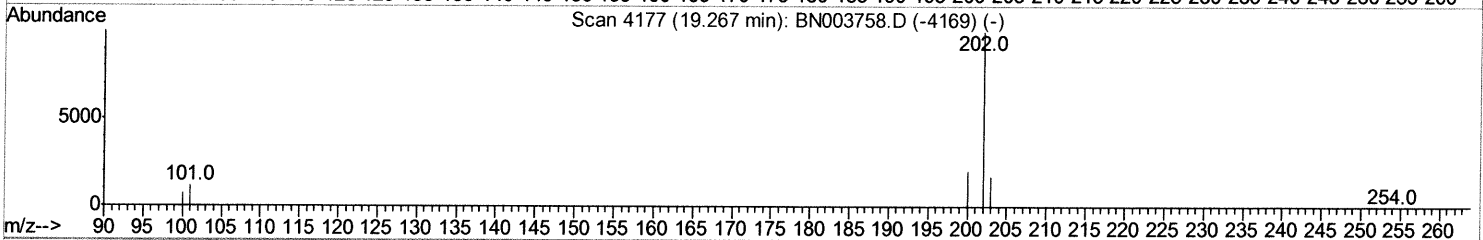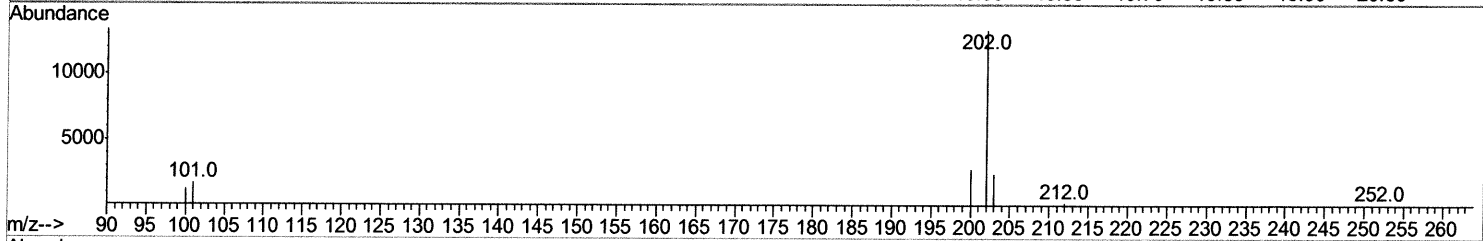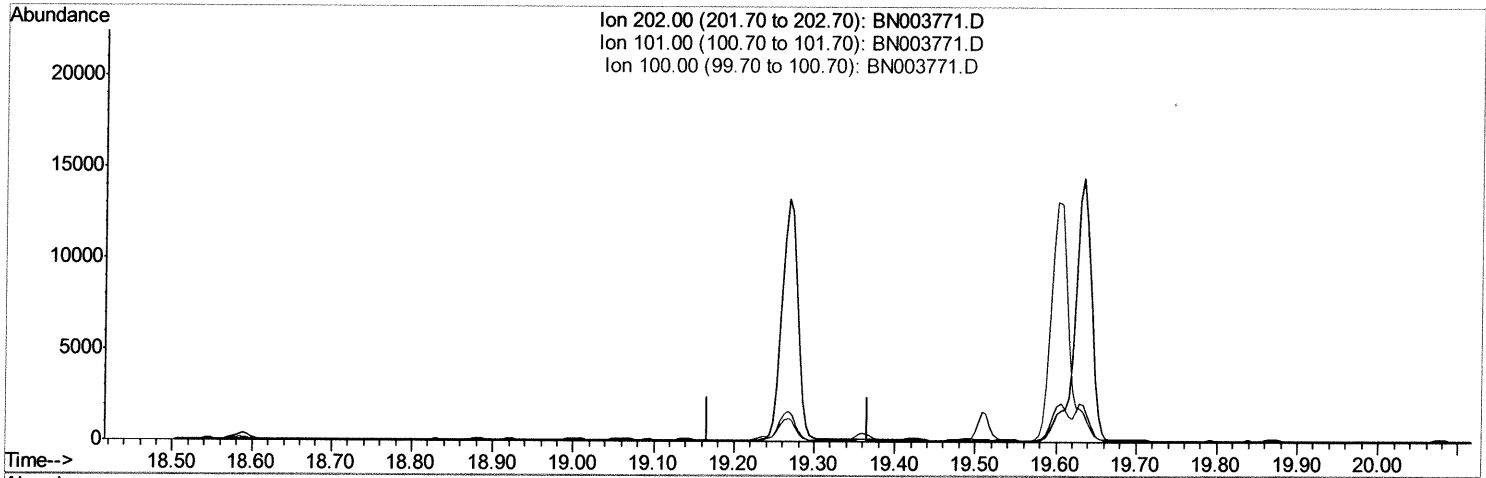

TIC: BN003771.D

(15) Fluoranthene (C)

19.267min (-19.267) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.70	0.00
100.00	8.10	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:49:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

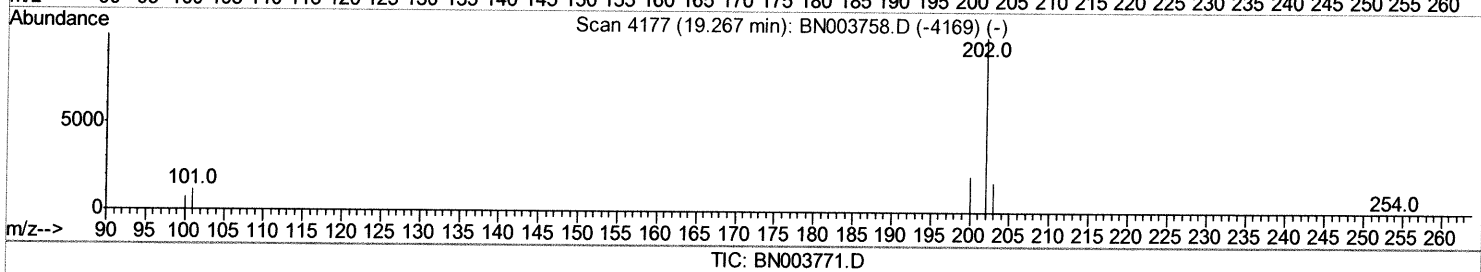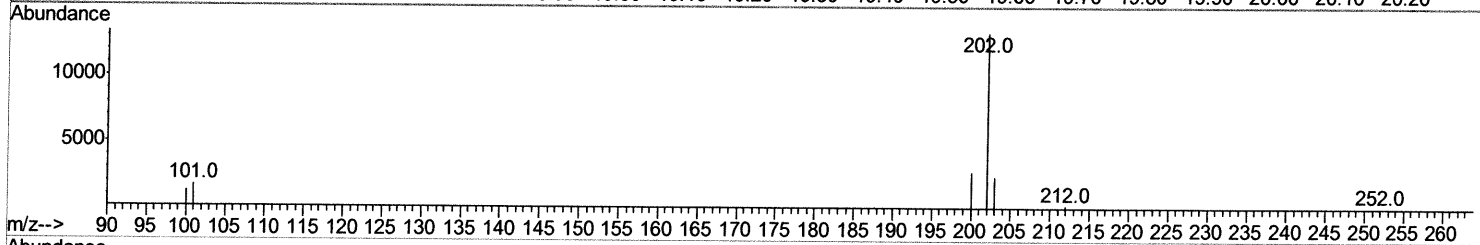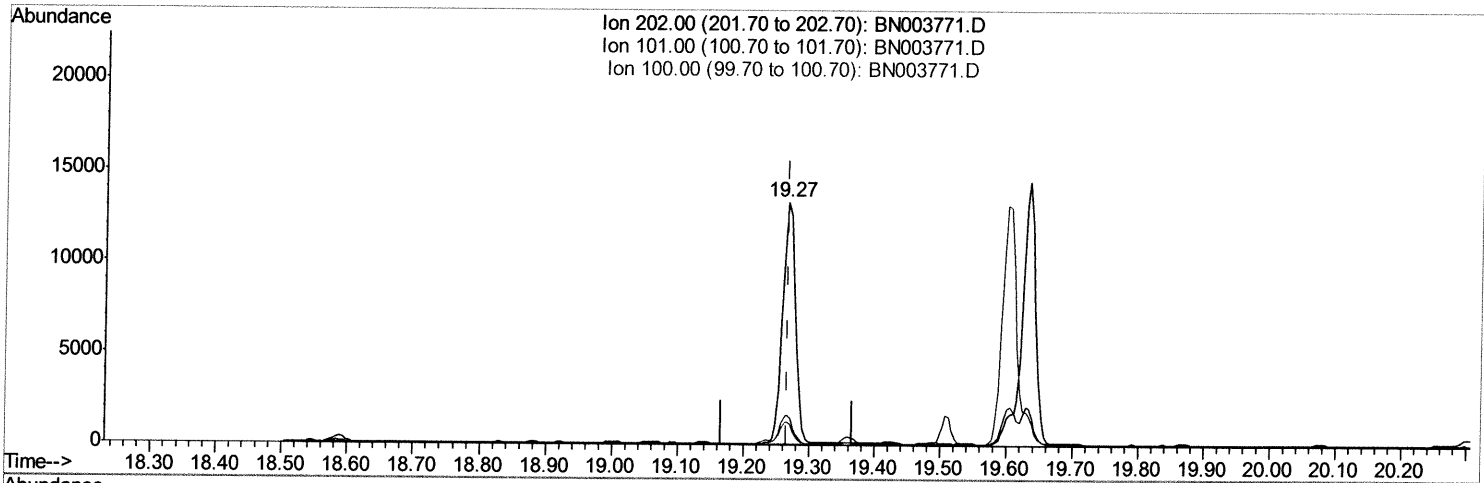

TIC: BN003771.D

(15) Fluoranthene (C)

19.267min (-0.000) 0.20ng/ul m

response 18221

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	12.50
100.00	8.10	9.53
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:49:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

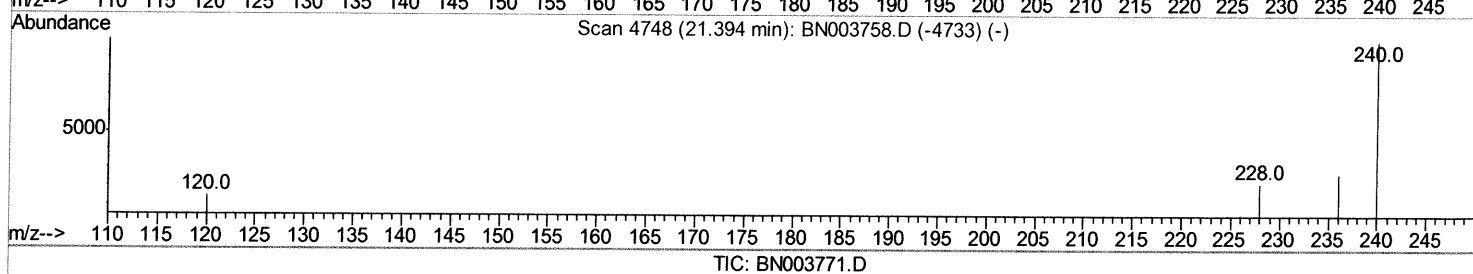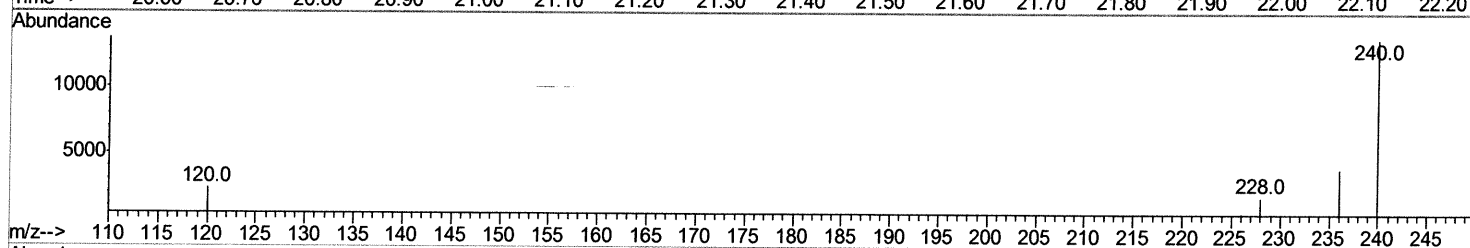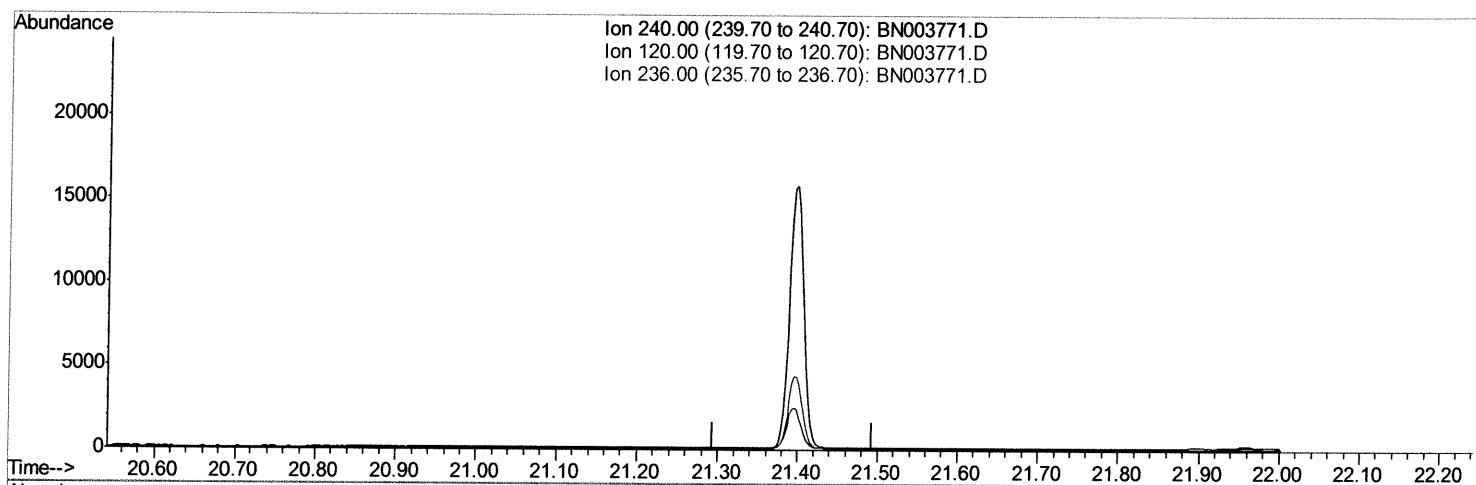

(16) Chrysene-d12 (I)

21.394min (-21.394) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:49:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

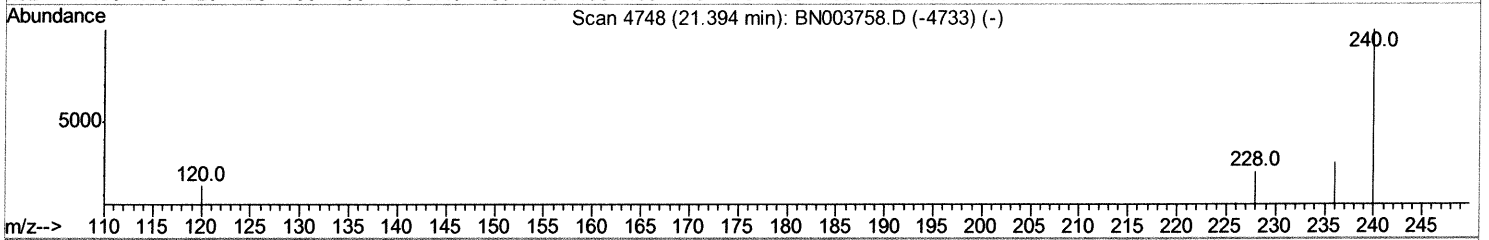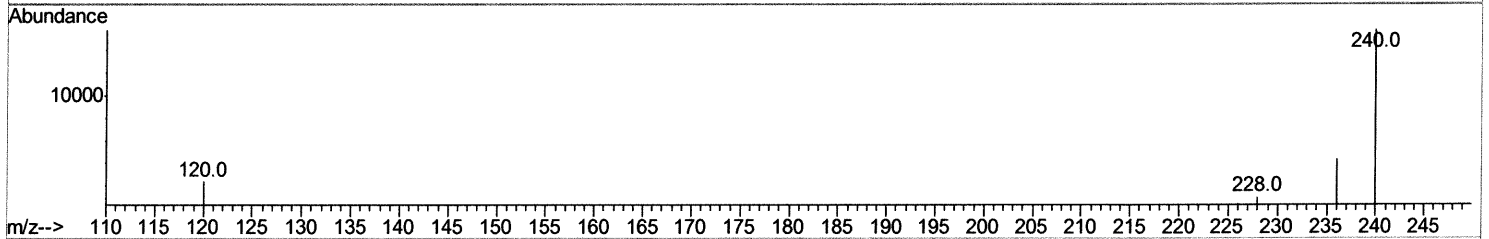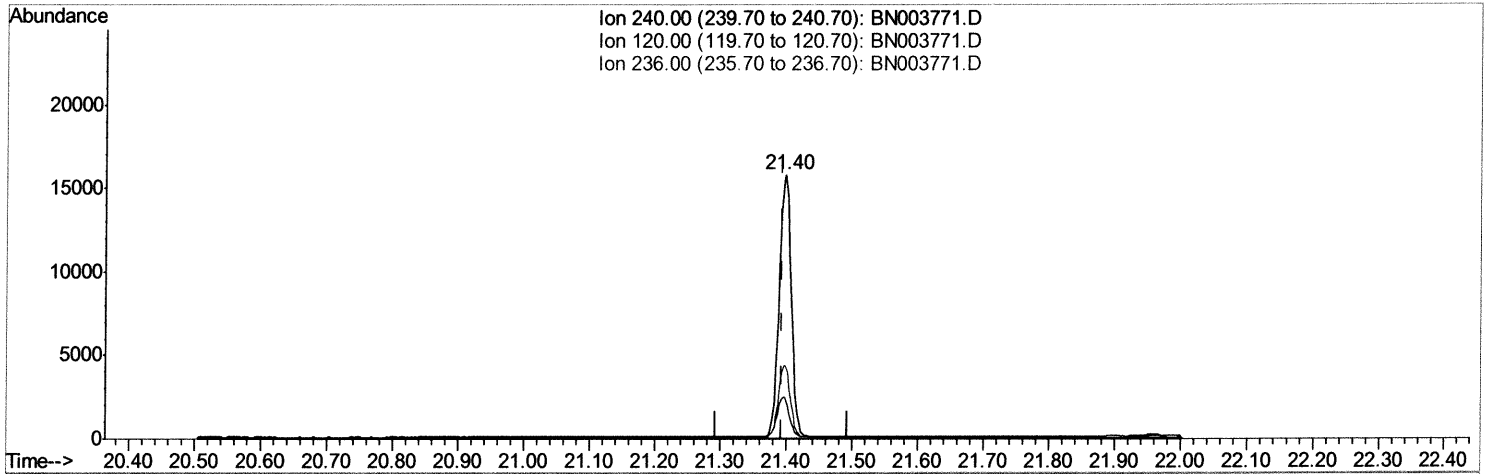

Scan 4748 (21.394 min): BN003758.D (-4733) (-)

TIC: BN003771.D

(16) Chrysene-d12 (I)

21.398min (+0.005) 0.40ng/ul m

response 20001

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	15.26
236.00	27.60	27.77
0.00	0.00	0.00

MA
12/11/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:51:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

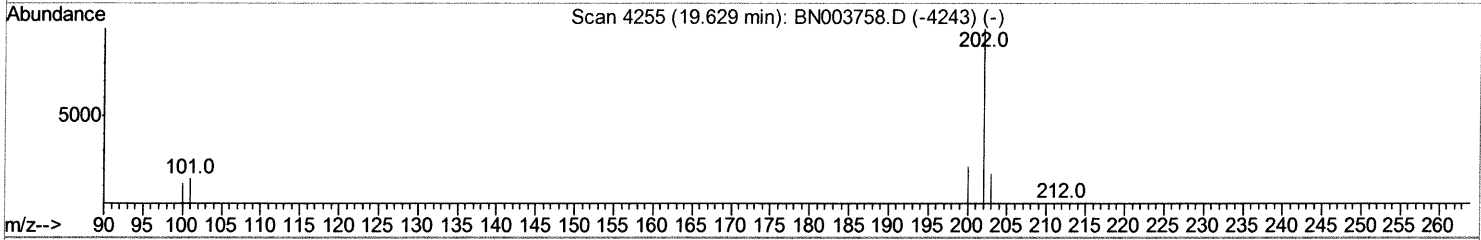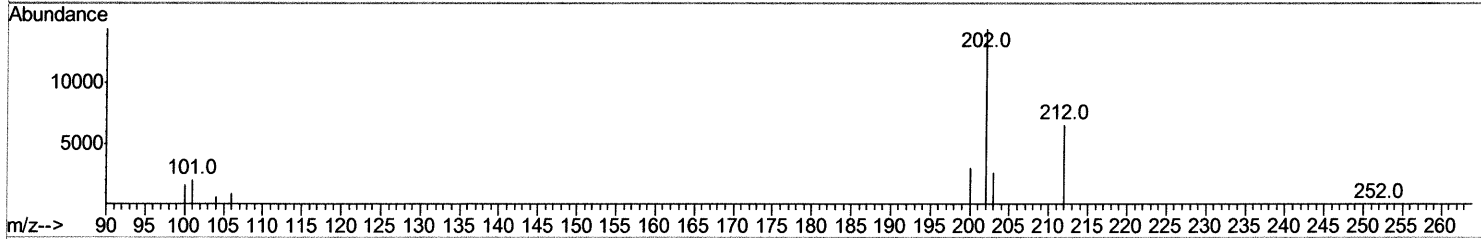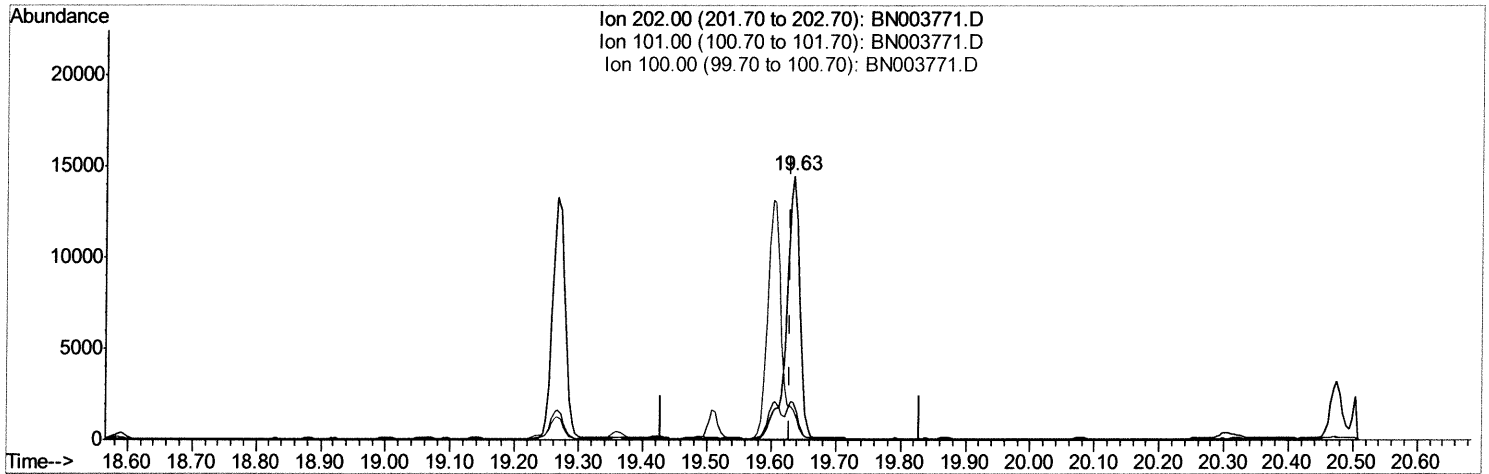

TIC: BN003771.D

(17) Pyrene

19.634min (+0.005) 0.29ng/ul

response 20780

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	14.16
100.00	10.60	11.53
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:51:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

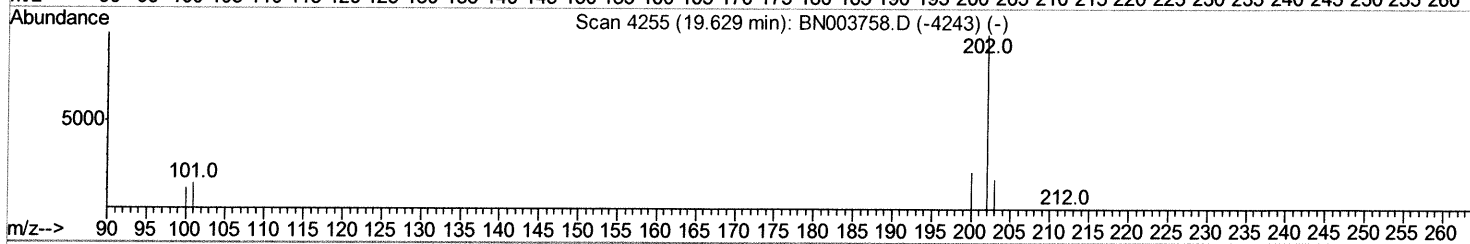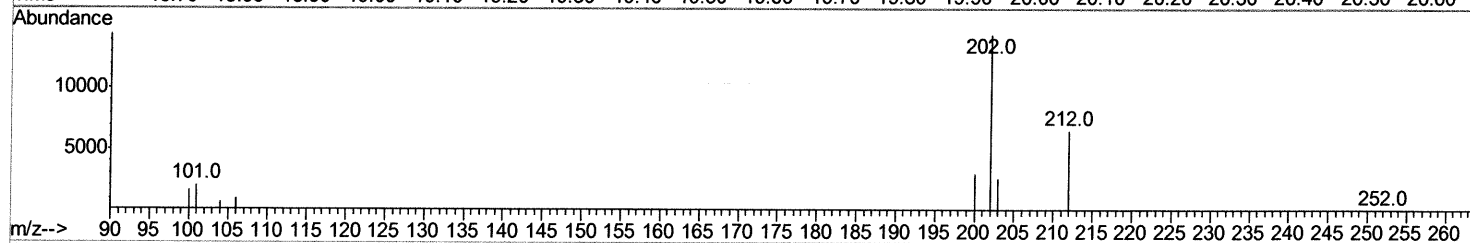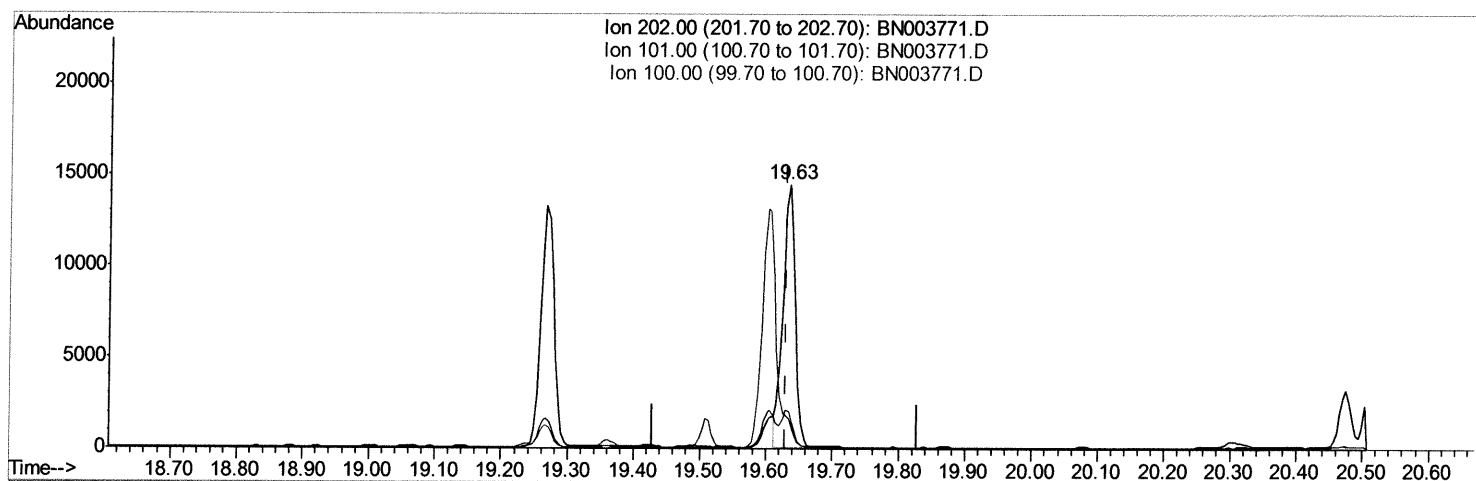

TIC: BN003771.D

(17) Pyrene

19.634min (+0.005) 0.26ng/ul m

response 18914

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	14.16
100.00	10.60	11.53
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:51:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

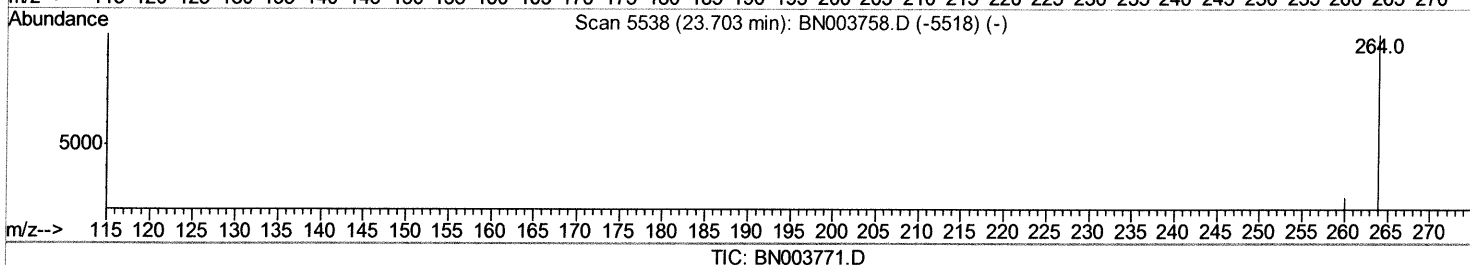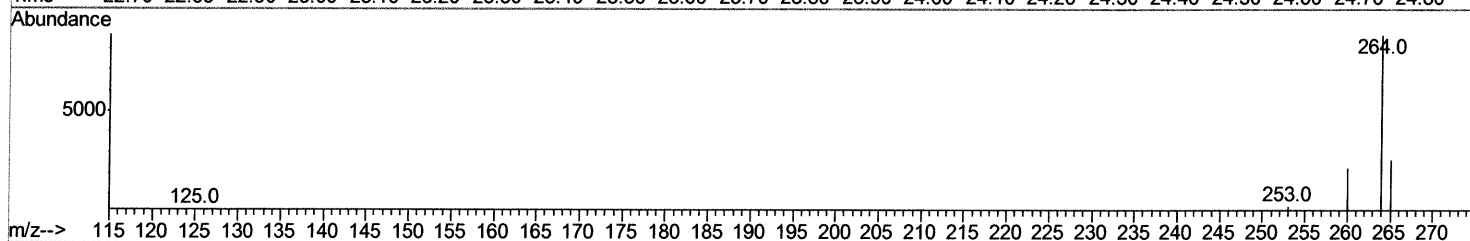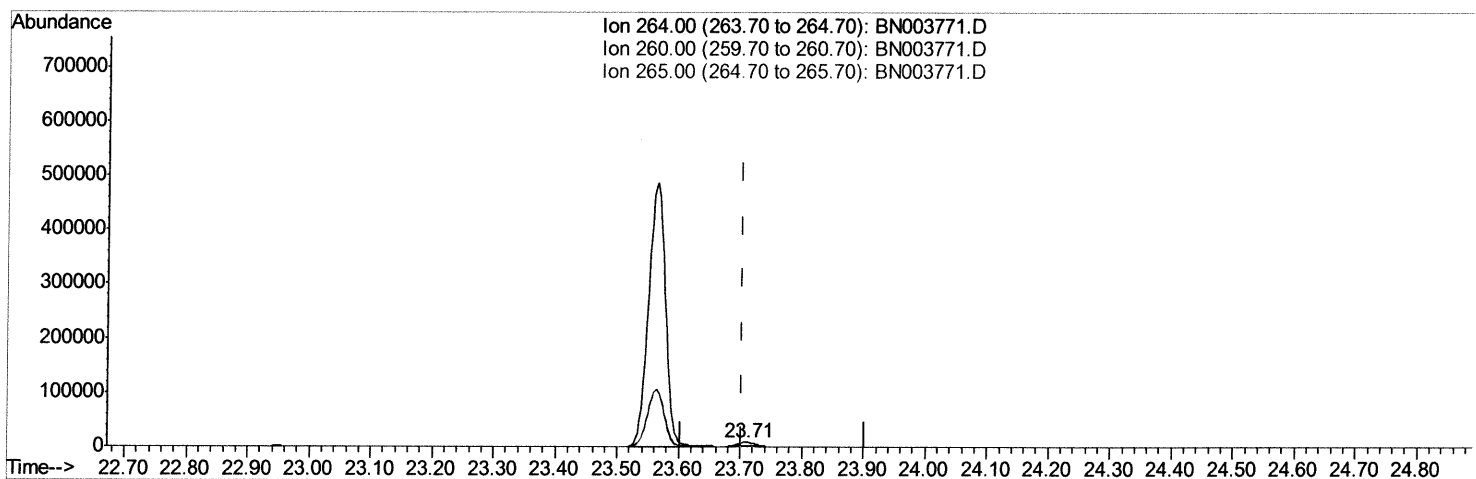

(20) Perylene-d12 (I)
 23.711min (+0.008) 0.40ng/ul
 response 18459

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.10
265.00	33.50	31.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:51:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

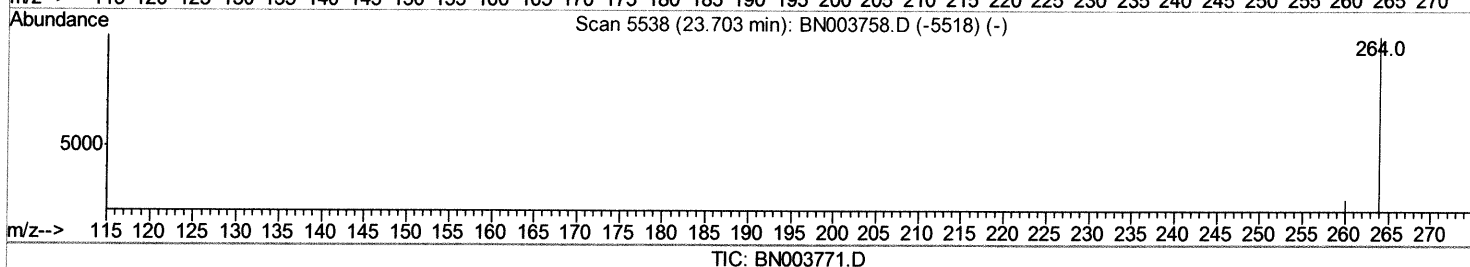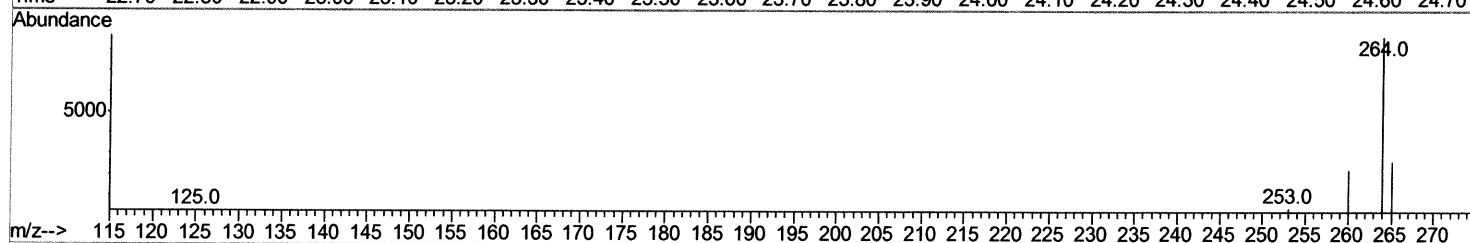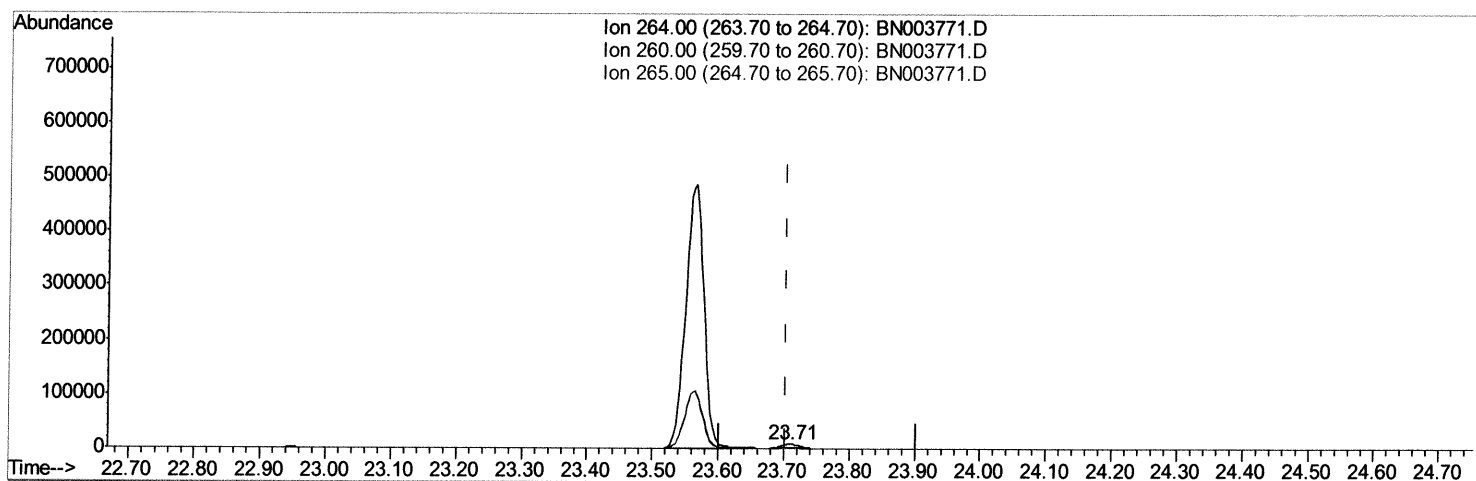

(20) Perylene-d12 (I)

23.711min (+0.008) 0.40ng/ul m

response 15023

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.10
265.00	33.50	31.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:52:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

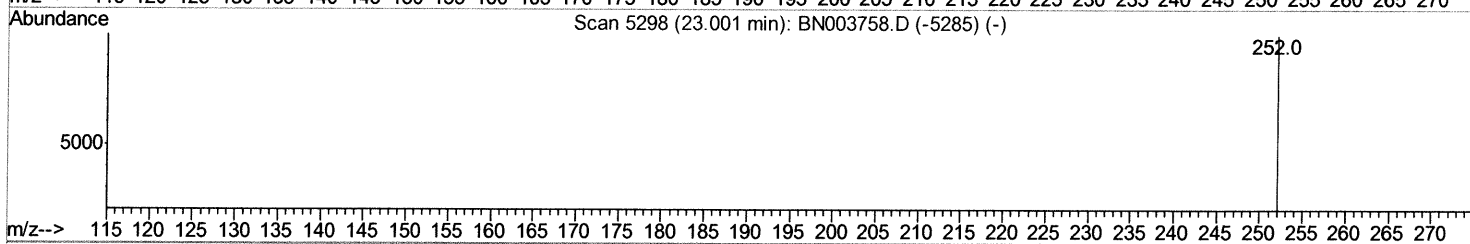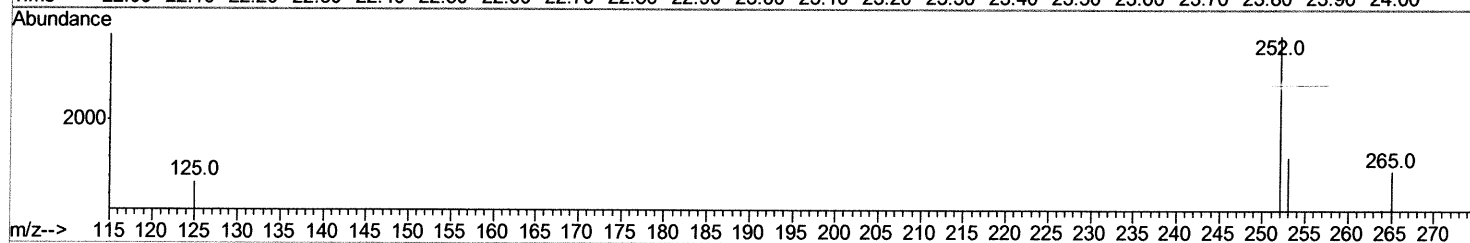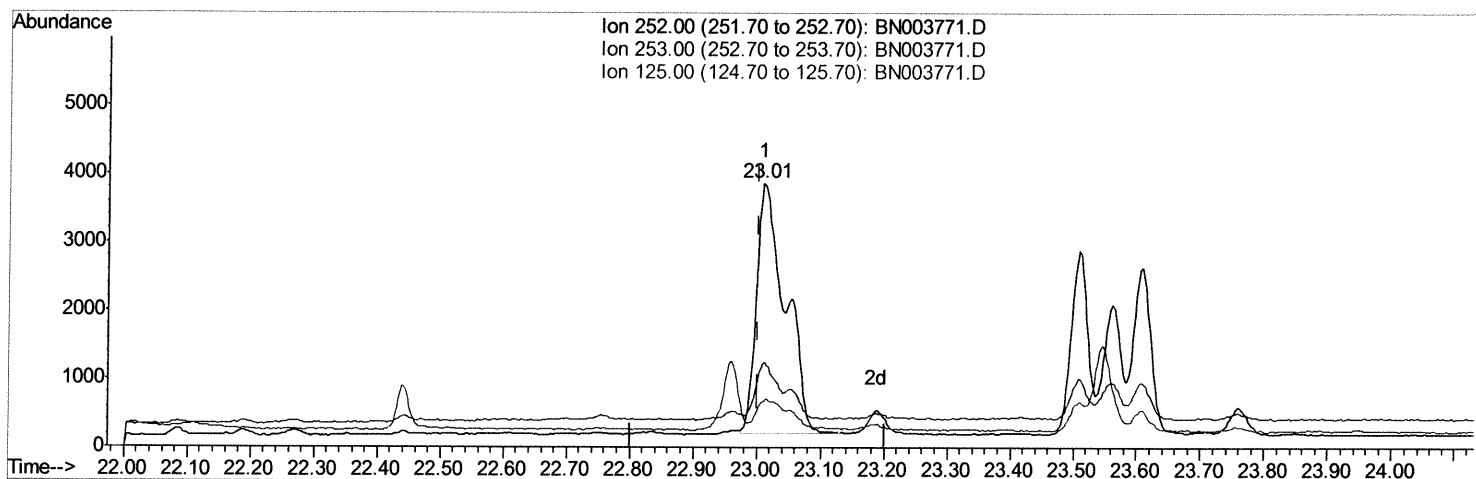

TIC: BN003771.D

(21) Benzo(b)fluoranthene
 23.009min (+0.008) 0.18ng/ul
 response 11456

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	31.60
125.00	11.20	17.33
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:52:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

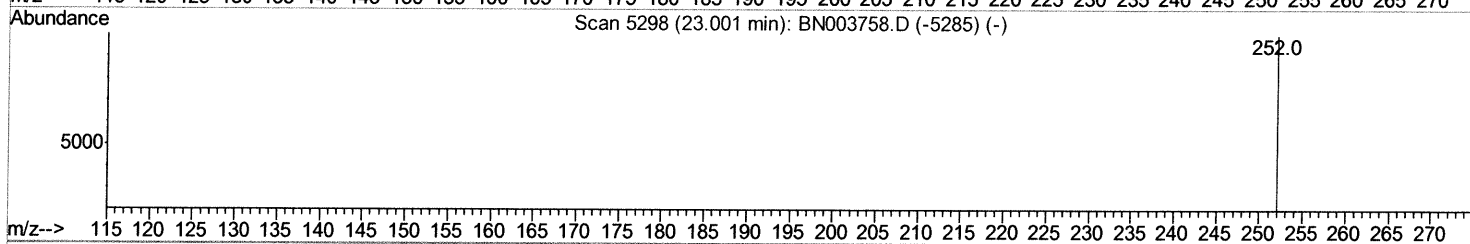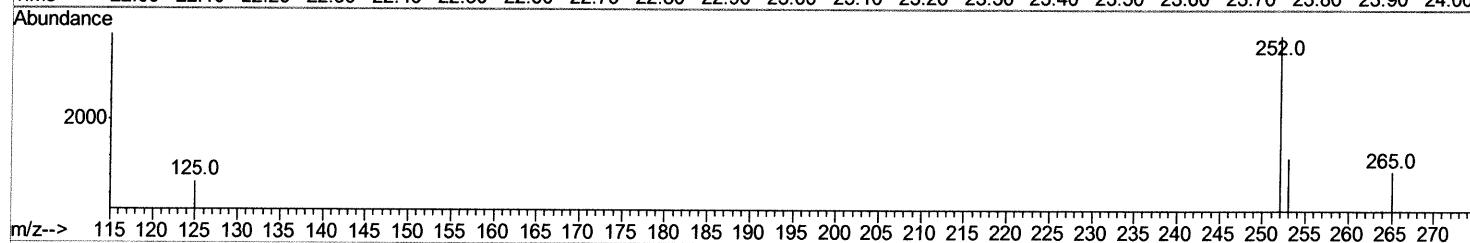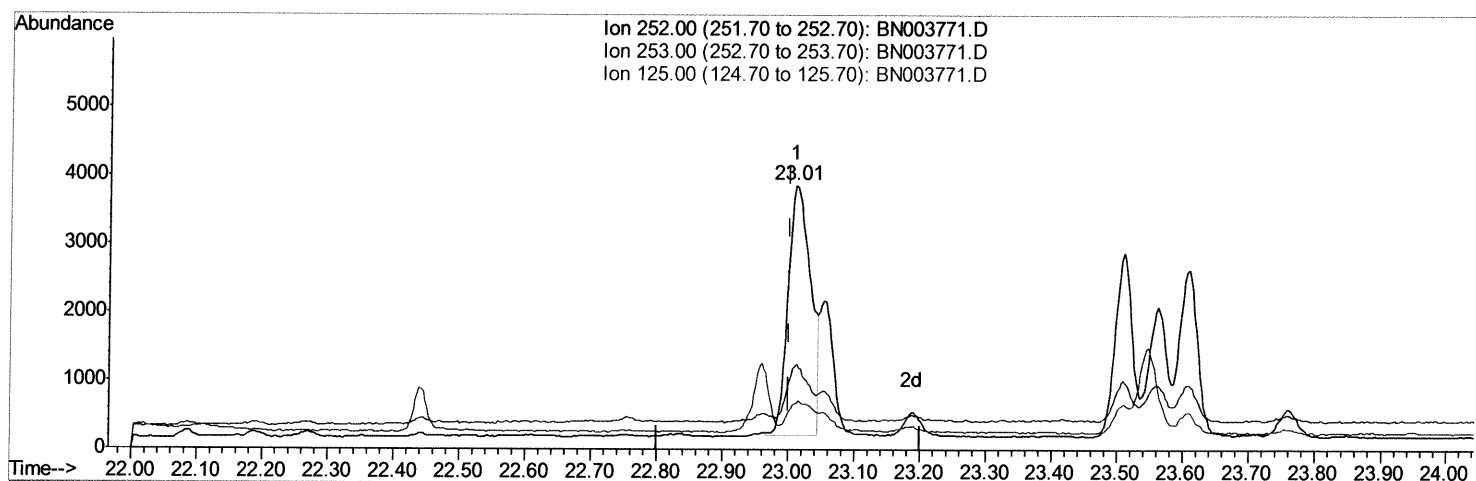

TIC: BN003771.D

(21) Benzo(b)fluoranthene
 23.009min (+0.008) 0.14ng/ul m
 response 8644

msd
12/11/18

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	31.60
125.00	11.20	17.33
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:52:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

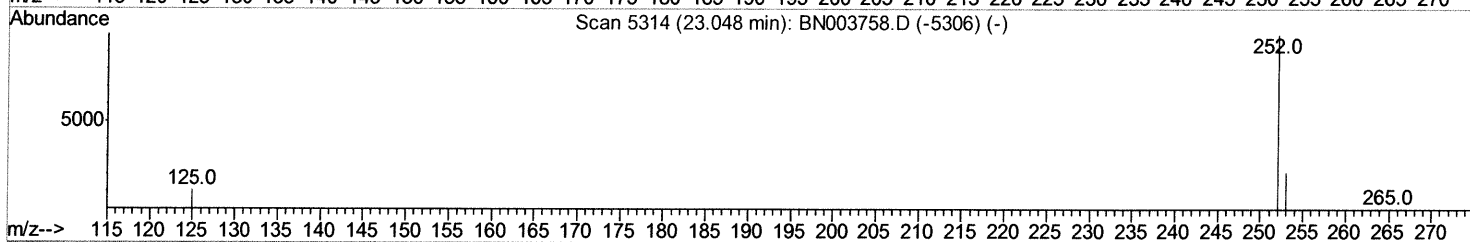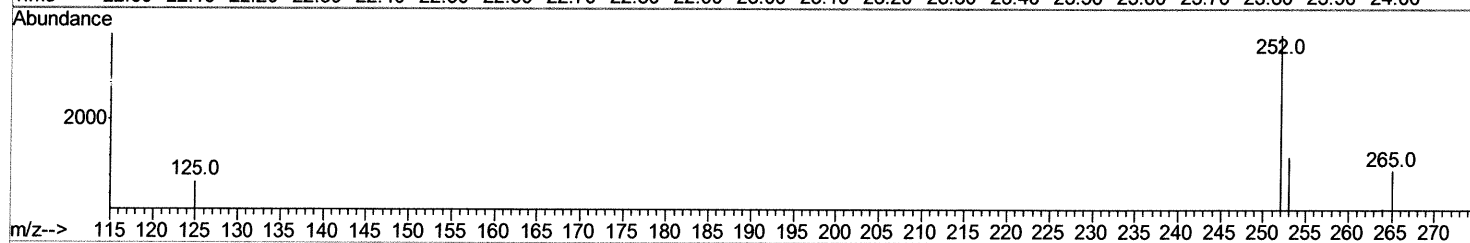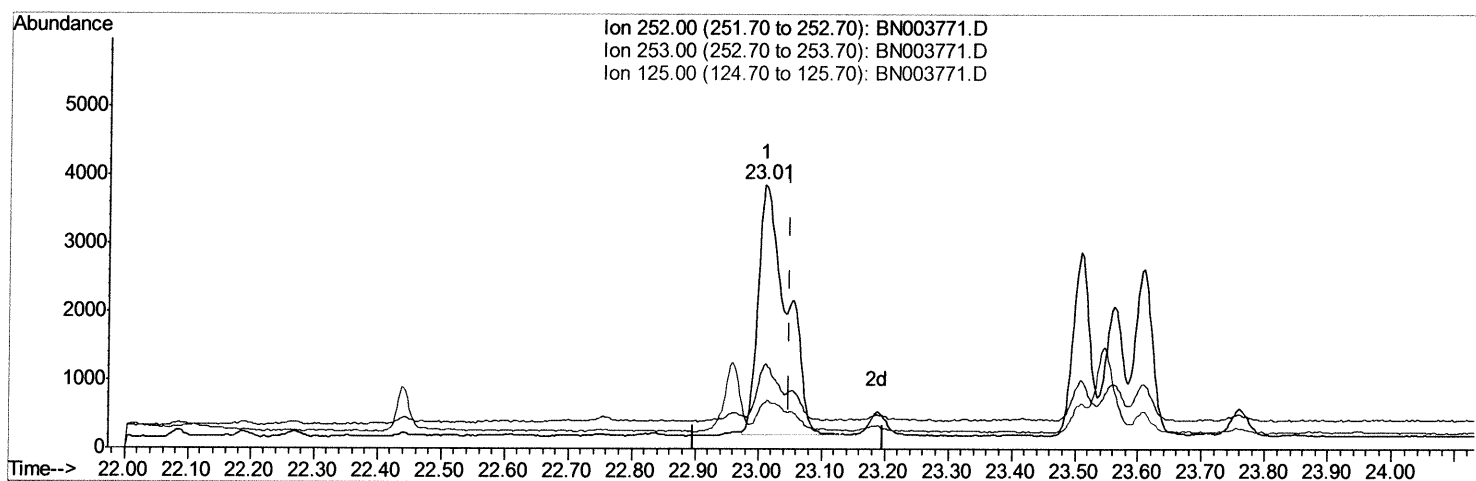

TIC: BN003771.D

(22) Benzo(k)fluoranthene
 23.009min (-0.039) 0.19ng/ul
 response 11456

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	31.60#
125.00	11.30	17.33#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:52:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

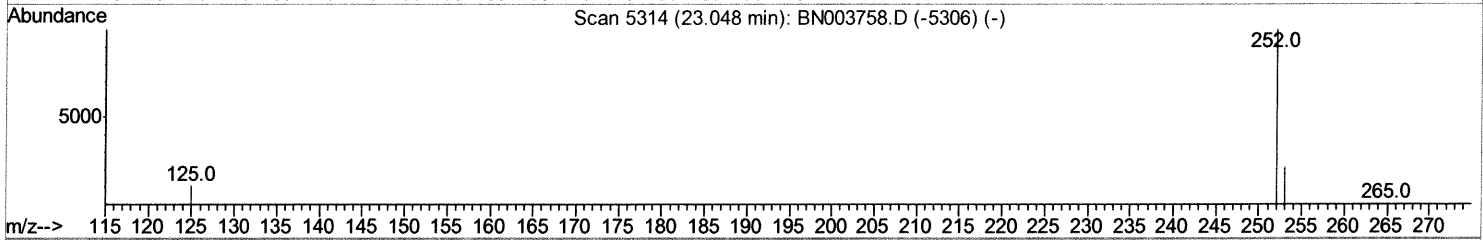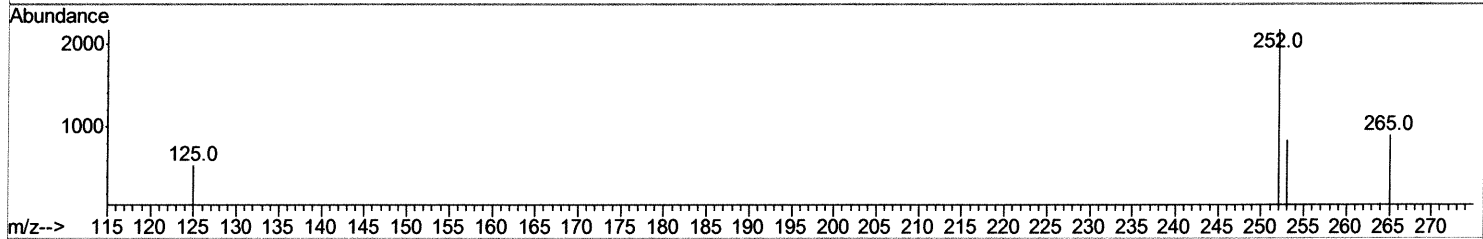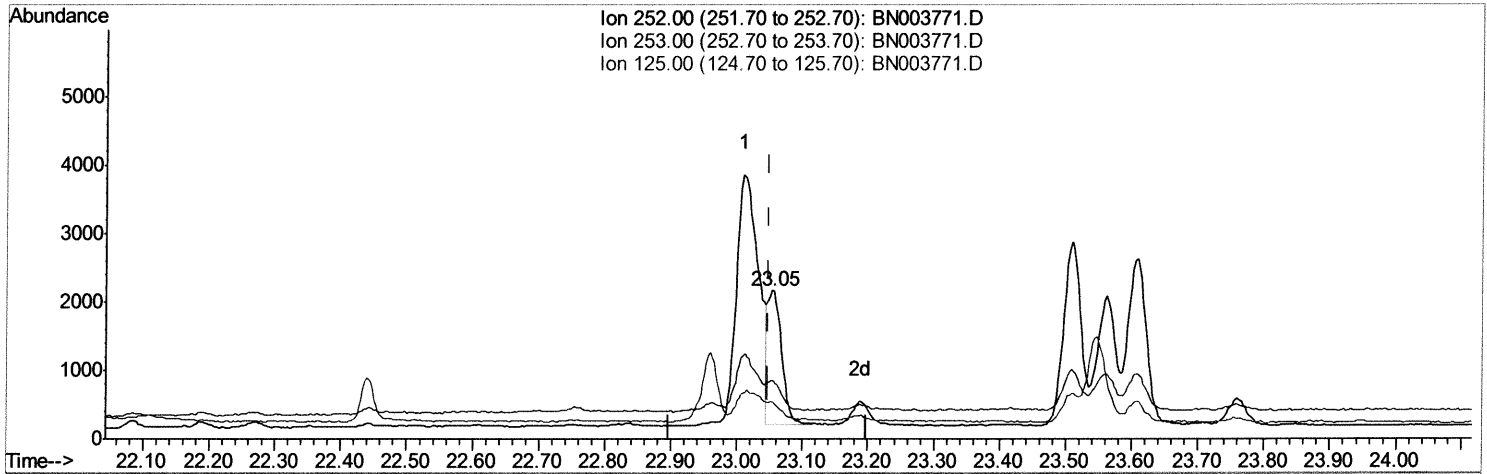

TIC: BN003771.D

(22) Benzo(k)fluoranthene

23.053min (+0.005) 0.05ng/ul m

response 2832

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	39.27#
125.00	11.30	24.78#
0.00	0.00	0.00

MP 12/11/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003771.D
 Acq On : 07 Dec 2018 17:54
 Operator : JU/SJ
 Sample : J6228-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E53

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:52:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4945	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	20344	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11104	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	23915m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	20001m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	15023m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	6531	0.21	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	14370m	0.21	ng/ul	0.00
Target Compounds						
					Ovalue	
12) Phenanthrene	17.25	178	15308	0.195	ng/ul	99
13) Anthracene	17.34	178	2229m	0.035	ng/ul	
15) Fluoranthene	19.27	202	18221m	0.197	ng/ul	
17) Pyrene	19.63	202	18914m	0.264	ng/ul	
18) Benzo(a)anthracene	21.38	228	5720	0.091	ng/ul	95
19) Chrysene	21.43	228	10150	0.140	ng/ul	98
21) Benzo(b)fluoranthene	23.01	252	8644m	0.139	ng/ul	
22) Benzo(k)fluoranthene	23.05	252	2832m	0.047	ng/ul	
23) Benzo(a)pyrene	23.61	252	4535	0.084	ng/ul#	77
24) Indeno(1,2,3-cd)pyrene	26.06	276	3116	0.050	ng/ul#	98
26) Benzo(g,h,i)perylene	26.79	276	3346	0.062	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003771.D
Acq On : 07 Dec 2018 17:54
Operator : JU/SJ
Sample : J6228-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E53

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:23 AM

Quant Time: Dec 08 00:52:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

