

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:37:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

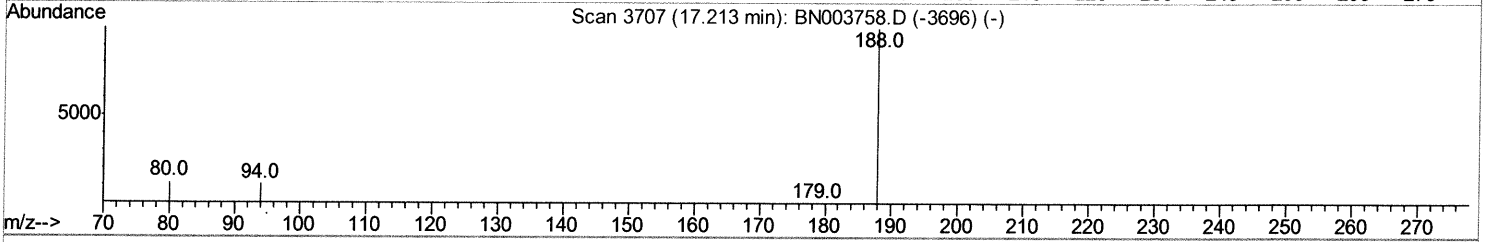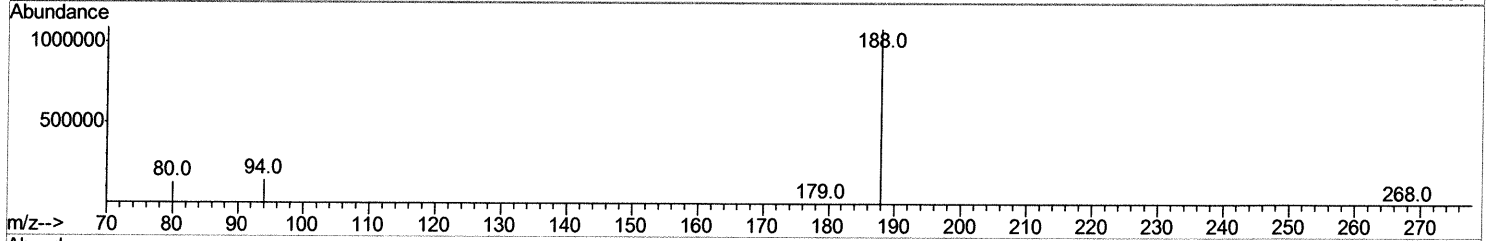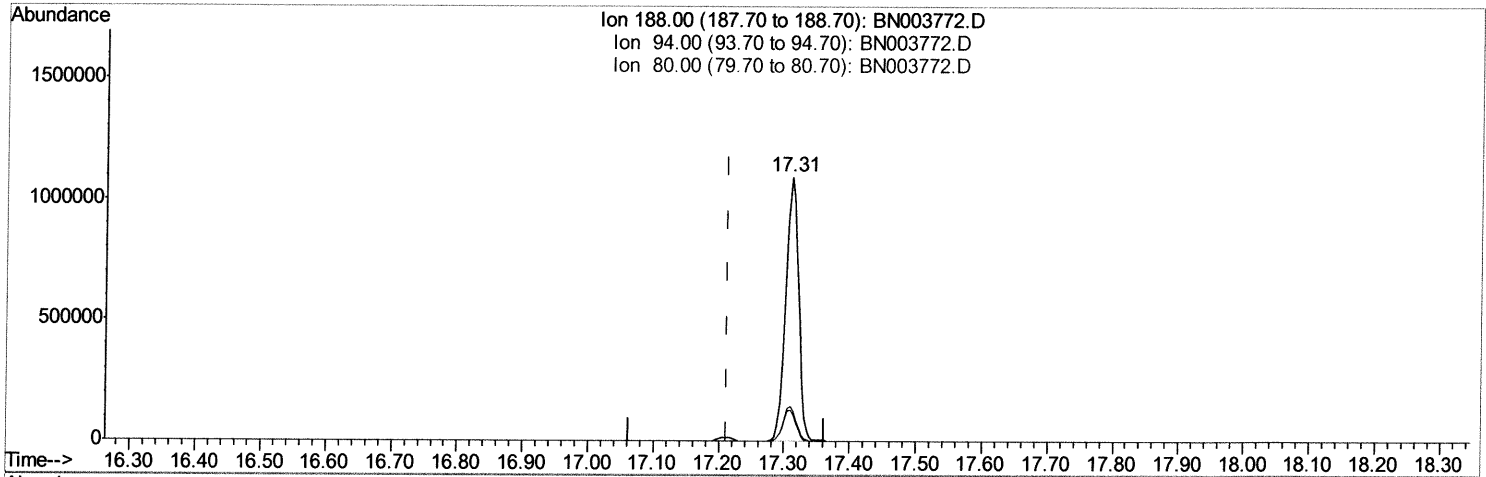

TIC: BN003772.D

(10) Phenanthrene-d10 (I)
 17.310min (+0.097) 0.40ng/ul
 response 1493537

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.30#
80.00	11.60	11.94
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:37:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

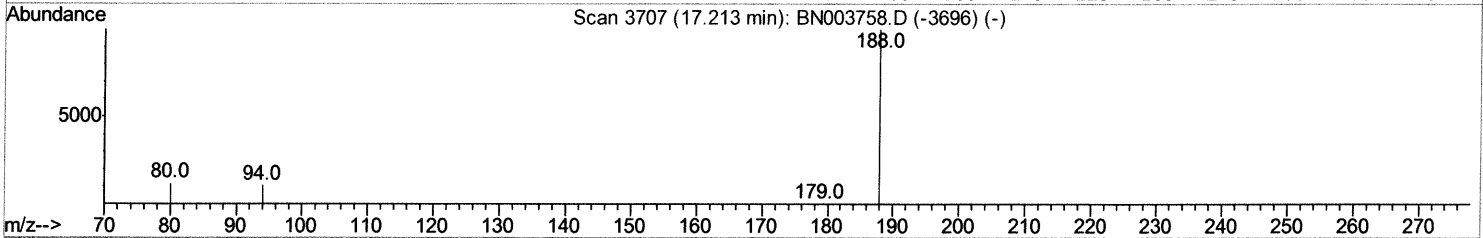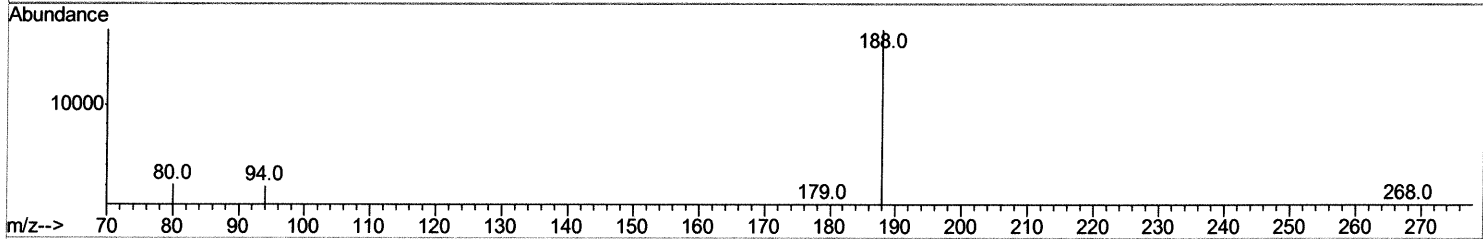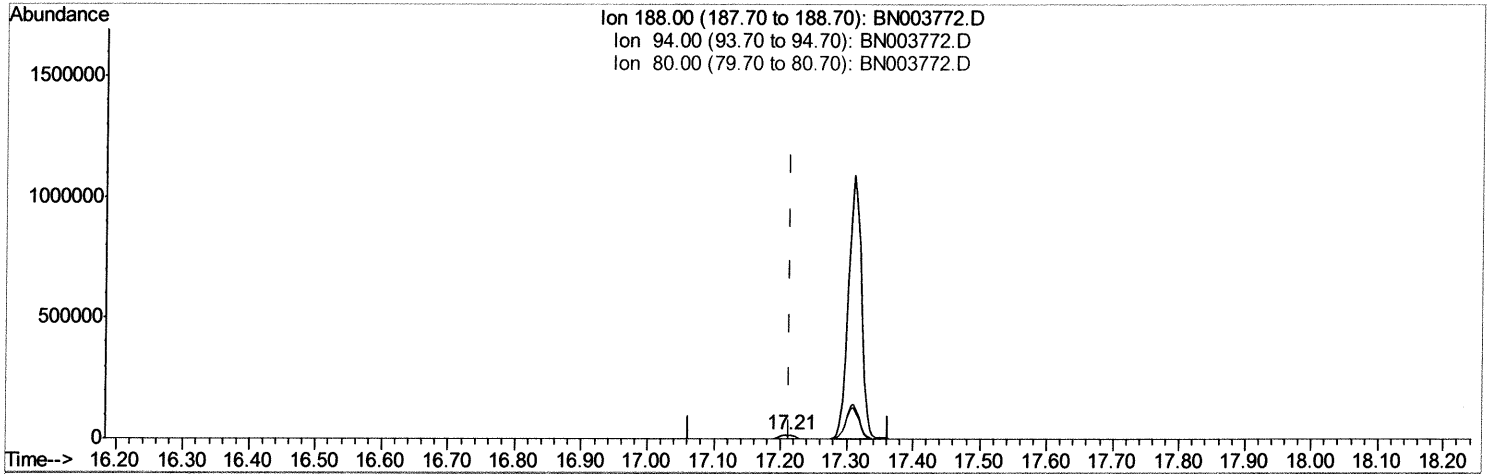

TIC: BN003772.D

(10) Phenanthrene-d10 (I)

17.213min (-0.000) 0.40ng/ul m

response 24294

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.78
80.00	11.60	11.71
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:53:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

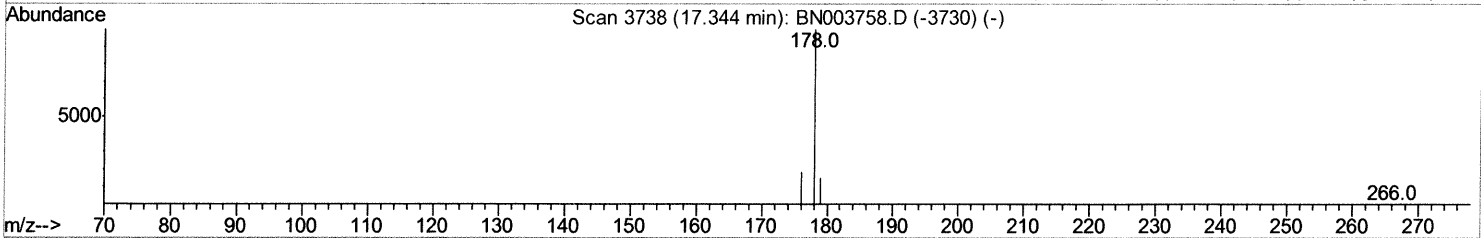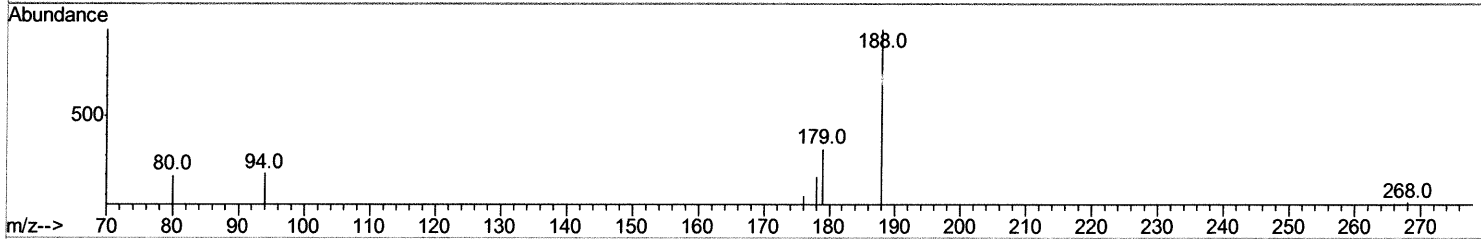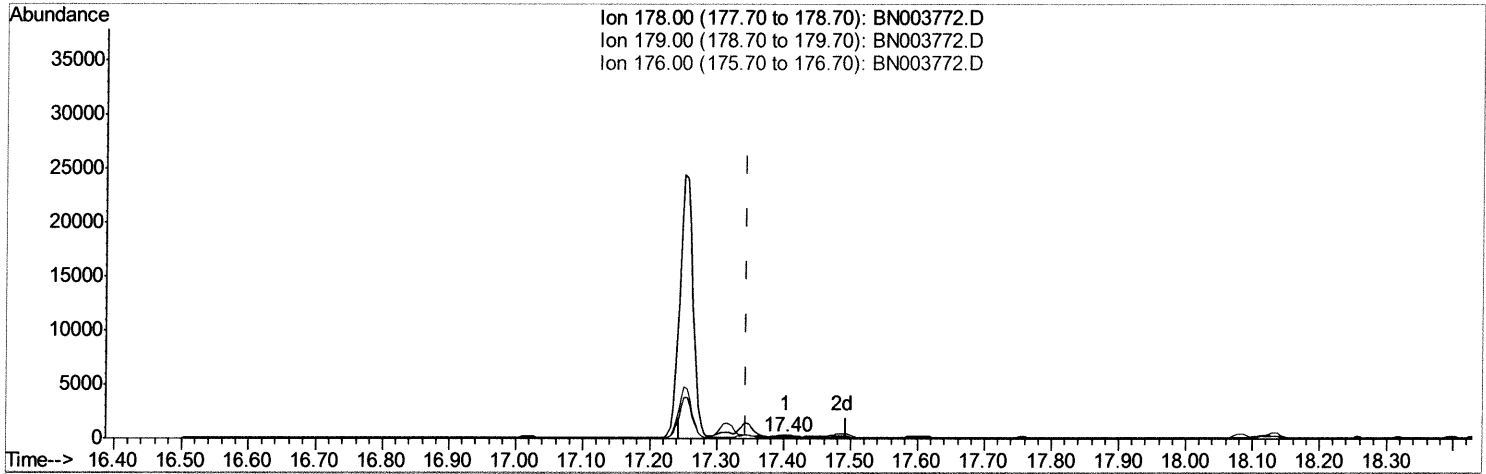

TIC: BN003772.D

(13) Anthracene

17.403min (+0.059) 0.00ng/ul

response 93

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	177.54#
176.00	18.50	49.20#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:53:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

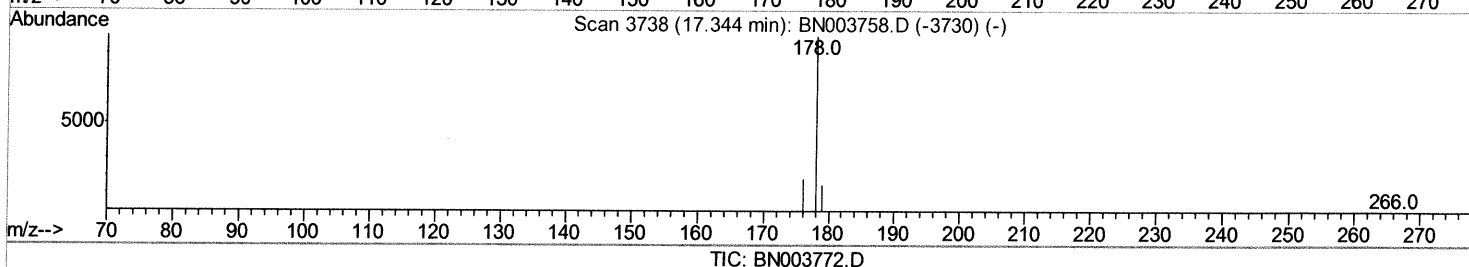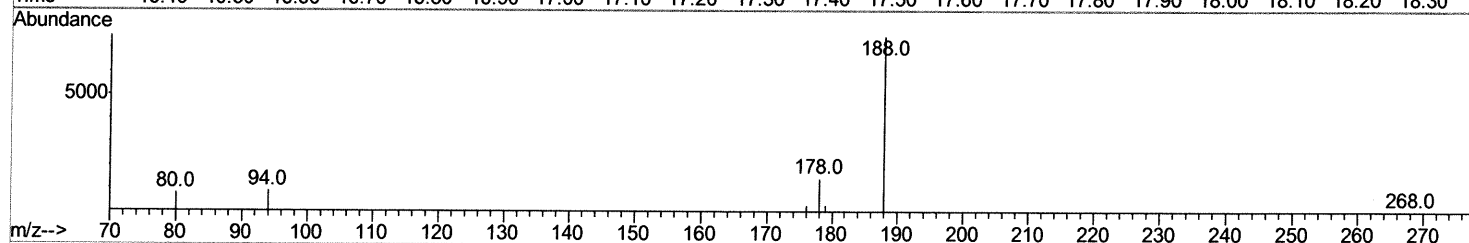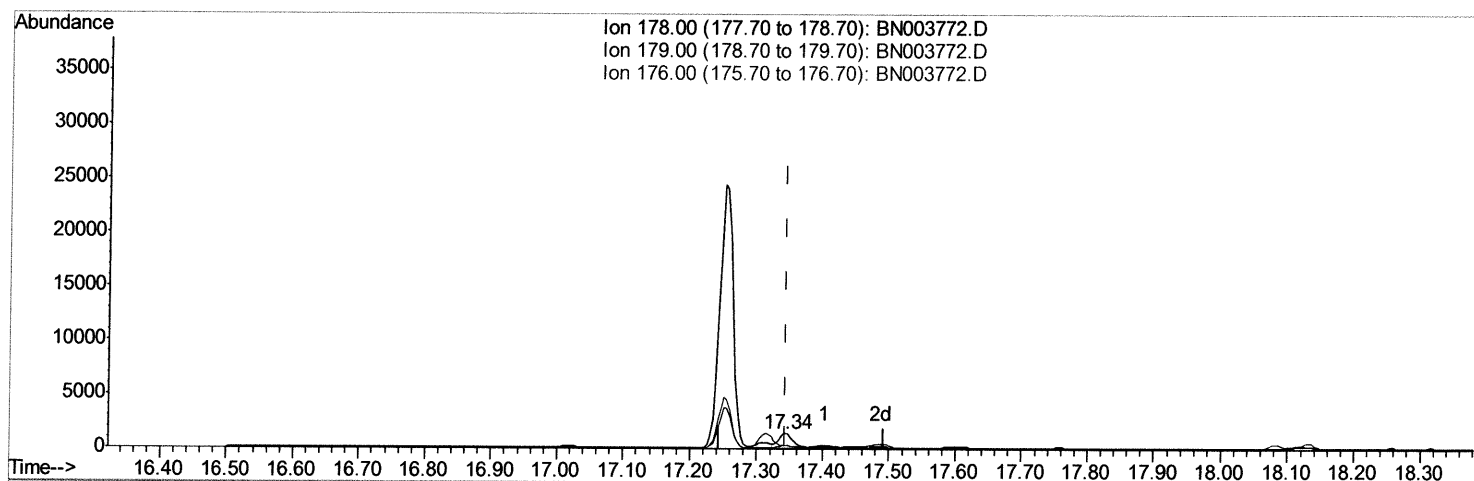

TIC: BN003772.D

(13) Anthracene

17.343min (-0.000) 0.03ng/ul m

response 2083

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	21.99#
176.00	18.50	21.99
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003772.D
Acq On : 07 Dec 2018 18:29
Operator : JU/SJ
Sample : J6228-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E59

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:53:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

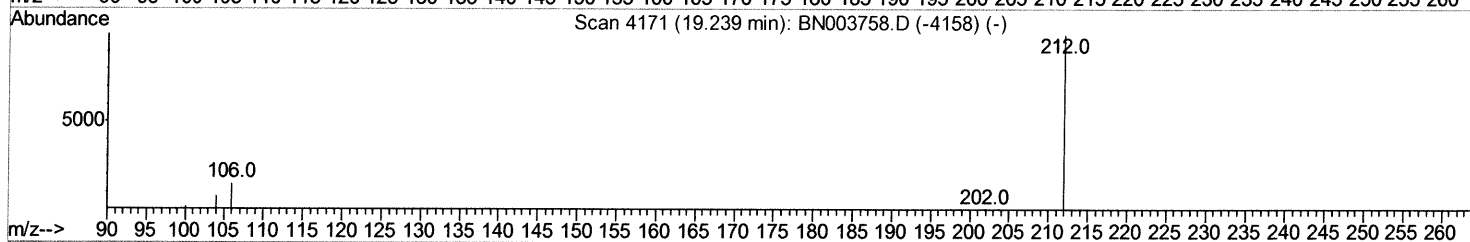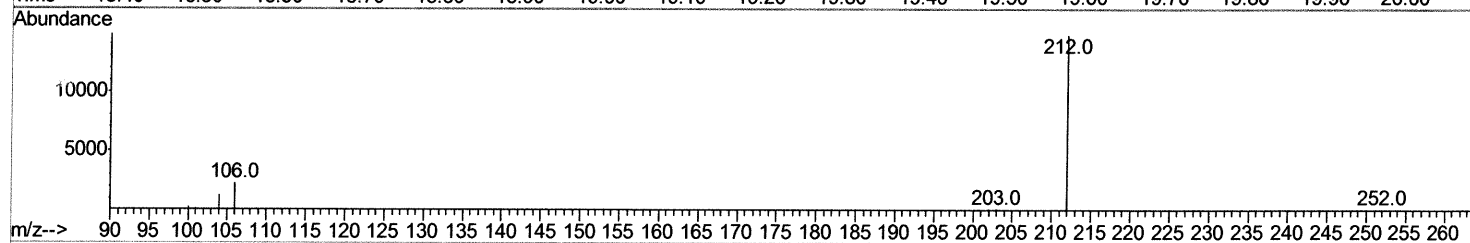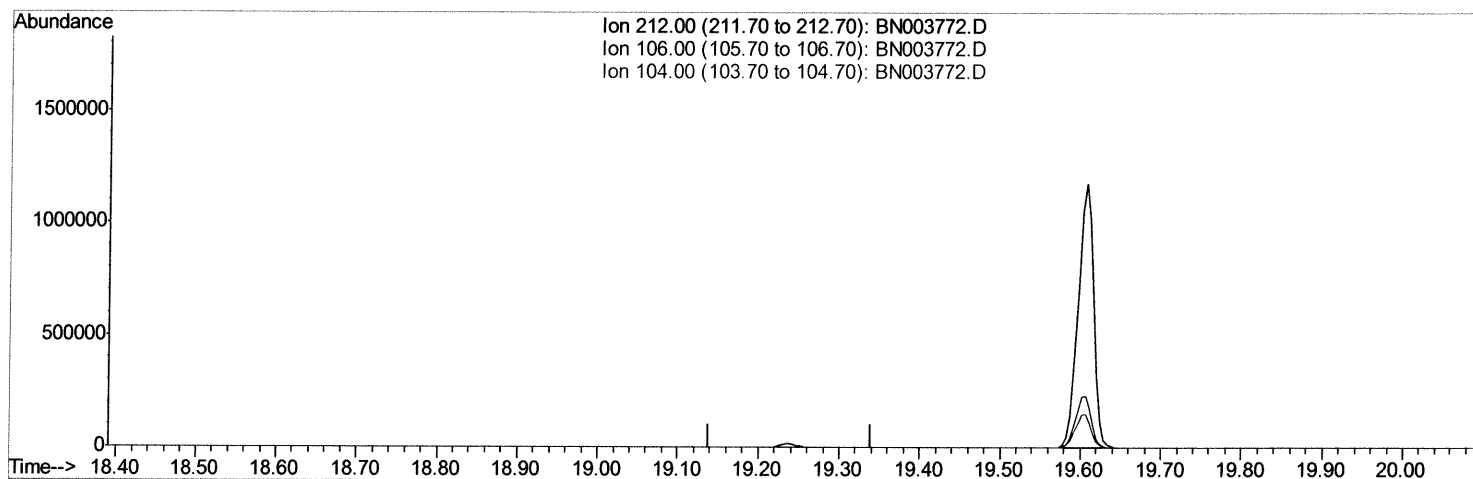

TIC: BN003772.D

(14) Fluoranthene-d10 (SURRE)

19.239min (-19.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:53:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

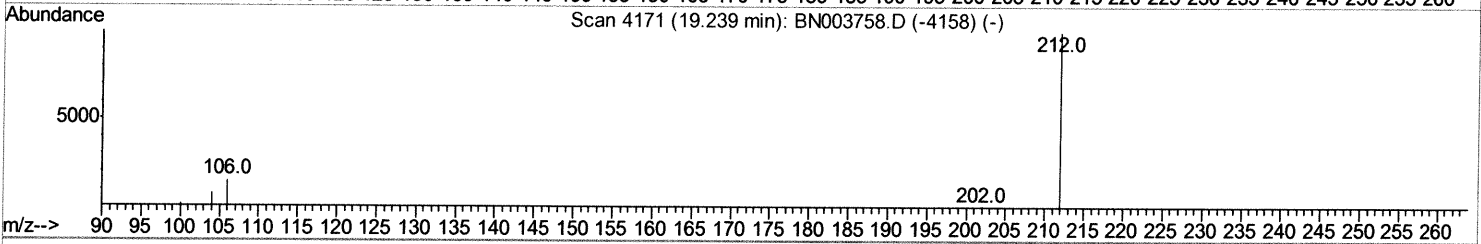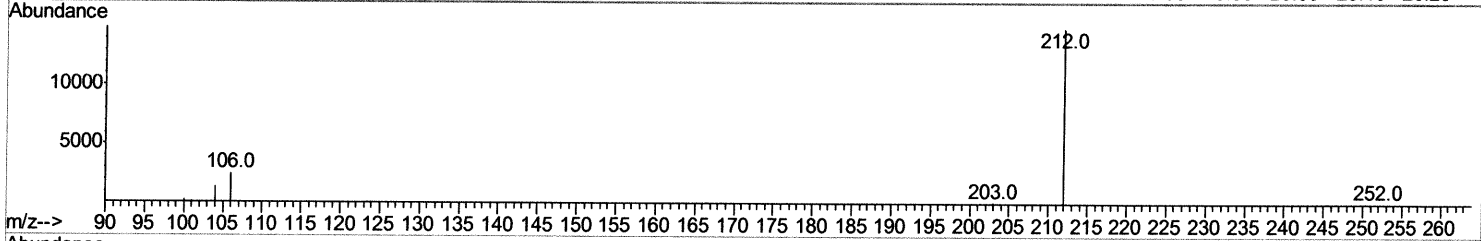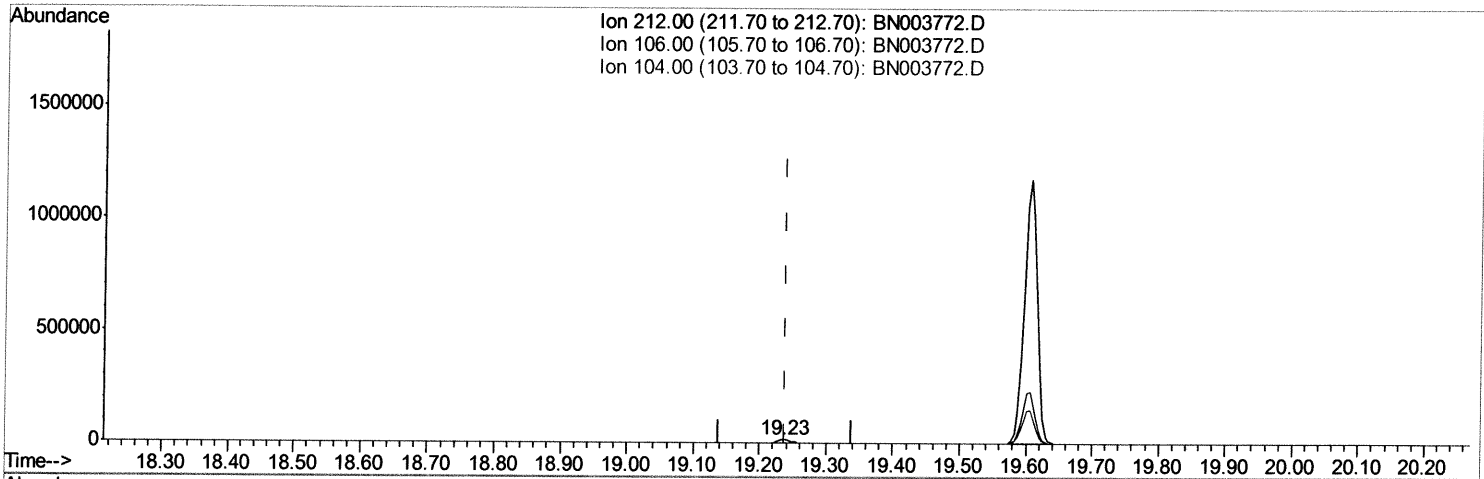

TIC: BN003772.D

(14) Fluoranthene-d10 (SURR)

19.234min (-0.005) 0.28ng/ul m

response 20138

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003772.D
Acq On : 07 Dec 2018 18:29
Operator : JU/SJ
Sample : J6228-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E59

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:53:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

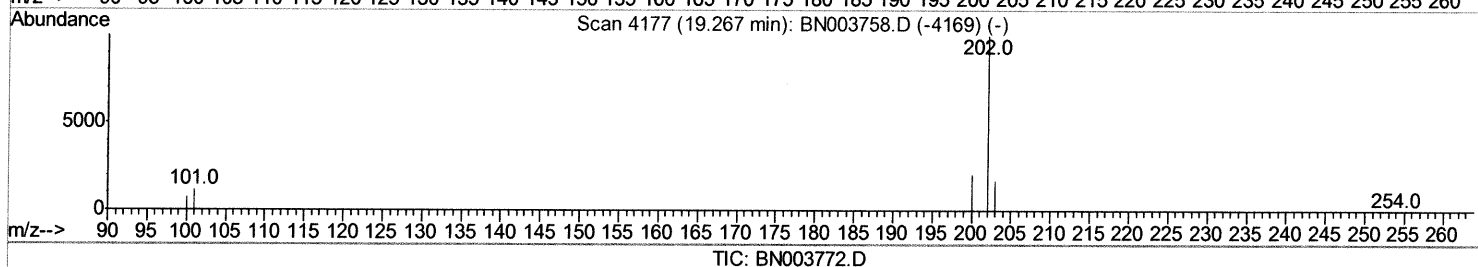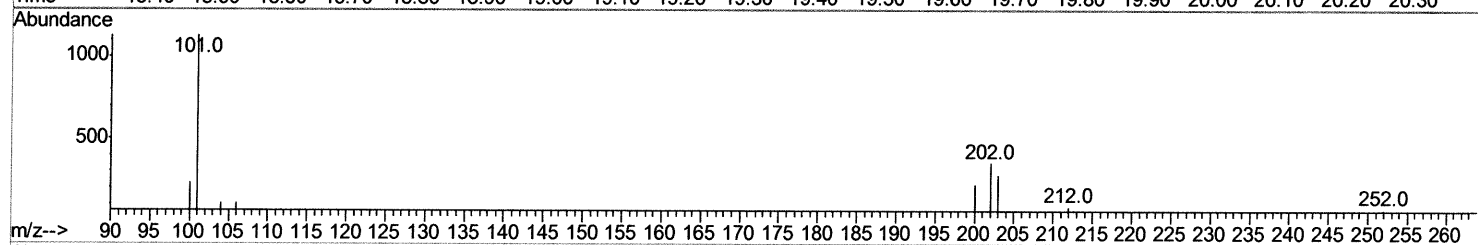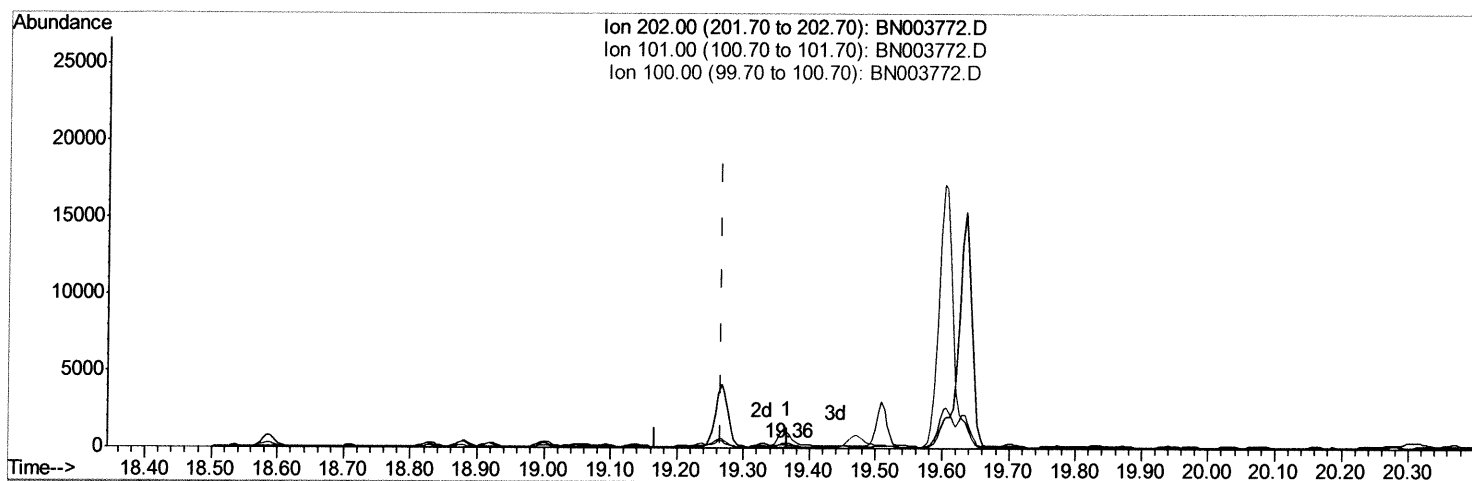

(15) Fluoranthene (C)

19.364min (+0.097) 0.00ng/ul

response 330

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	322.29#
100.00	8.10	64.86#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:53:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

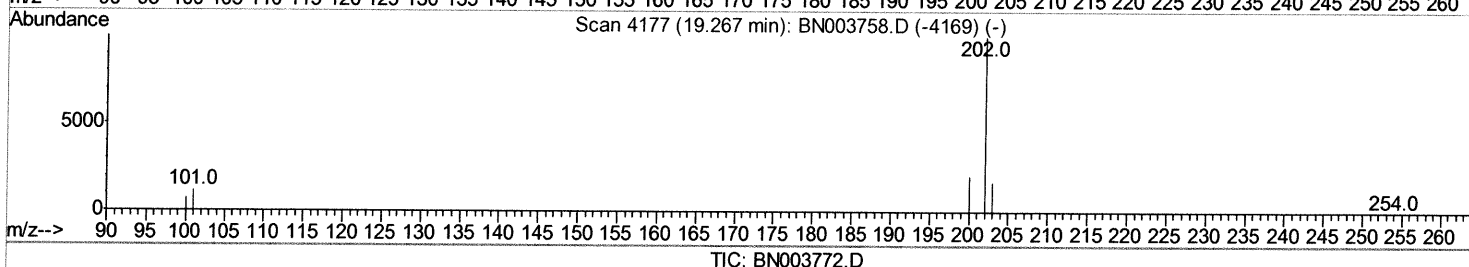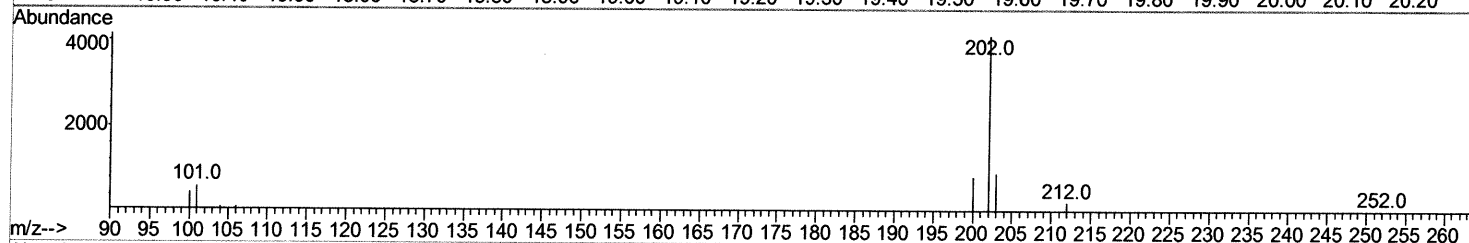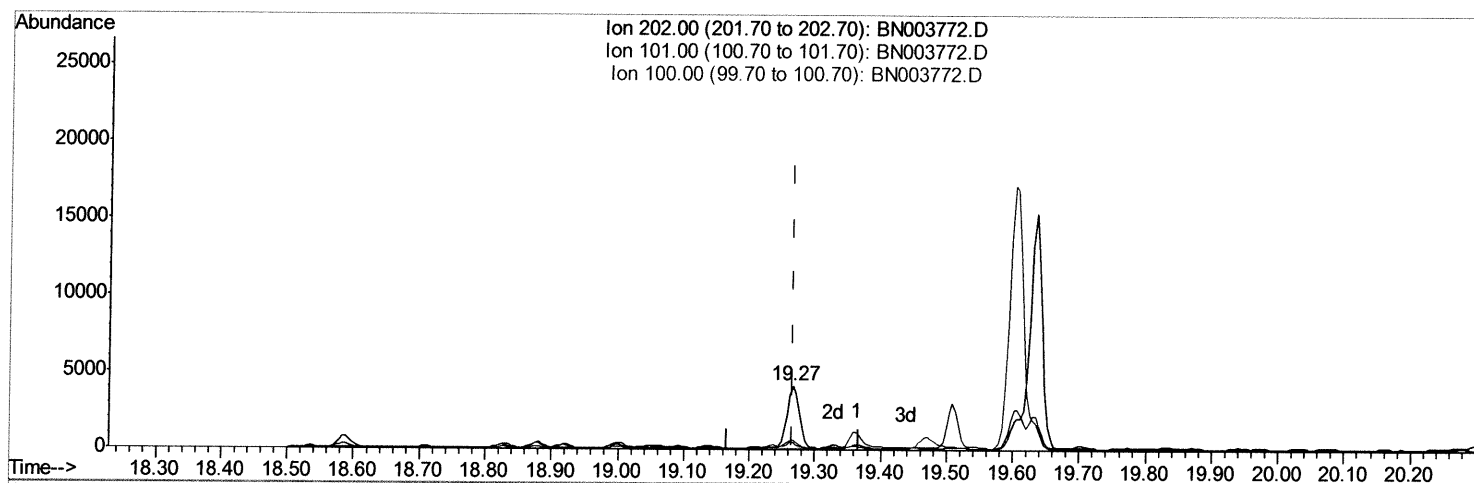

(15) Fluoranthene (C)

19.267min (-0.000) 0.06ng/ul m

response 5373

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	14.45
100.00	8.10	10.52
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:53:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

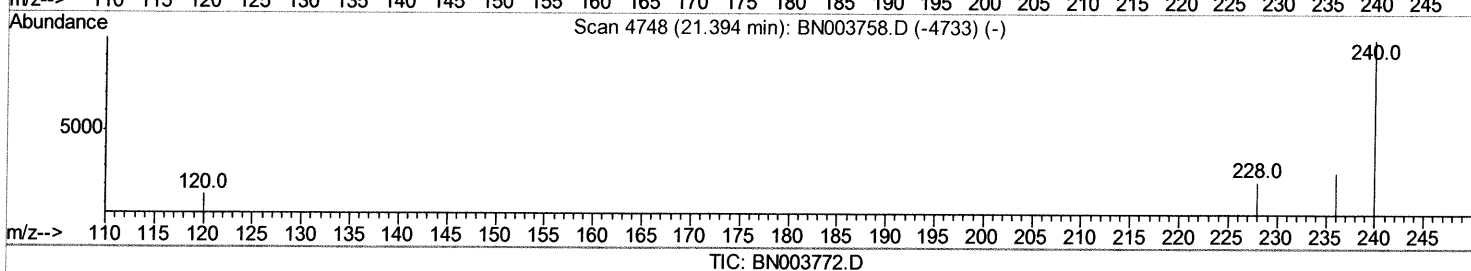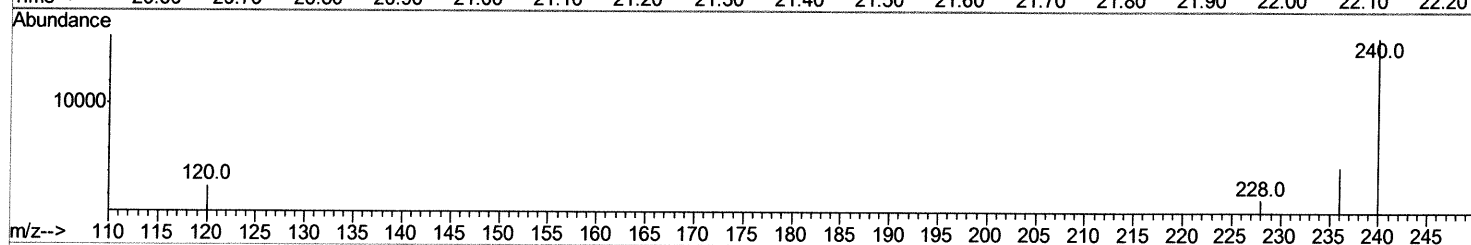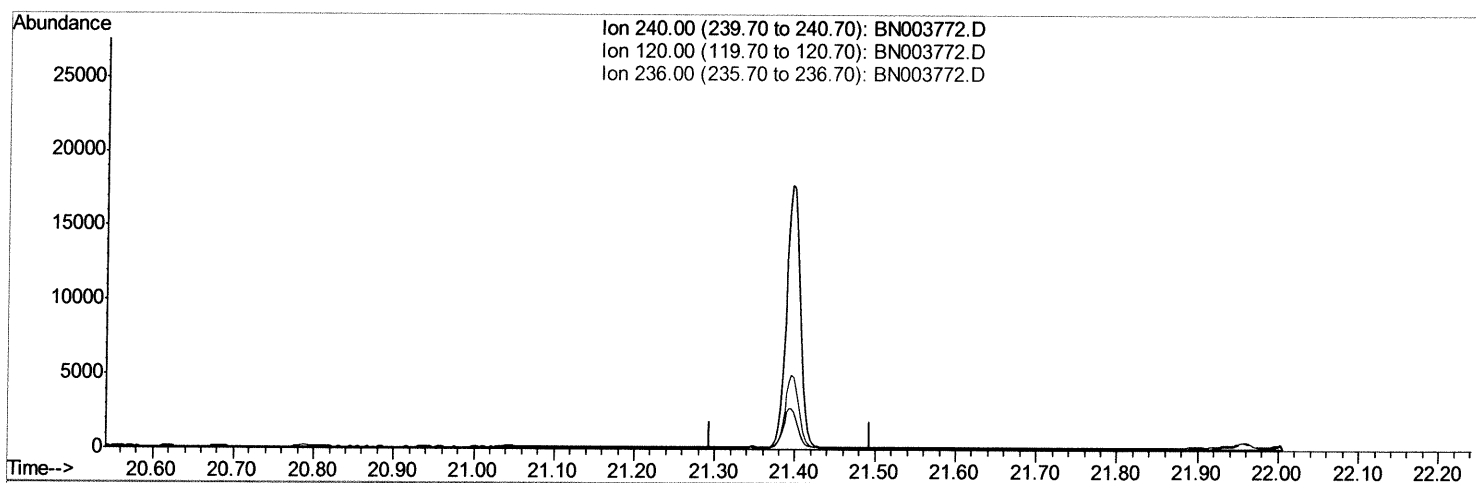

(16) Chrysene-d12 (I)

21.394min (-21.394) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:53:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

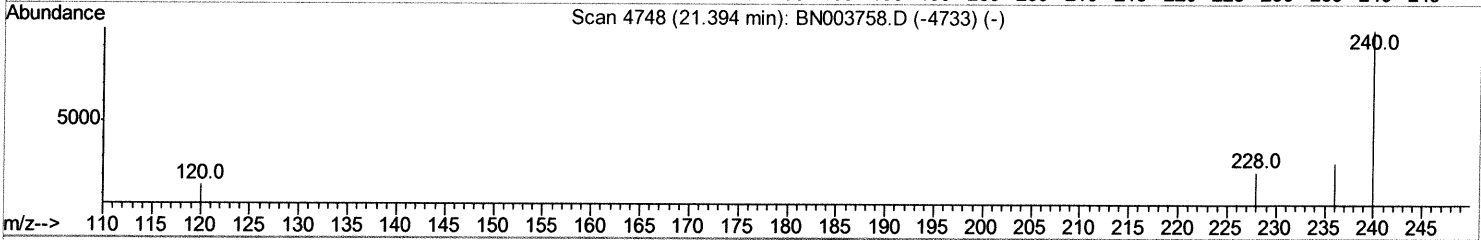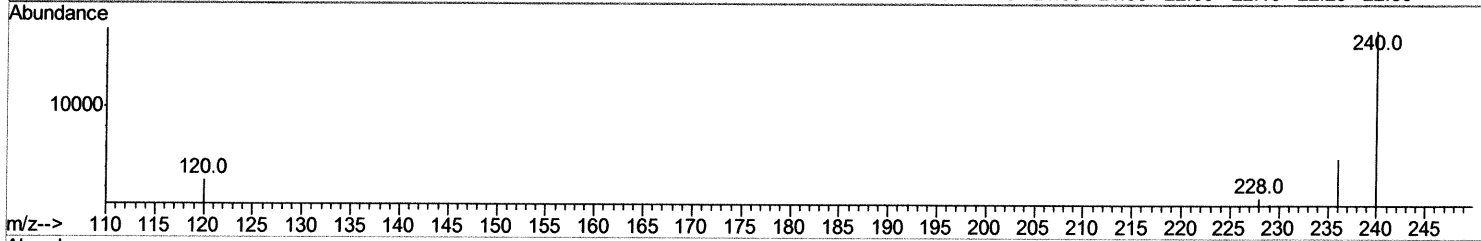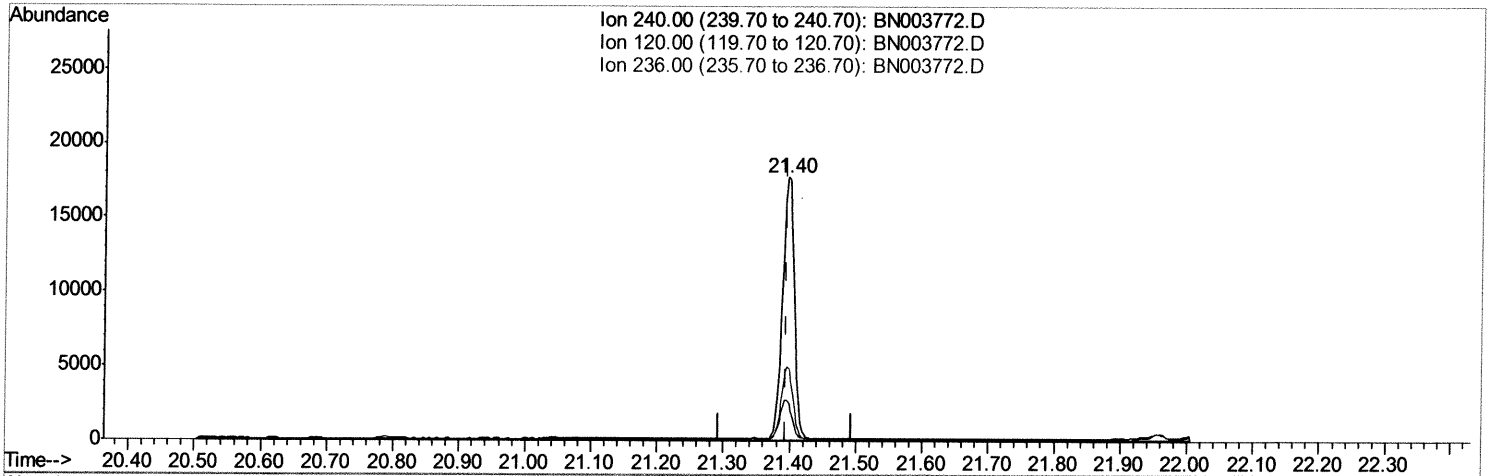

TIC: BN003772.D

(16) Chrysene-d12 (I)

21.395min (+0.002) 0.40ng/ul m

response 21916

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	15.63
236.00	27.60	28.40
0.00	0.00	0.00

MA 12/11/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:55:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

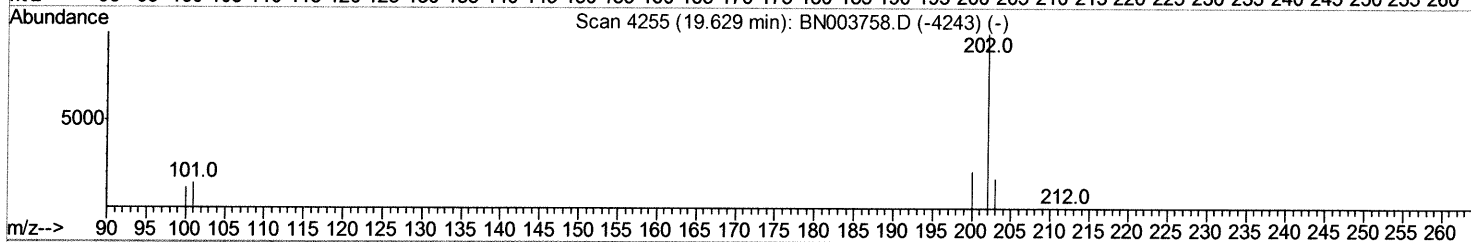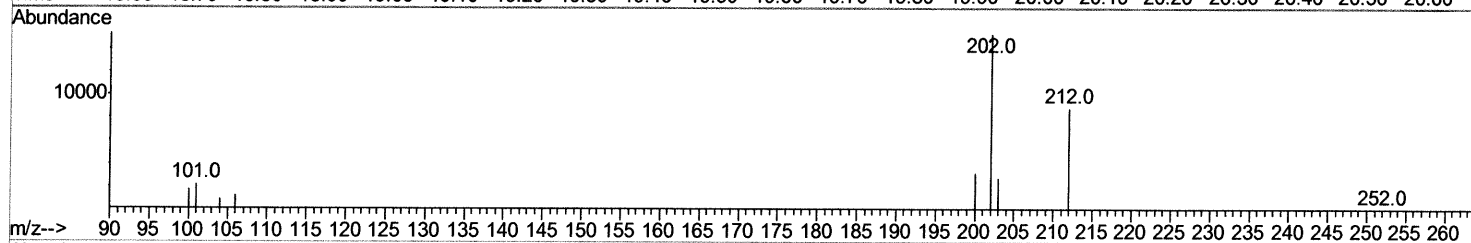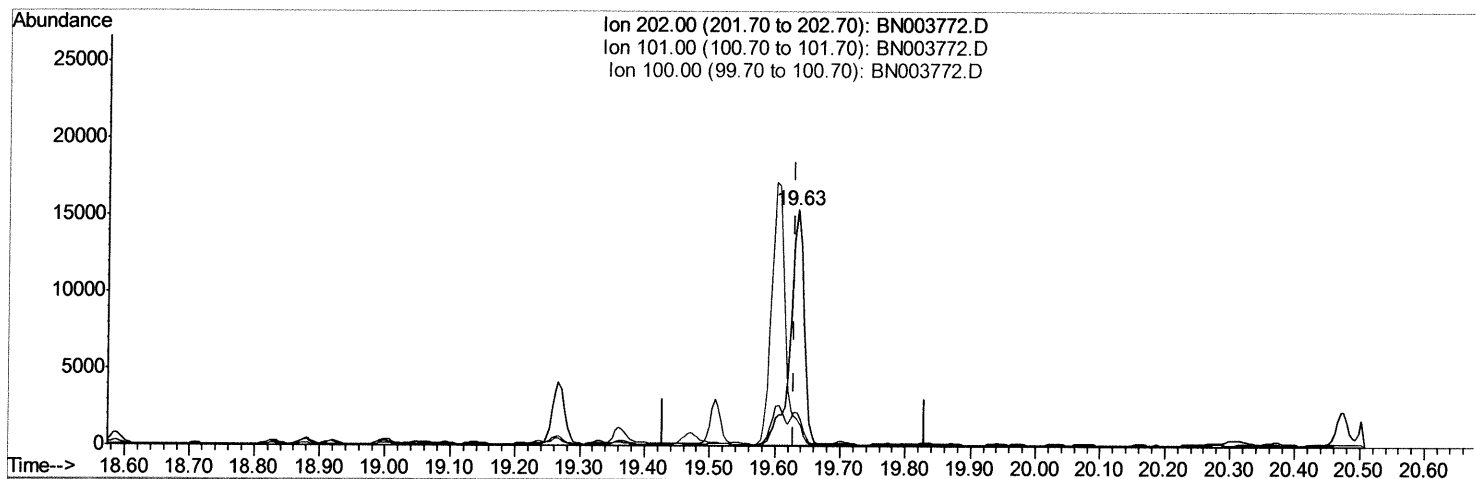

TIC: BN003772.D

(17) Pyrene

19.634min (+0.004) 0.28ng/ul

response 21752

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	14.17
100.00	10.60	11.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003772.D
Acq On : 07 Dec 2018 18:29
Operator : JU/SJ
Sample : J6228-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E59

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:55:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

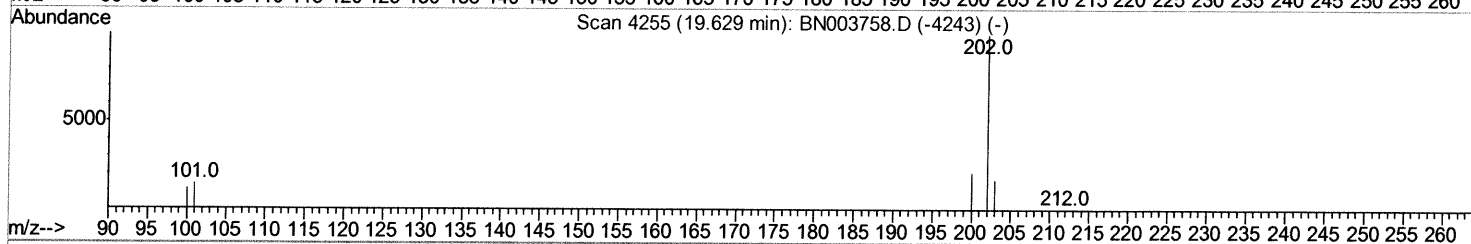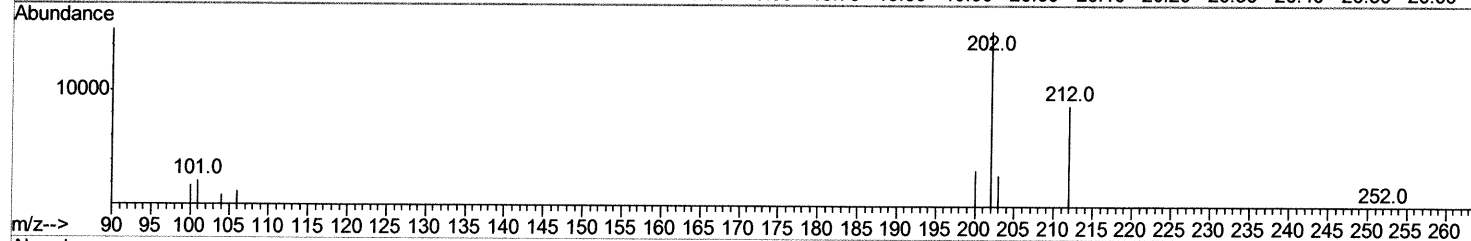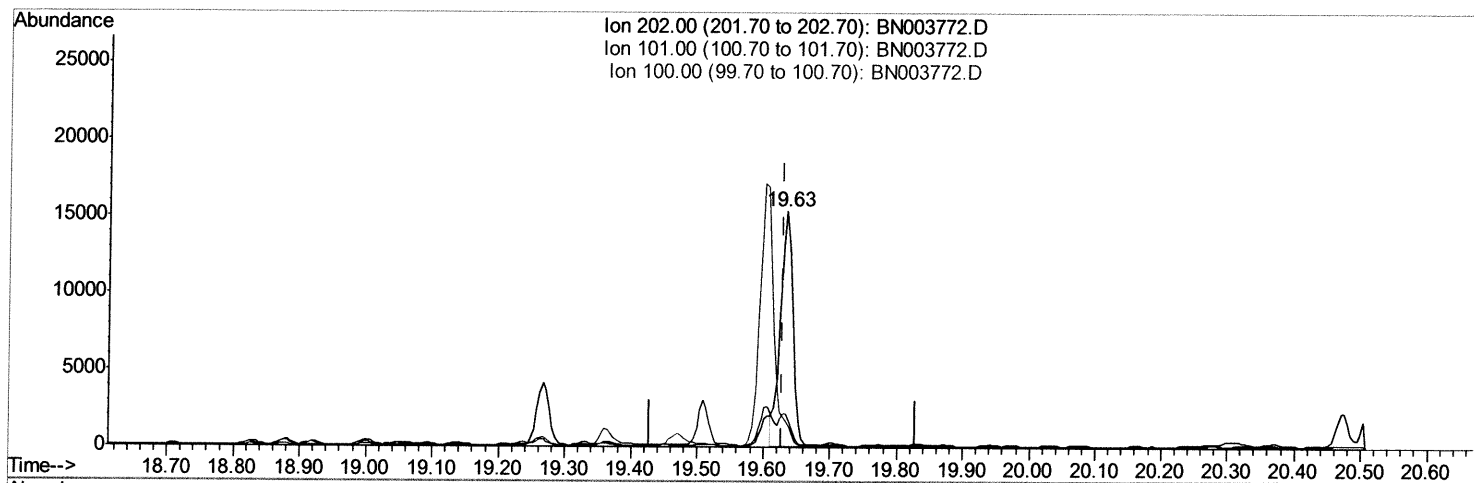

TIC: BN003772.D

(17) Pyrene

19.634min (+0.004) 0.25ng/ul m

response 19612

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	14.17
100.00	10.60	11.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:55:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

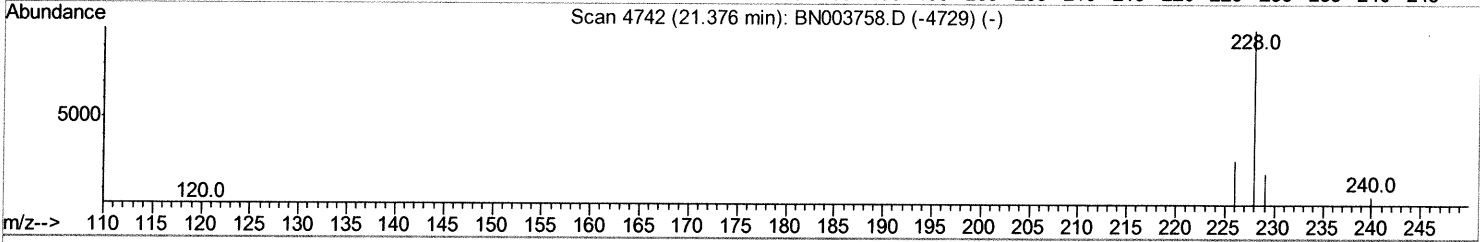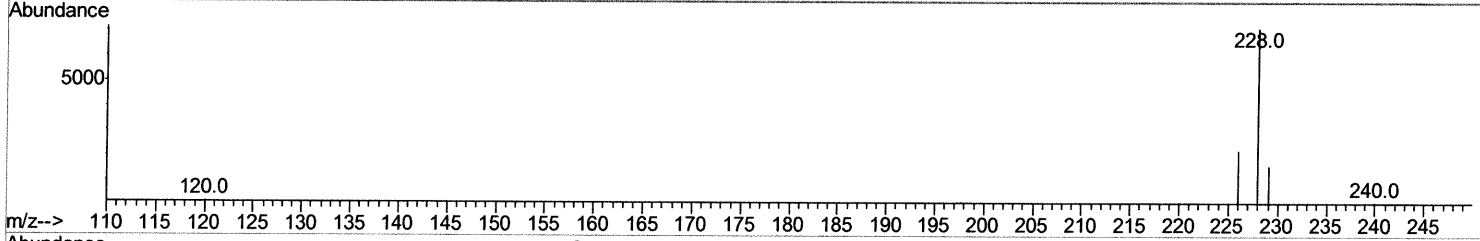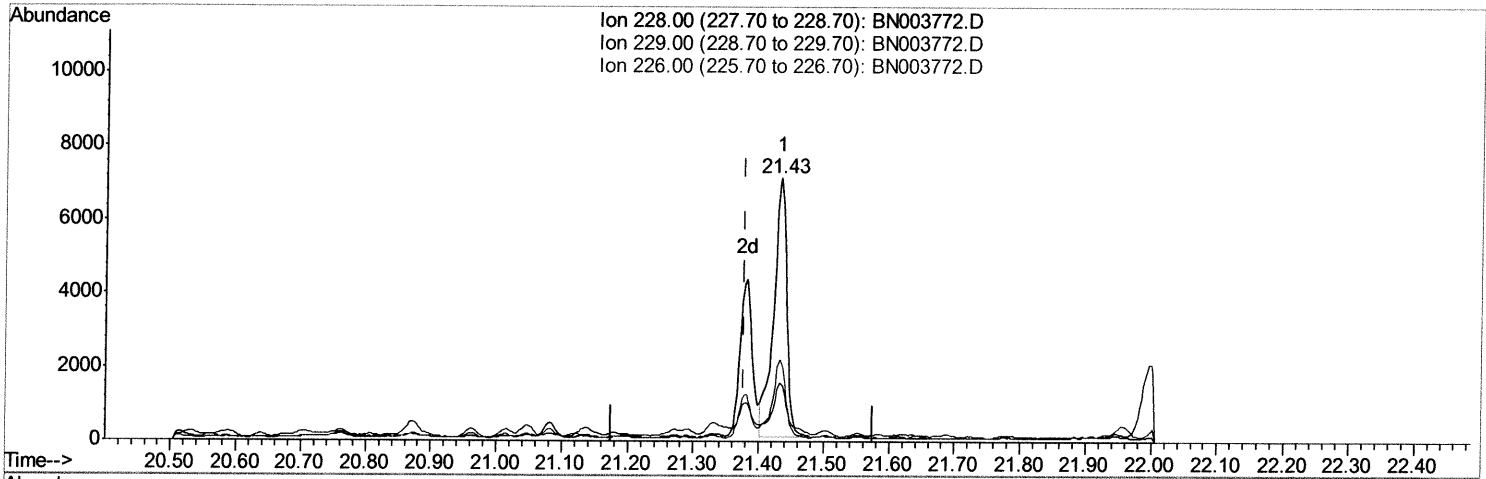

TIC: BN003772.D

(18) Benzo(a)anthracene
 21.433min (+0.057) 0.14ng/ul
 response 9933

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	22.37
226.00	26.40	31.12
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:55:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

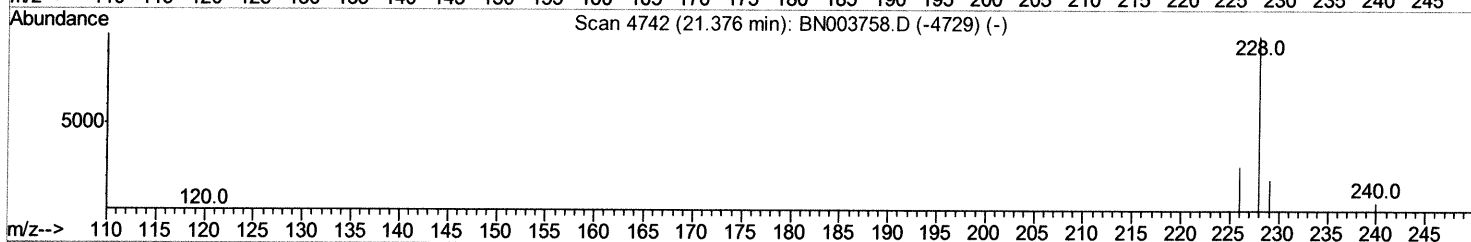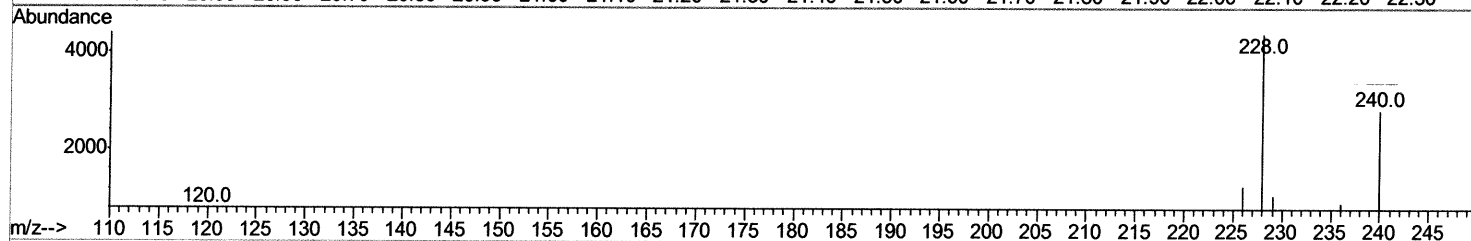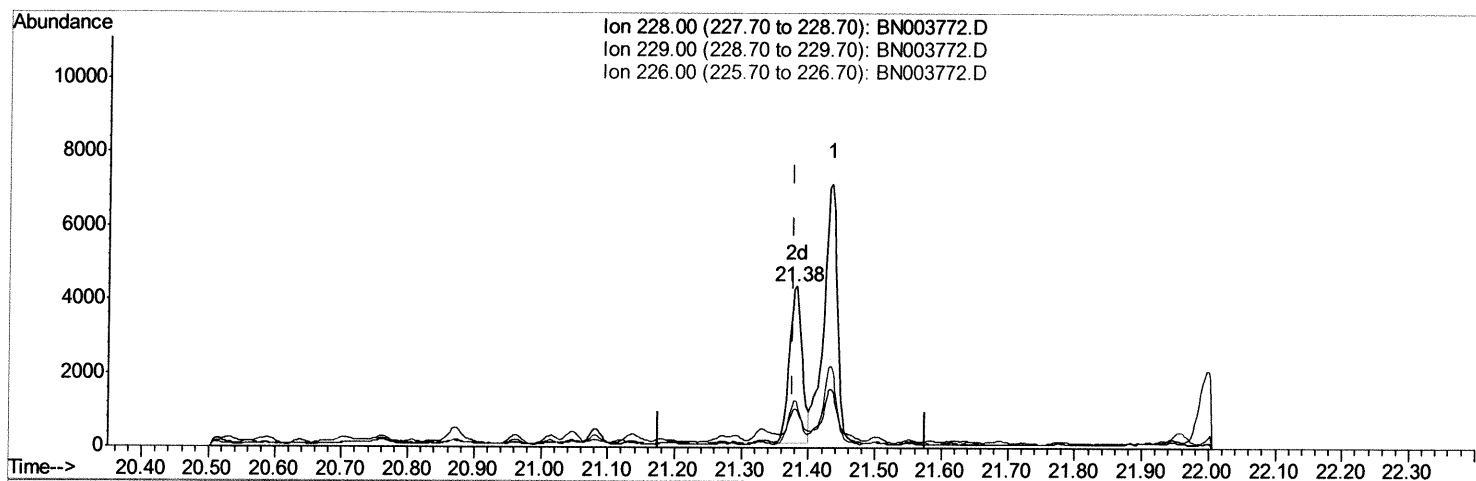

TIC: BN003772.D

(18) Benzo(a)anthracene

21.381min (+0.004) 0.08ng/ul m

response 5549

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	24.09#
226.00	26.40	28.76
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:55:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

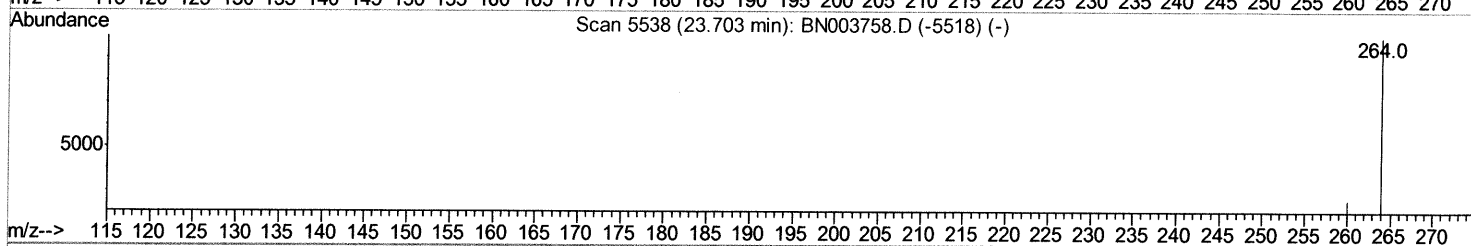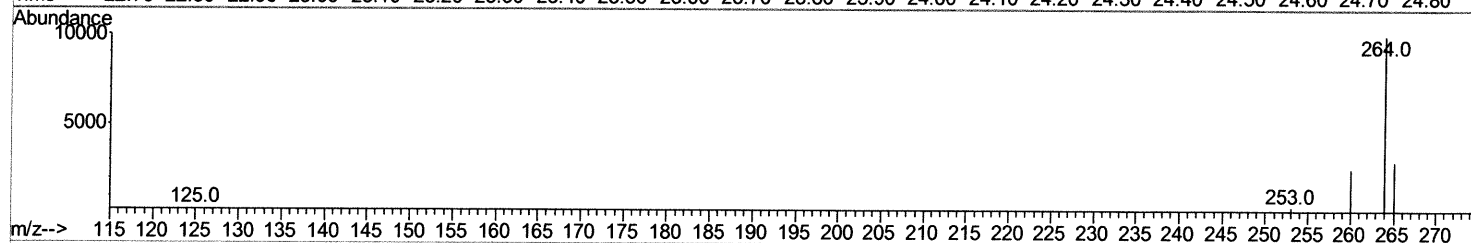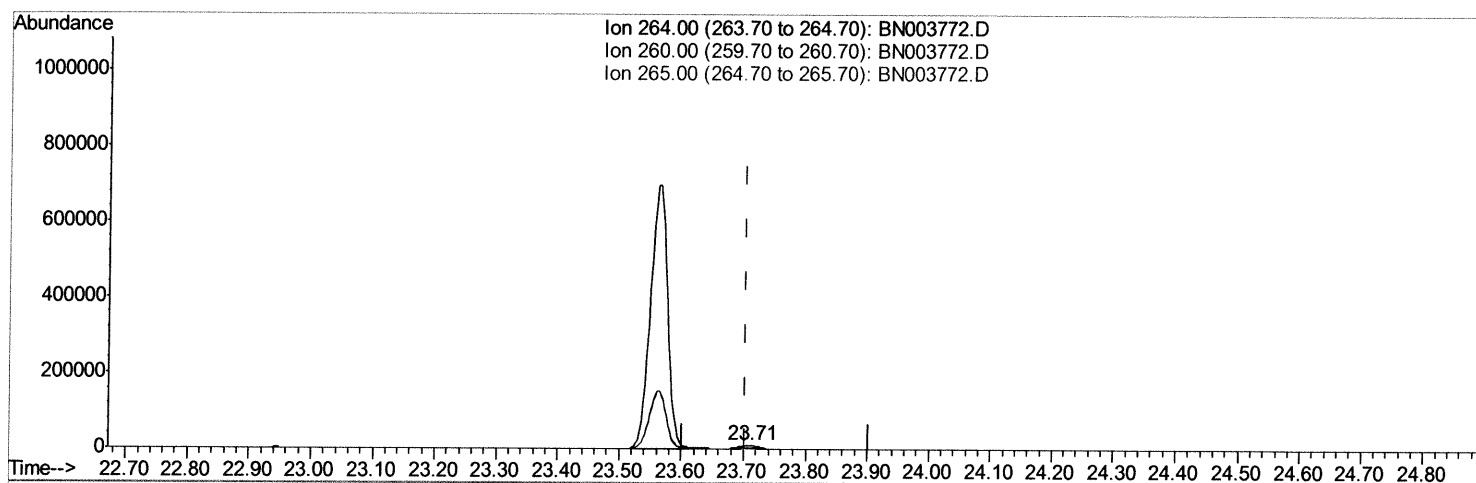

TIC: BN003772.D

(20) Perylene-d12 (I)
 23.710min (+0.007) 0.40ng/ul
 response 21215

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.08
265.00	33.50	30.03
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:55:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

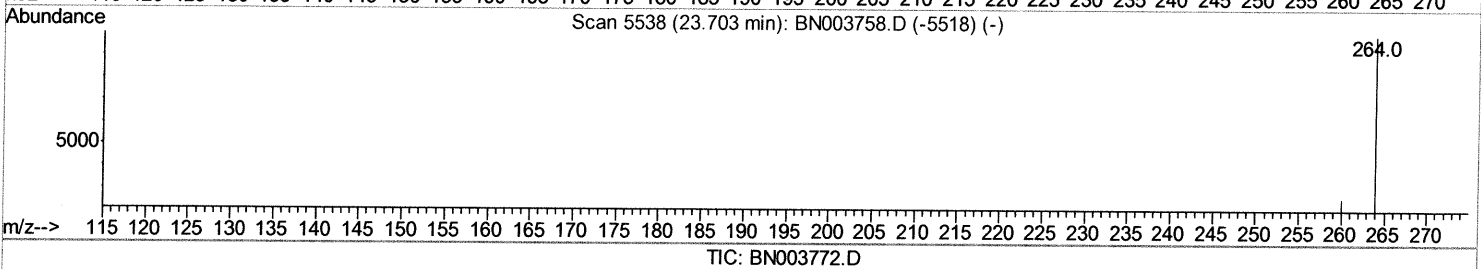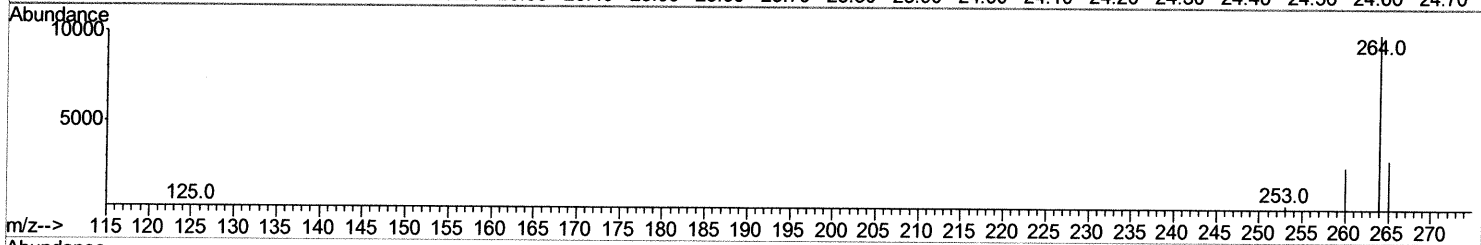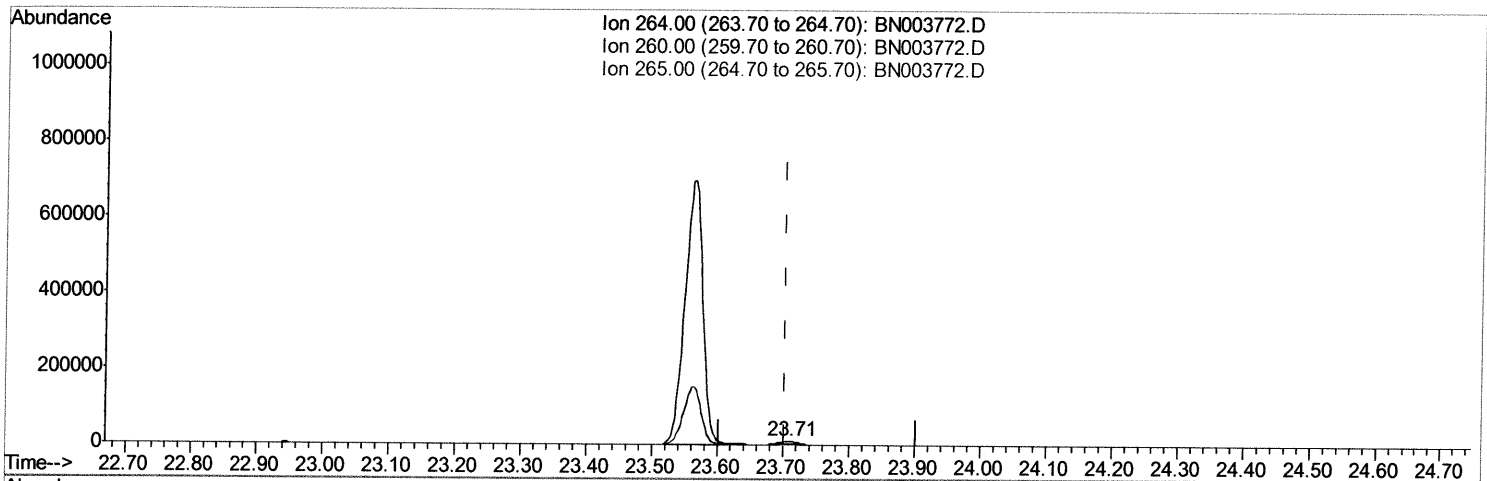

(20) Perylene-d12 (I)

23.710min (+0.007) 0.40ng/ul m

response 16887

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.08
265.00	33.50	30.03
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003772.D
Acq On : 07 Dec 2018 18:29
Operator : JU/SJ
Sample : J6228-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E59

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:56:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

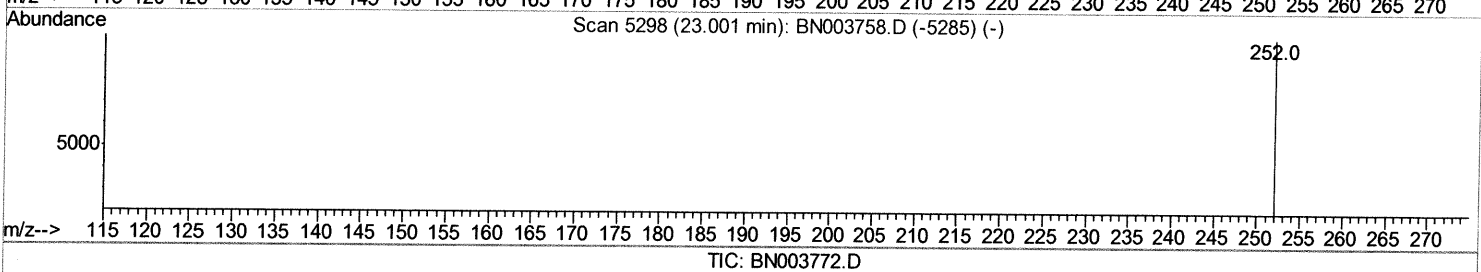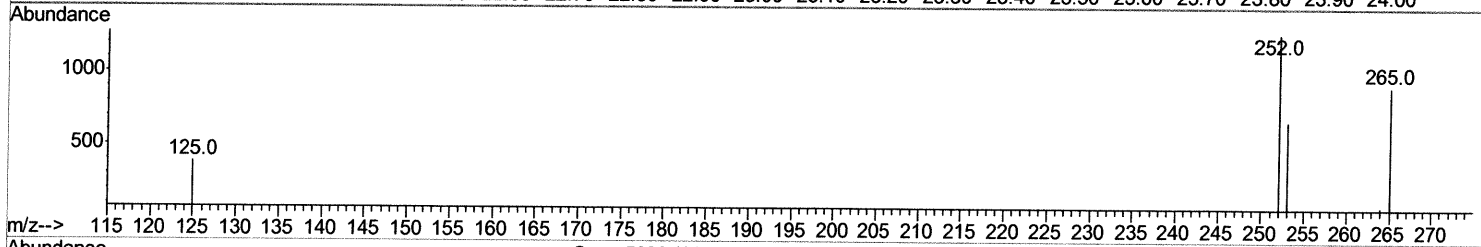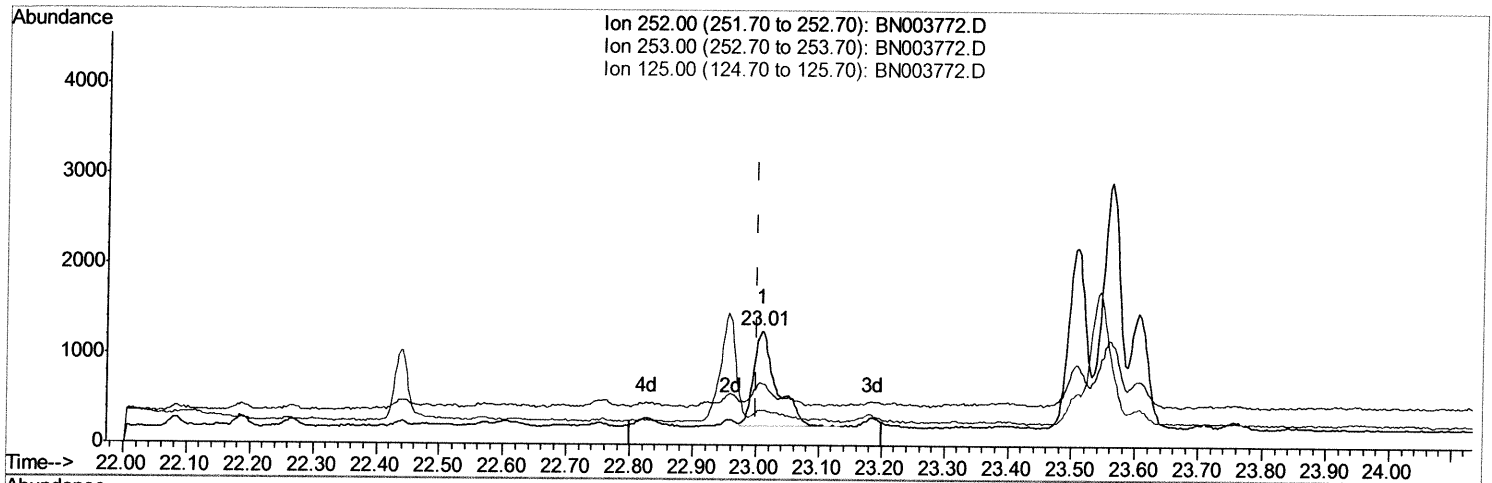

(21) Benzo(b)fluoranthene

23.009min (+0.007) 0.04ng/ul

response 2697

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	53.10#
125.00	11.20	30.16#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:56:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

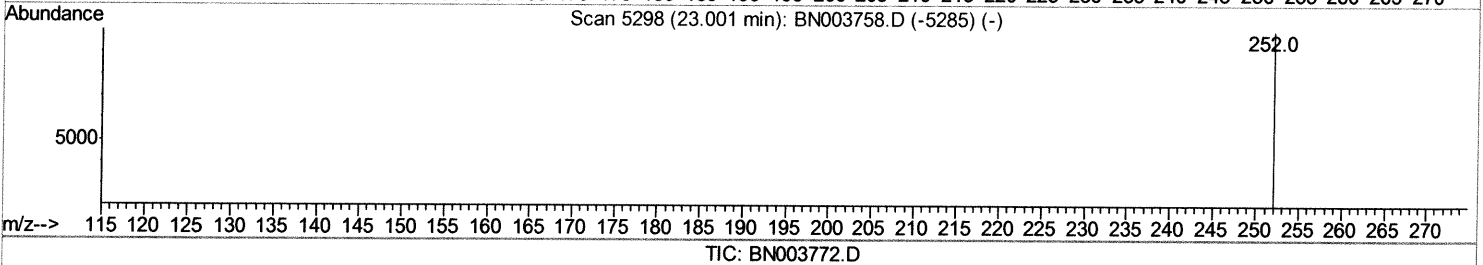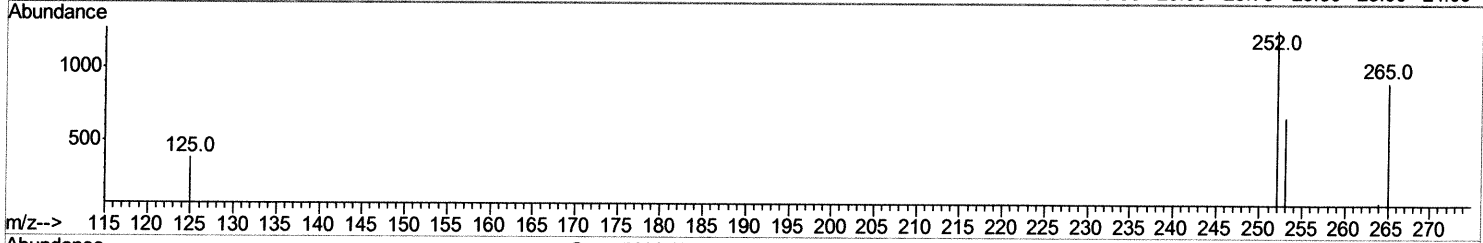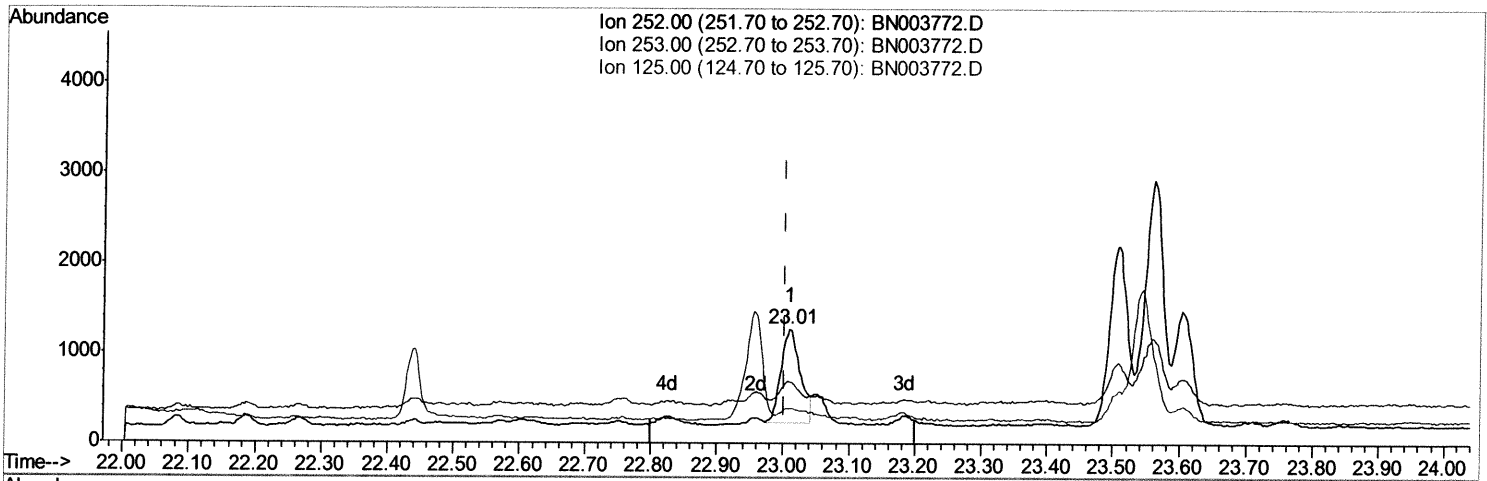

(21) Benzo(b)fluoranthene

23.009min (+0.007) 0.03ng/ul m

response 2113

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	53.10#
125.00	11.20	30.16#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003772.D
 Acq On : 07 Dec 2018 18:29
 Operator : JU/SJ
 Sample : J6228-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E59

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:57:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 08 00:32:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4793	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	19914	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11063	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	24294m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	21916m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	16887m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	8837	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.23	212	20138m	0.28	ng/ul	0.00
Target Compounds						
					Ovalue	
5) 2-Methylnaphthalene	12.29	142	1221	0.031	ng/ul	98
12) Phenanthrene	17.25	178	33991	0.426	ng/ul	99
13) Anthracene	17.34	178	2083m	0.032	ng/ul	
15) Fluoranthene	19.27	202	5373m	0.057	ng/ul	
17) Pyrene	19.63	202	19612m	0.250	ng/ul	
18) Benzo(a)anthracene	21.38	228	5549m	0.080	ng/ul	
19) Chrysene	21.43	228	9933	0.125	ng/ul	
21) Benzo(b)fluoranthene	23.01	252	2113m	0.030	ng/ul	
23) Benzo(a)pyrene	23.61	252	2289	0.038	ng/ul#	54
26) Benzo(a,h,i)perylene	26.78	276	1304	0.022	ng/ul#	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003772.D
Acq On : 07 Dec 2018 18:29
Operator : JU/SJ
Sample : J6228-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E59

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:24 AM

Quant Time: Dec 08 00:57:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 08 00:32:32 2018
Response via : Initial Calibration

