

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
 Data File : BN003759.D
 Acq On : 07 Dec 2018 10:45
 Operator : JU/SJ
 Sample : J6077-05DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9Y38DL

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:46:13 AM

Quant Time: Dec 07 11:25:06 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 07 04:08:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5664	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	23808	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12963	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	28477	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	24125	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	22253	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	3317	0.09	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	7169	0.09	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.68	128	42831	0.640	ng/ul	97
5) 2-Methylnaphthalene	12.29	142	40380	0.865	ng/ul	100
8) Acenaphthene	14.53	153	1193	0.023	ng/ul	97
9) Fluorene	15.52	166	1360	0.023	ng/ul#	97
12) Phenanthrene	17.25	178	10147	0.109	ng/ul	98
17) Pyrene	19.63	202	3561m	0.041	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120718\
Data File : BN003759.D
Acq On : 07 Dec 2018 10:45
Operator : JU/SJ
Sample : J6077-05DL 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
F9Y38DL

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:13 AM

Quant Time: Dec 07 11:25:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 07 04:08:50 2018
Response via : Initial Calibration

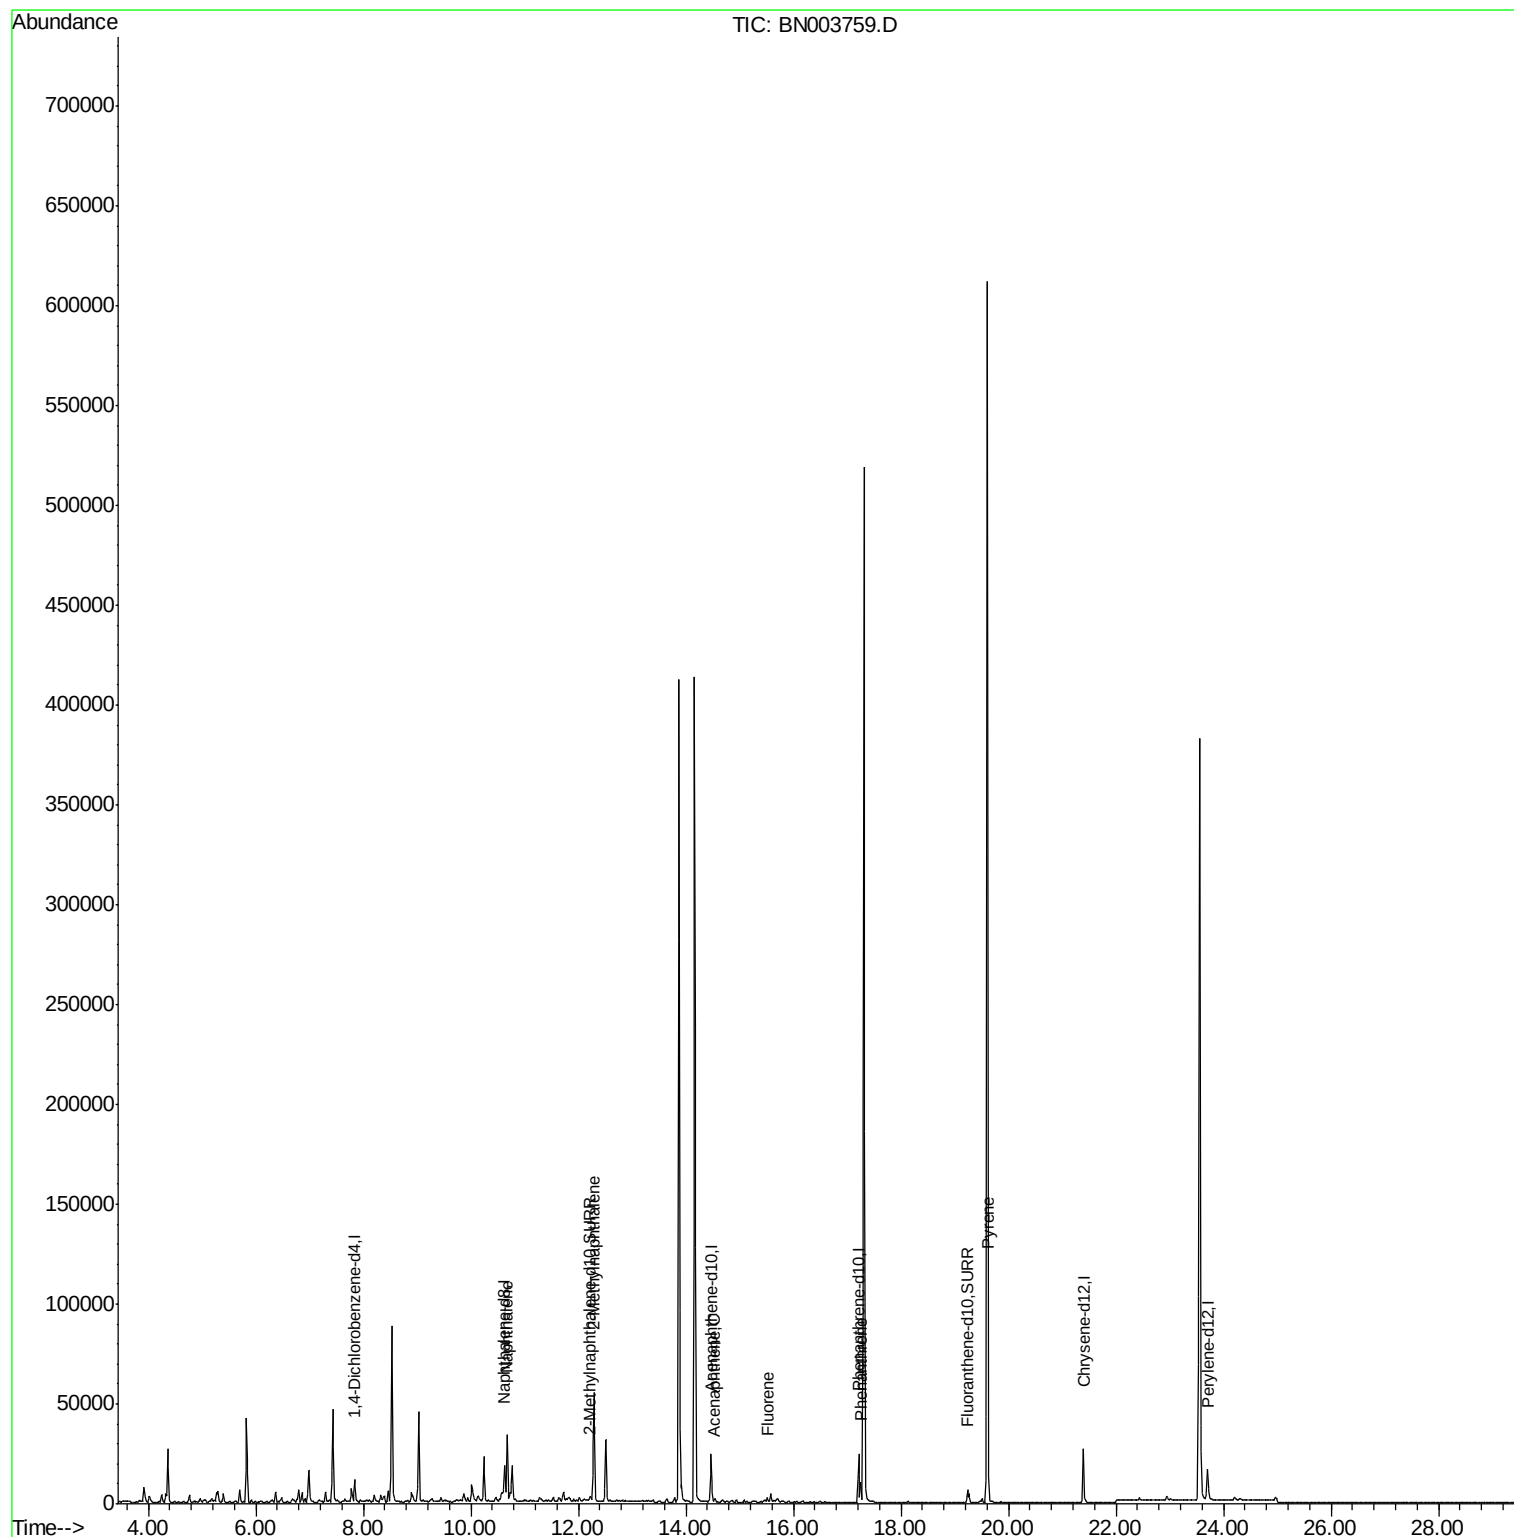

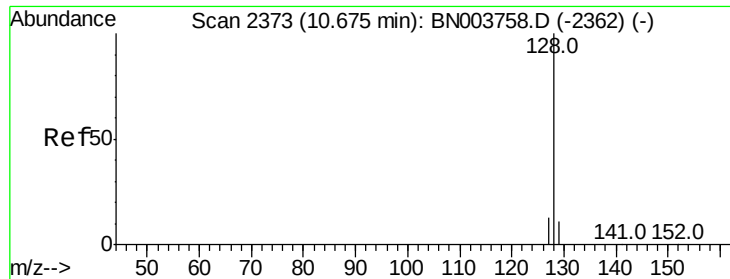

#3

Naphthalene

Concen: 0.640 ng/ul

RT: 10.68 min Scan# 2373

Delta R.T. -0.01 min

Lab File: BN003759.D

Acq: 07 Dec 2018 10:45

Instrument :

BNA_N


ClientSampleId :

F9Y38DL




Tot Ion:	128	Resp:	42831
Ion	Ratio	Lower	Upper
128	100		
129	12.7	9.0	13.6
127	13.7	10.5	15.7

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:13 AM

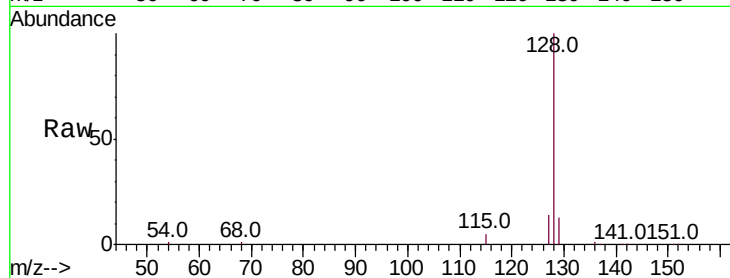

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

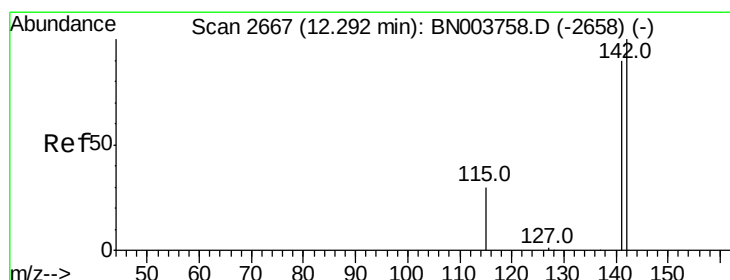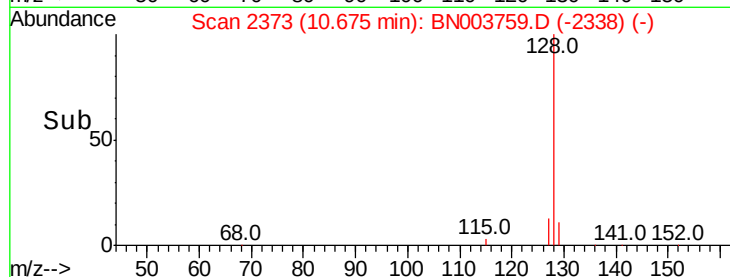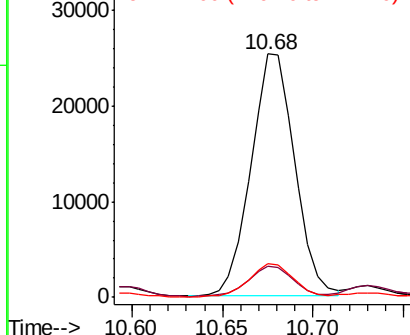

#5

2-Methylnaphthalene

Concen: 0.865 ng/ul


RT: 12.29 min Scan# 2666

Delta R.T. -0.01 min



Lab File: BN003759.D


Acq: 07 Dec 2018 10:45

Tgt Ion:	142	Resp:	40380
Ion	Ratio	Lower	Upper
142	100		
141	89.3	71.5	107.3

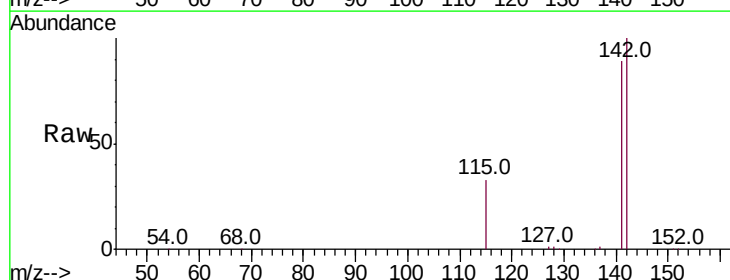

Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E

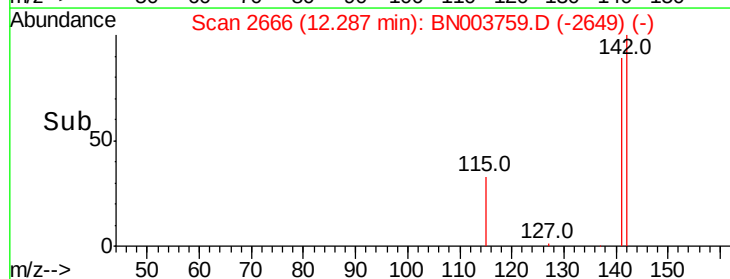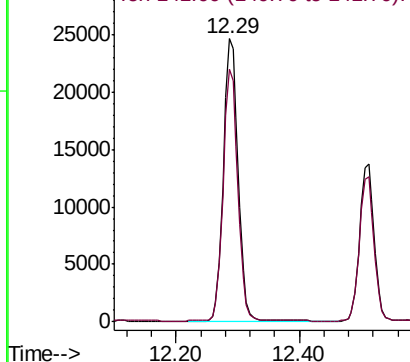

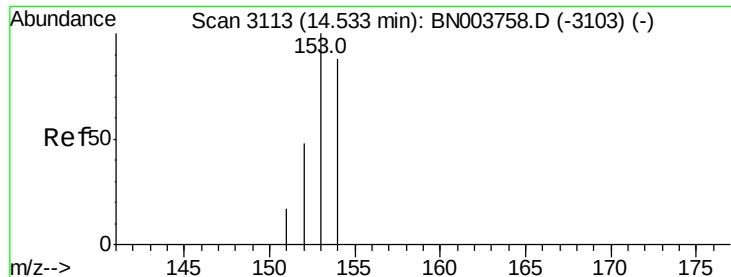

#8

Acenaphthene

Concen: 0.023 ng/ul

RT: 14.53 min Scan# 3113

Delta R.T. 0.00 min

Lab File: BN003759.D

Acq: 07 Dec 2018 10:45

Instrument :

BNA_N





ClientSampled :

F9Y38DL

Tot Ion:	153	Resp:	1193
Ion	Ratio	Lower	Upper
153	100		
152	54.1	39.3	58.9
154	87.3	70.3	105.5

Manual Integrations
APPROVED

Sohil
12/11/2018 8:46:13 AM

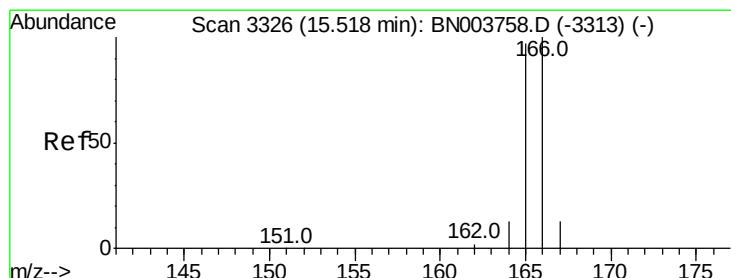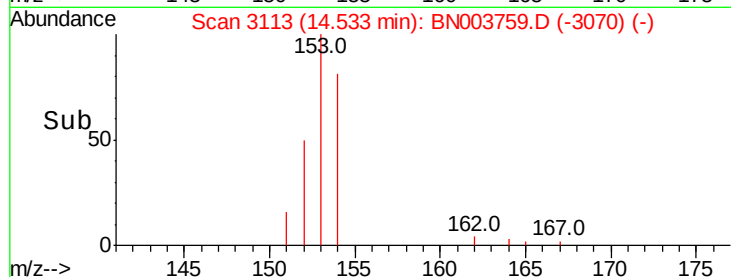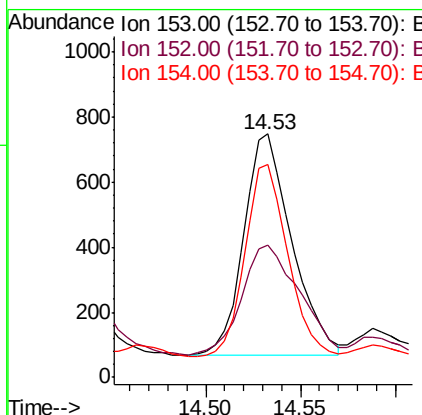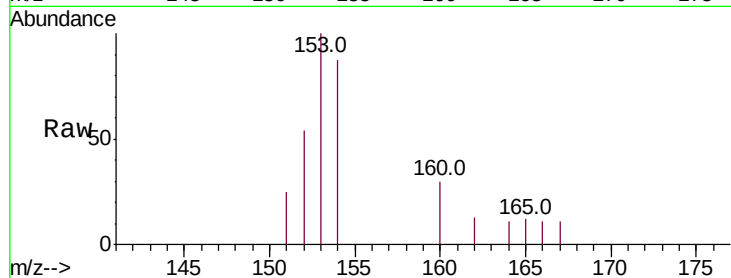

#9

Fluorene

Concen: 0.023 ng/ul




RT: 15.52 min Scan# 3326


Delta R.T. 0.00 min

Lab File: BN003759.D

Acq: 07 Dec 2018 10:45

Tgt Ion:	166	Resp:	1360
Ion	Ratio	Lower	Upper
166	100		
165	98.7	78.3	117.5
167	21.2	11.3	16.9#

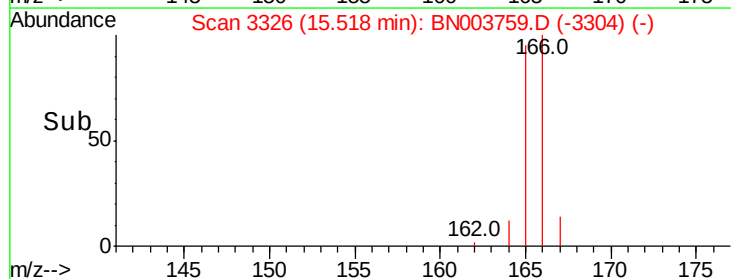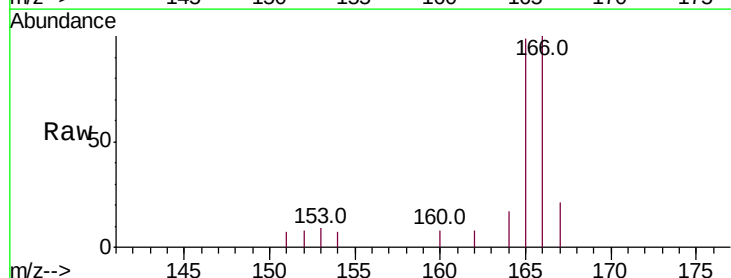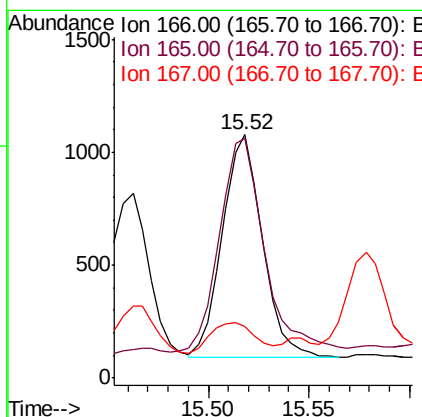

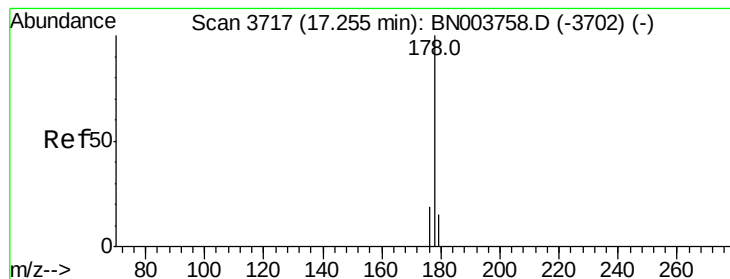

#12

Phenanthrene

Concen: 0.109 ng/ul

RT: 17.25 min Scan# 3717

Delta R.T. 0.00 min

Lab File: BN003759.D

Acq: 07 Dec 2018 10:45

Instrument :

BNA_N

ClientSampled :

F9Y38DL

Tot Ion:178 Resp: 10147

Ion Ratio Lower Upper


178 100

179 16.4 12.5 18.7

176 19.9 15.0 22.4

Manual Integrations
APPROVED




Sohil
12/11/2018 8:46:13 AM

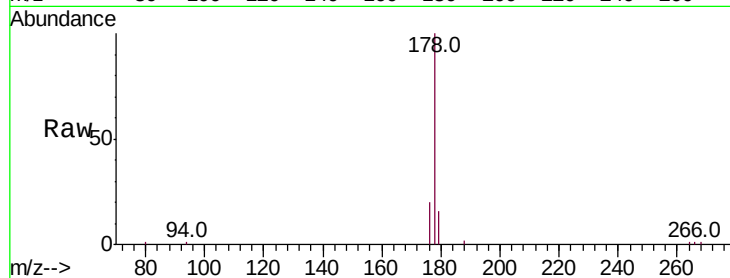

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

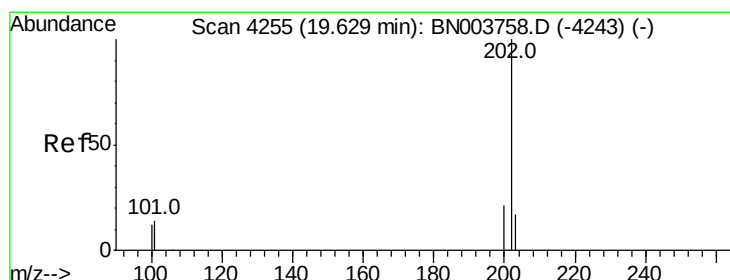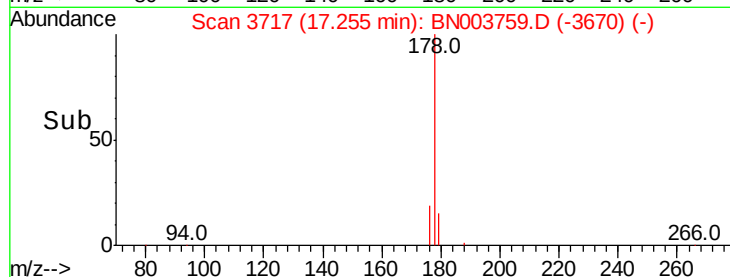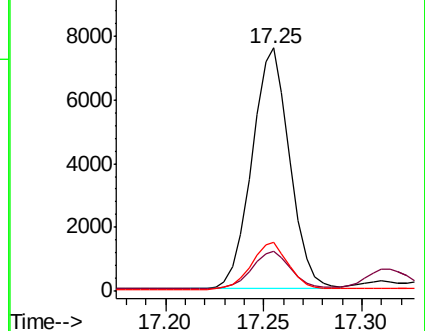

#17

Pyrene

Concen: 0.041 ng/ul m

RT: 19.63 min Scan# 4255

Delta R.T. -0.00 min

Lab File: BN003759.D

Acq: 07 Dec 2018 10:45


Tgt Ion:202 Resp: 3561

Ion Ratio Lower Upper

202 100

101 16.1 10.3 15.5#

100 14.3 8.5 12.7#

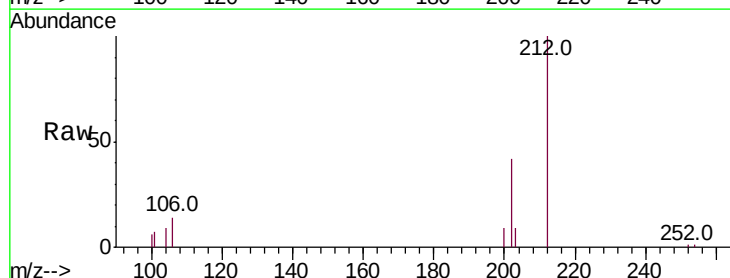

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

