
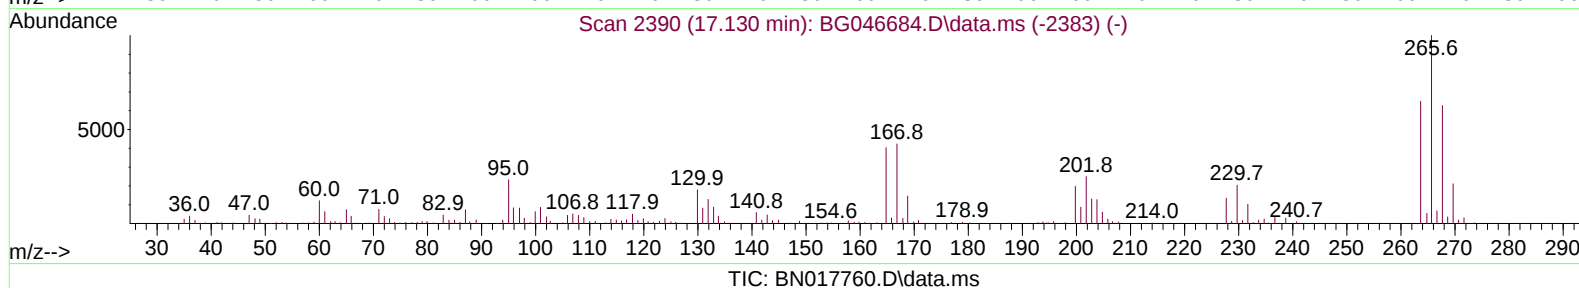
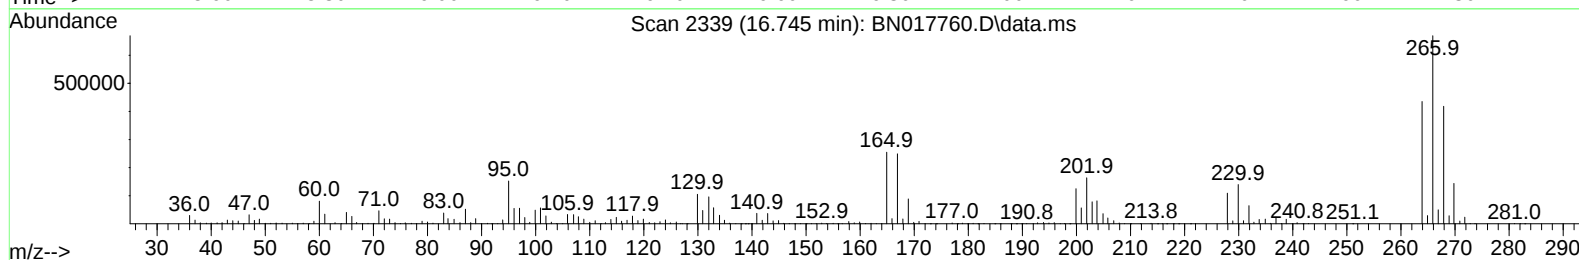


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120721\
Data File : BN017760.D
Acq On : 07 Dec 2021 12:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 09:39:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 08 09:39:40 2021
Response via : Initial Calibration

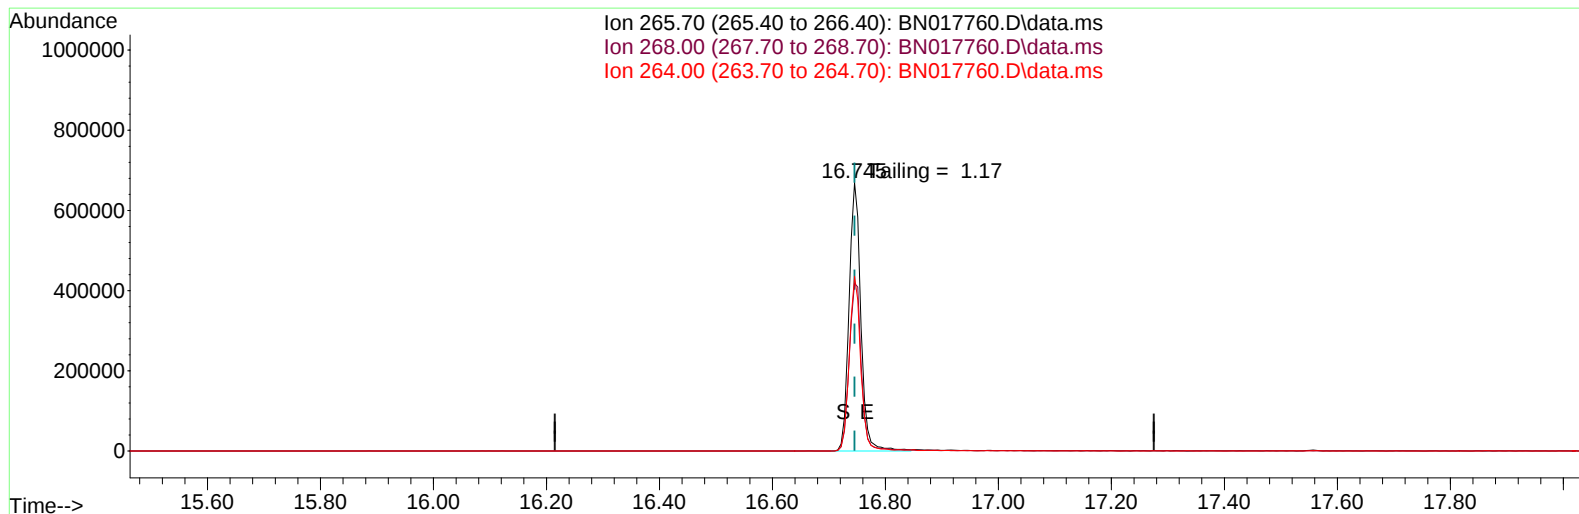

TIC: BN017760.D\data.ms

(70) Pentachlorophenol (C)




16.745min (0.000) 28865.90 ng

response 971597

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.50
264.00	61.60	65.03
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120721\  
Data File : BN017760.D  
Acq On    : 07 Dec 2021  12:11  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 08 09:39:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 08 09:39:40 2021
Response via : Initial Calibration

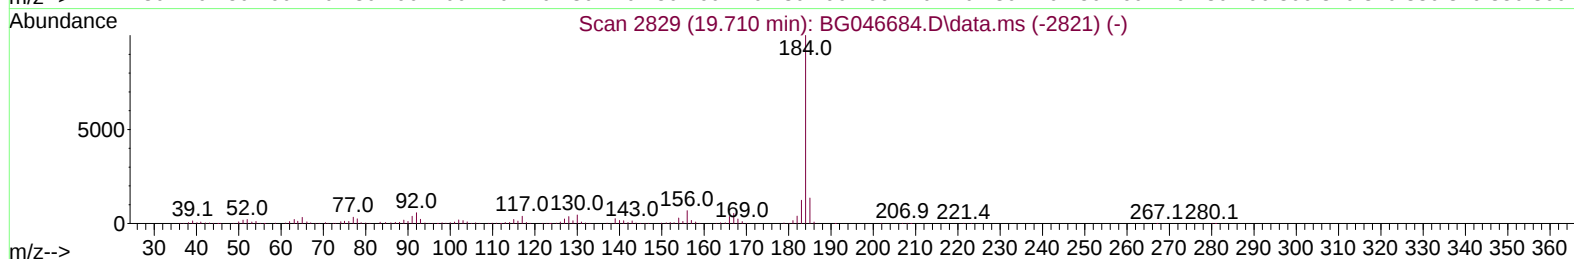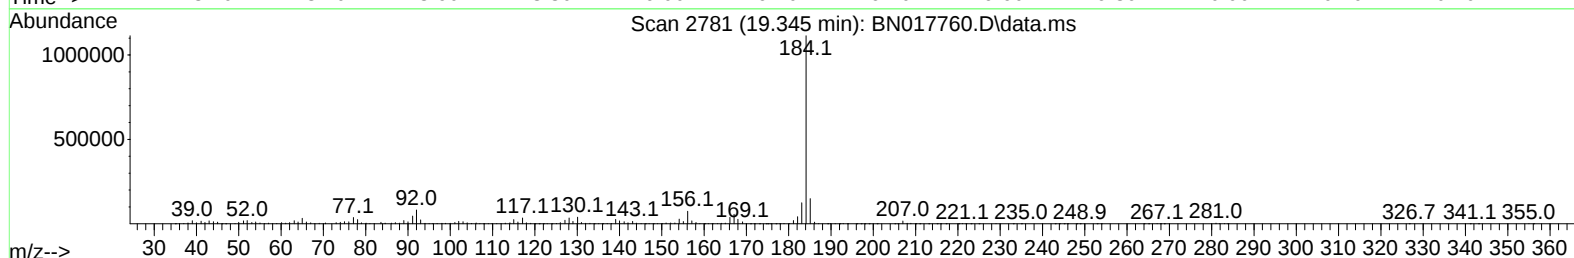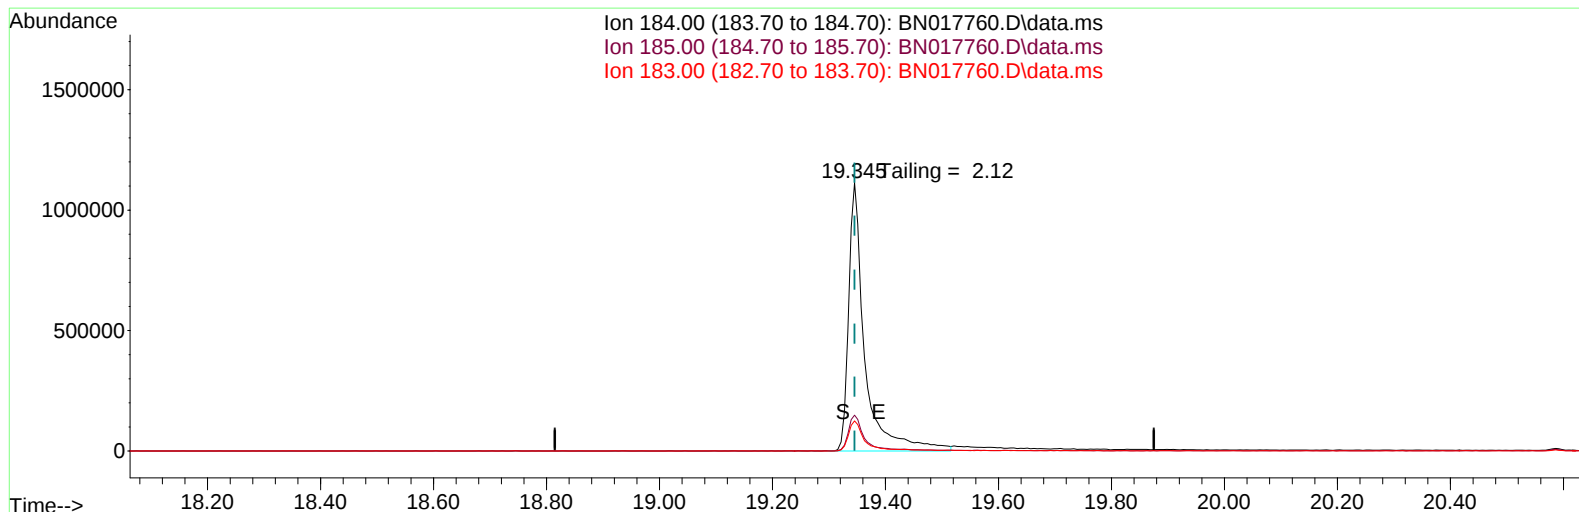

TIC: BN017760.D\data.ms

(77) Benzidine

19.345min (0.000) 348892.15 ng

response **2312267**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.50	13.39
--------	-------	-------

183.00	13.20	11.20
--------	-------	-------

0.00 0.00 0.00