
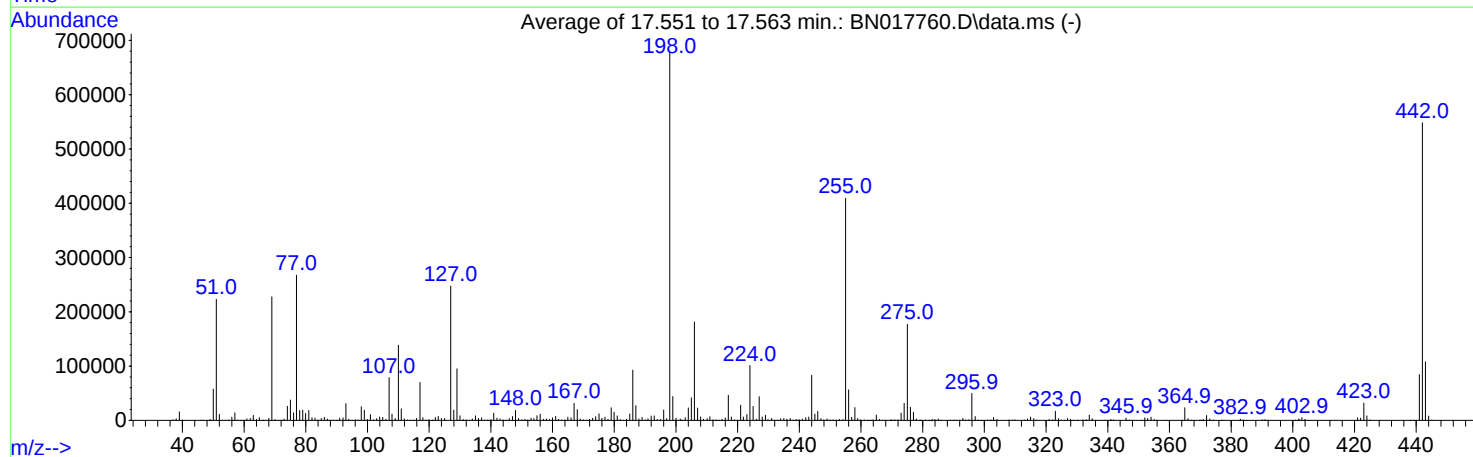


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120721\
 Data File : BN017760.D
 Acq On : 07 Dec 2021 12:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 08 01:18:09 2021

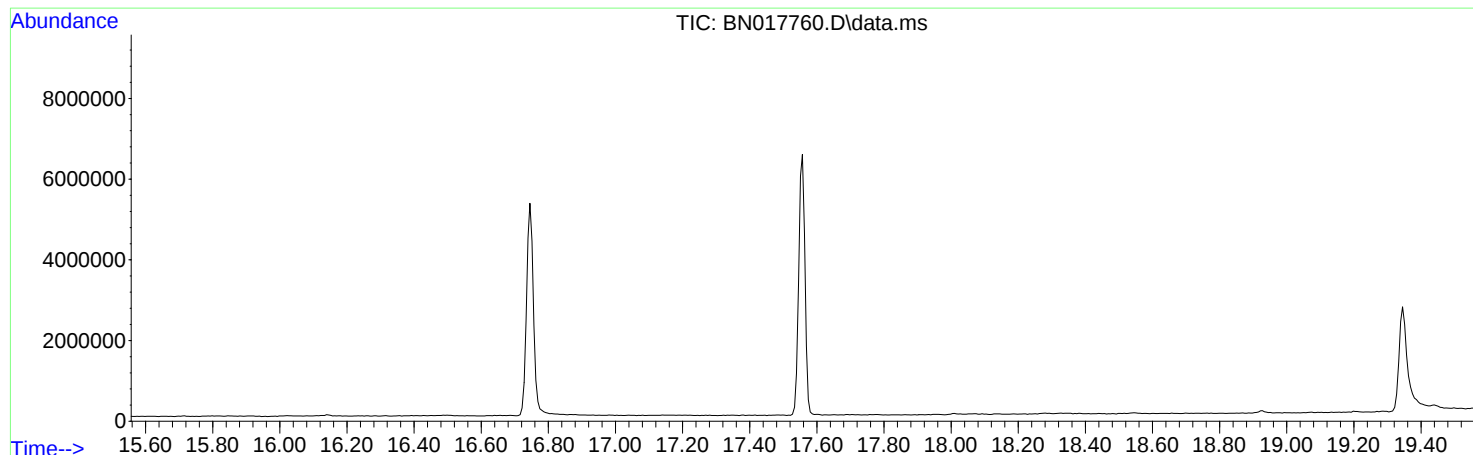




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	223295	PASS
68	69	0.00	2	1.7	3969	PASS
69	198	0.00	100	33.6	227509	PASS
70	69	0.00	2	0.6	1438	PASS
127	198	10	80	36.5	247381	PASS
197	198	0.00	2	0.5	3179	PASS
198	198	100	100	100.0	677717	PASS
199	198	5	9	6.5	43952	PASS
275	198	10	60	26.1	177003	PASS
365	198	1	100	3.4	23371	PASS
441	198	0.01	100	12.5	84400	PASS
442	442	50	100	100.0	548181	PASS
443	442	15	24	19.7	108061	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120721\
 Data File : BN017760.D
 Acq On : 07 Dec 2021 12:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 08 09:39:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 08 09:39:40 2021
 Response via : Initial Calibration

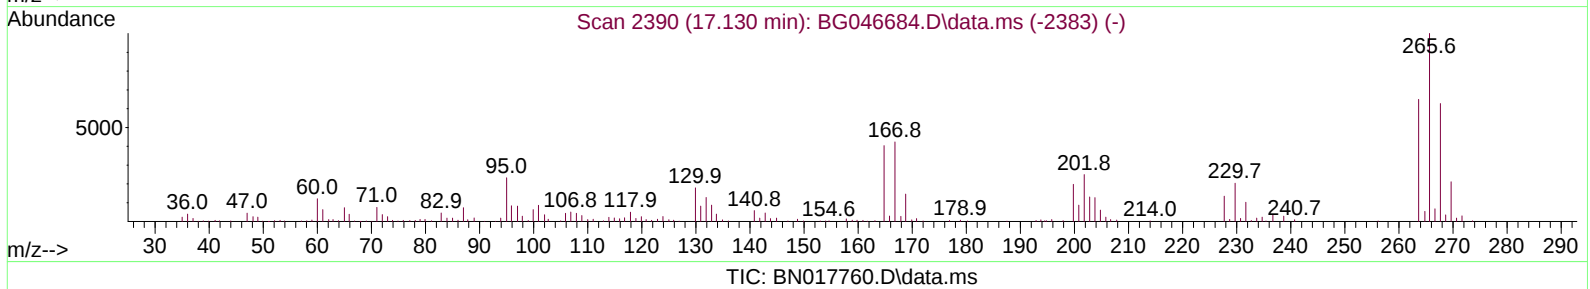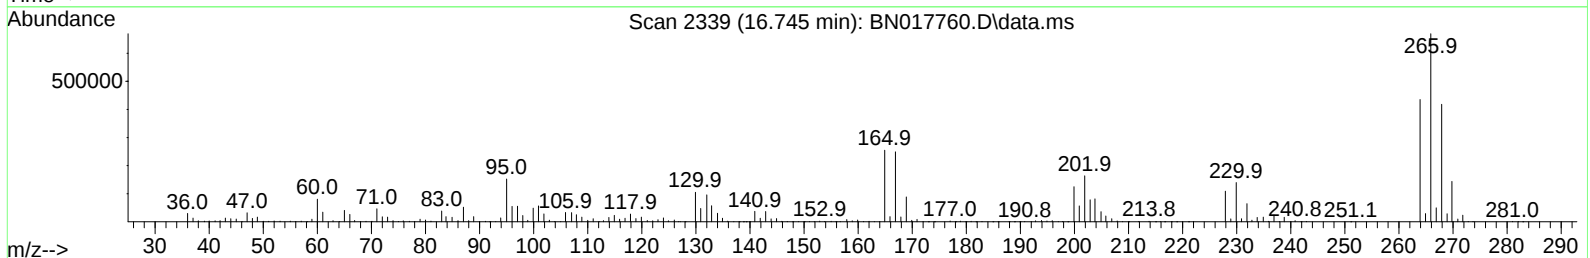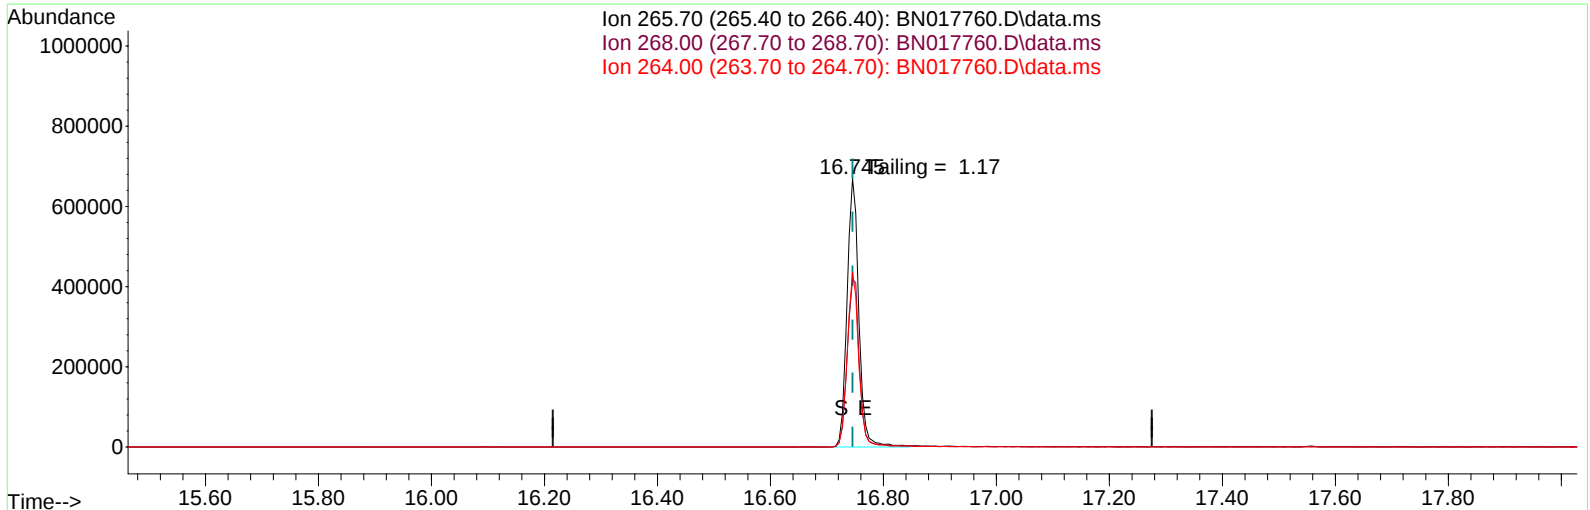

(70) Pentachlorophenol (C)

16.745min (0.000) 28865.90 ng




response 971597

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.50
264.00	61.60	65.03
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120721\  
Data File : BN017760.D  
Acq On    : 07 Dec 2021  12:11  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 08 09:39:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 08 09:39:40 2021
Response via : Initial Calibration

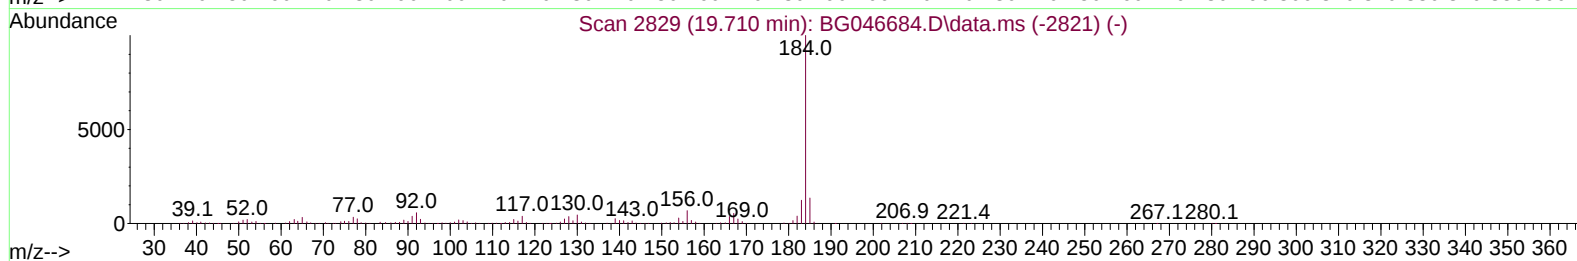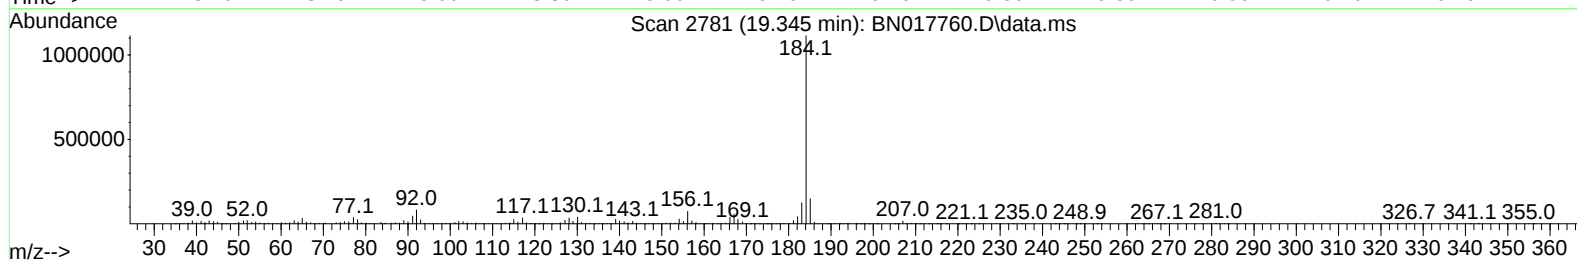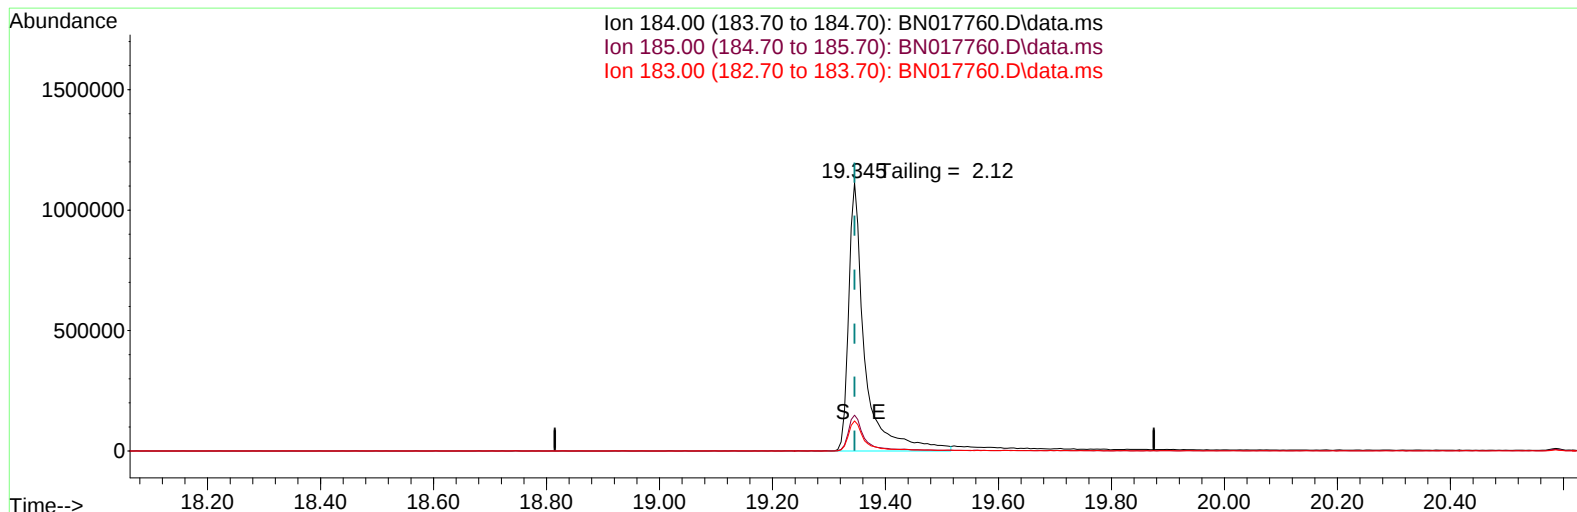

TIC: BN017760.D\data.ms

(77) Benzidine

19.345min (0.000) 348892.15 ng

response **2312267**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.50	13.39
--------	-------	-------

183.00	13.20	11.20
--------	-------	-------

0.00 0.00 0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/7/2021	BNA_N	<u>BN017760.D</u>
Compound Name	Response	Retention Time
DDT	2001388	20.586
DDD	39299	20.145
DDE	4137	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43436	2044824	2.12

Instrument :
BNA_N
ClientSampleId :
DFTPP