
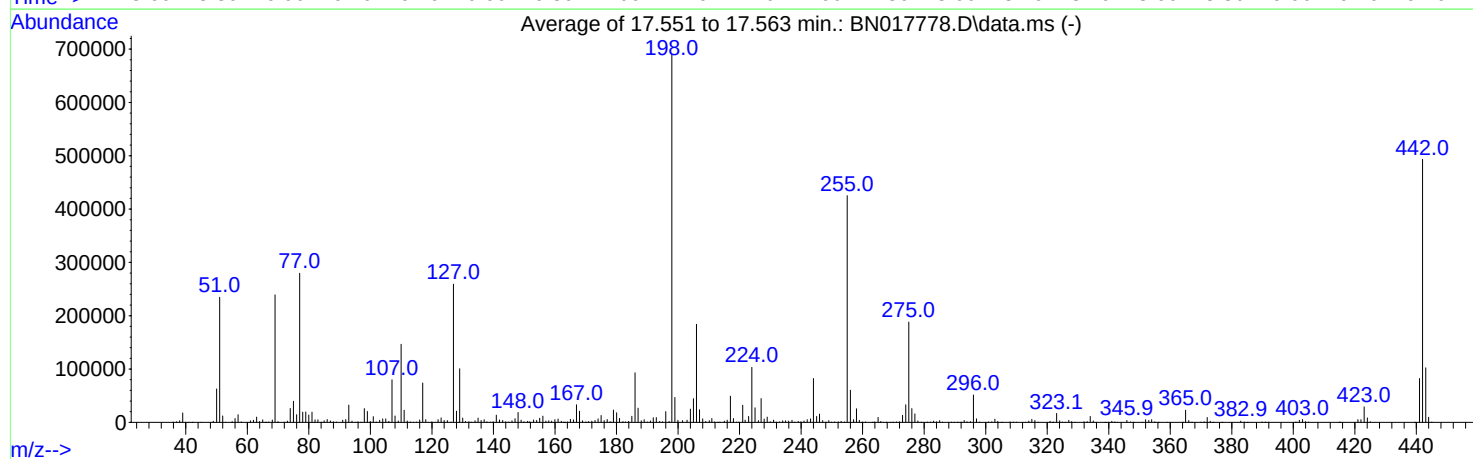


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120721\
 Data File : BN017778.D
 Acq On : 08 Dec 2021 00:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 08 01:18:09 2021

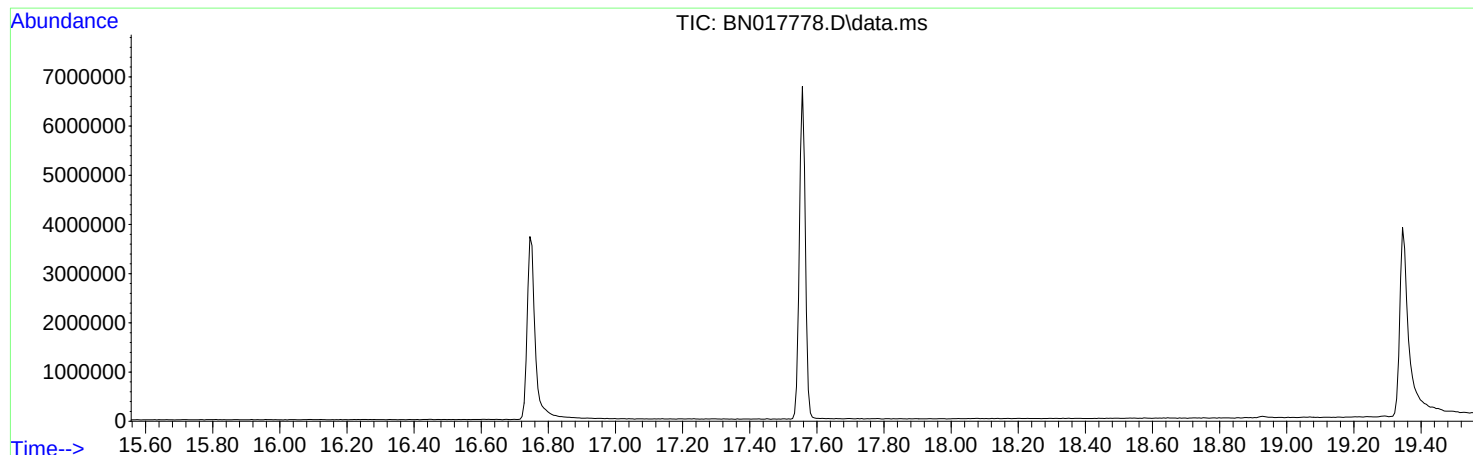




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	234562	PASS
68	69	0.00	2	1.9	4510	PASS
69	198	0.00	100	34.7	239099	PASS
70	69	0.00	2	0.4	973	PASS
127	198	10	80	37.6	259307	PASS
197	198	0.00	2	0.3	1800	PASS
198	198	100	100	100.0	689899	PASS
199	198	5	9	6.8	46883	PASS
275	198	10	60	27.3	188203	PASS
365	198	1	100	3.3	22837	PASS
441	198	0.01	100	11.9	82355	PASS
442	442	50	100	100.0	493269	PASS
443	442	15	24	20.8	102408	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120721\
 Data File : BN017778.D
 Acq On : 08 Dec 2021 00:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 08 09:41:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 08 09:39:40 2021
 Response via : Initial Calibration

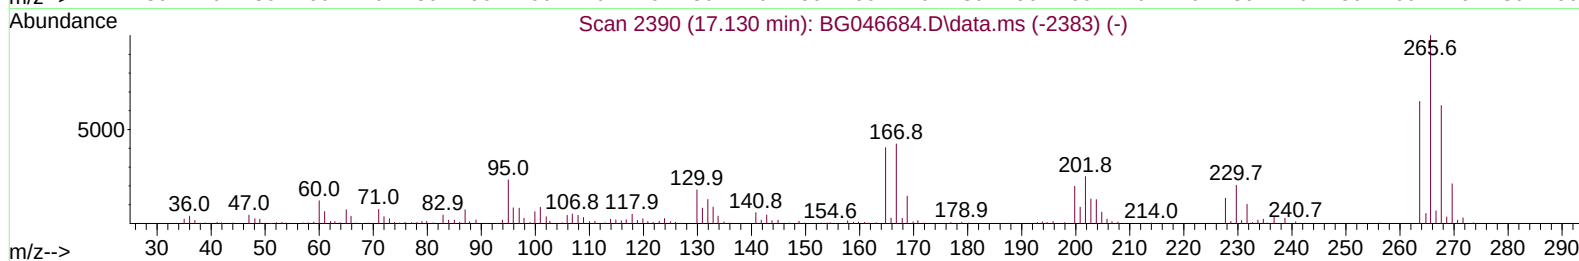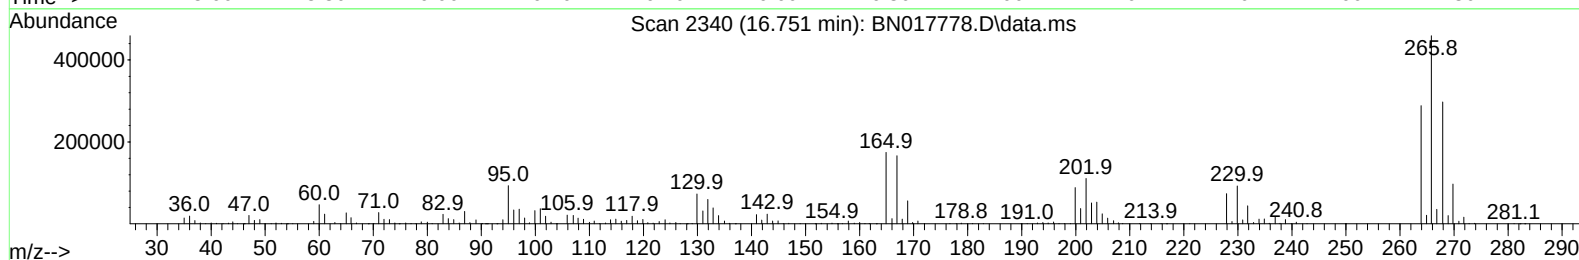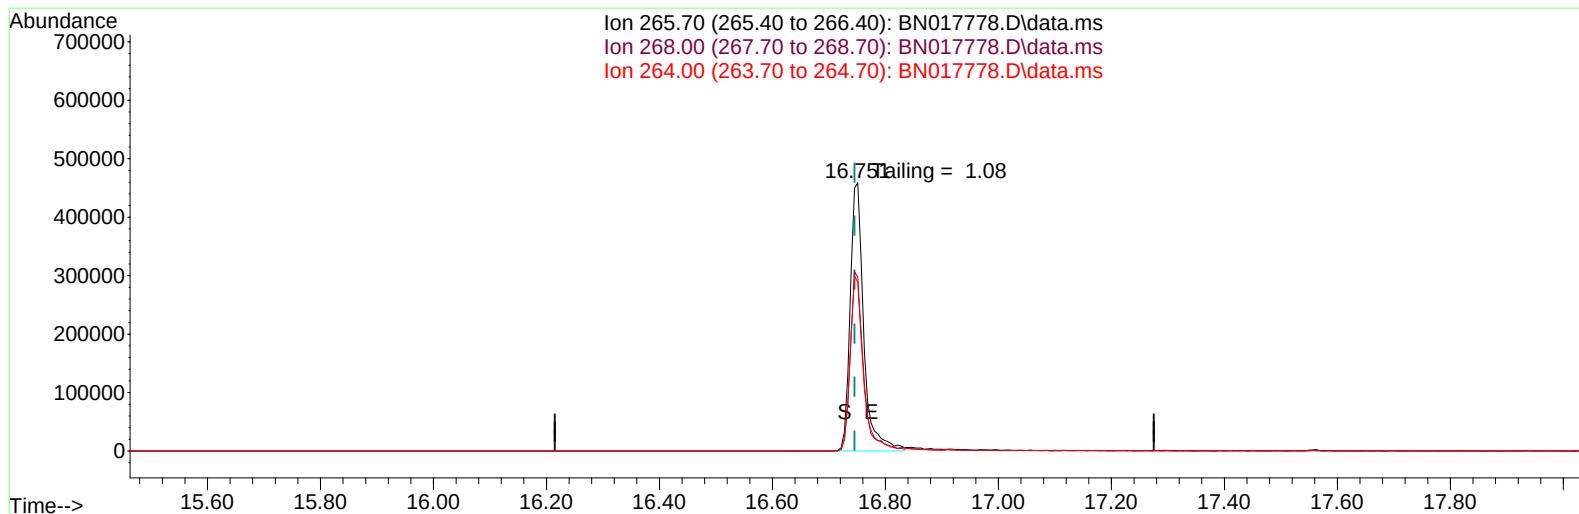

TIC: BN017778.D\data.ms

(70) Pentachlorophenol (C)

16.751min (+ 0.006) 24674.53 ng




response 782110

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.80
264.00	61.60	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120721\
 Data File : BN017778.D
 Acq On : 08 Dec 2021 00:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 08 09:41:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 08 09:39:40 2021
 Response via : Initial Calibration

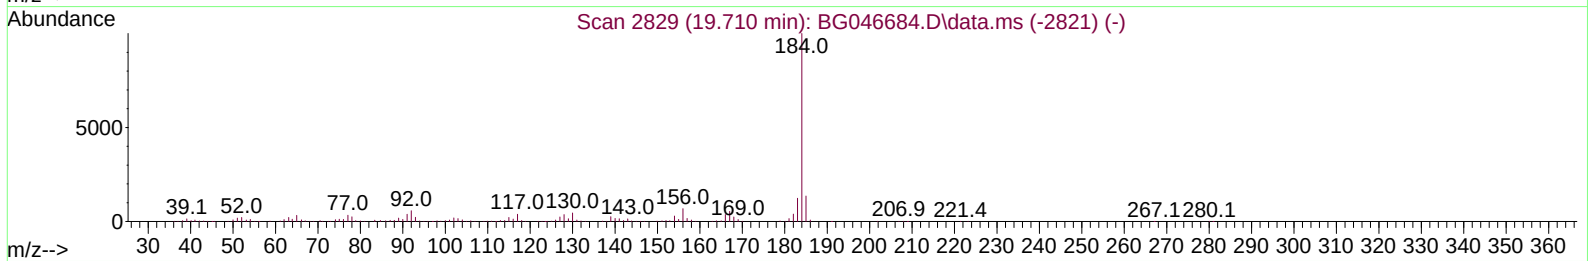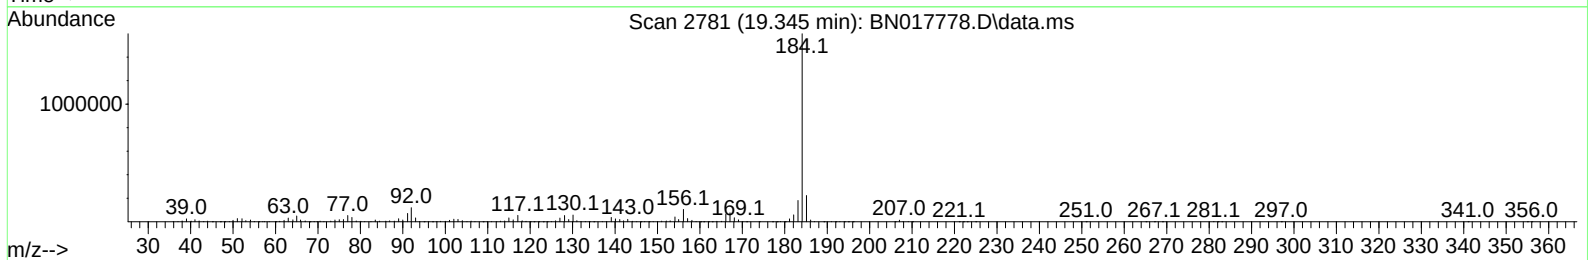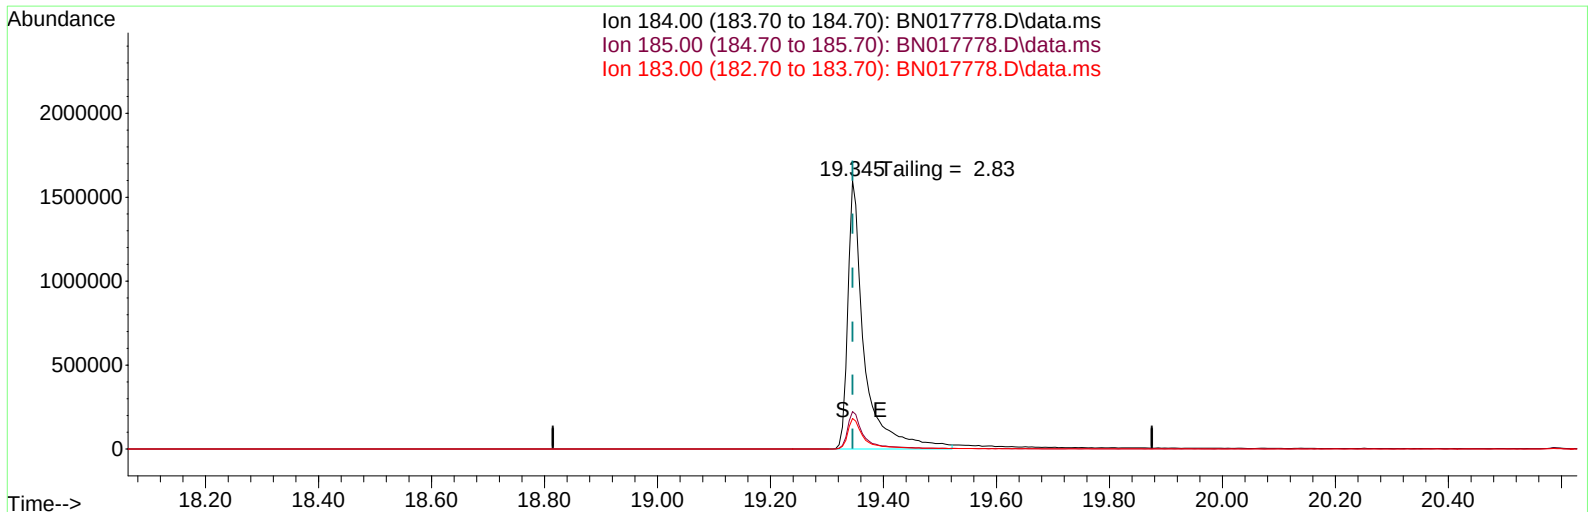

TIC: BN017778.D\data.ms

(77) Benzidine**19.345min (+ 0.000) 454847.27 ng****response 3336959**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	11.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/7/2021	BNA_N	<u>BN017778.D</u>
Compound Name	Response	Retention Time
DDT	1701522	20.586
DDD	57923	20.157
DDE	4501	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
62424	1763946	3.54

Instrument :
BNA_N
ClientSampleId :
DFTPP