
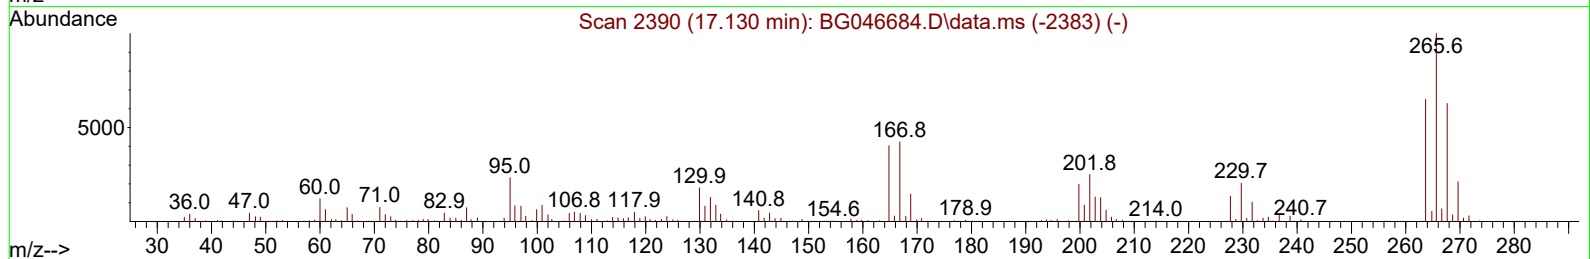
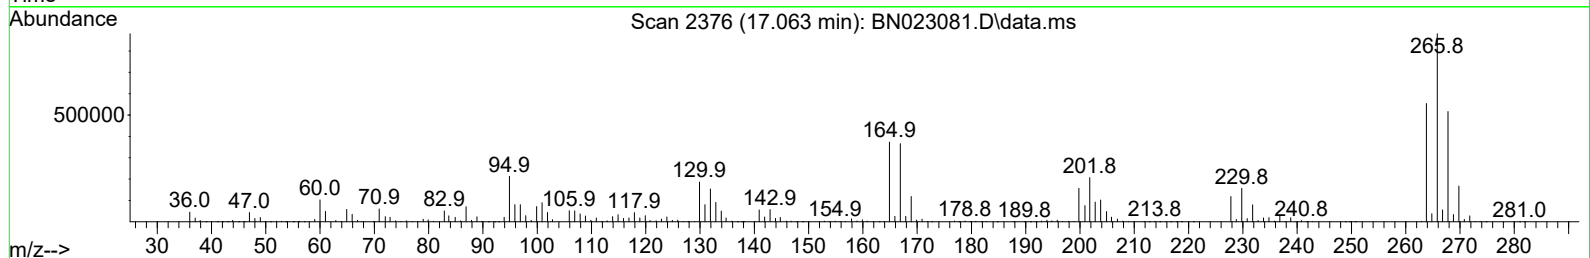


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120722\
Data File : BN023081.D
Acq On : 07 Dec 2022 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 06:43:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 08 06:43:23 2022
Response via : Initial Calibration

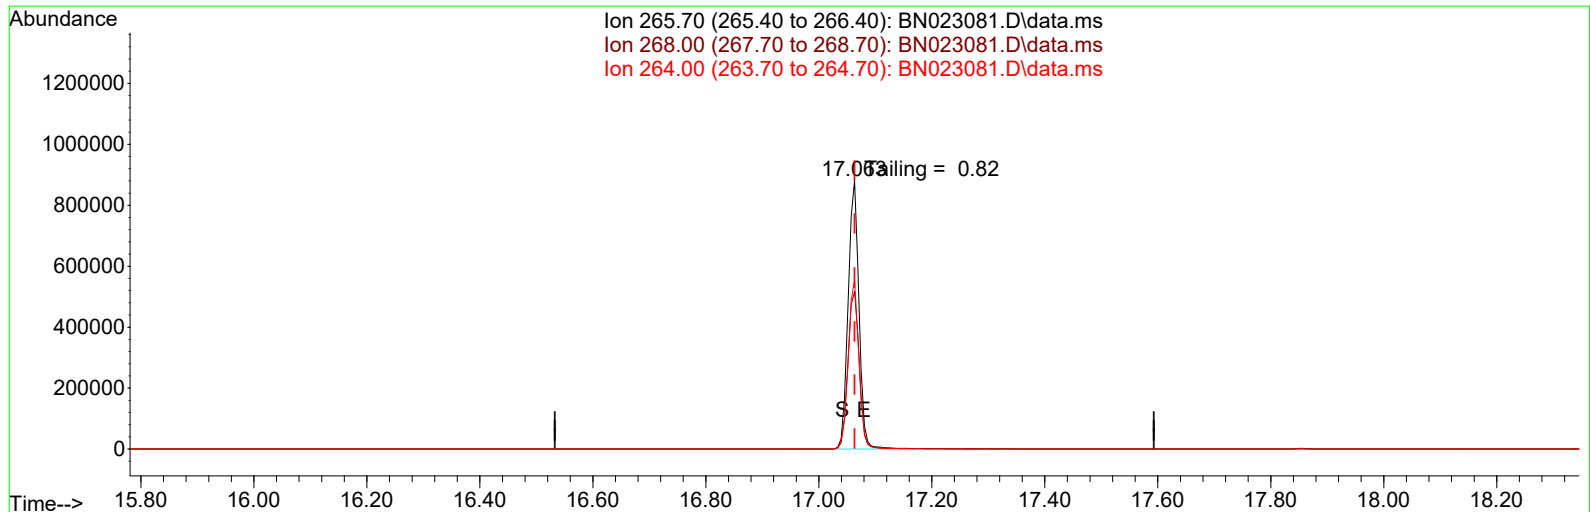

TIC: BN023081.D\data.ms

(70) Pentachlorophenol (C)




17.063min (0.000) 23435.33 ng

response 1177973

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.67
264.00	61.60	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120722\
Data File : BN023081.D
Acq On : 07 Dec 2022 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 06:43:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 08 06:43:23 2022
Response via : Initial Calibration

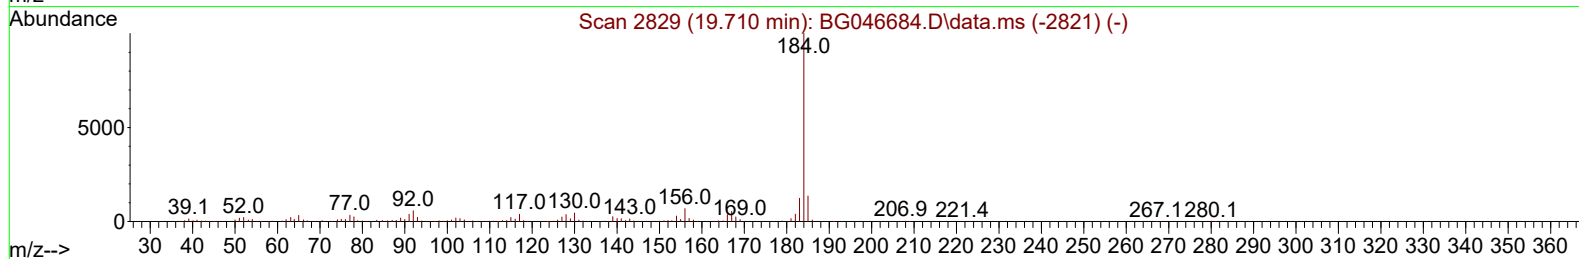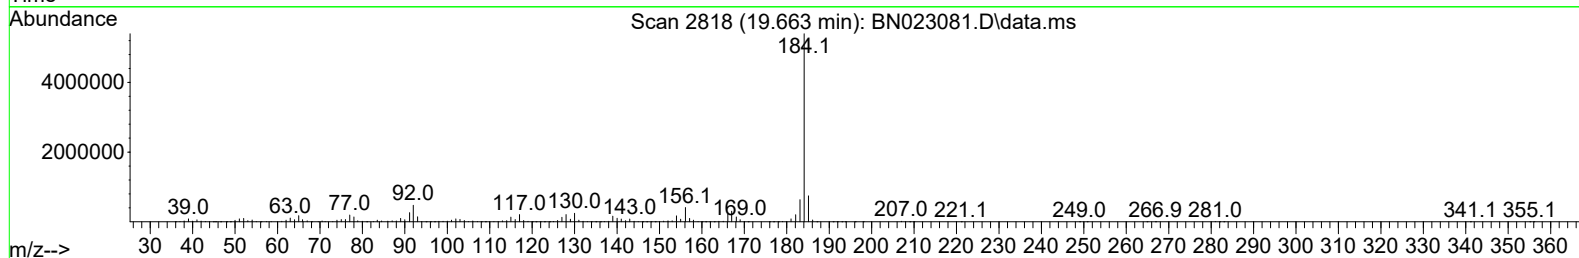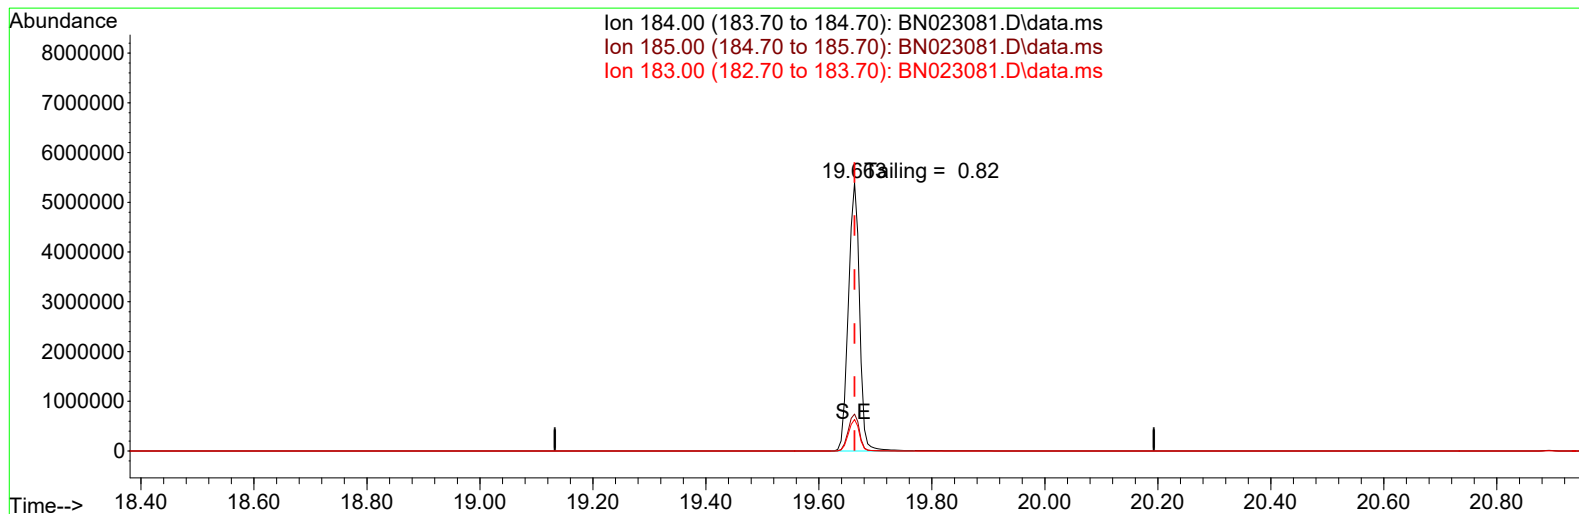

TIC: BN023081.D\data.ms

(77) Benzidine

19.663min (0.000) 0.00 ng

response 7434389

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.80
183.00	13.20	11.74
0.00	0.00	0.00