
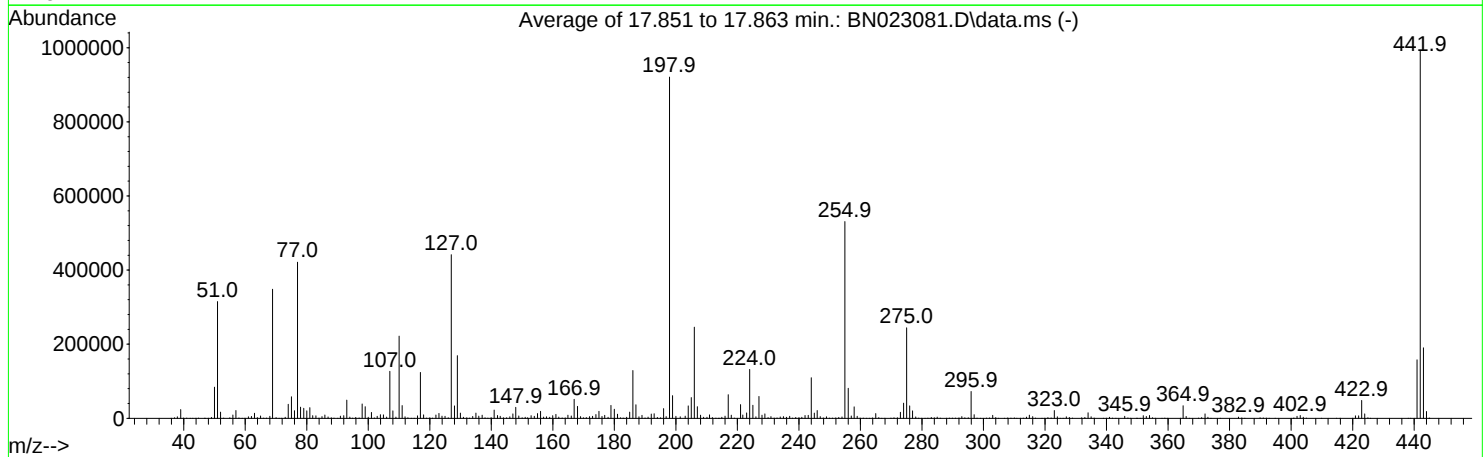


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120722\
 Data File : BN023081.D
 Acq On : 07 Dec 2022 10:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 08 02:58:10 2022

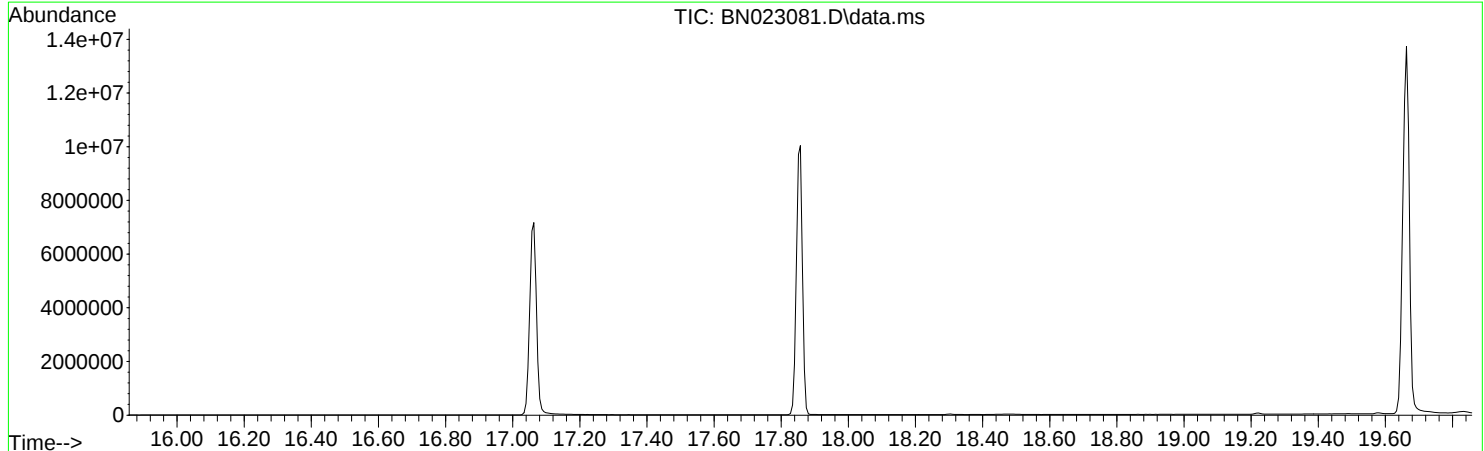




AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	314965	PASS
68	69	0.00	2	1.6	5568	PASS
69	198	0.00	100	37.8	348117	PASS
70	69	0.00	2	0.5	1868	PASS
127	198	10	80	48.0	441643	PASS
197	198	0.00	2	0.5	4612	PASS
198	198	100	100	100.0	920875	PASS
199	198	5	9	6.6	61136	PASS
275	198	10	60	26.5	244117	PASS
365	198	1	100	3.7	33752	PASS
441	198	0.01	100	17.1	157787	PASS
442	442	50	100	100.0	992768	PASS
443	442	15	24	19.2	190400	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120722\
Data File : BN023081.D
Acq On : 07 Dec 2022 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 08 06:43:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 08 06:43:23 2022
Response via : Initial Calibration

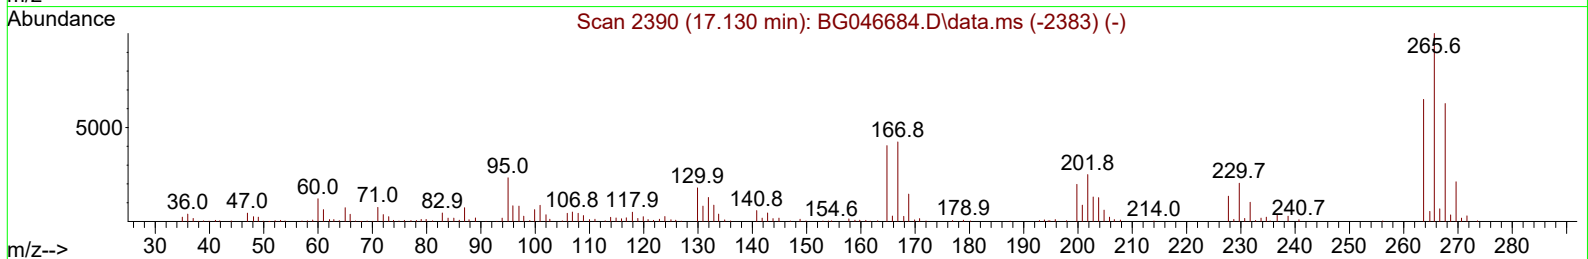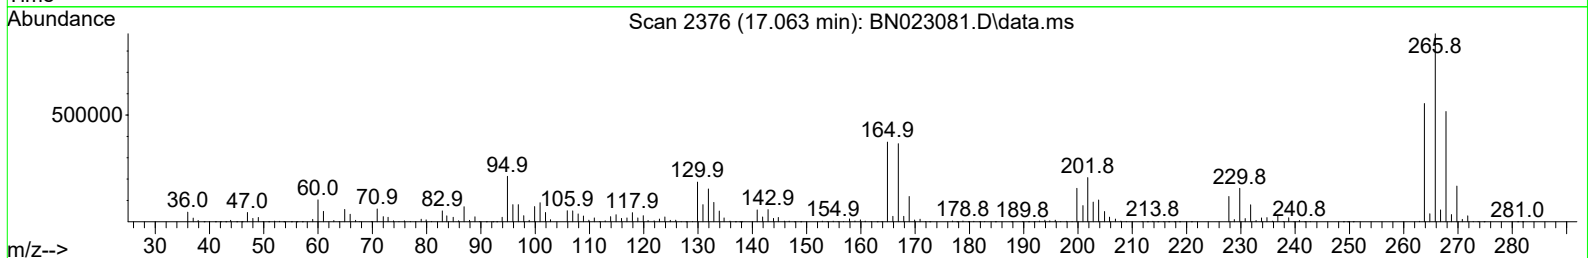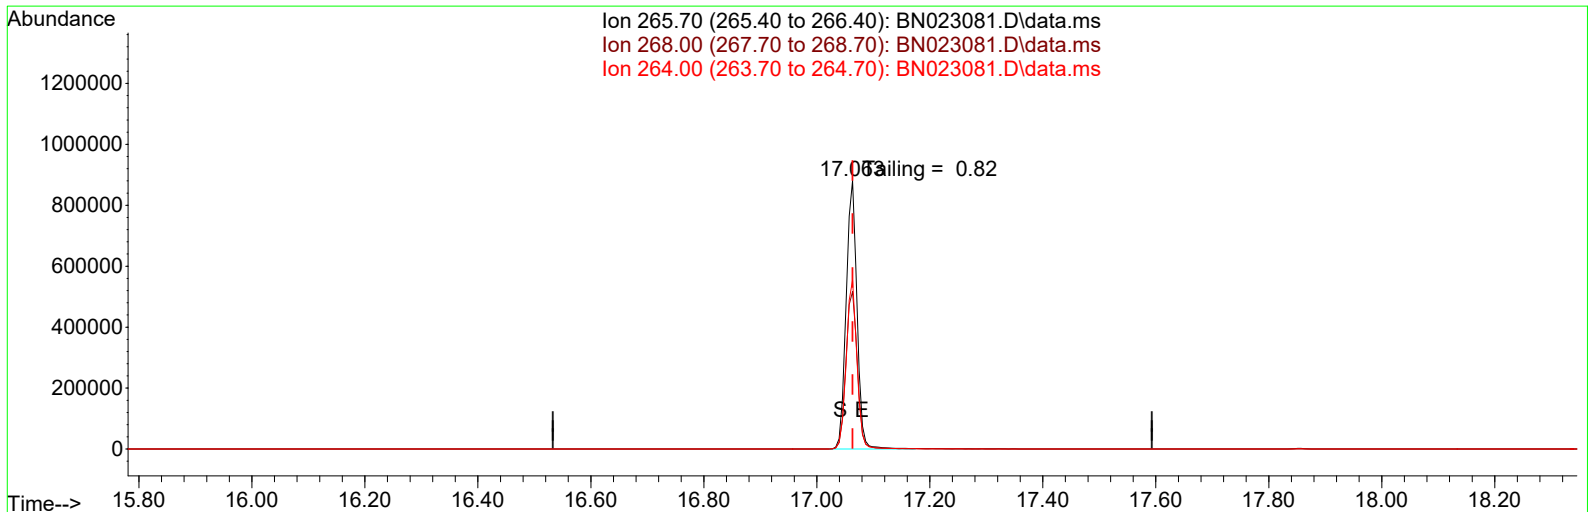

TIC: BN023081.D\data.ms

(70) Pentachlorophenol (C)

17.063min (0.000) 23435.33 ng




response 1177973

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.67
264.00	61.60	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120722\
Data File : BN023081.D
Acq On : 07 Dec 2022 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 08 06:43:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 08 06:43:23 2022
Response via : Initial Calibration

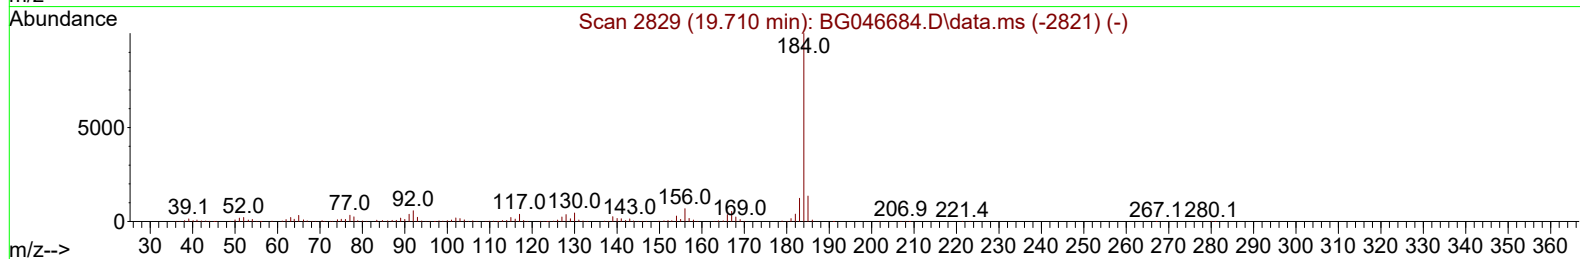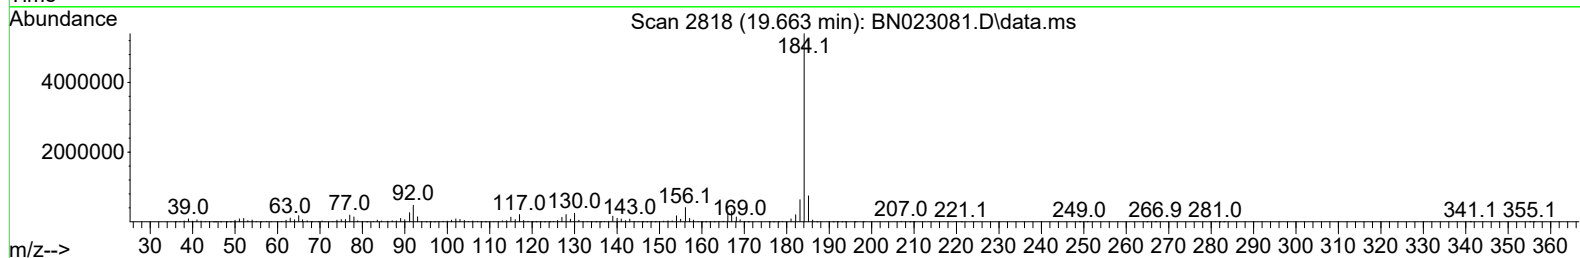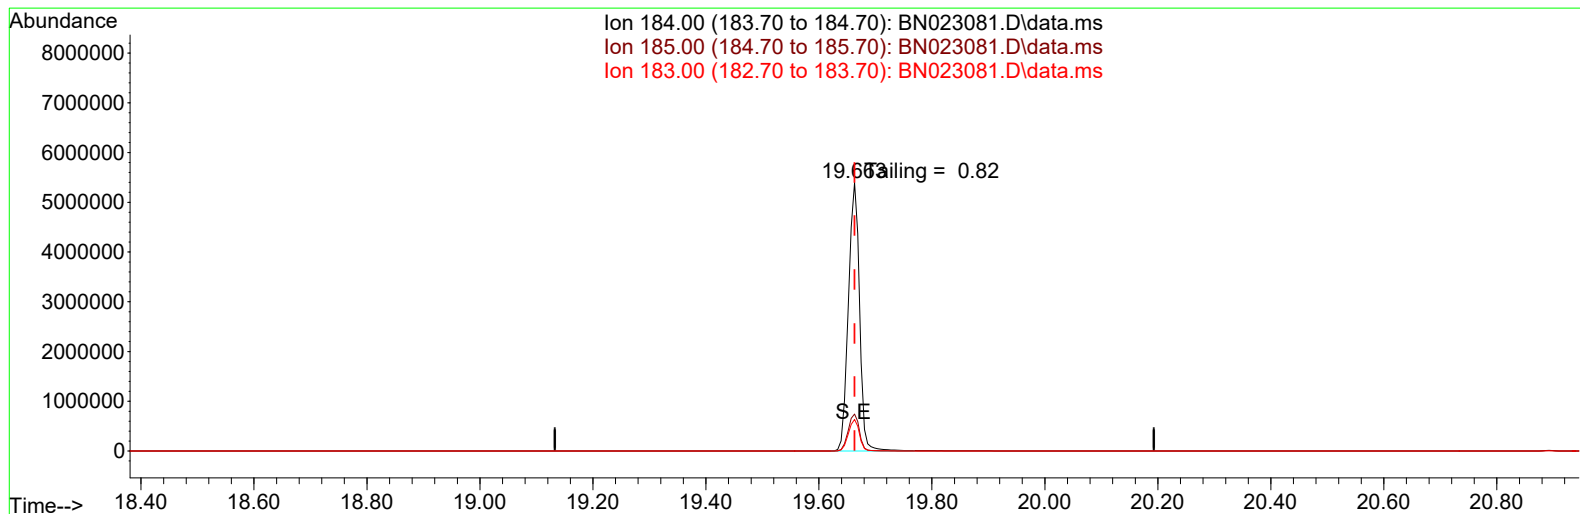

TIC: BN023081.D\data.ms

(77) Benzidine

19.663min (0.000) 0.00 ng

response 7434389

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.80
183.00	13.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/7/2022	BNA_N	<u>BN023081.D</u>
Compound Name	Response	Retention Time
DDT	3013868	20.892
DDD	23851	20.504
DDE	165	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24016	3037884	0.79

Instrument :
BNA_N
ClientSampleId :
DFTPP