

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120821\
 Data File : BN017798.D
 Acq On : 08 Dec 2021 14:03
 Operator : CG/JU
 Sample : PB141179BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB141179BL

Quant Time: Dec 09 11:03:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 08 01:18:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.715	152	21032	0.400	ng	0.00
7) Naphthalene-d8	10.507	136	75824	0.400	ng	0.01
13) Acenaphthene-d10	14.347	164	52098	0.400	ng	0.00
19) Phenanthrene-d10	17.105	188	102266	0.400	ng	# 0.01
29) Chrysene-d12	21.304	240	107299	0.400	ng	# 0.02
35) Perylene-d12	23.596	264	89712	0.400	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.345	112	14535	0.286	ng	0.02
5) Phenol-d6	6.913	99	10281	0.214	ng	0.00
8) Nitrobenzene-d5	8.859	82	15484	0.307	ng	0.00
11) 2-Methylnaphthalene-d10	12.103	152	39075	0.258	ng	0.01
14) 2,4,6-Tribromophenol	15.870	330	2634	0.097	ng	0.03
15) 2-Fluorobiphenyl	12.977	172	45749	0.240	ng	0.01
27) Fluoranthene-d10	19.134	212	103557	0.303	ng	0.00
31) Terphenyl-d14	19.745	244	82694	0.359	ng	0.00
Target Compounds						
20) 4,6-Dinitro-2-methylph...	15.502	198	9	0.089	ng	# 33
24) Pentachlorophenol	16.800	266	23	0.281	ng	# 27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120821\
Data File : BN017798.D
Acq On : 08 Dec 2021 14:03
Operator : CG/JU
Sample : PB141179BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB141179BL

Quant Time: Dec 09 11:03:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 08 01:18:09 2021
Response via : Initial Calibration




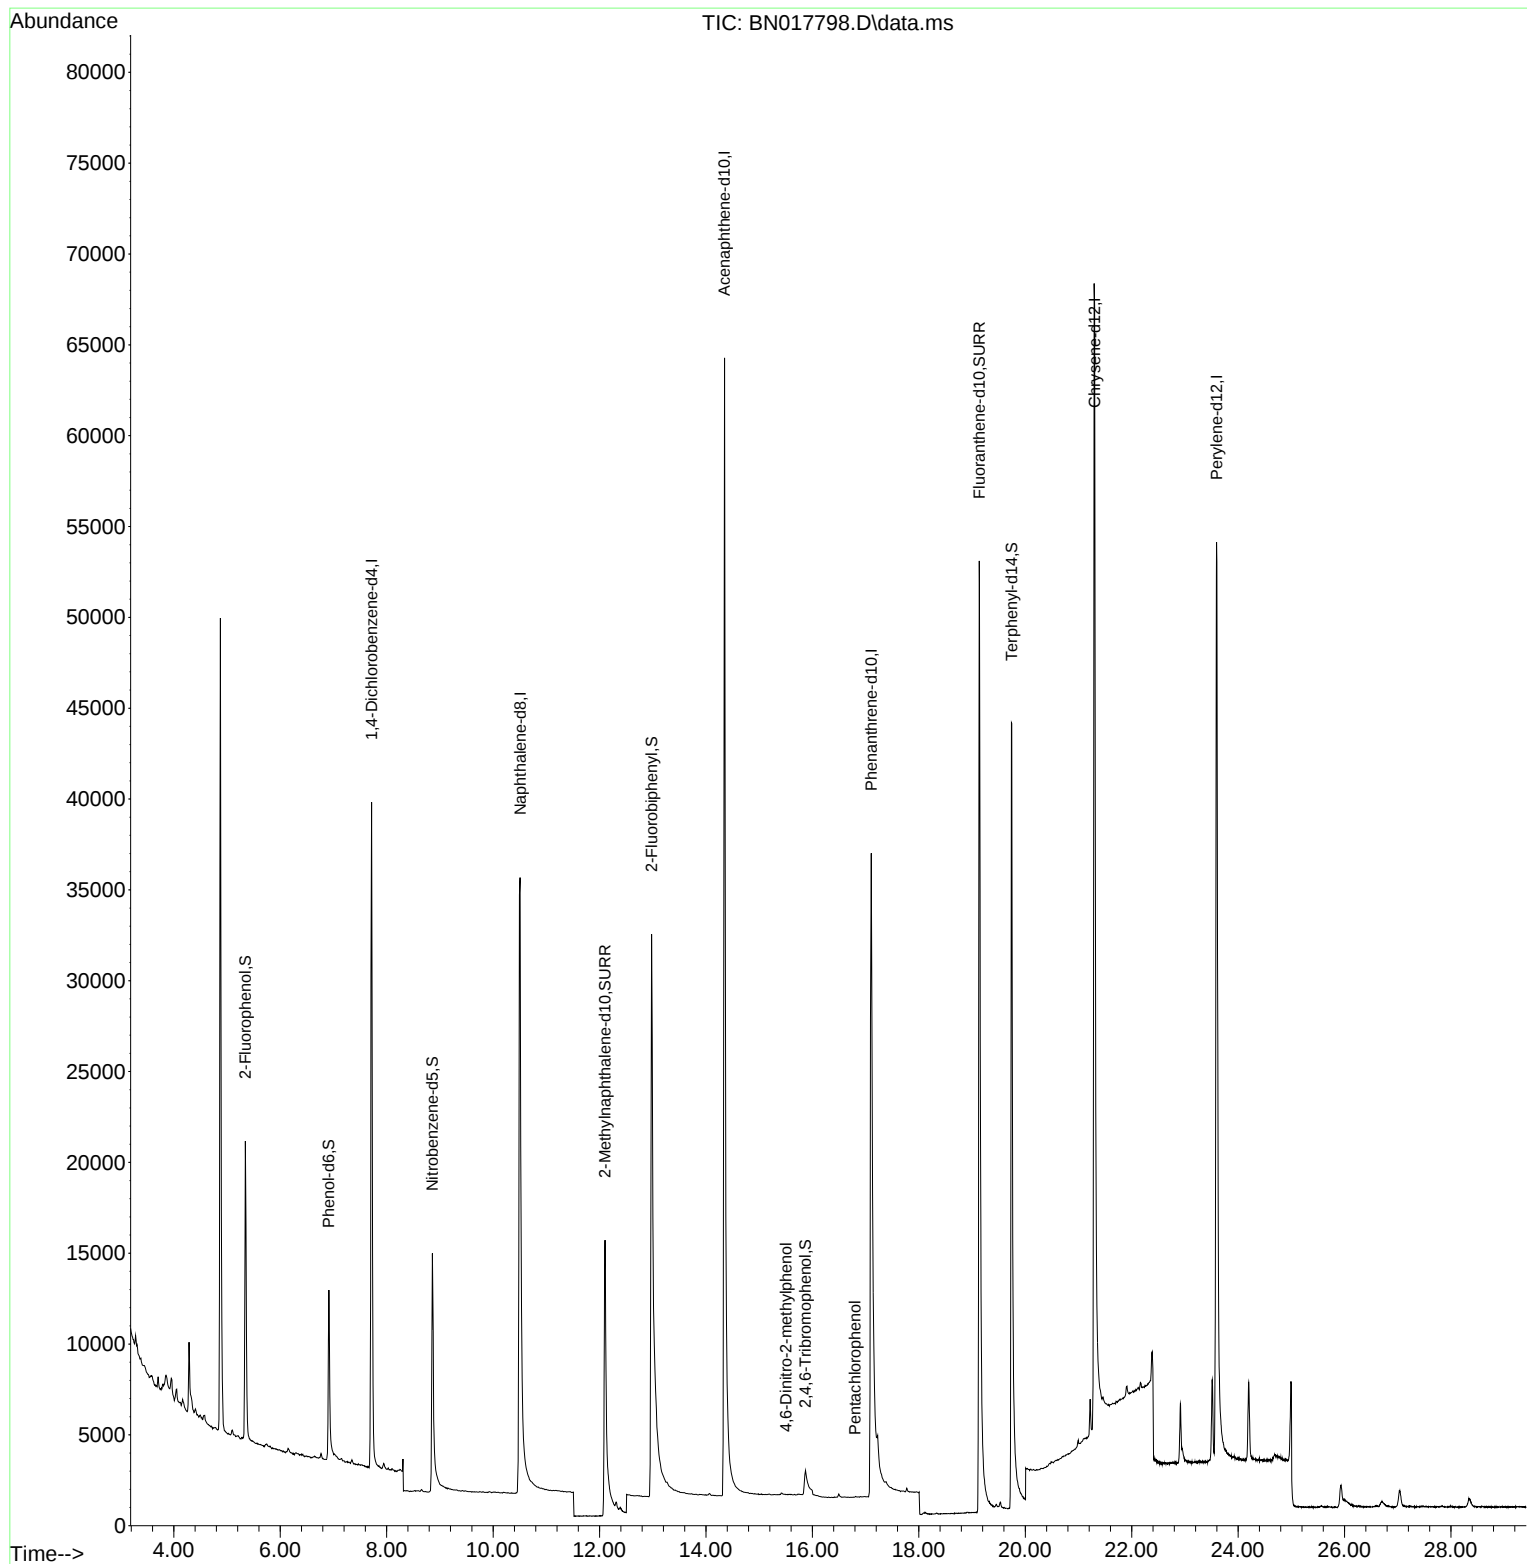


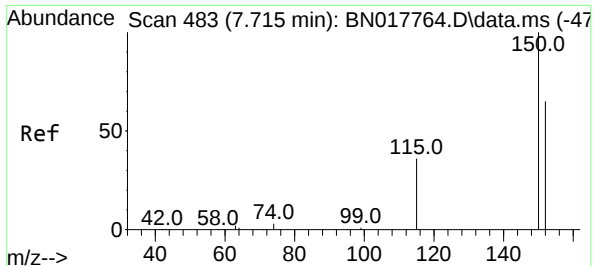

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.715 min Scan# 483
 Delta R.T. -0.000 min
 Lab File: BN017798.D
 Acq: 08 Dec 2021 14:03




Instrument :
 BNA_N
 ClientSampleId :
 PB141179BL


Tgt Ion:152 Resp: 21032
 Ion Ratio Lower Upper
 152 100
 150 154.9 123.0 184.4
 115 57.4 45.3 67.9

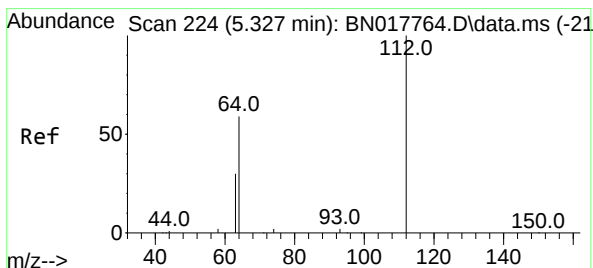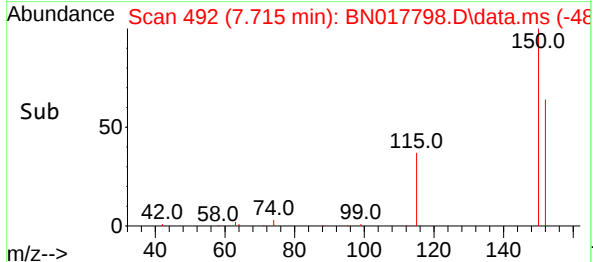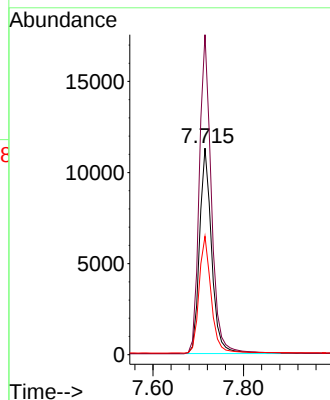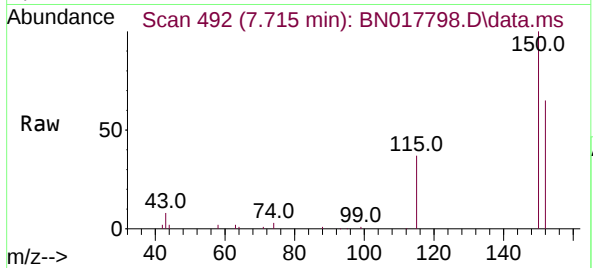

#4
 2-Fluorophenol
 Concen: 0.286 ng
 RT: 5.345 min Scan# 235
 Delta R.T. 0.018 min
 Lab File: BN017798.D
 Acq: 08 Dec 2021 14:03

Tgt Ion:112 Resp: 14535
 Ion Ratio Lower Upper
 112 100
 64 61.6 49.3 73.9
 63 33.5 25.8 38.8


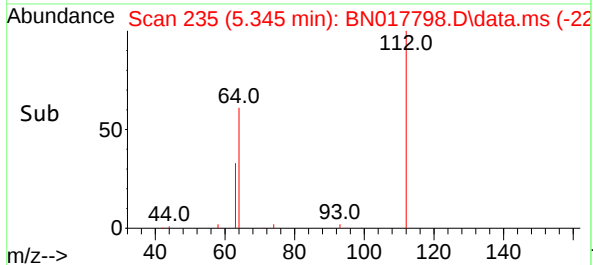
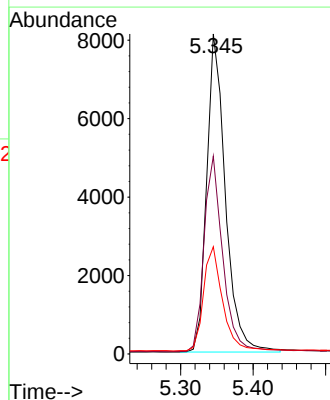
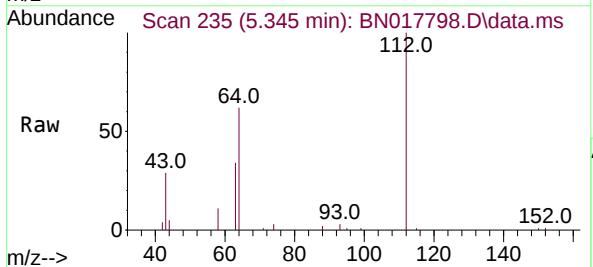


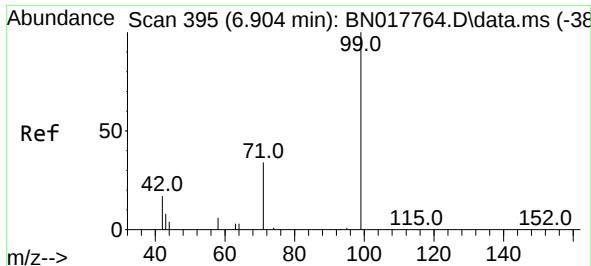

#5
Phenol-d6
Concen: 0.214 ng
RT: 6.913 min Scan# 40
Delta R.T. 0.009 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03




Instrument :
BNA_N
ClientSampleId :
PB141179BL


Tgt Ion: 99 Resp: 10281
Ion Ratio Lower Upper
99 100
42 20.2 16.6 25.0
71 37.0 29.0 43.4

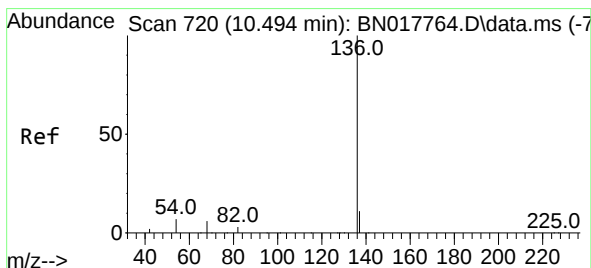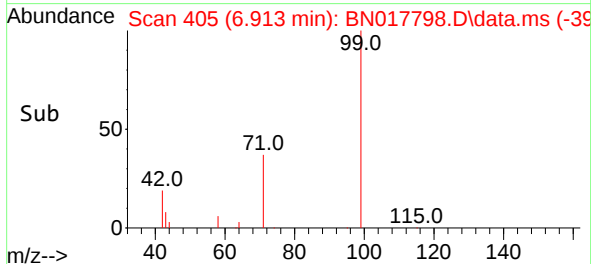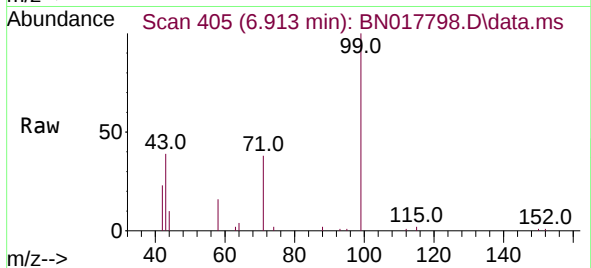

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.507 min Scan# 730
Delta R.T. 0.012 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03

Tgt Ion: 136 Resp: 75824
Ion Ratio Lower Upper
136 100
137 11.1 8.8 13.2
54 6.6 5.9 8.9
68 5.4 5.0 7.6


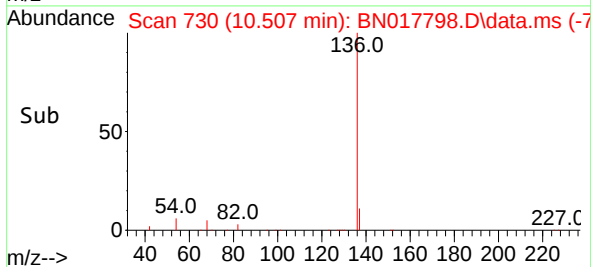

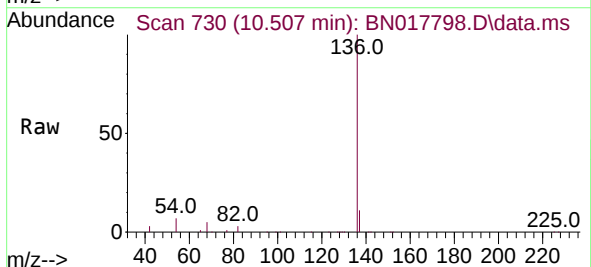


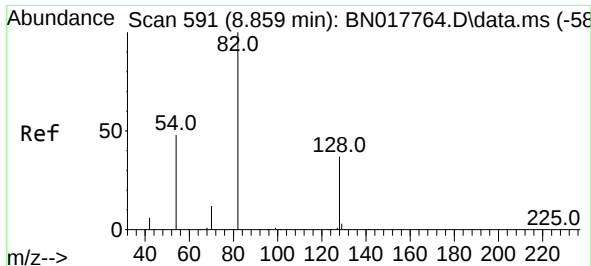

#8
Nitrobenzene-d5
Concen: 0.307 ng
RT: 8.859 min Scan# 60
Delta R.T. -0.000 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03




Instrument :
BNA_N
ClientSampleId :
PB141179BL


Tgt Ion: 82 Resp: 15484
Ion Ratio Lower Upper
82 100
128 34.8 30.2 45.2
54 51.3 39.0 58.6

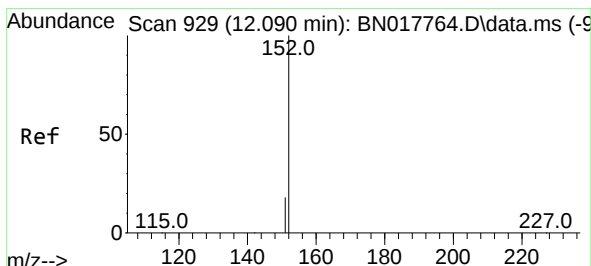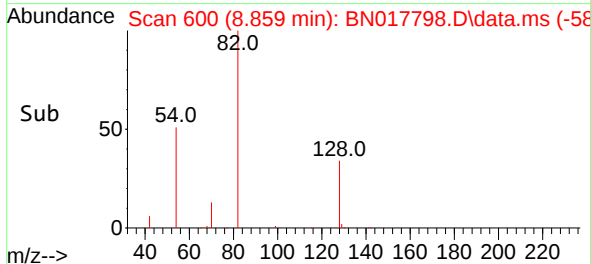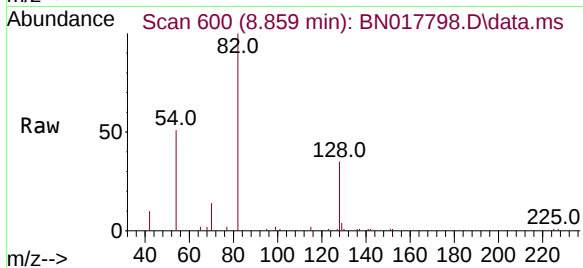

#11
2-Methylnaphthalene-d10
Concen: 0.258 ng
RT: 12.103 min Scan# 941
Delta R.T. 0.013 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03

Tgt Ion: 152 Resp: 39075
Ion Ratio Lower Upper
152 100
151 20.6 16.4 24.6


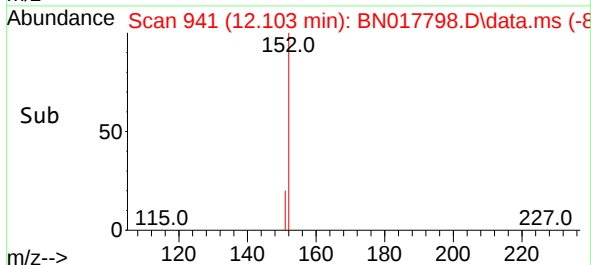

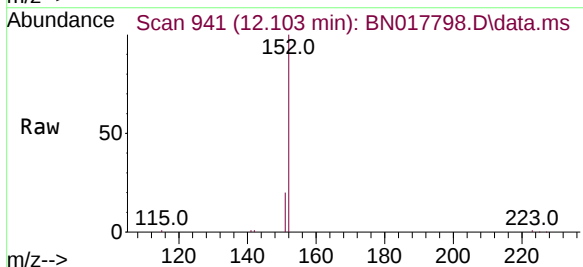


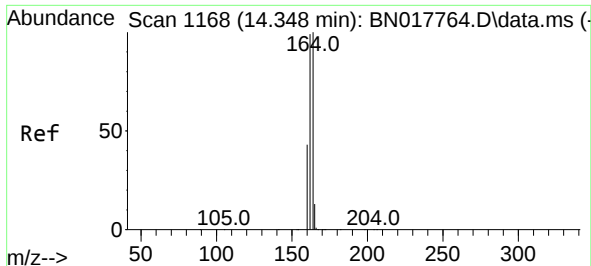

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.347 min Scan# 1168
Delta R.T. -0.000 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03




Instrument :
BNA_N
ClientSampleId :
PB141179BL


Tgt Ion:164 Resp: 52098
Ion Ratio Lower Upper
164 100
162 100.7 79.0 118.6
160 45.2 34.6 52.0

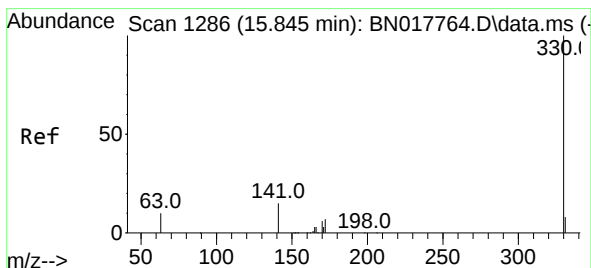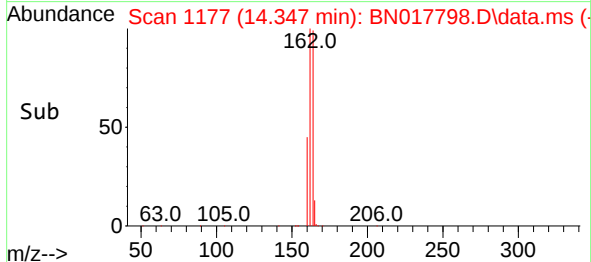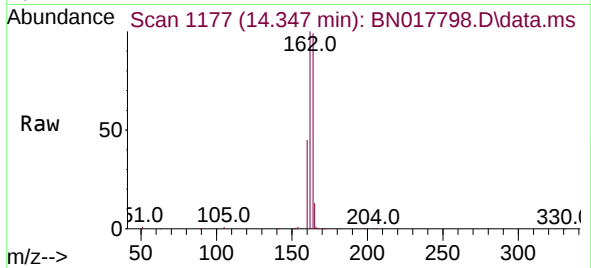

#14
2,4,6-Tribromophenol
Concen: 0.097 ng
RT: 15.870 min Scan# 1297
Delta R.T. 0.025 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03

Tgt Ion:330 Resp: 2634
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.5 21.5 32.3


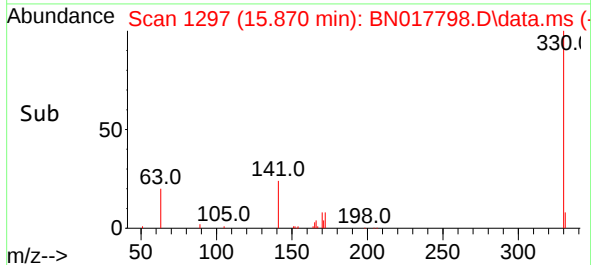

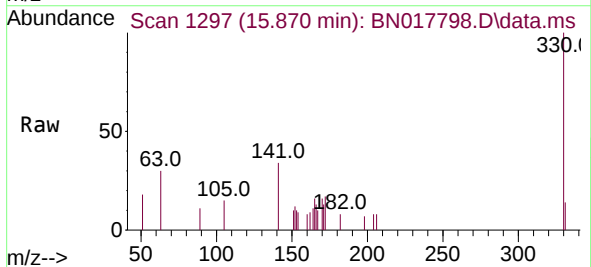


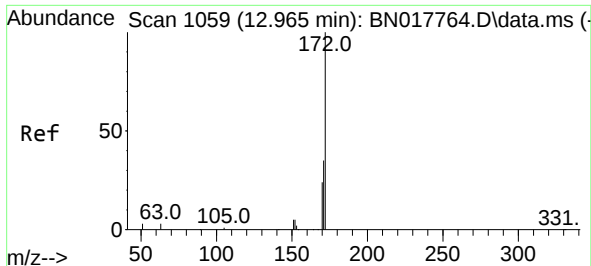

#15
2-Fluorobiphenyl
Concen: 0.240 ng
RT: 12.977 min Scan# 1069
Delta R.T. 0.012 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03




Instrument :
BNA_N
ClientSampleId :
PB141179BL


Tgt Ion:172 Resp: 45749
Ion Ratio Lower Upper
172 100
171 35.4 28.1 42.1
170 23.2 18.9 28.3

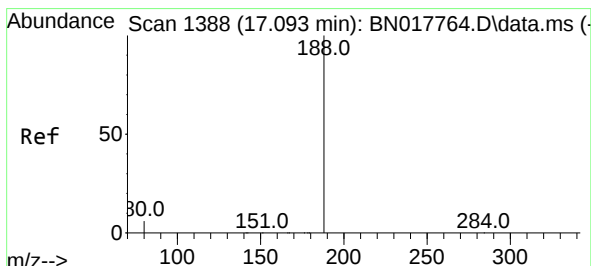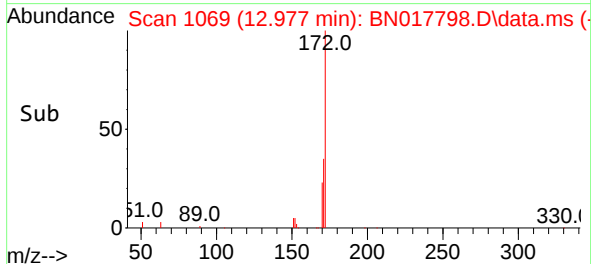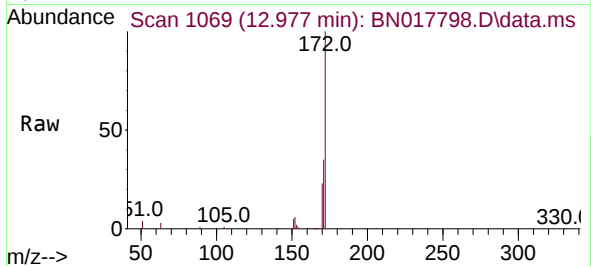

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.105 min Scan# 1398
Delta R.T. 0.012 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03

Tgt Ion:188 Resp: 102266
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.4 5.1 7.7#


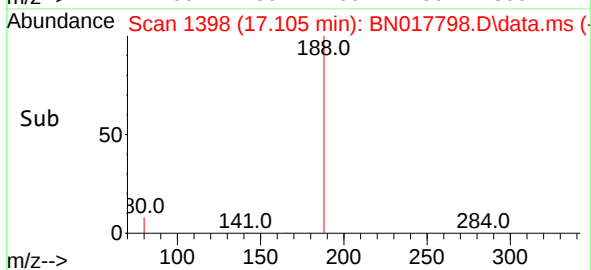

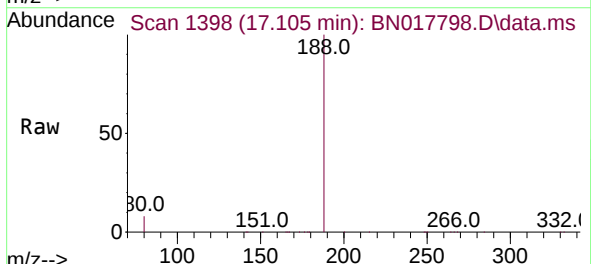


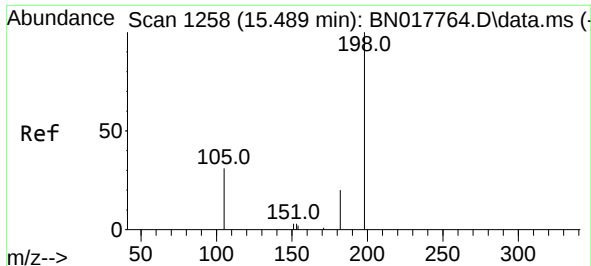

#20
4,6-Dinitro-2-methylphenol
Concen: 0.089 ng
RT: 15.502 min Scan# 1372
Delta R.T. 0.013 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03




Instrument :
BNA_N
ClientSampleId :
PB141179BL


Tgt Ion:198 Resp: 9
Ion Ratio Lower Upper
198 100
182 103.7 44.2 66.2#
77 0.0 0.0 0.0

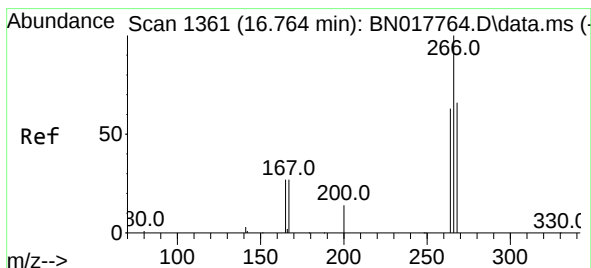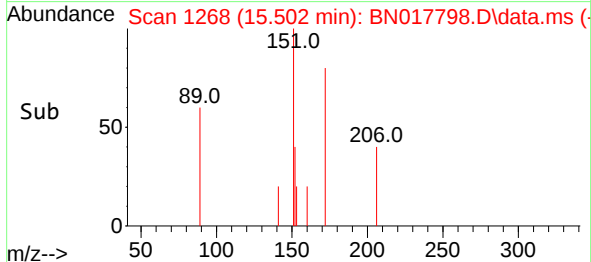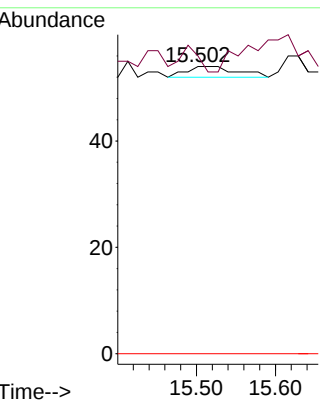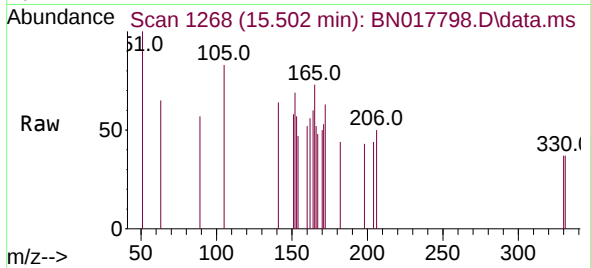

#24
Pentachlorophenol
Concen: 0.281 ng
RT: 16.800 min Scan# 1373
Delta R.T. 0.036 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03

Tgt Ion:266 Resp: 23
Ion Ratio Lower Upper
266 100
264 113.0 50.8 76.2#
268 0.0 51.8 77.6#


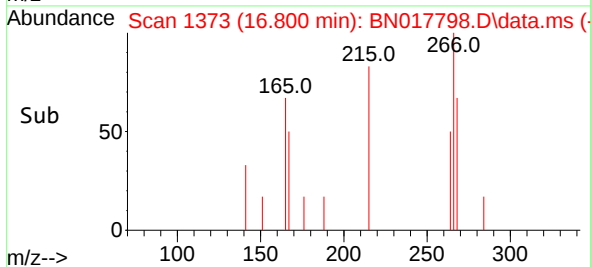
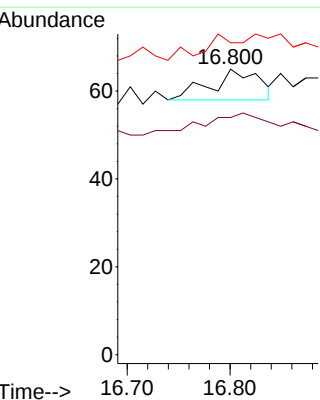
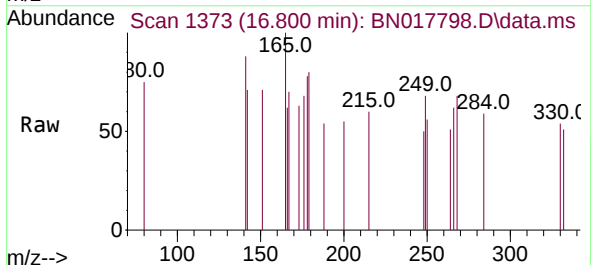


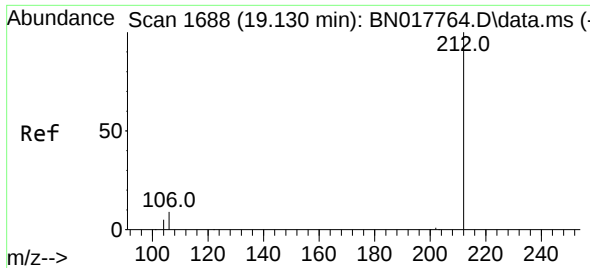

#27
Fluoranthene-d10
Concen: 0.303 ng
RT: 19.134 min Scan# 1
Delta R.T. 0.005 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03




Instrument :
BNA_N
ClientSampleId :
PB141179BL


Tgt Ion:212 Resp: 103557
Ion Ratio Lower Upper
212 100
106 10.1 8.2 12.2
104 5.6 4.6 6.8

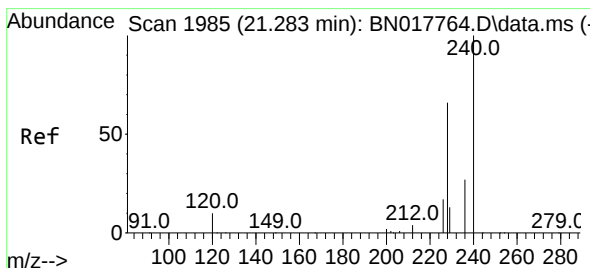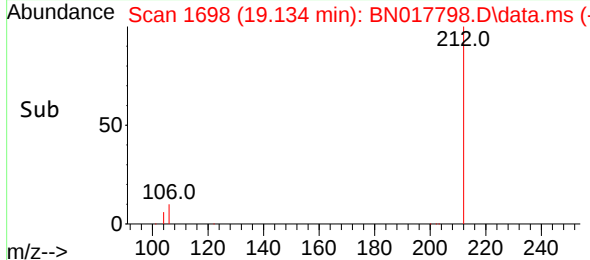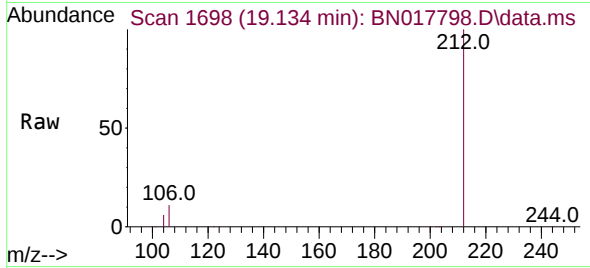

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.304 min Scan# 1996
Delta R.T. 0.021 min
Lab File: BN017798.D
Acq: 08 Dec 2021 14:03

Tgt Ion:240 Resp: 107299
Ion Ratio Lower Upper
240 100
120 6.4 7.9 11.9#
236 25.7 21.4 32.2


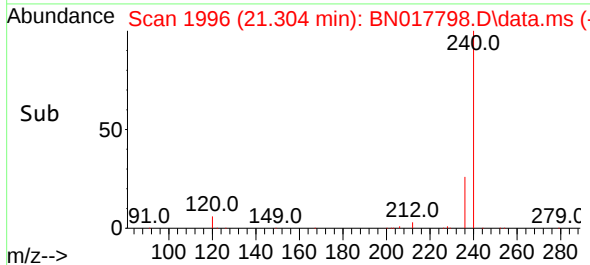

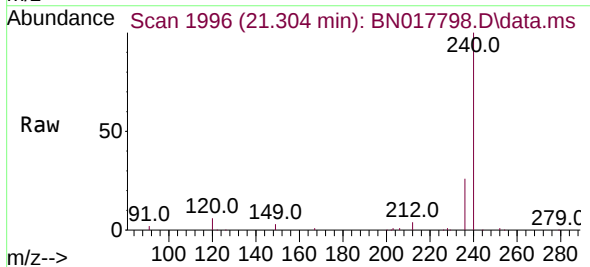


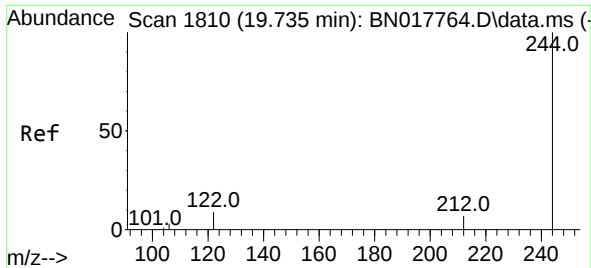

#31
 Terphenyl-d14
 Concen: 0.359 ng
 RT: 19.745 min Scan# 1810
 Delta R.T. 0.010 min
 Lab File: BN017798.D
 Acq: 08 Dec 2021 14:03

Instrument :
 BNA_N
 ClientSampleId :
 PB141179BL

Tgt Ion:244 Resp: 82694
 Ion Ratio Lower Upper
 244 100
 212 7.7 5.8 8.8
 122 9.1 7.1 10.7

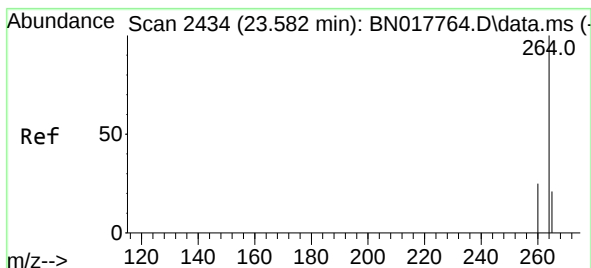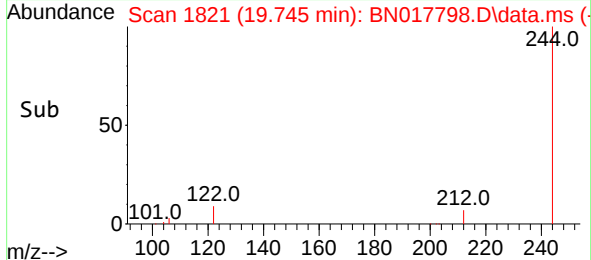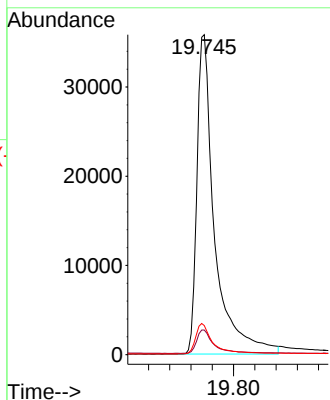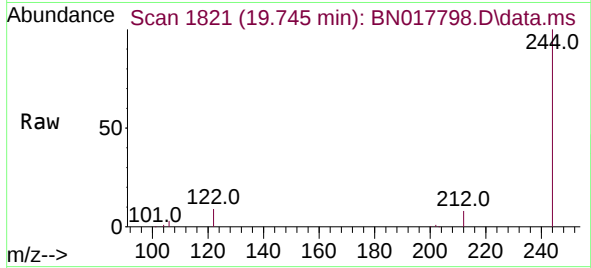

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.596 min Scan# 2447
 Delta R.T. 0.013 min
 Lab File: BN017798.D
 Acq: 08 Dec 2021 14:03

Tgt Ion:264 Resp: 89712
 Ion Ratio Lower Upper
 264 100
 260 24.8 20.0 30.0
 265 26.5 20.5 30.7

