
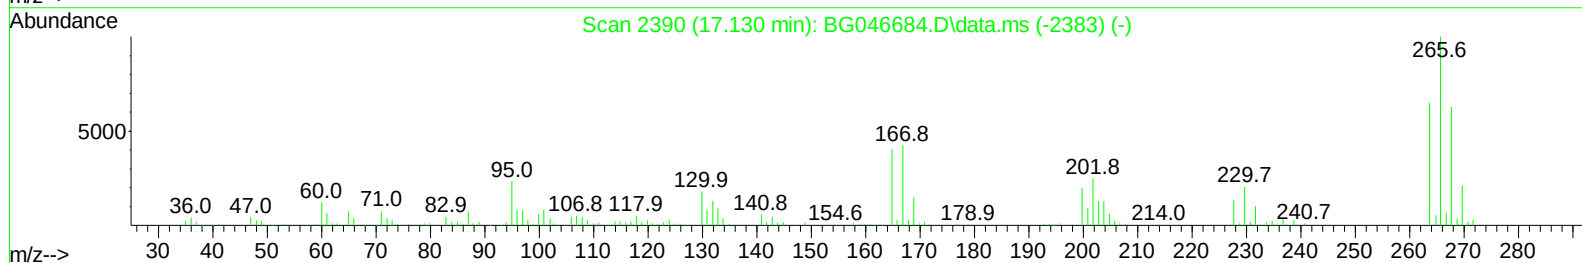
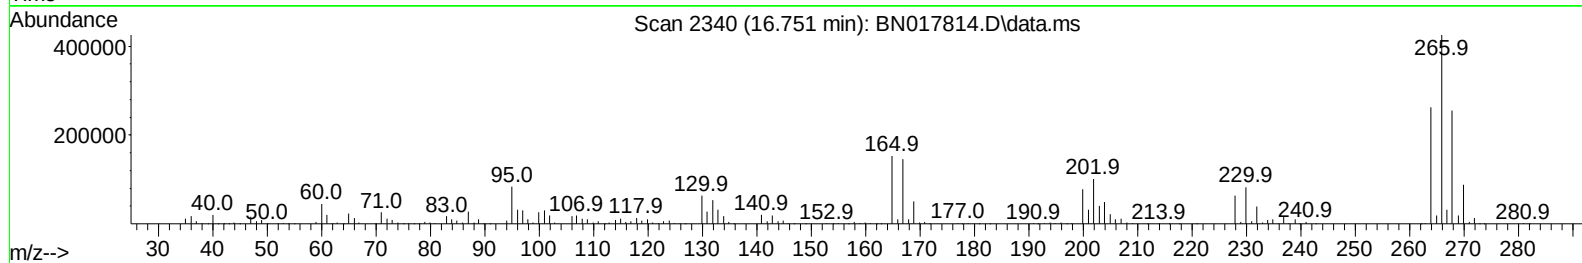


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120821\
Data File : BN017814.D
Acq On : 09 Dec 2021 00:25
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 02:51:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 12:31:20 2021
Response via : Initial Calibration

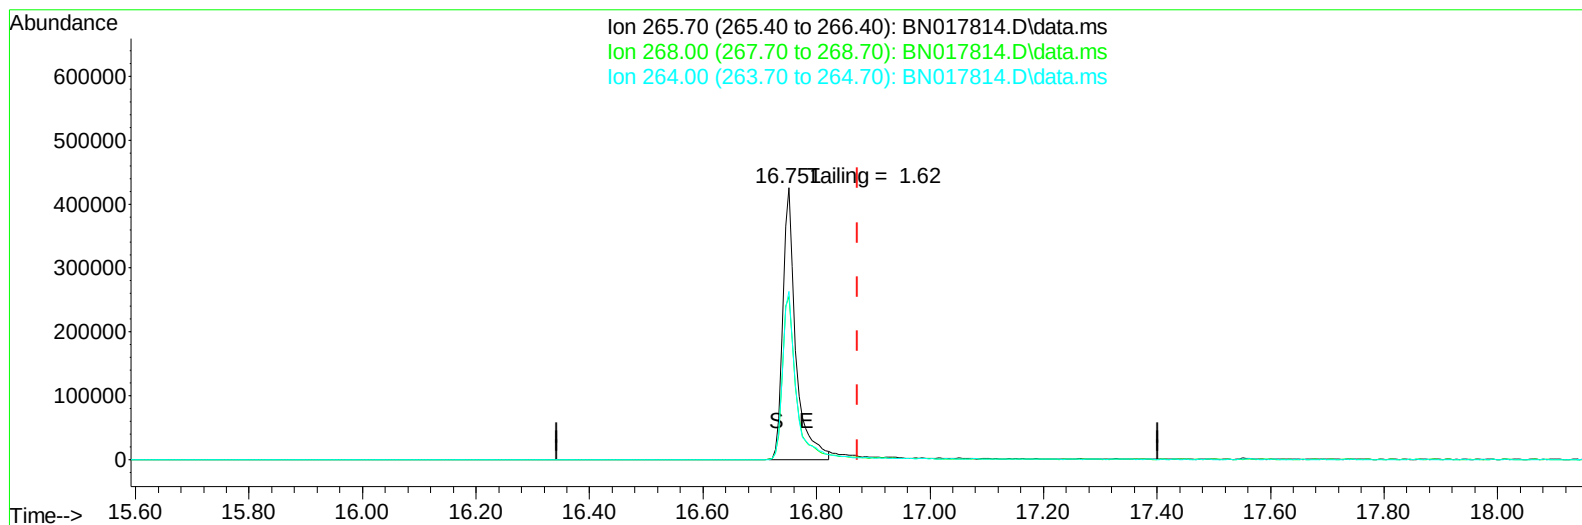




TIC: BN017814.D\data.ms

(70) Pentachlorophenol (C)**16.751min (-0.121) 21217.52 ng****response 715326**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.05
264.00	61.60	61.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120821\
 Data File : BN017814.D
 Acq On : 09 Dec 2021 00:25
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 02:51:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 12:31:20 2021
 Response via : Initial Calibration

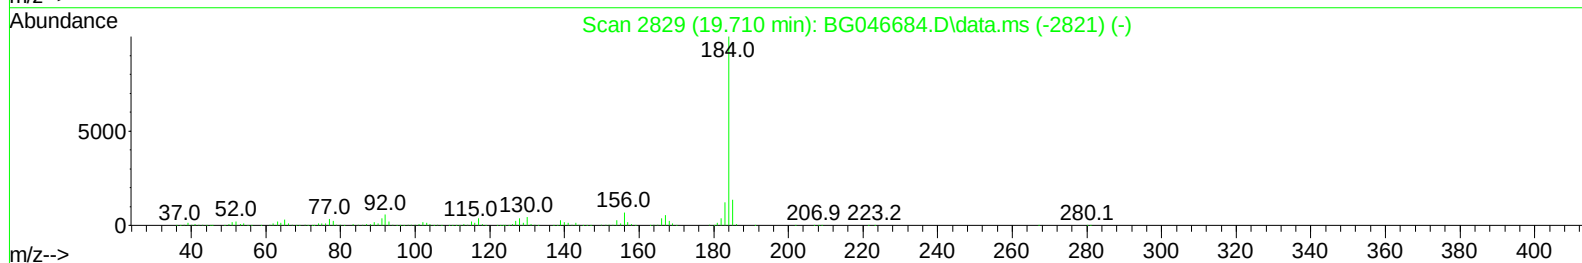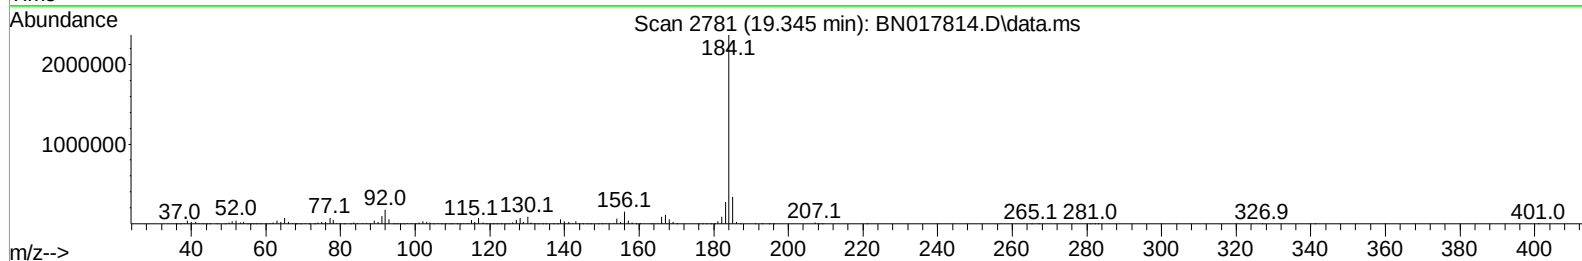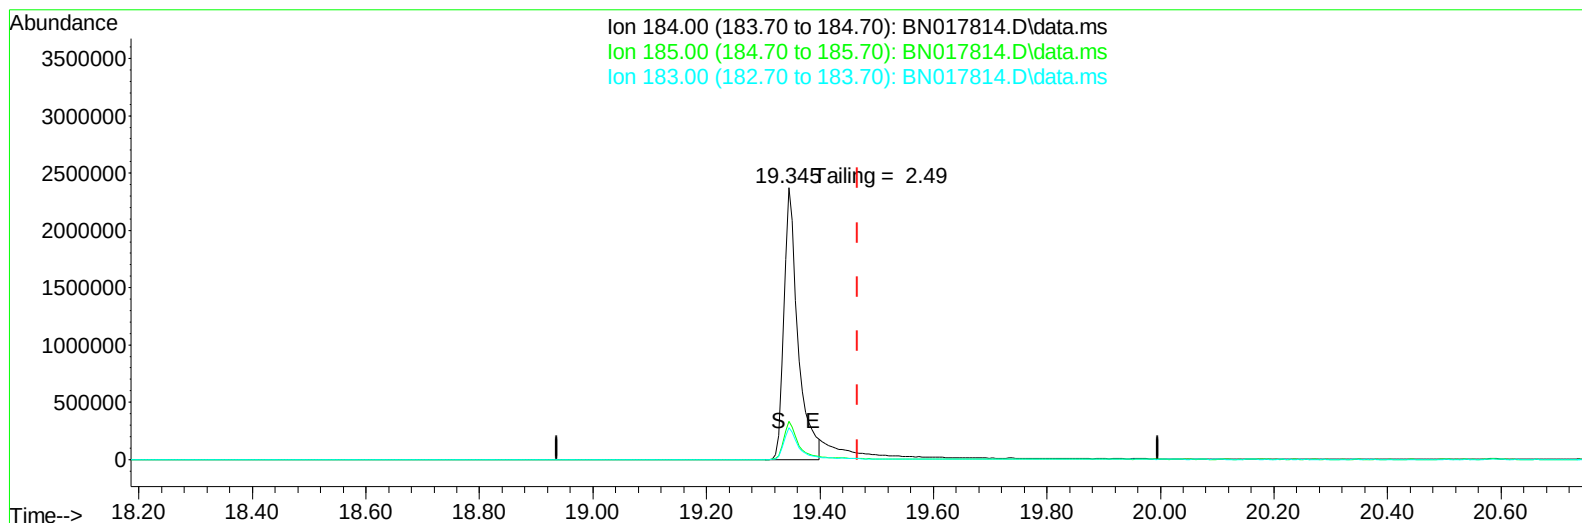

TIC: BN017814.D\data.ms

(77) Benzidine**19.345min (-0.121) 1172023.55 ng****response 4696648**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	11.61
0.00	0.00	0.00