
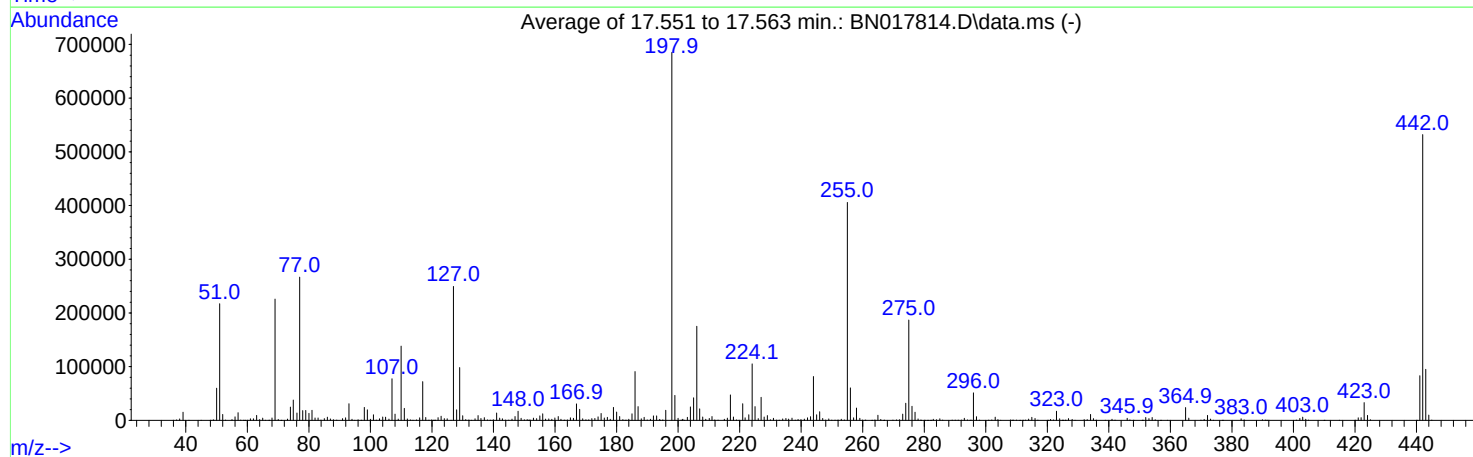


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120821\
 Data File : BN017814.D
 Acq On : 09 Dec 2021 00:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 08 01:18:09 2021

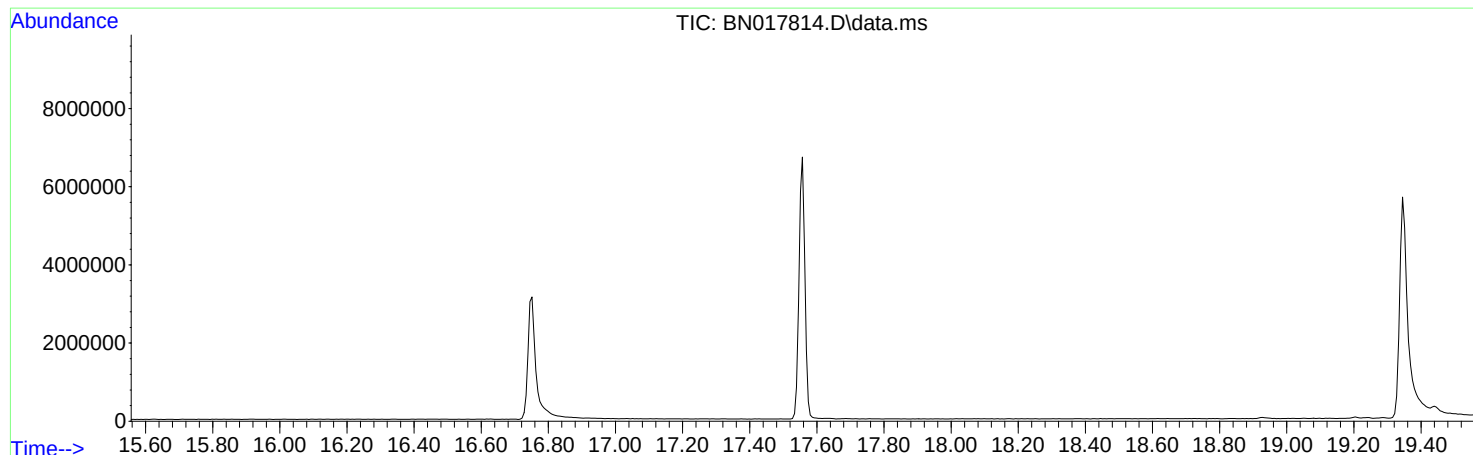




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	217301	PASS
68	69	0.00	2	1.9	4356	PASS
69	198	0.00	100	33.0	225920	PASS
70	69	0.00	2	0.7	1673	PASS
127	198	10	80	36.4	249451	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	684949	PASS
199	198	5	9	6.8	46347	PASS
275	198	10	60	27.3	186837	PASS
365	198	1	100	3.5	23875	PASS
441	198	0.01	100	12.1	83136	PASS
442	442	50	100	100.0	531989	PASS
443	442	15	24	17.9	95115	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120821\
 Data File : BN017814.D
 Acq On : 09 Dec 2021 00:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 10 02:51:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 12:31:20 2021
 Response via : Initial Calibration

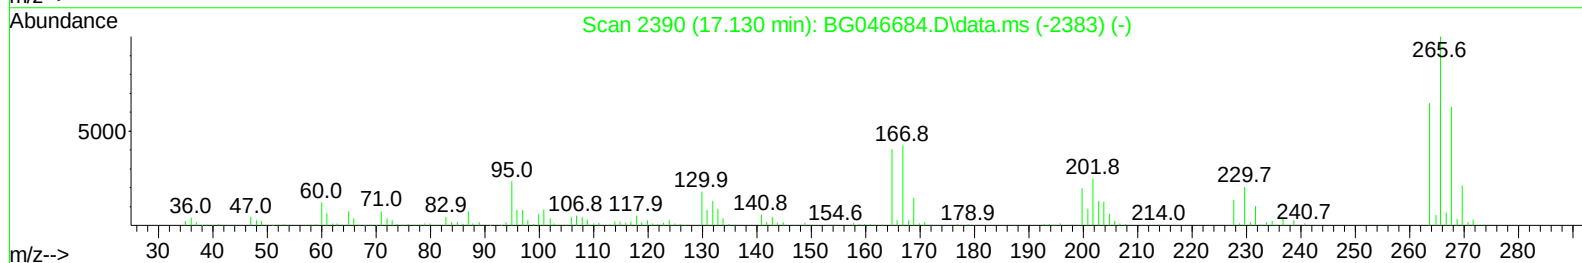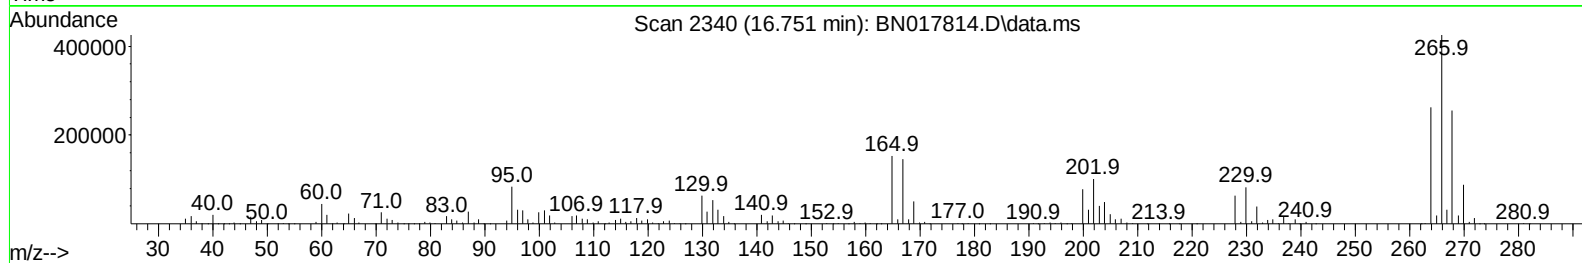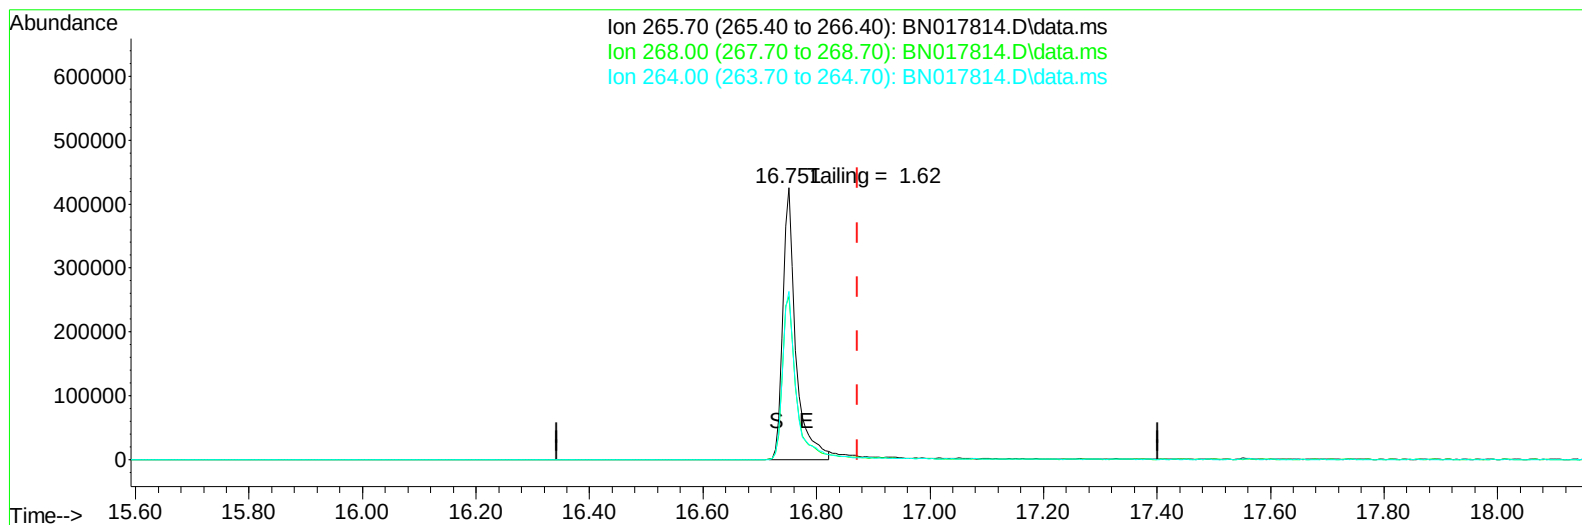

TIC: BN017814.D\data.ms




(70) Pentachlorophenol (C)**16.751min (-0.121) 21217.52 ng****response 715326**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.05
264.00	61.60	61.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120821\
Data File : BN017814.D
Acq On : 09 Dec 2021 00:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 10 02:51:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 12:31:20 2021
Response via : Initial Calibration

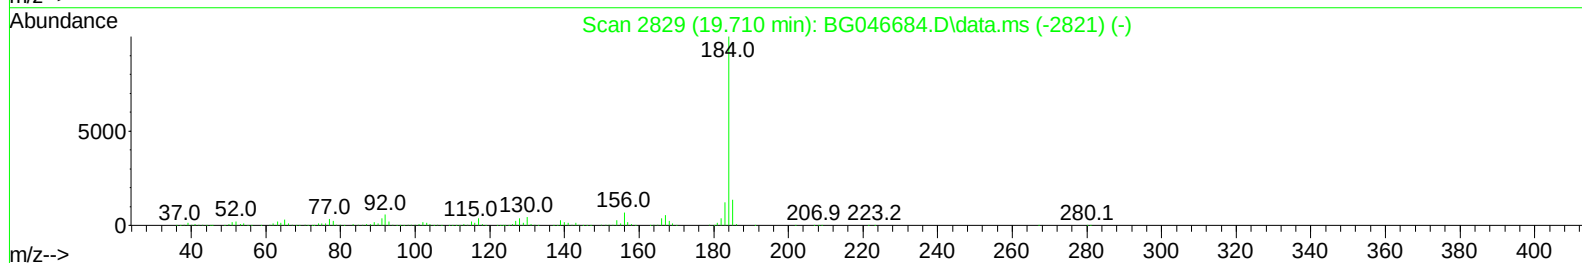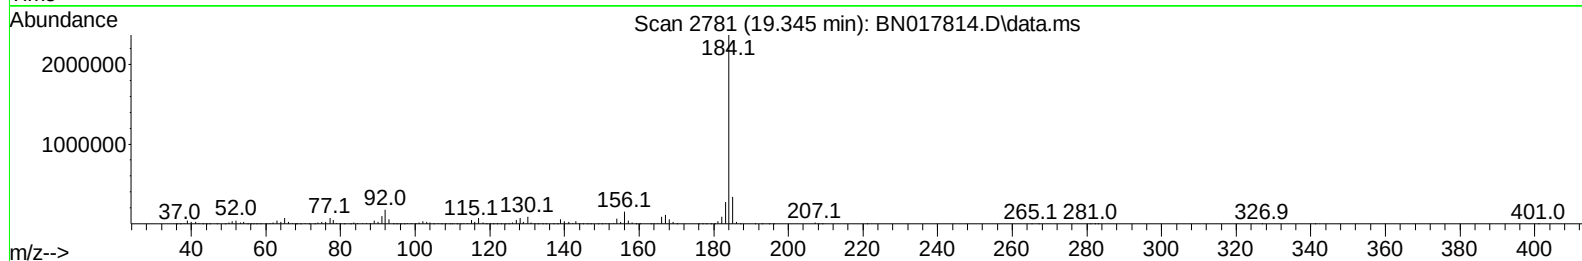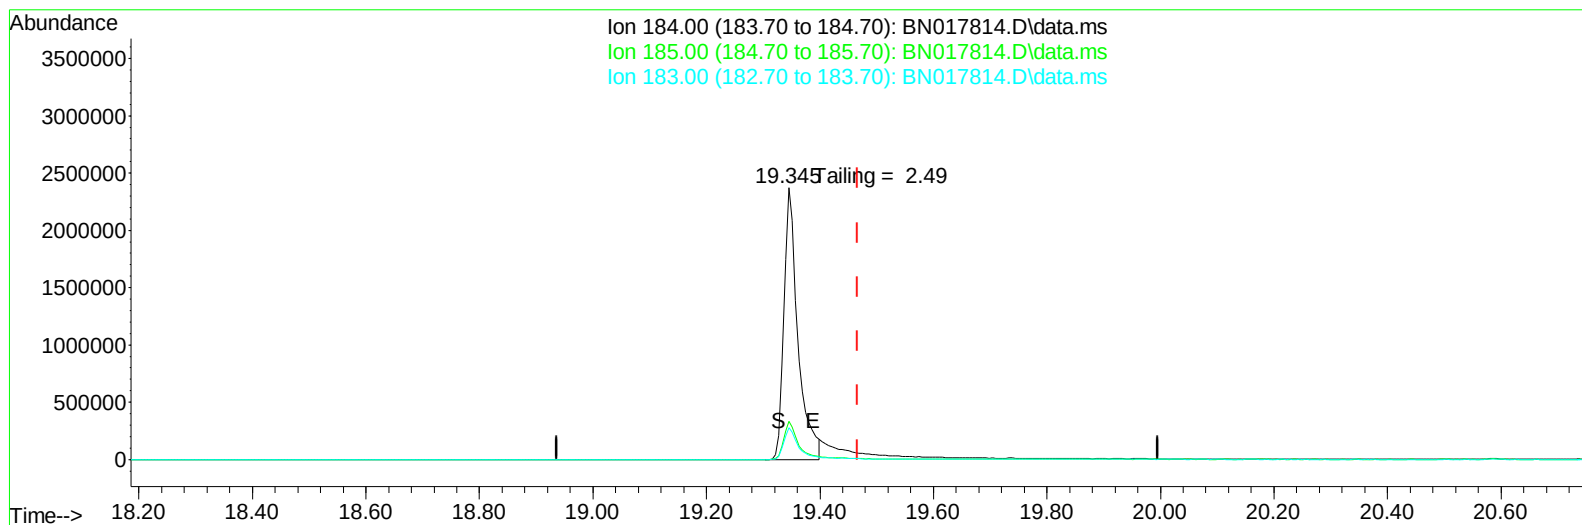

TIC: BN017814.D\data.ms

(77) Benzidine

19.345min (-0.121) 1172023.55 ng

response 4696648

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	11.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/8/2021	BNA_N	<u>BN017814.D</u>
Compound Name	Response	Retention Time
DDT	2170975	20.586
DDD	138427	20.145
DDE	5451	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
143878	2314853	6.22

Instrument :
BNA_N
ClientSampleId :
DFTPP