
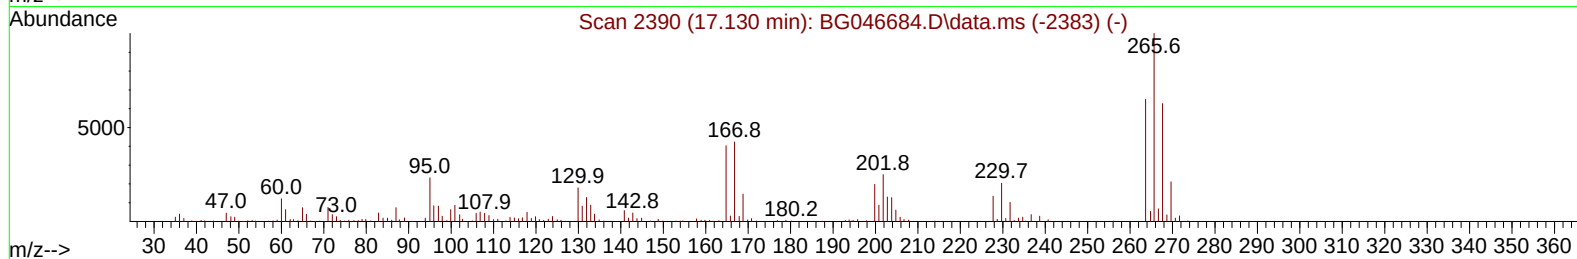
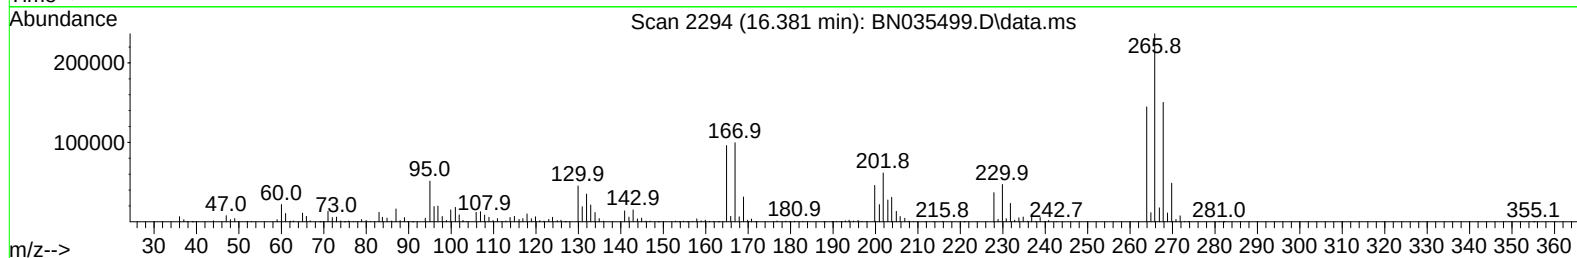


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035499.D
Acq On : 09 Dec 2024 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 12:54:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 23:08:29 2024
Response via : Initial Calibration

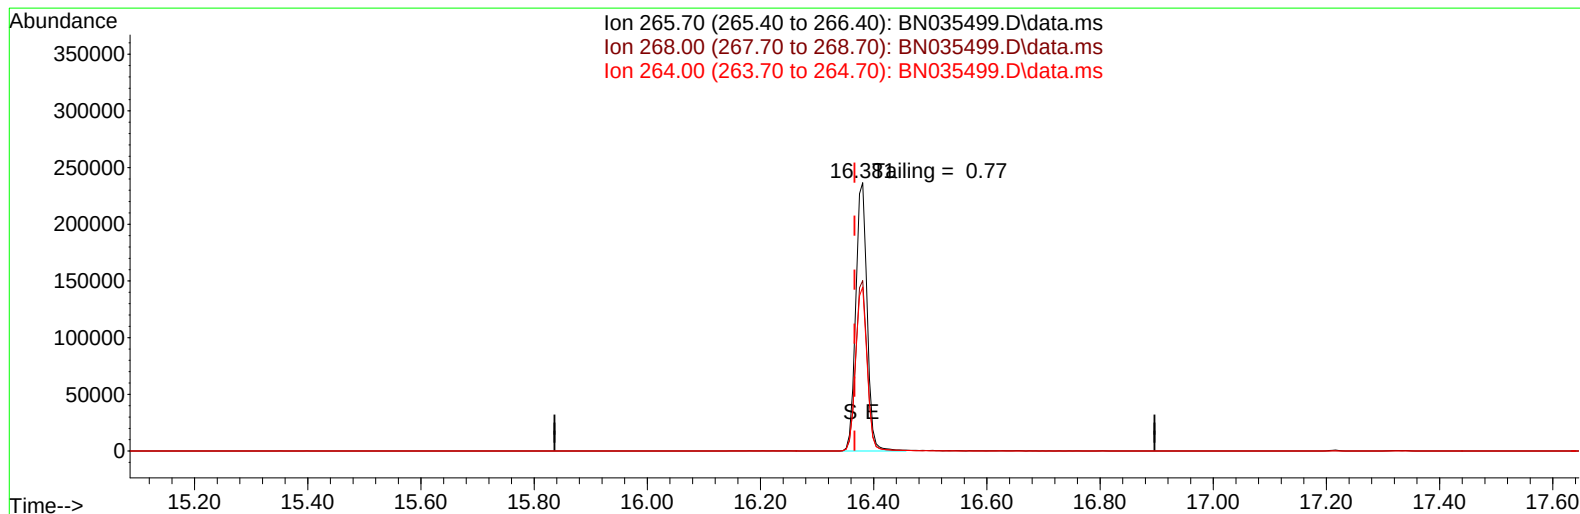

TIC: BN035499.D\data.ms

(70) Pentachlorophenol (C)




16.381min (+ 0.015) 26216.12 ng

response 333912

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.48
264.00	61.60	61.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035499.D
Acq On : 09 Dec 2024 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 12:59:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 23:08:29 2024
Response via : Initial Calibration

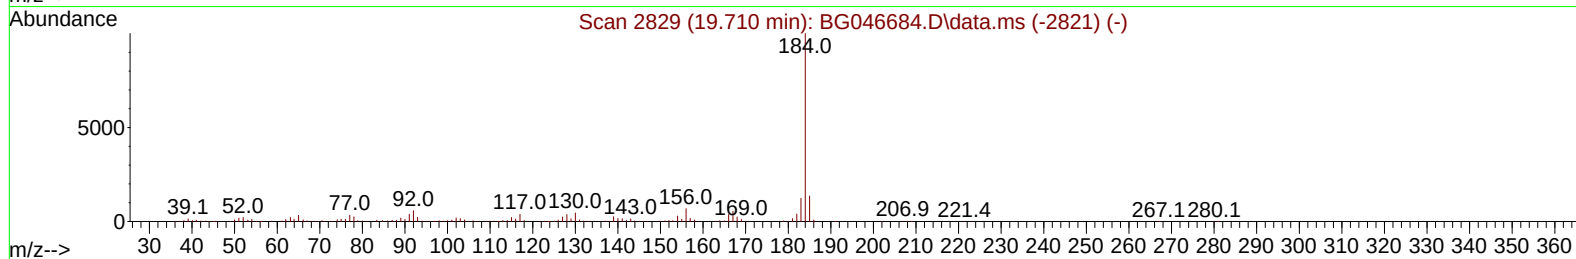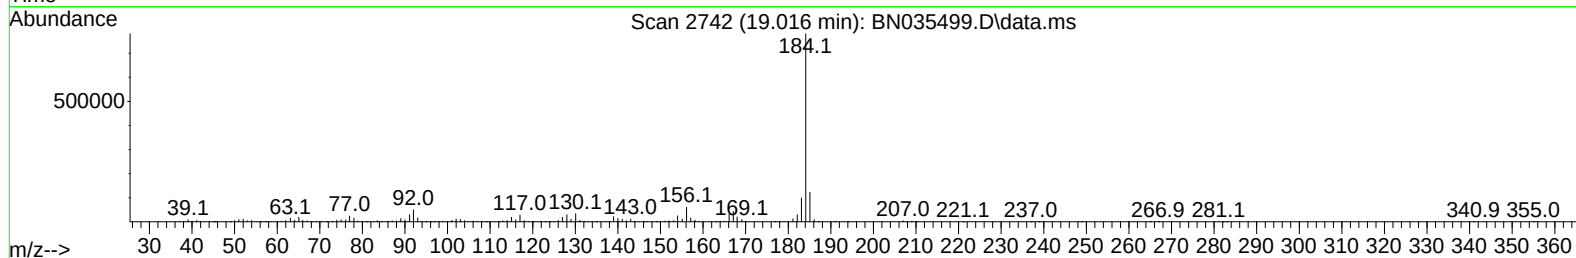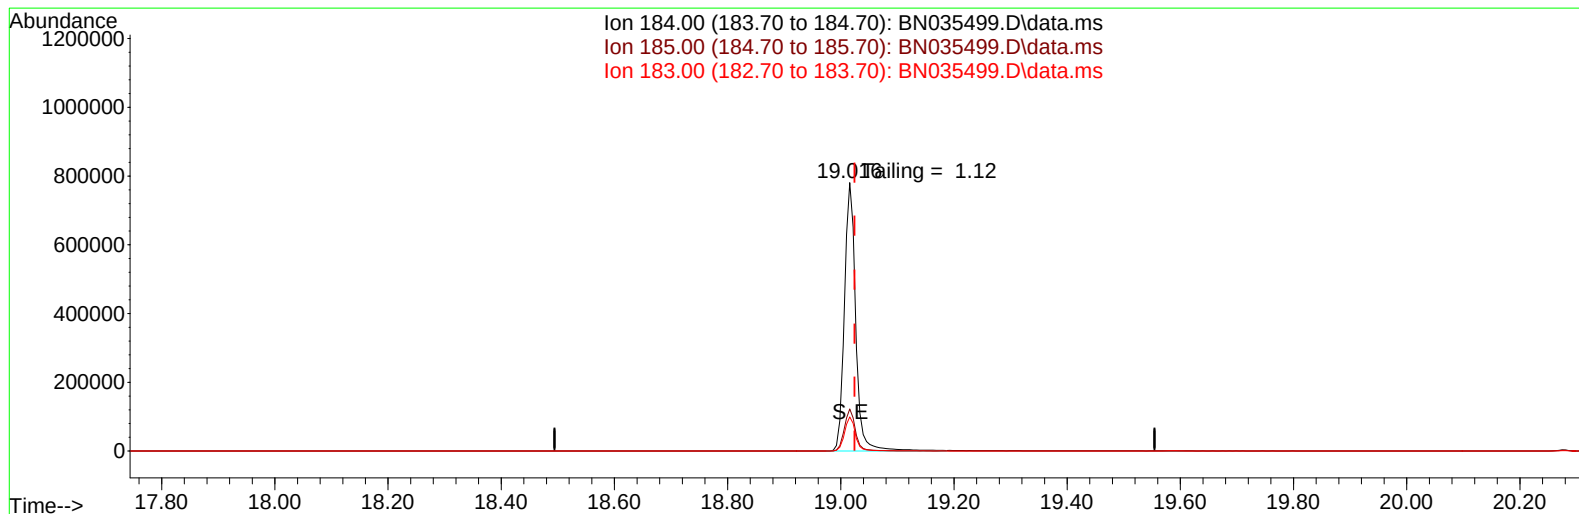

TIC: BN035499.D\data.ms

(77) Benzidine

19.016min (-0.008) 0.00 ng

response 1097531

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.72
183.00	13.20	12.71
0.00	0.00	0.00