
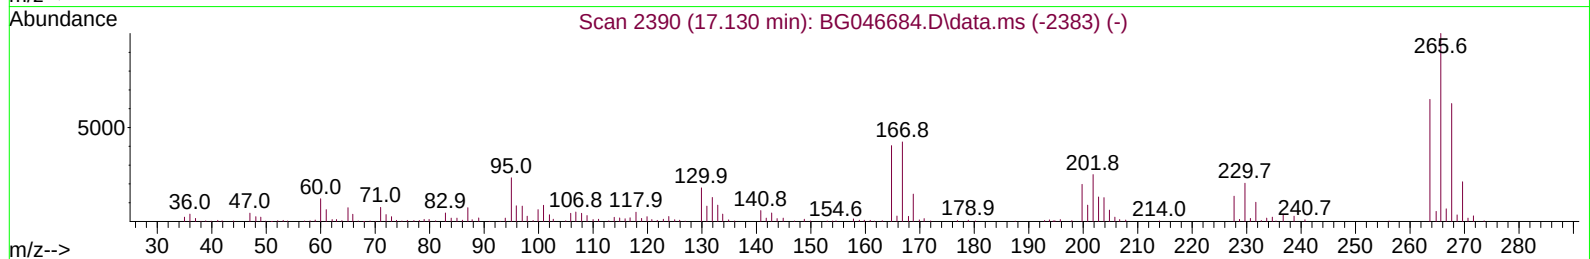
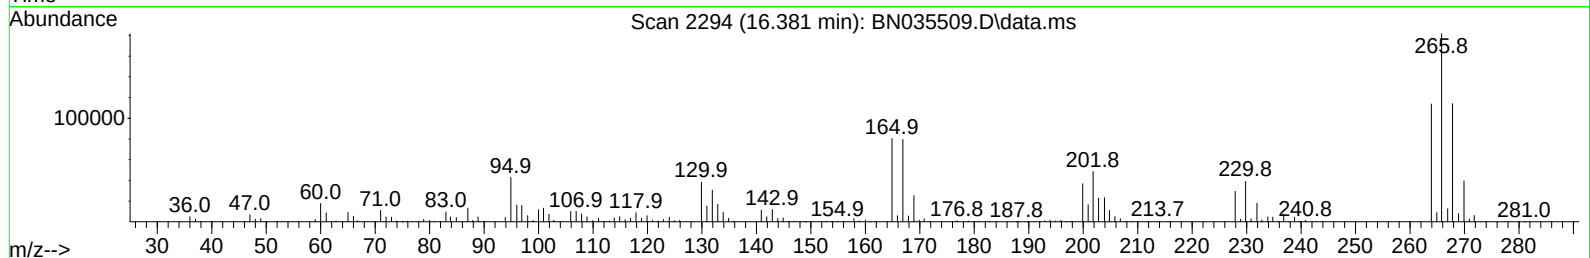


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035509.D
Acq On : 09 Dec 2024 16:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 03:57:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 03:57:32 2024
Response via : Initial Calibration

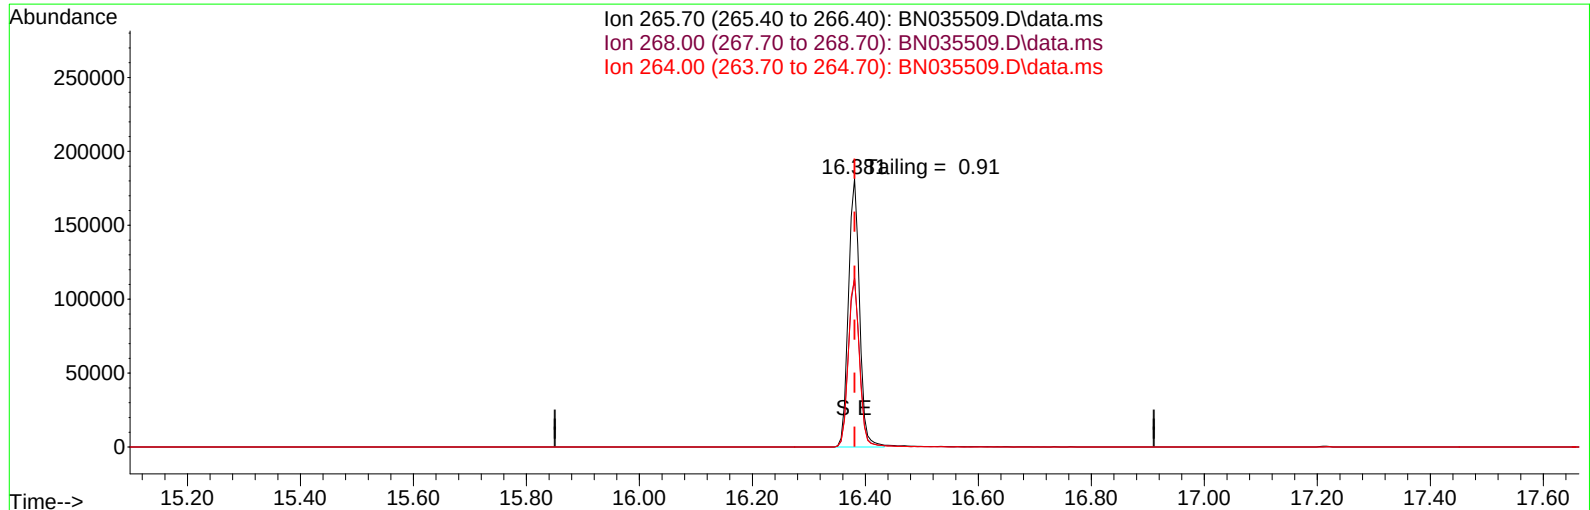

TIC: BN035509.D\data.ms

(70) Pentachlorophenol (C)




16.381min (0.000) 23065.04 ng

response 251964

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.83
264.00	61.60	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035509.D
Acq On : 09 Dec 2024 16:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 03:57:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 03:57:32 2024
Response via : Initial Calibration

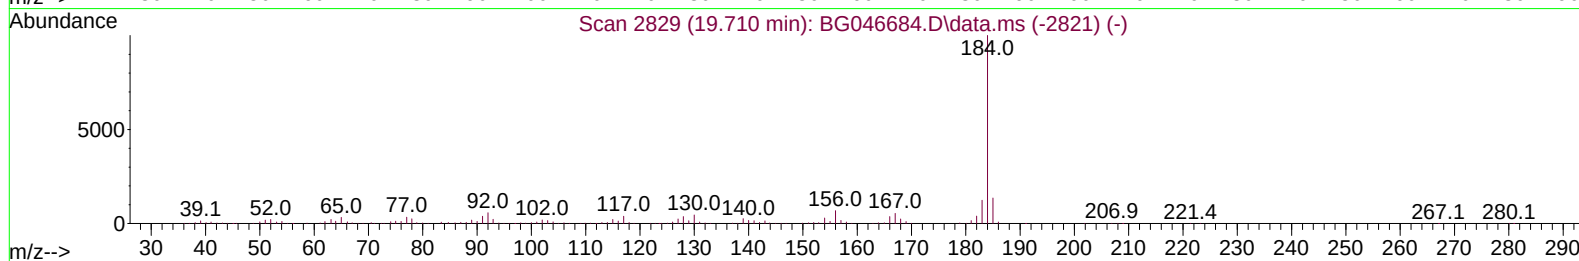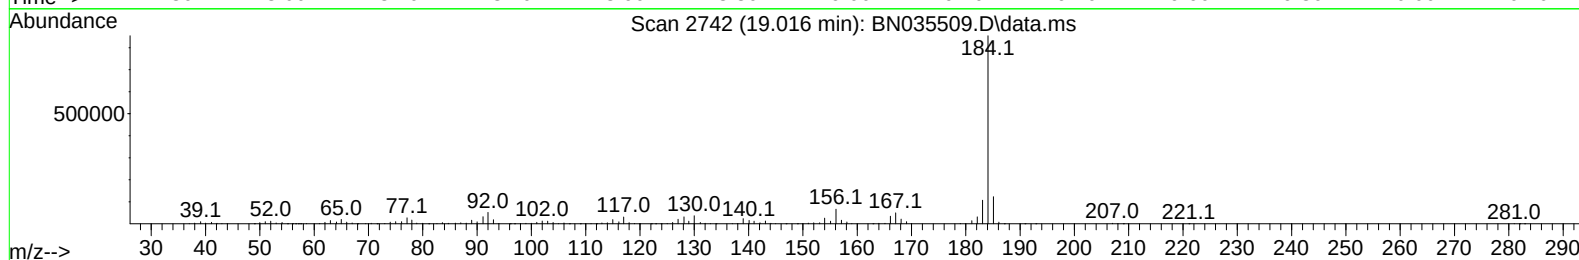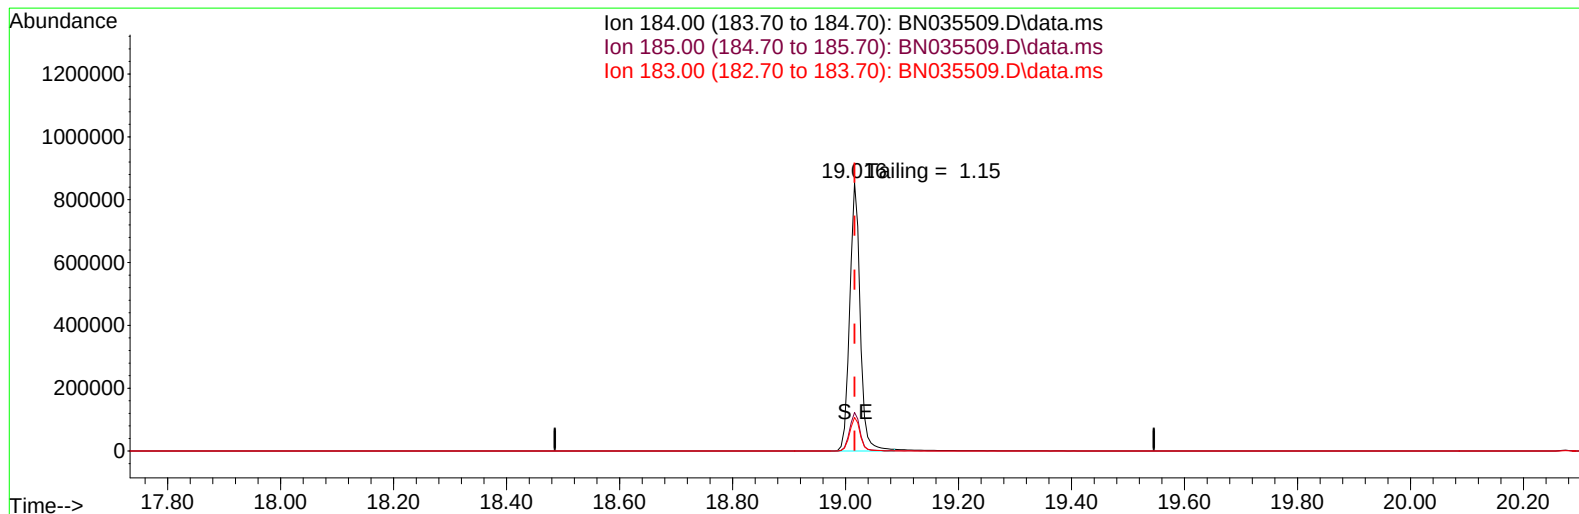

TIC: BN035509.D\data.ms

(77) Benzidine

19.016min (0.000) 0.00 ng

response 1117982

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	12.52
0.00	0.00	0.00