
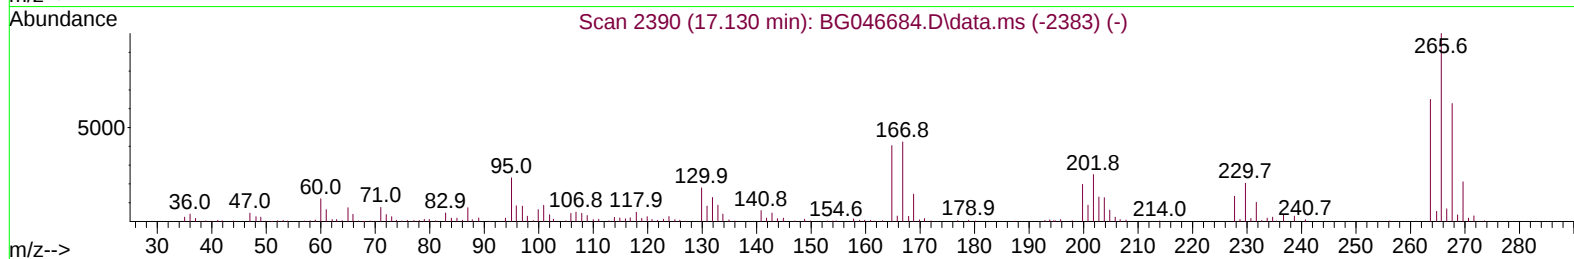
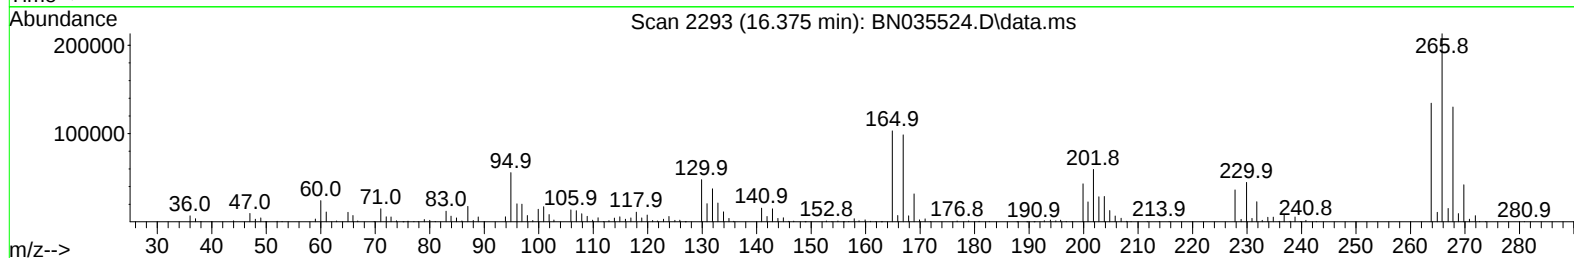


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035524.D
Acq On : 10 Dec 2024 08:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 06:13:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 06:13:05 2024
Response via : Initial Calibration

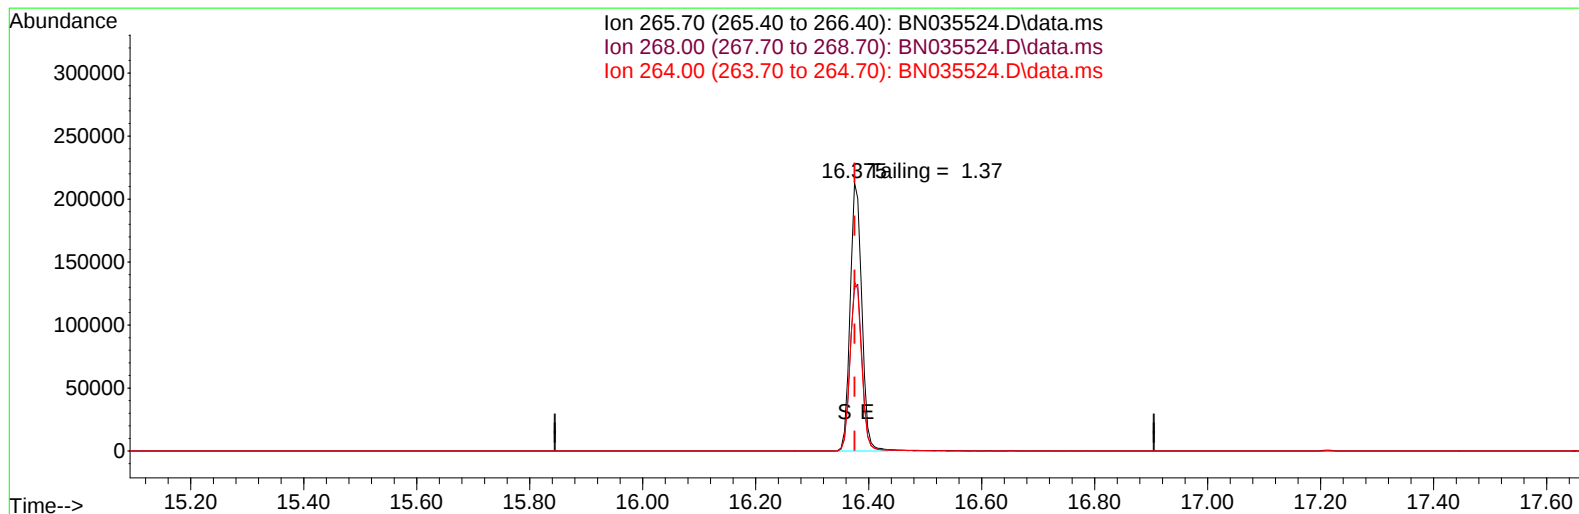

TIC: BN035524.D\data.ms

(70) Pentachlorophenol (C)




16.375min (0.000) 25281.71 ng

response 307527

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.01
264.00	61.60	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035524.D
Acq On : 10 Dec 2024 08:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 06:13:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 06:13:05 2024
Response via : Initial Calibration

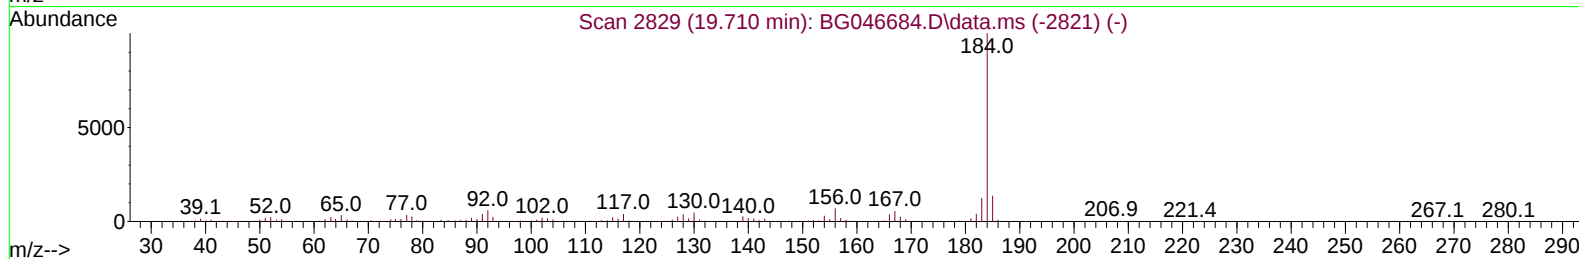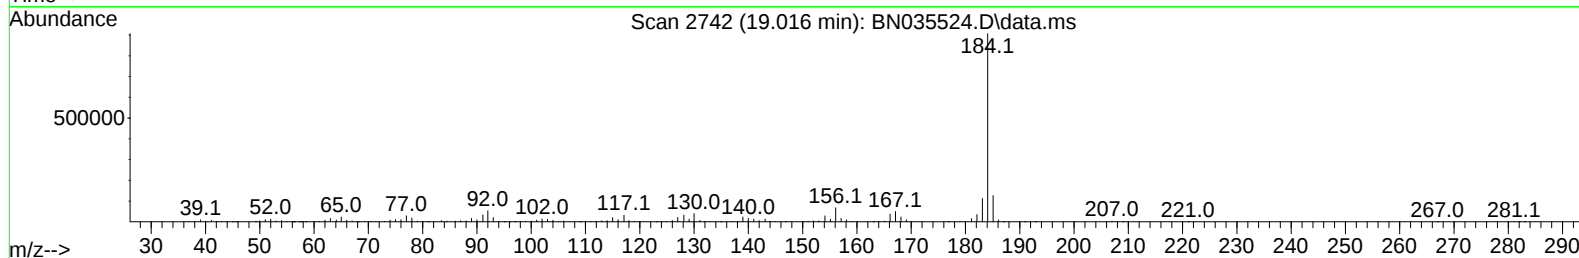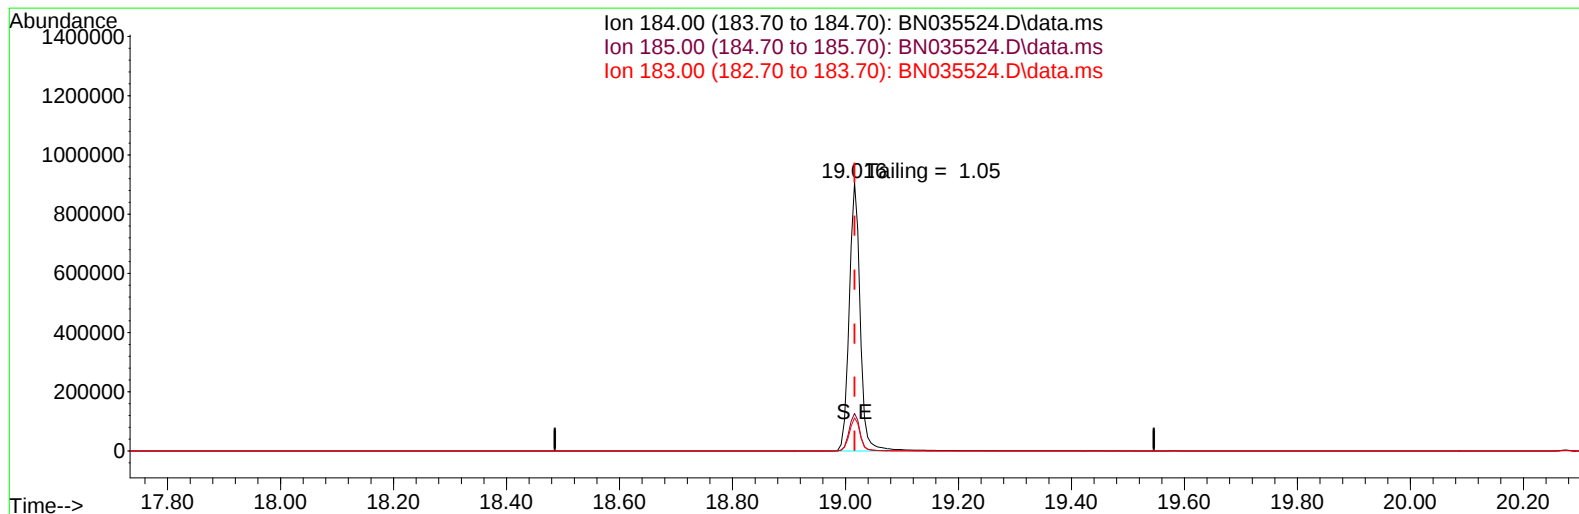

TIC: BN035524.D\data.ms

(77) Benzidine

19.016min (0.000) 0.00 ng

response 1233878

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	12.36
0.00	0.00	0.00