


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035499.D
Acq On : 09 Dec 2024 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 27 23:03:24 2024

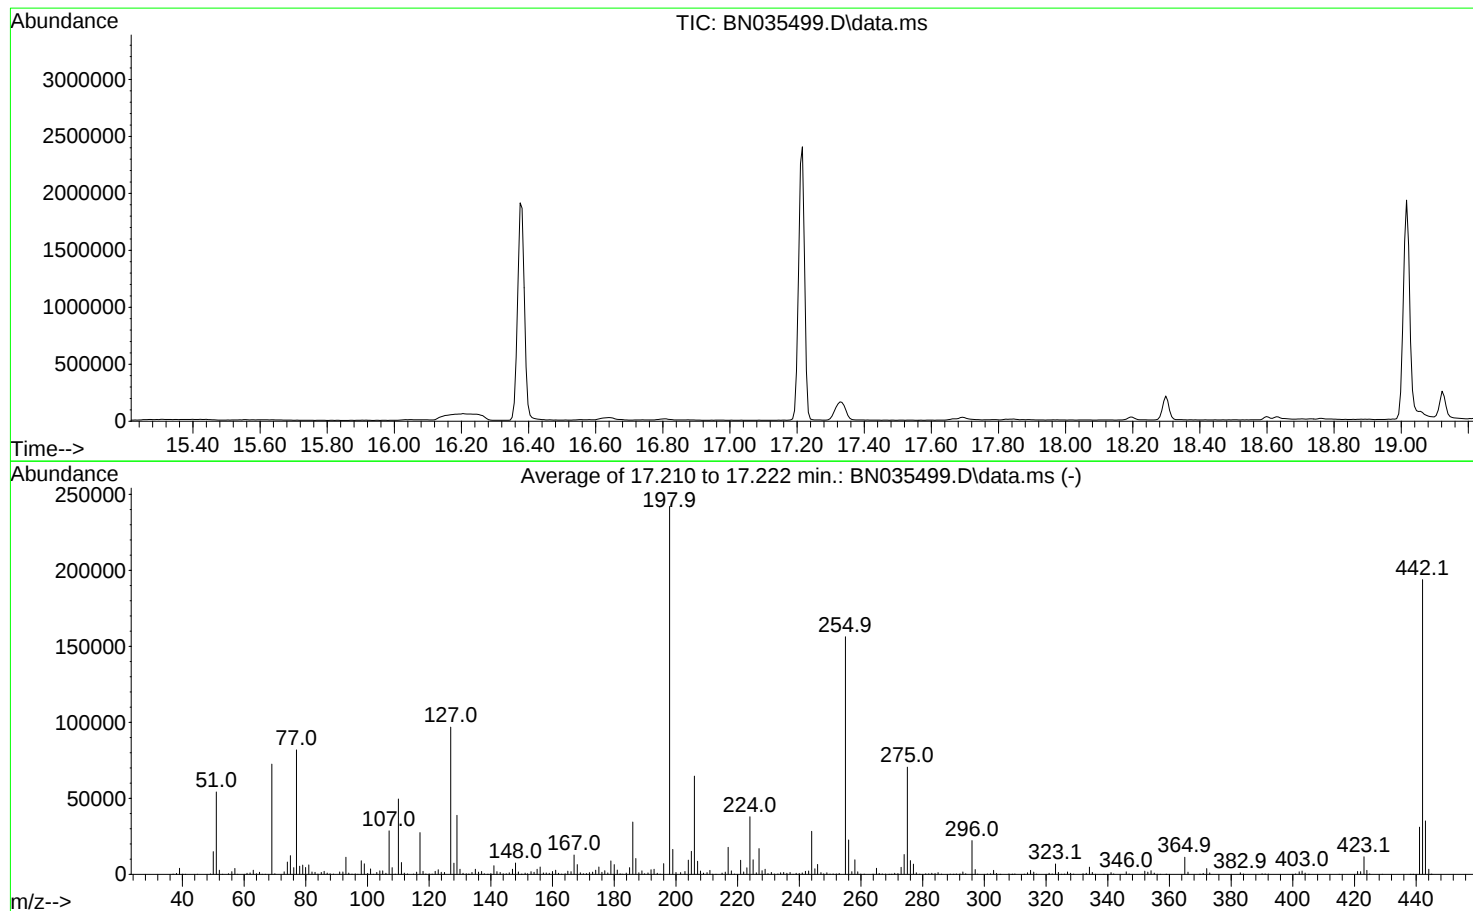

AutoFind: Scans 2435, 2436, 2437; Background Corrected with Scan 2428

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	54219	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.0	72555	PASS
70	69	0.00	2	0.6	416	PASS
127	198	10	80	40.0	96861	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	242027	PASS
199	198	5	9	6.8	16411	PASS
275	198	10	60	29.2	70568	PASS
365	198	1	100	4.6	11235	PASS
441	198	0.01	100	12.8	31048	PASS
442	442	50	100	100.0	193899	PASS
443	442	15	24	18.1	35123	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/9/2024	BNA_N	<u>BN035499.D</u>
Compound Name	Response	Retention Time
DDT	748822	20.281
DDD	24676	19.828
DDE	4486	19.316
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29162	777984	3.75

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035499.D
Acq On : 09 Dec 2024 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 09 12:54:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 23:08:29 2024
Response via : Initial Calibration

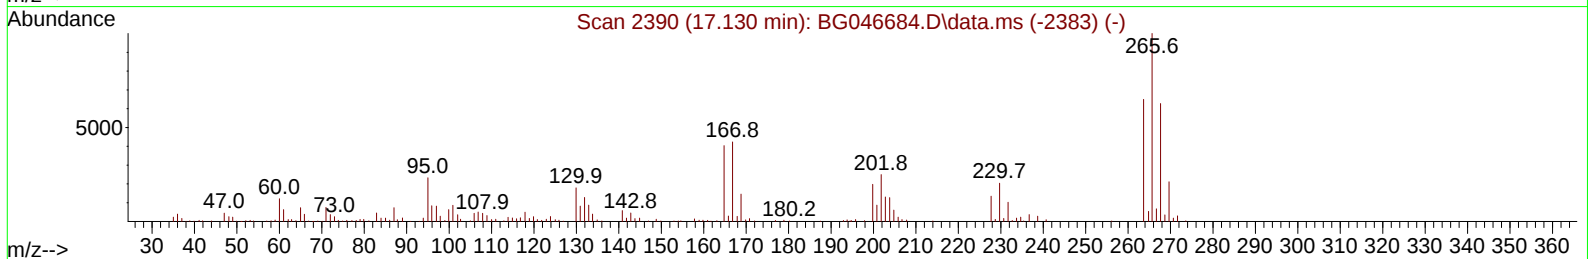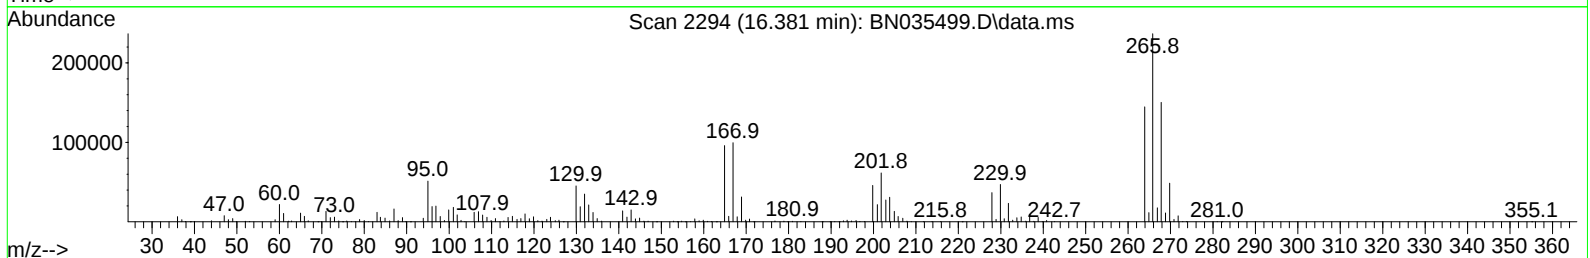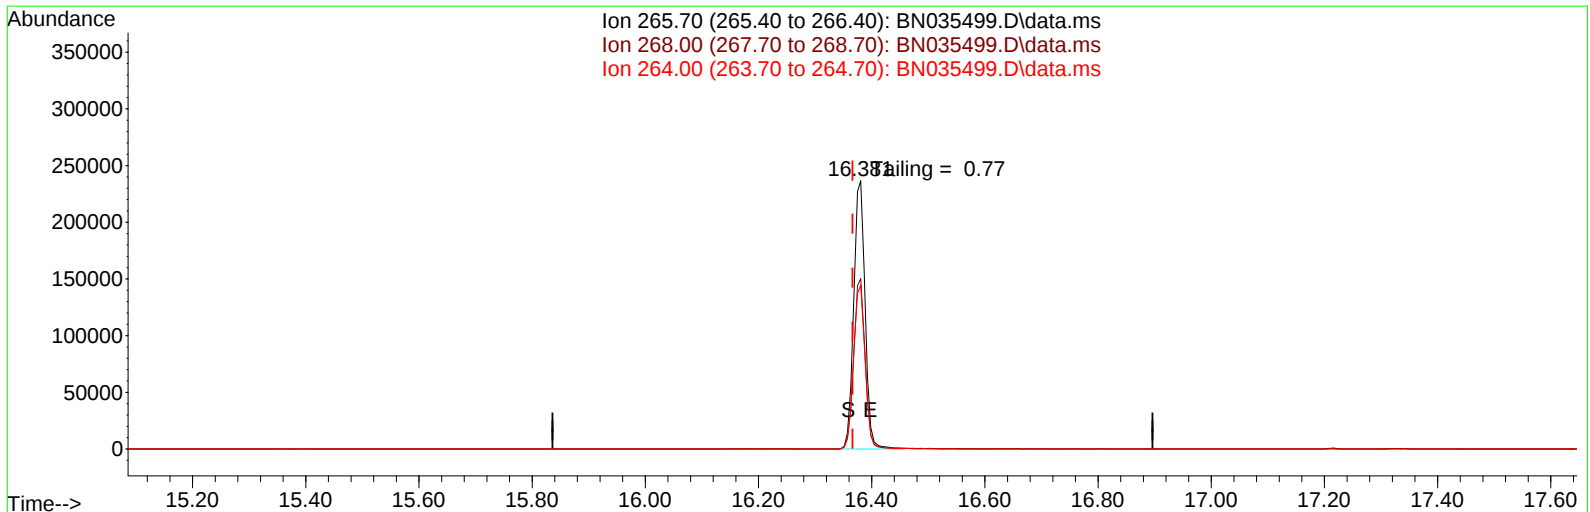

TIC: BN035499.D\data.ms

(70) Pentachlorophenol (C)

16.381min (+ 0.015) 26216.12 ng




response 333912

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.48
264.00	61.60	61.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035499.D
Acq On : 09 Dec 2024 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 09 12:59:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 03 23:08:29 2024
Response via : Initial Calibration

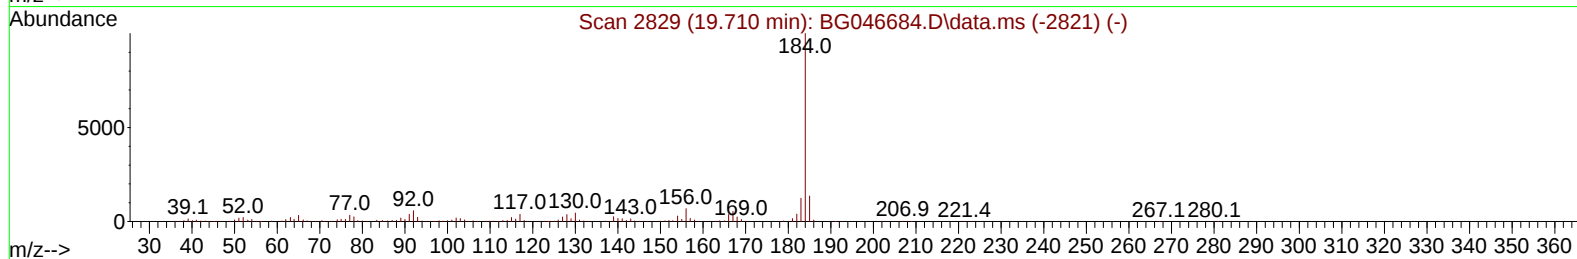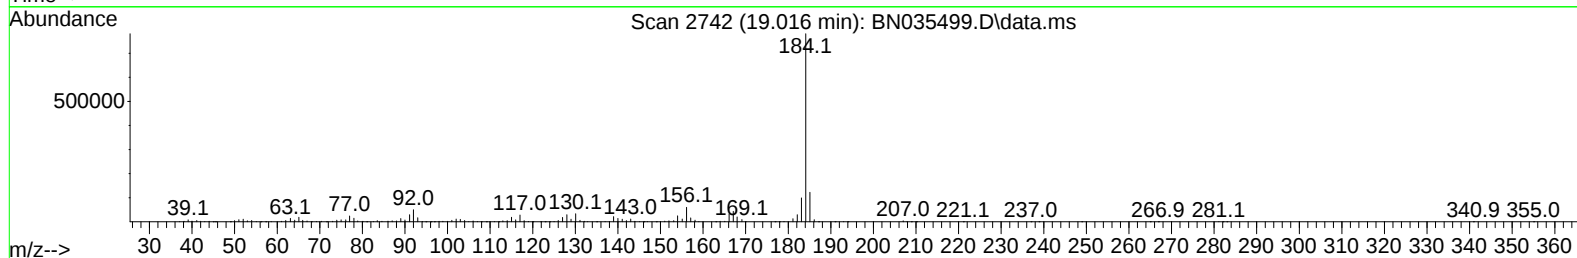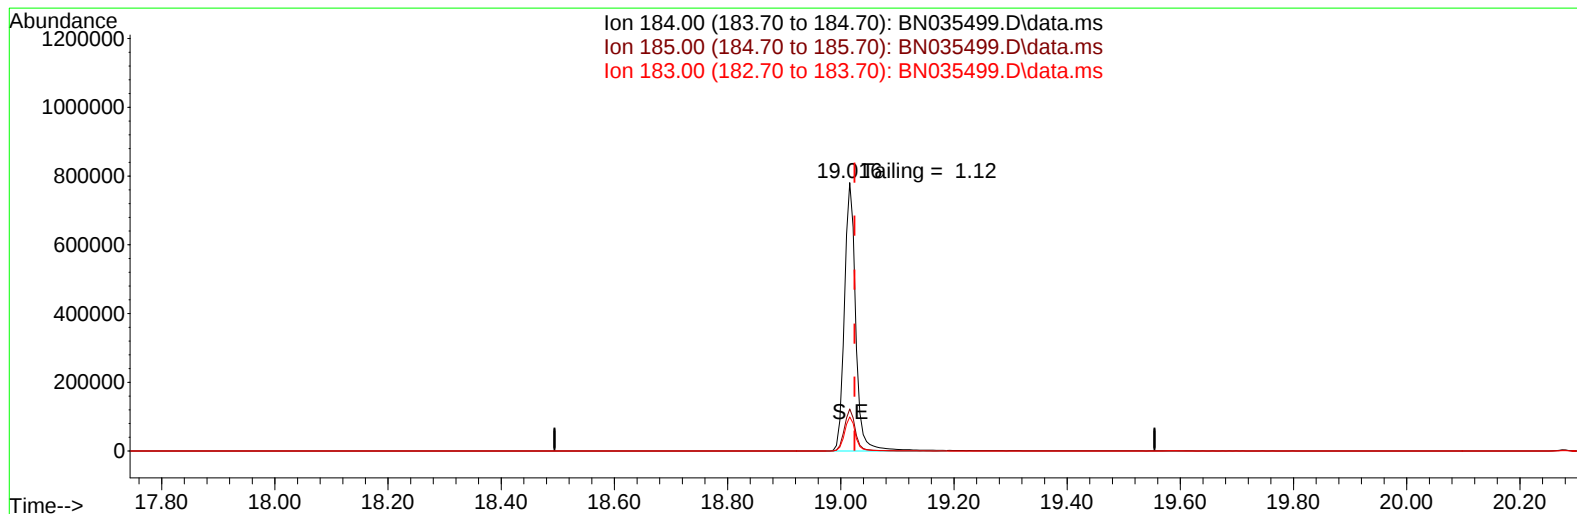

TIC: BN035499.D\data.ms

(77) Benzidine

19.016min (-0.008) 0.00 ng

response 1097531

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.72
183.00	13.20	12.71
0.00	0.00	0.00