


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035509.D
Acq On : 09 Dec 2024 16:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 27 23:03:24 2024

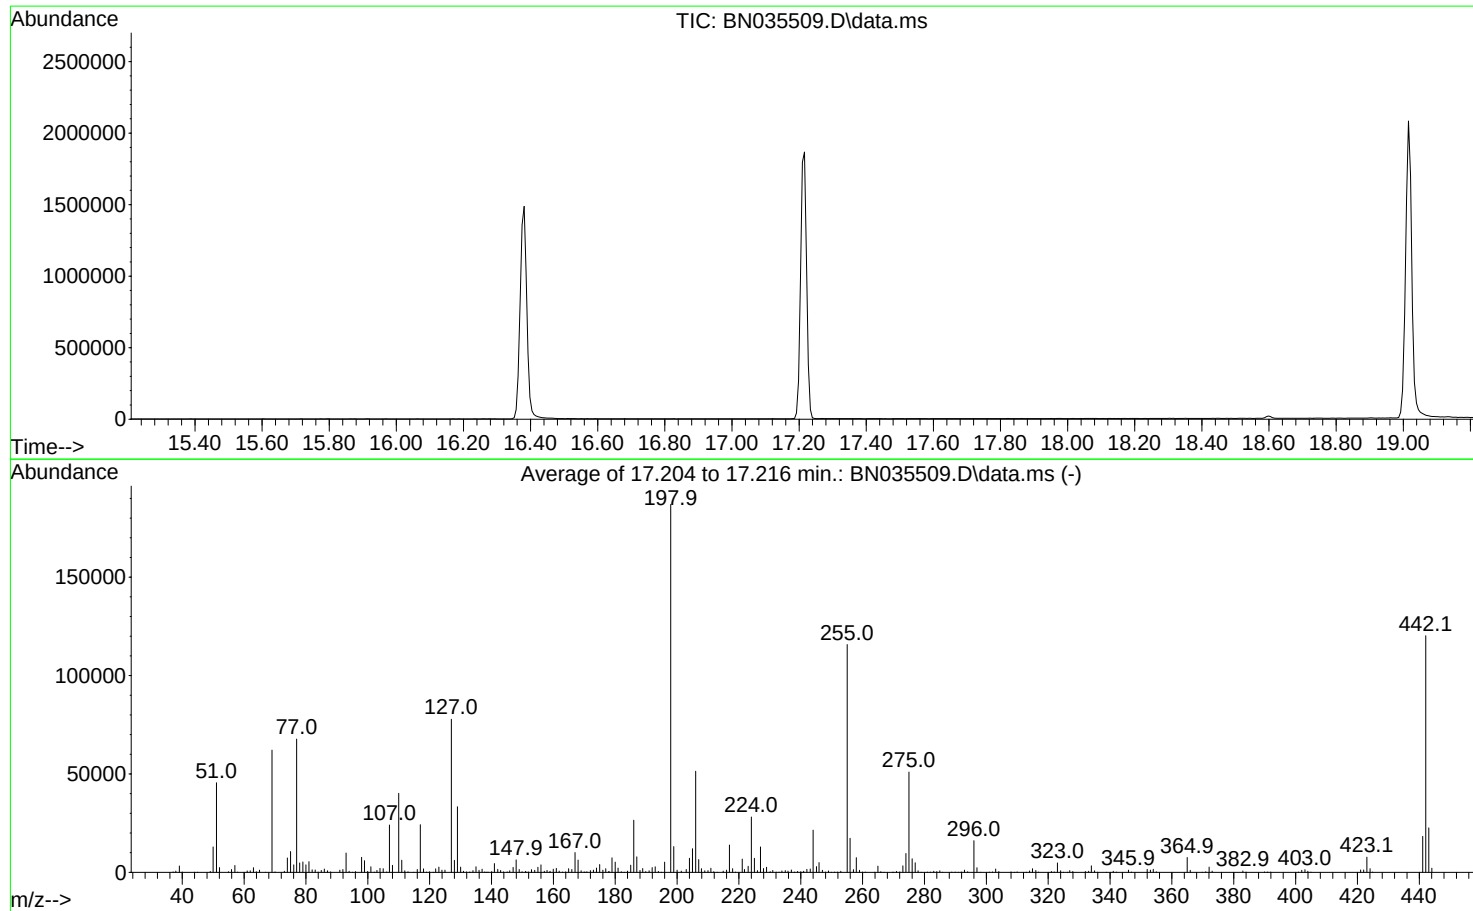

AutoFind: Scans 2434, 2435, 2436; Background Corrected with Scan 2428

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	45533	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.2	62101	PASS
70	69	0.00	2	0.4	269	PASS
127	198	10	80	41.6	77816	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	186941	PASS
199	198	5	9	7.0	13108	PASS
275	198	10	60	27.3	51029	PASS
365	198	1	100	4.1	7578	PASS
441	198	0.01	100	9.8	18314	PASS
442	442	50	100	100.0	120309	PASS
443	442	15	24	18.8	22619	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/9/2024	BNA_N	<u>BN035509.D</u>
Compound Name	Response	Retention Time
DDT	555028	20.274
DDD	56573	19.827
DDE	2168	19.316
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
58741	613769	9.57

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035509.D
Acq On : 09 Dec 2024 16:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 10 03:57:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 03:57:32 2024
Response via : Initial Calibration

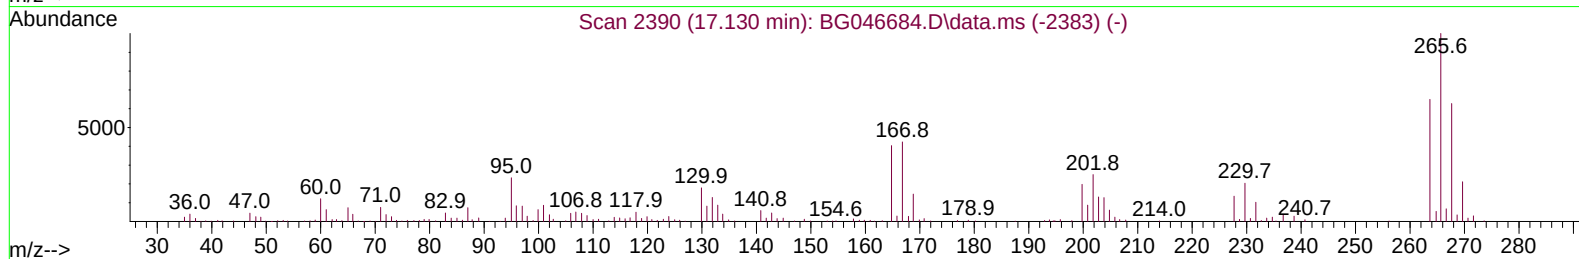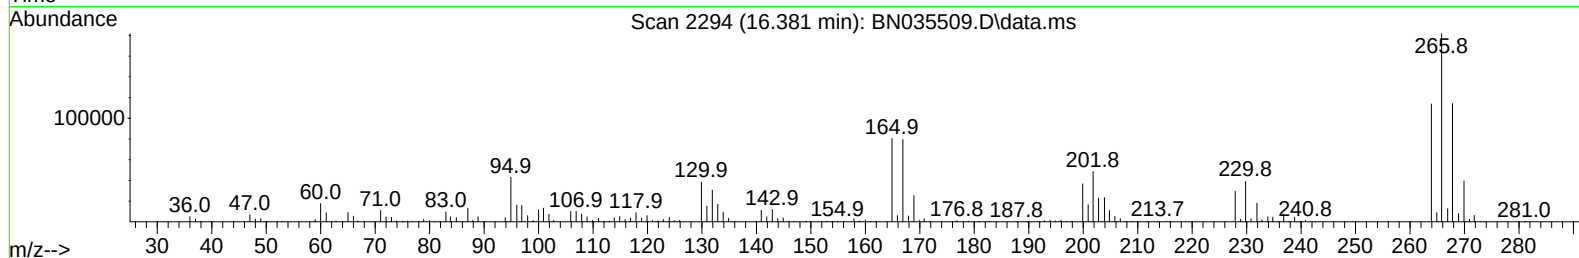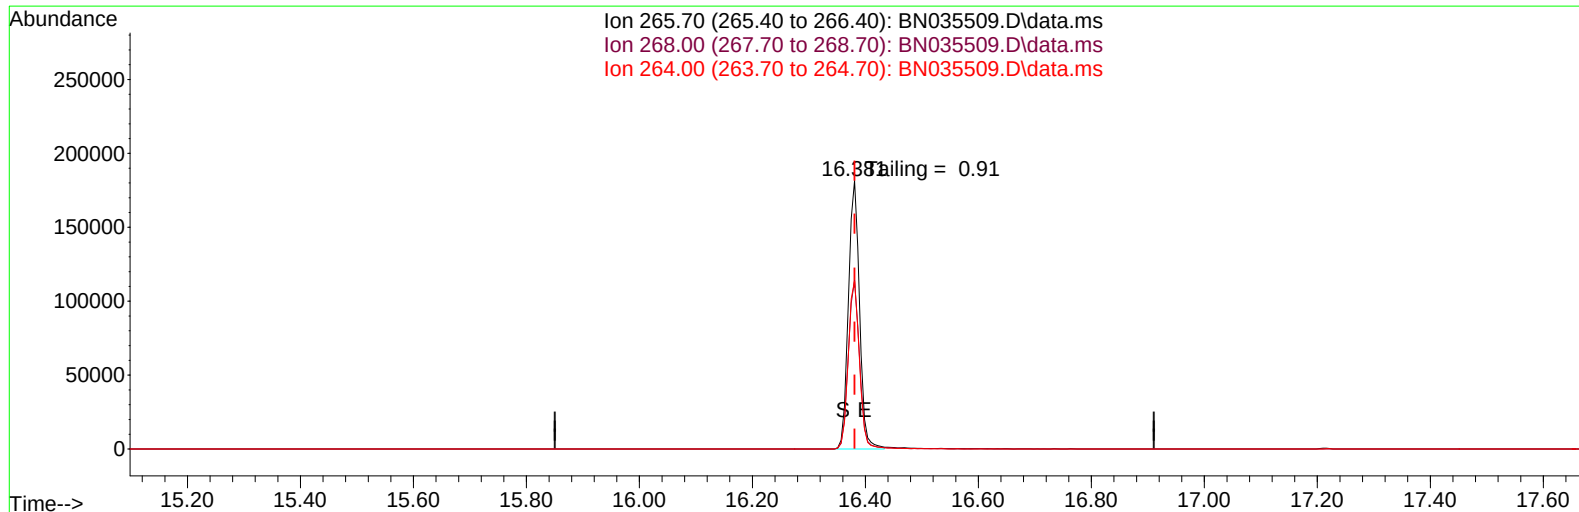

TIC: BN035509.D\data.ms

(70) Pentachlorophenol (C)

16.381min (0.000) 23065.04 ng




response 251964

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.83
264.00	61.60	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035509.D
Acq On : 09 Dec 2024 16:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 10 03:57:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 03:57:32 2024
Response via : Initial Calibration

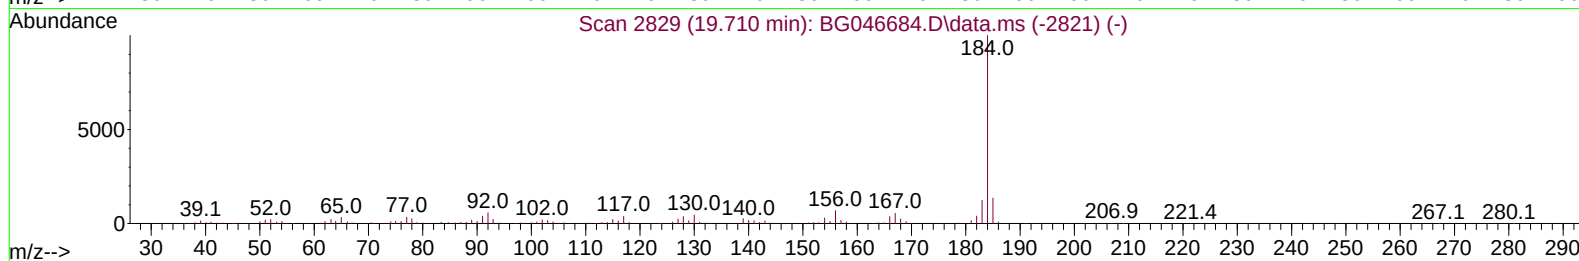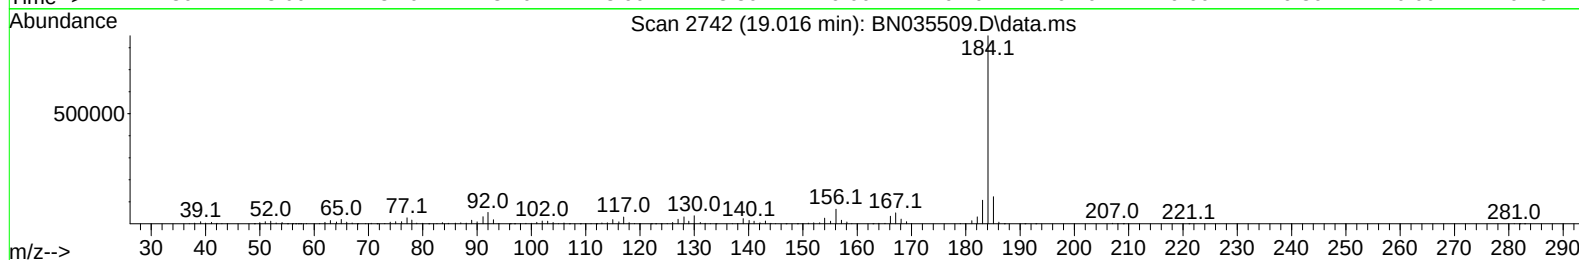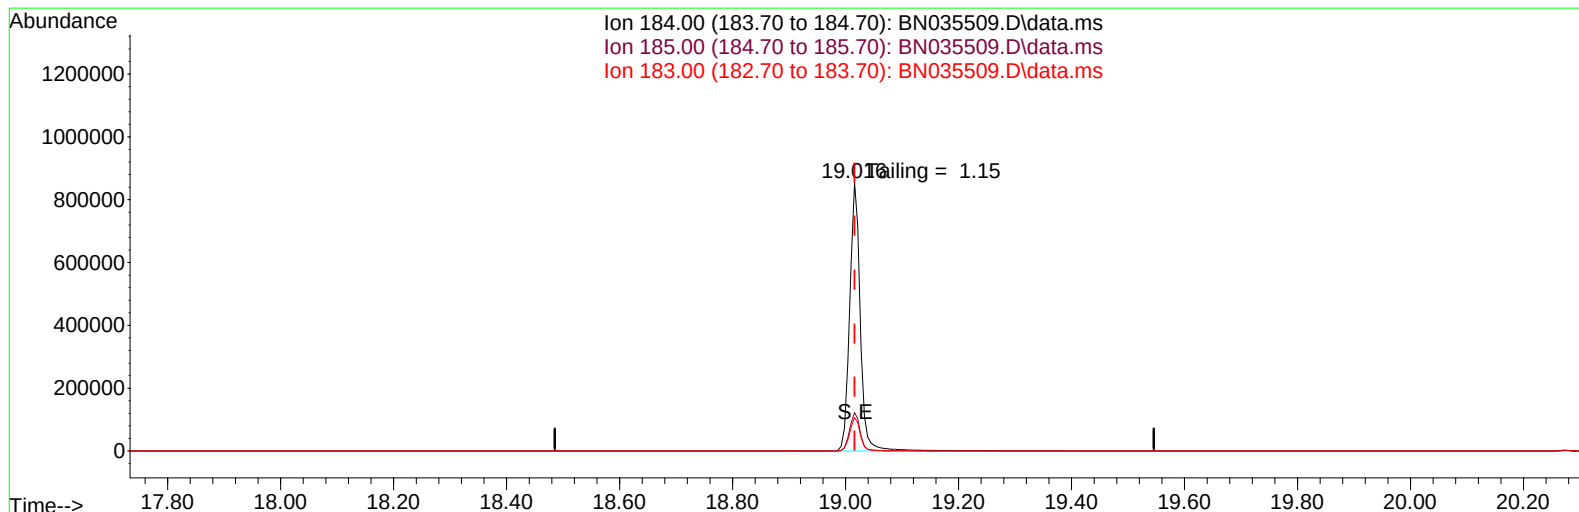

TIC: BN035509.D\data.ms

(77) Benzidine

19.016min (0.000) 0.00 ng

response 1117982

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	12.52
0.00	0.00	0.00