


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035524.D
Acq On : 10 Dec 2024 08:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 27 23:03:24 2024

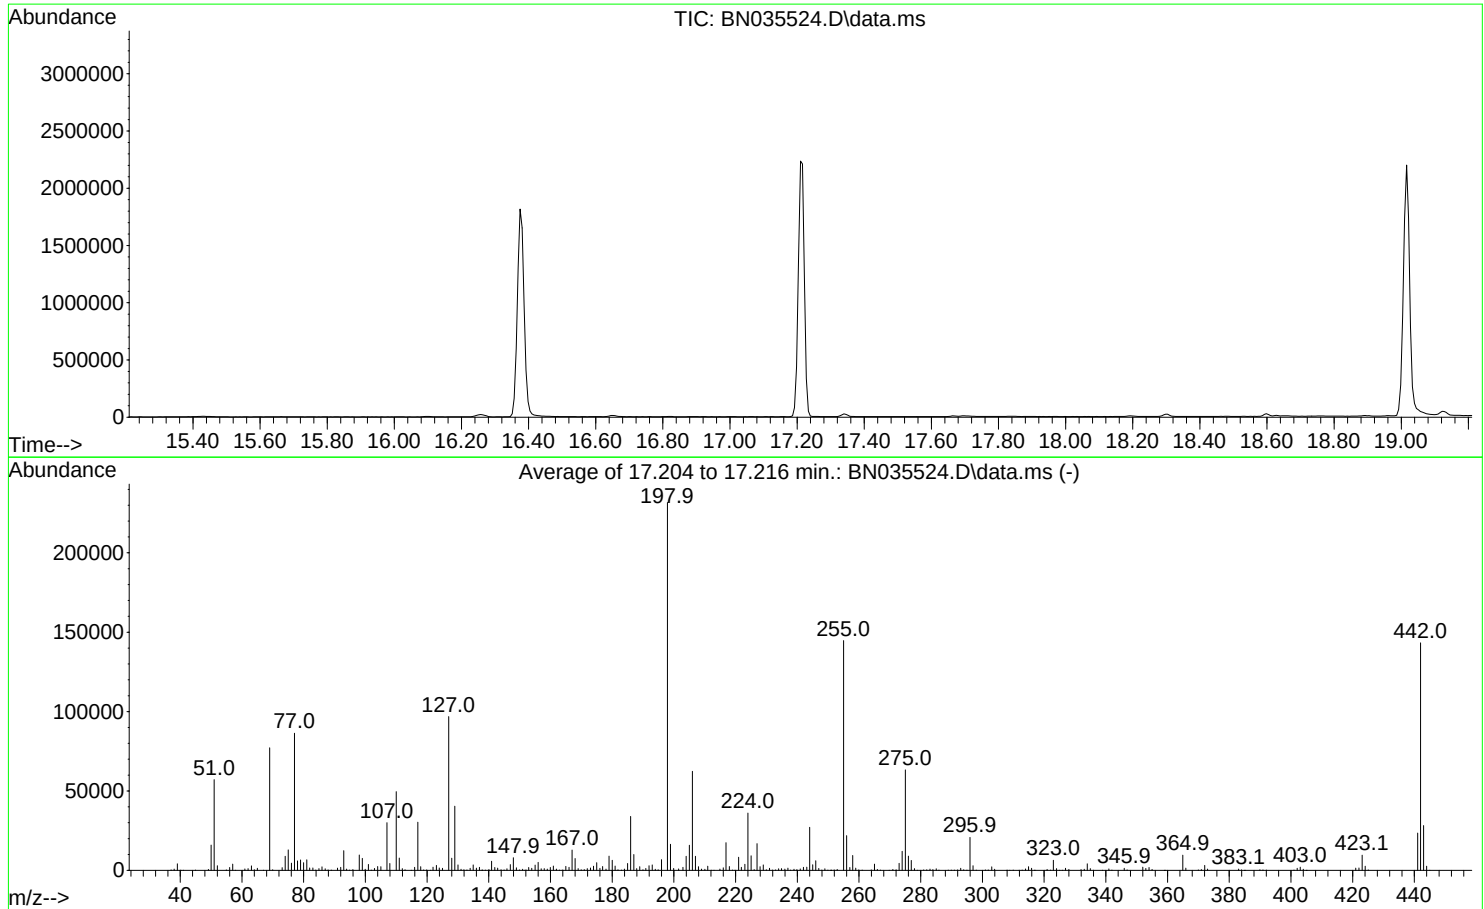

AutoFind: Scans 2434, 2435, 2436; Background Corrected with Scan 2428

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	57104	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.3	77235	PASS
70	69	0.00	2	0.6	434	PASS
127	198	10	80	41.8	96816	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	231701	PASS
199	198	5	9	7.1	16431	PASS
275	198	10	60	27.3	63328	PASS
365	198	1	100	4.1	9588	PASS
441	198	0.01	100	10.1	23464	PASS
442	442	50	100	100.0	143315	PASS
443	442	15	24	19.7	28188	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/9/2024	BNA_N	<u>BN035524.D</u>
Compound Name	Response	Retention Time
DDT	684763	20.275
DDD	62588	19.828
DDE	4137	19.31
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
66725	751488	8.88

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035524.D
Acq On : 10 Dec 2024 08:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 11 06:13:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 06:13:05 2024
Response via : Initial Calibration

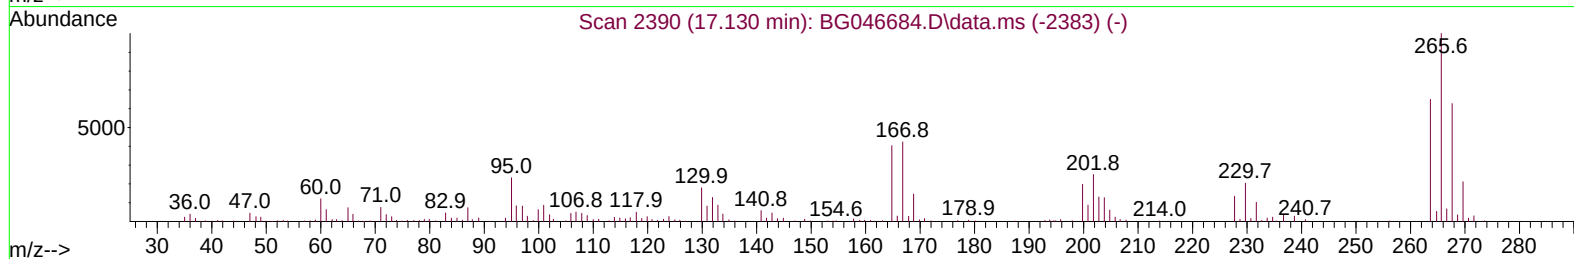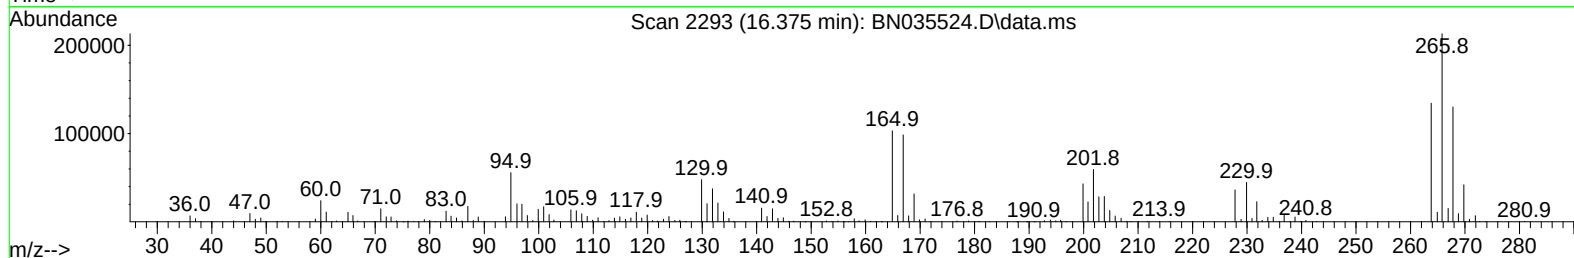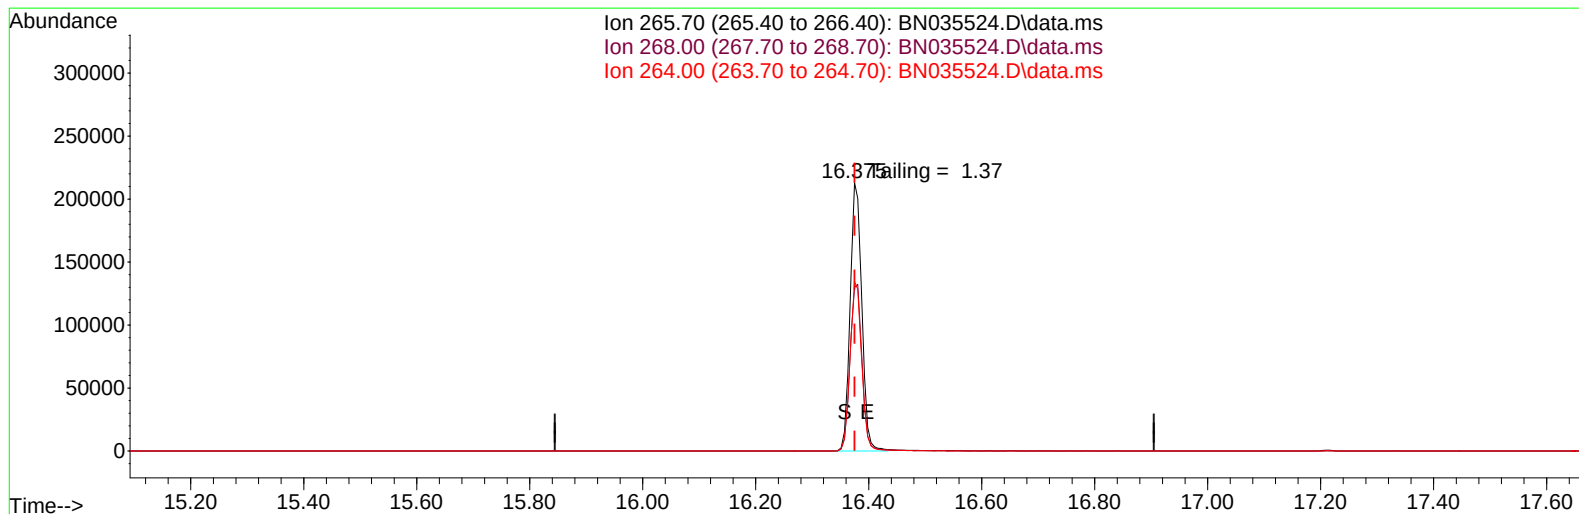

TIC: BN035524.D\data.ms

(70) Pentachlorophenol (C)

16.375min (0.000) 25281.71 ng




response 307527

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.01
264.00	61.60	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120924\
Data File : BN035524.D
Acq On : 10 Dec 2024 08:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 11 06:13:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 06:13:05 2024
Response via : Initial Calibration

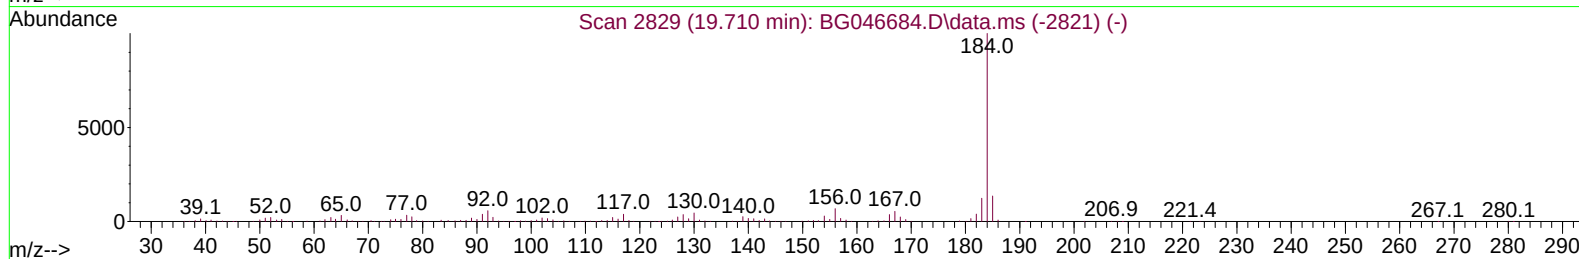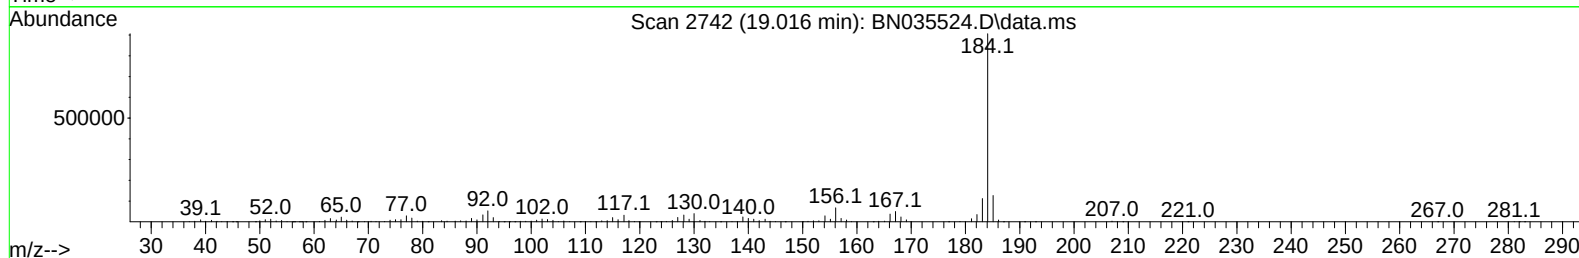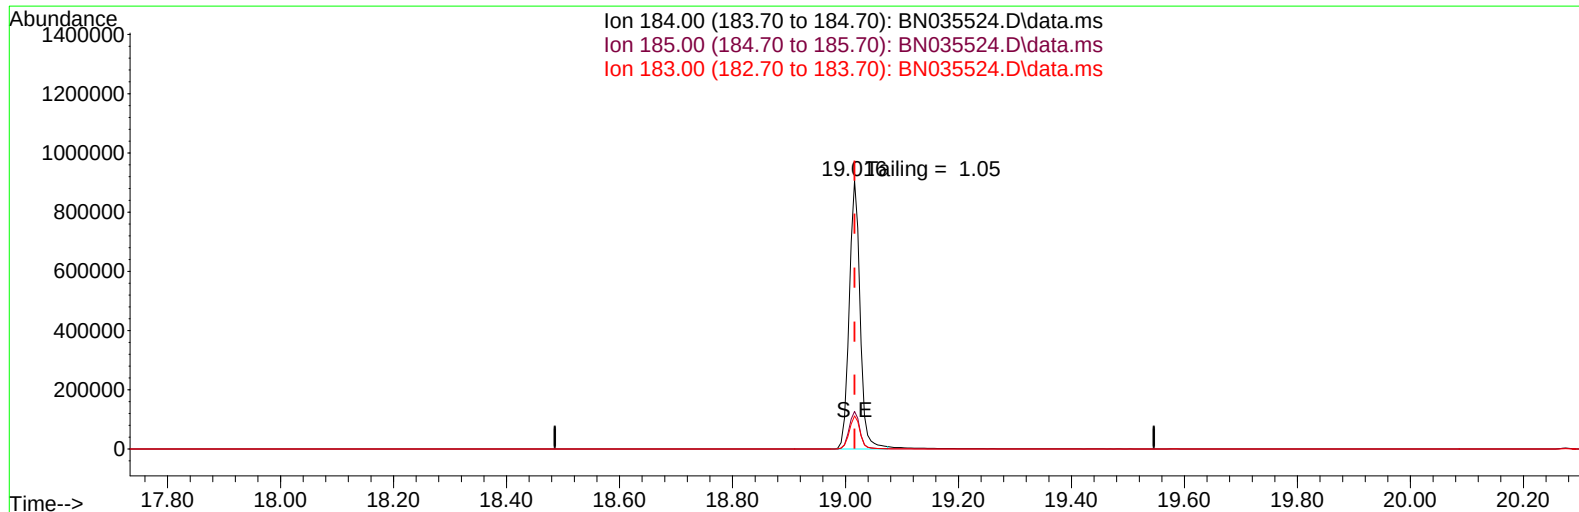

TIC: BN035524.D\data.ms

(77) Benzidine

19.016min (0.000) 0.00 ng

response 1233878

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	12.36
0.00	0.00	0.00