
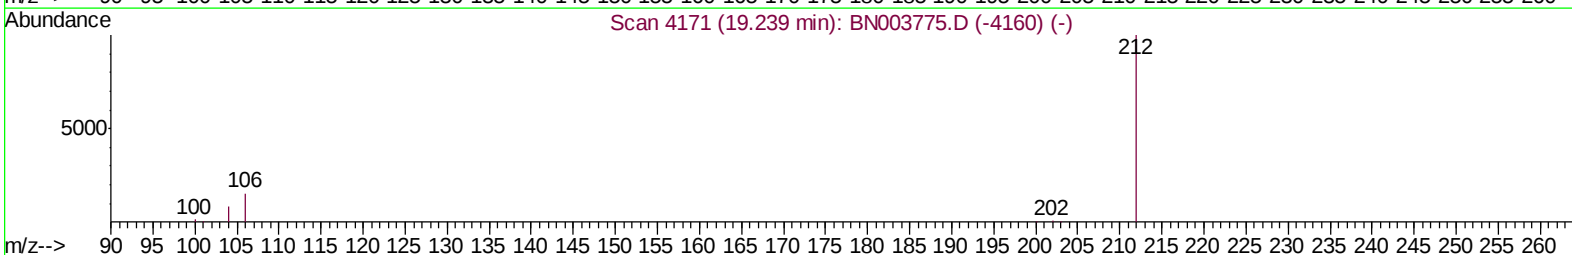
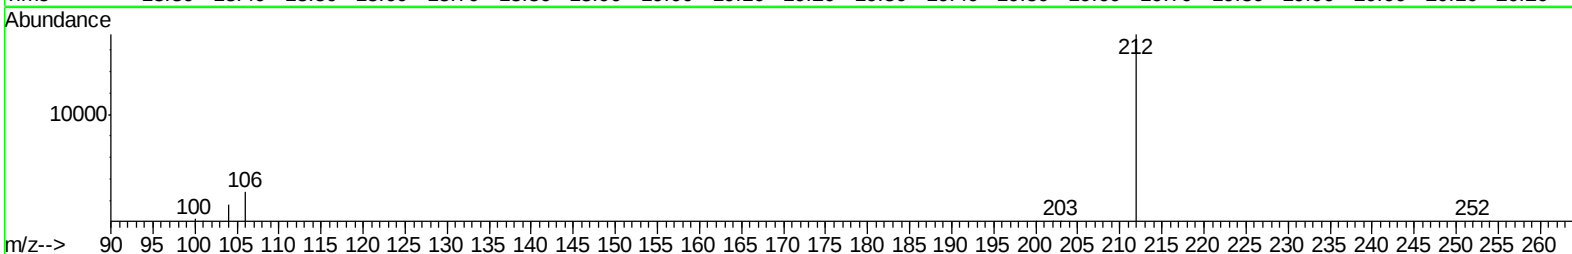


Data File : BN003778.D
Acq On : 10 Dec 2018 14:47
Operator : JU/SJ
Sample : PB115353BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 11 04:01:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 03:42:06 2018
Response via : Initial Calibration

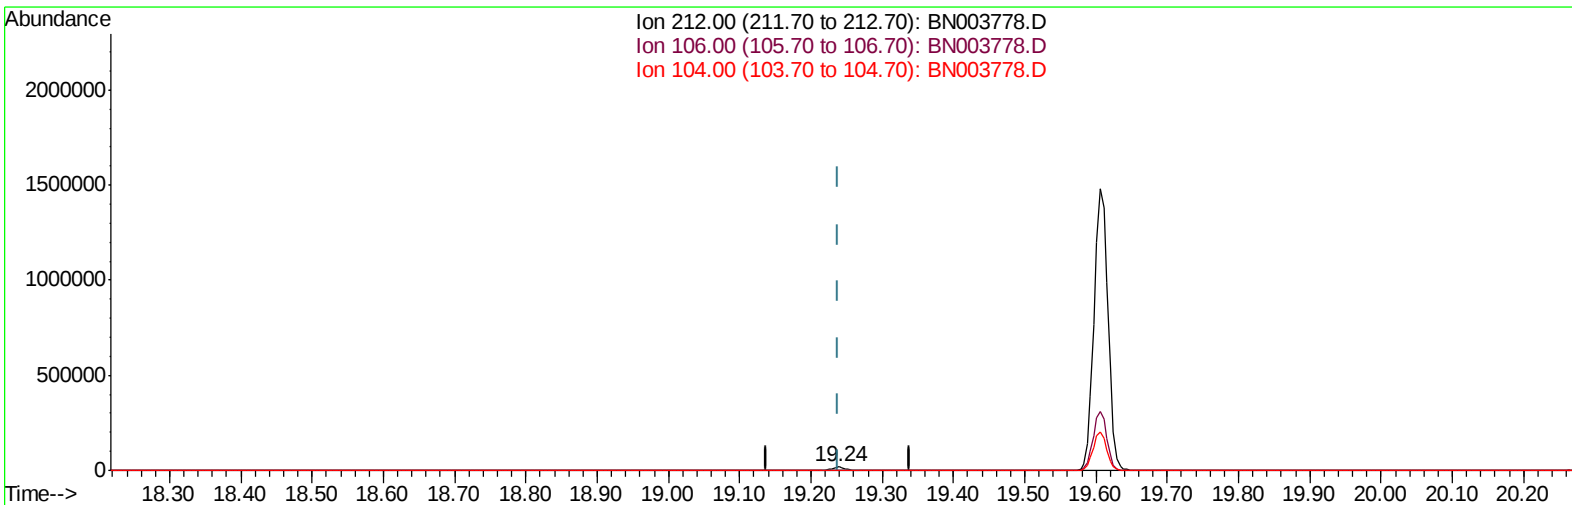

TIC: BN003778.D

(14) Fluoranthene-d10 (SURR)

19.239min (+0.000) 0.30ng/ul m

response 22942

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00