
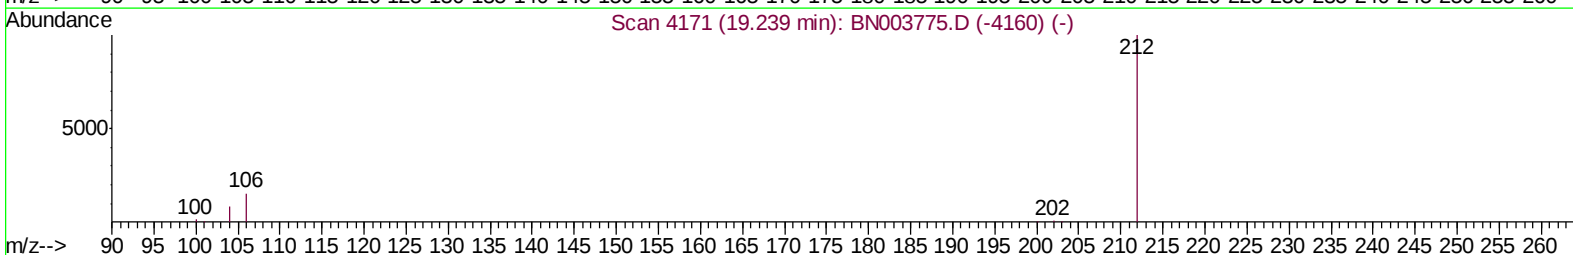
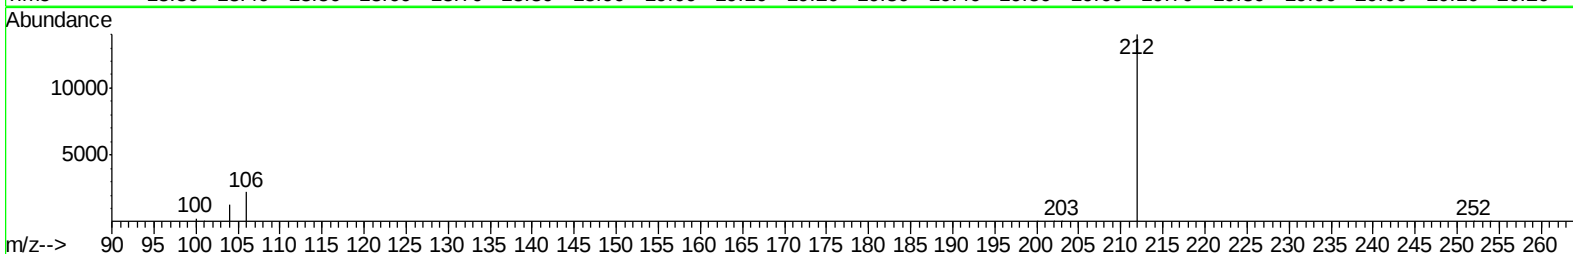


Data File : BN003780.D  
Acq On : 10 Dec 2018 15:57  
Operator : JU/SJ  
Sample : PB115355BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Dec 11 04:05:39 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 11 03:42:06 2018  
Response via : Initial Calibration

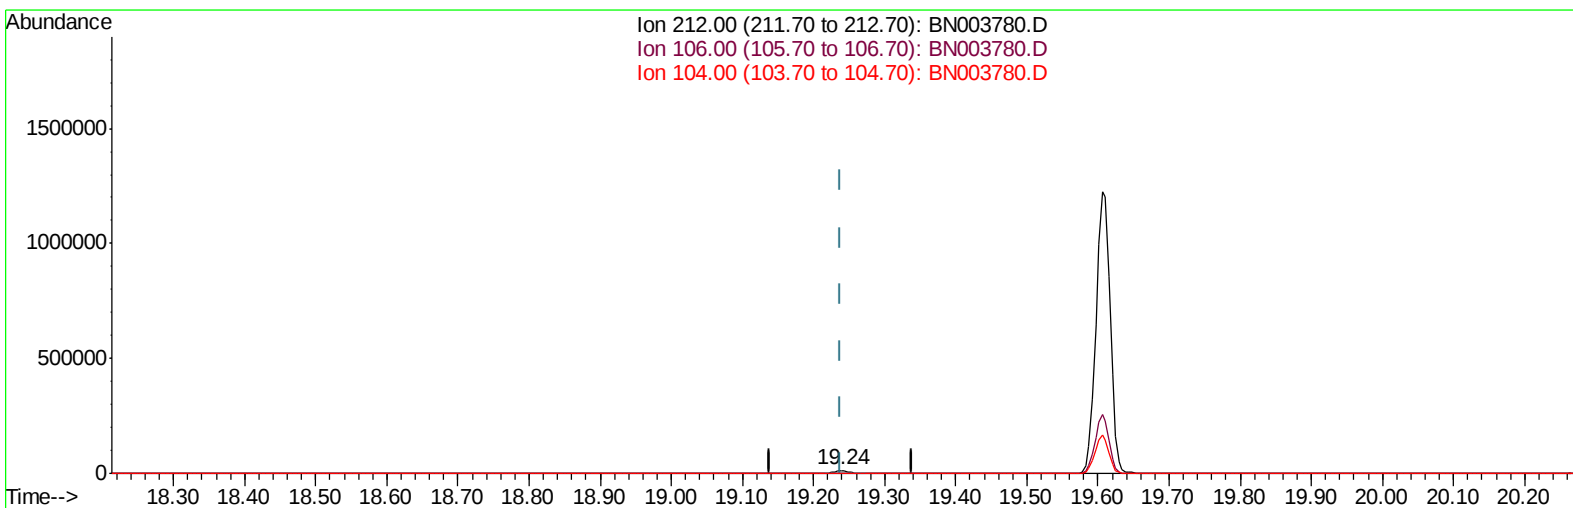

TIC: BN003780.D

(14) Fluoranthene-d10 (SURR)

19.239min (+0.000) 0.29ng/ul m

response 18581

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 212.00 | 100   | 100   |
| 106.00 | 14.20 | 0.00# |
| 104.00 | 8.00  | 0.00# |
| 0.00   | 0.00  | 0.00  |