

Data File : BN003781.D

Acq On : 10 Dec 2018 16:32

Operator : JU/SJ

Sample : J6155-14

Misc :

ALS Vial : 8 Sample Multiplier: 1




Quant Time: Dec 11 04:08:34 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 11 03:42:06 2018

Response via : Initial Calibration

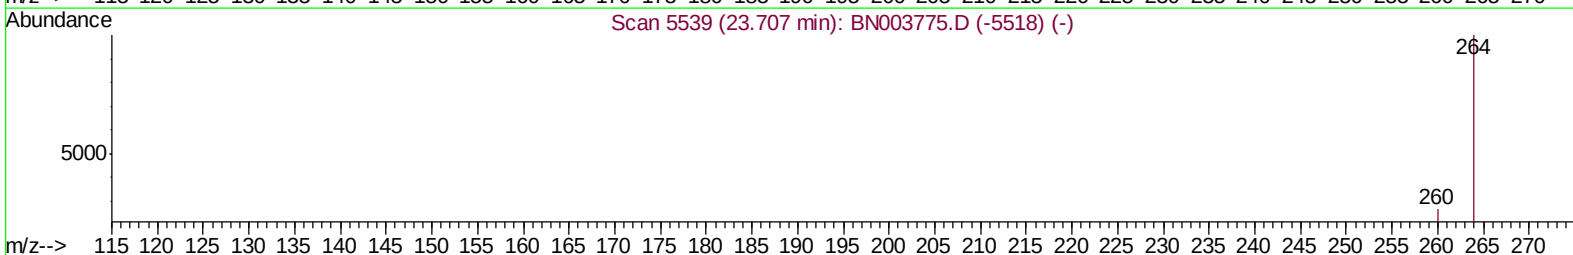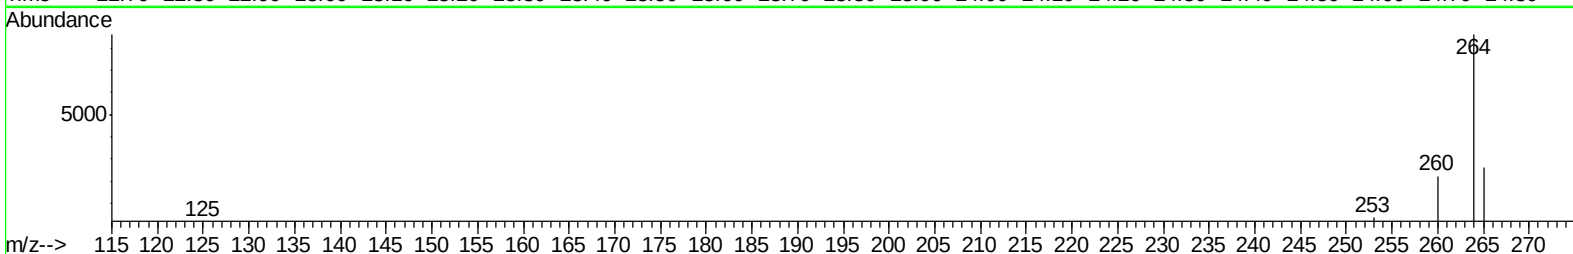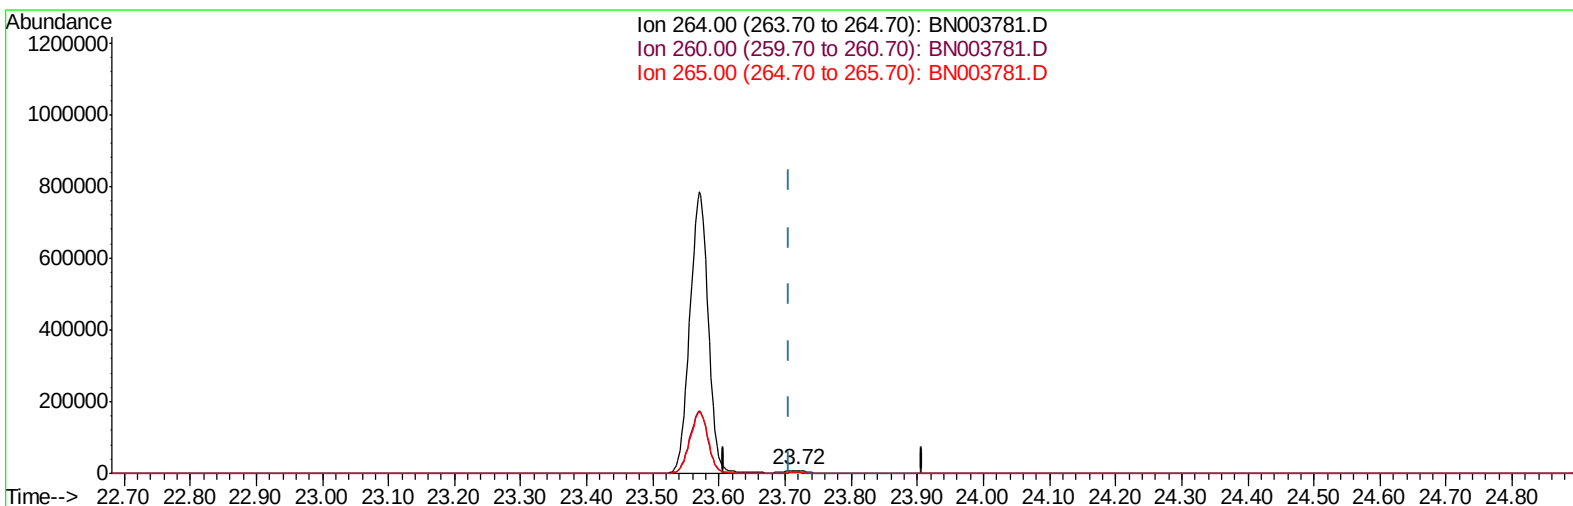

TIC: BN003781.D

(20) Perylene-d12 (I)

23.716min (+0.009) 0.40ng/ul

response 19909

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	25.96
265.00	33.50	30.16
0.00	0.00	0.00