
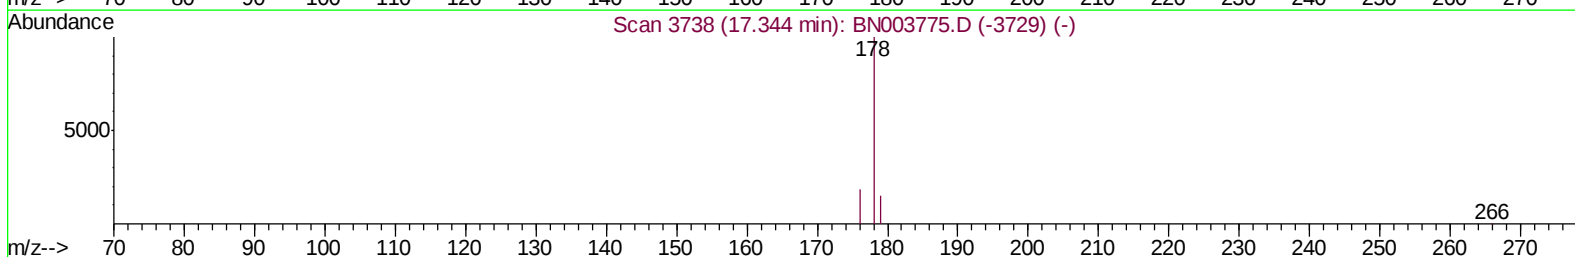
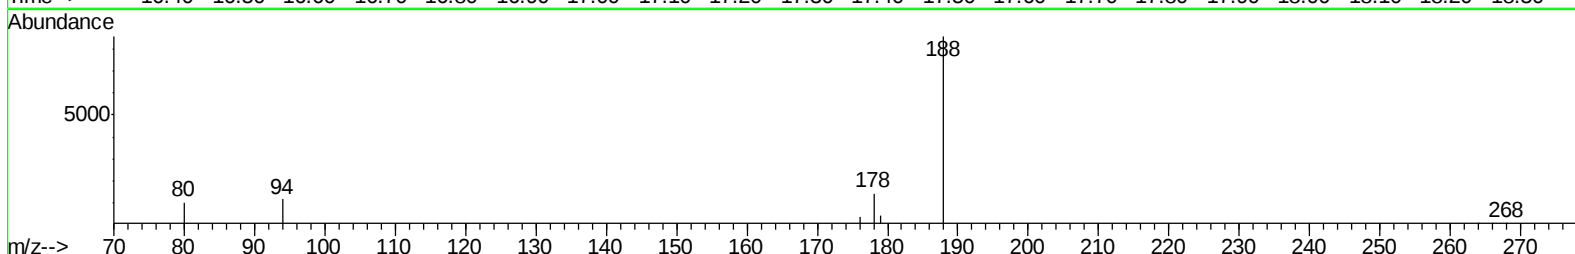


Data File : BN003784.D
Acq On : 10 Dec 2018 18:18
Operator : JU/SJ
Sample : J6155-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Dec 11 04:14:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 03:42:06 2018
Response via : Initial Calibration

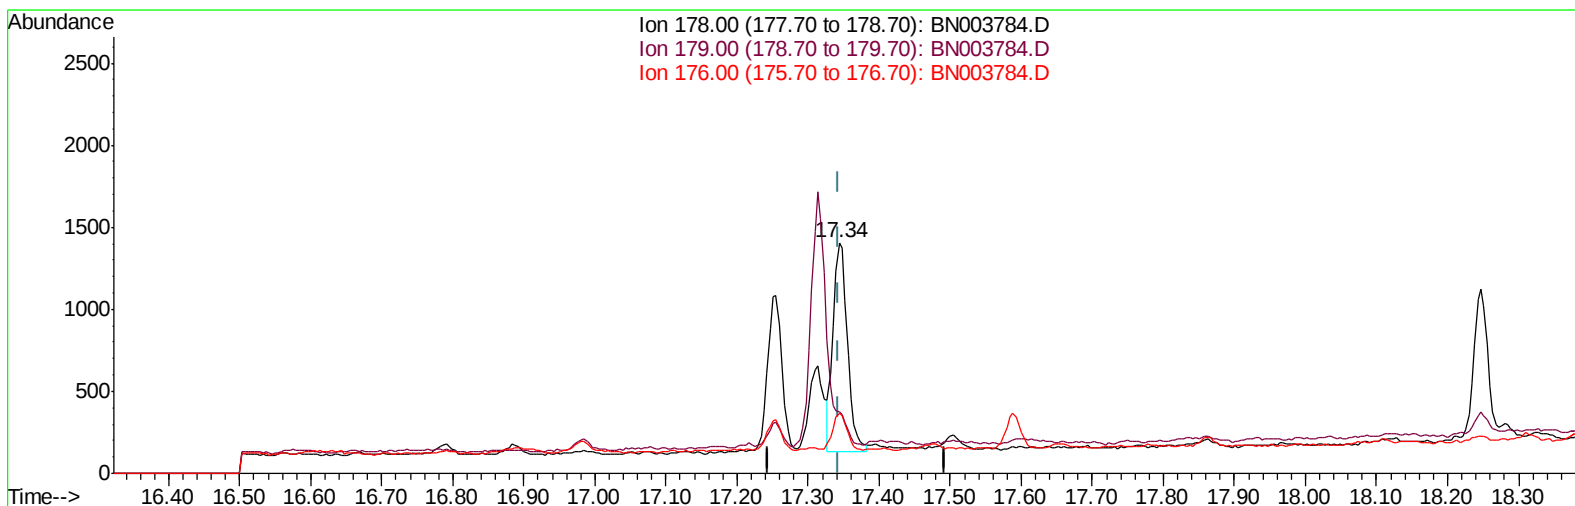

TIC: BN003784.D

(13) Anthracene

17.343min (-0.000) 0.02ng/ul m

response 1797

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	26.88#
176.00	18.50	25.89#
0.00	0.00	0.00