
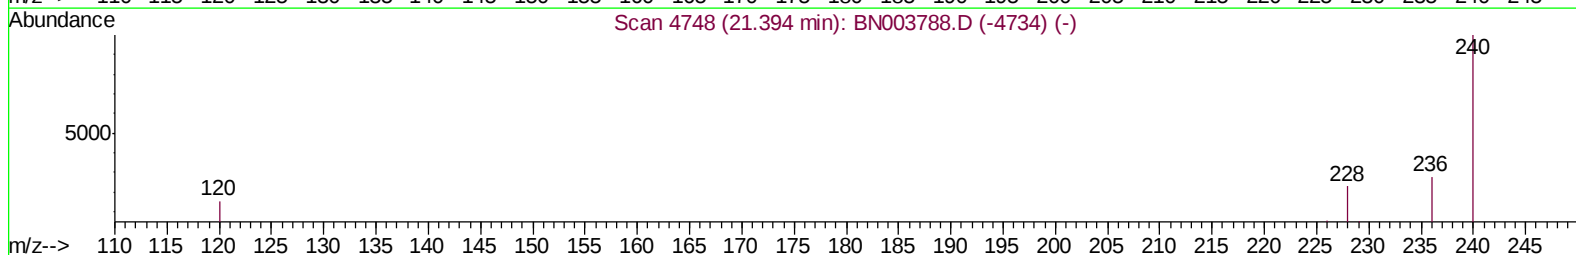
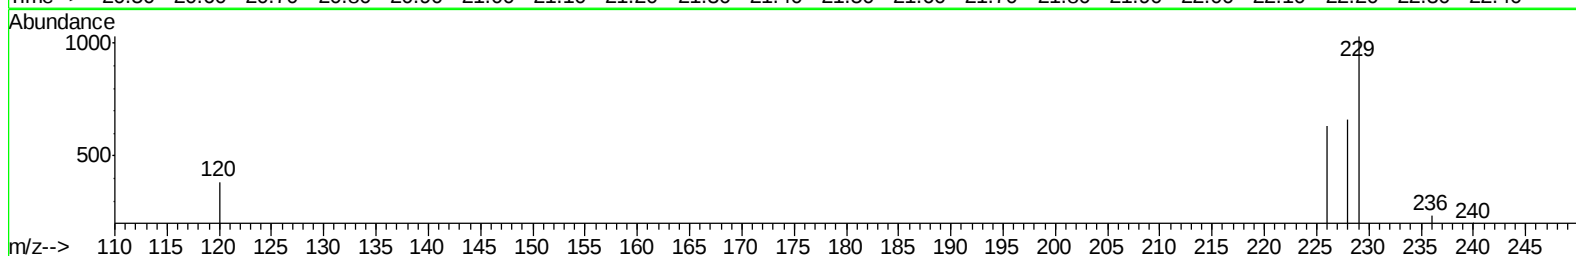


Data File : BN003789.D
Acq On : 10 Dec 2018 21:49
Operator : JU/SJ
Sample : J6077-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 11 04:34:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

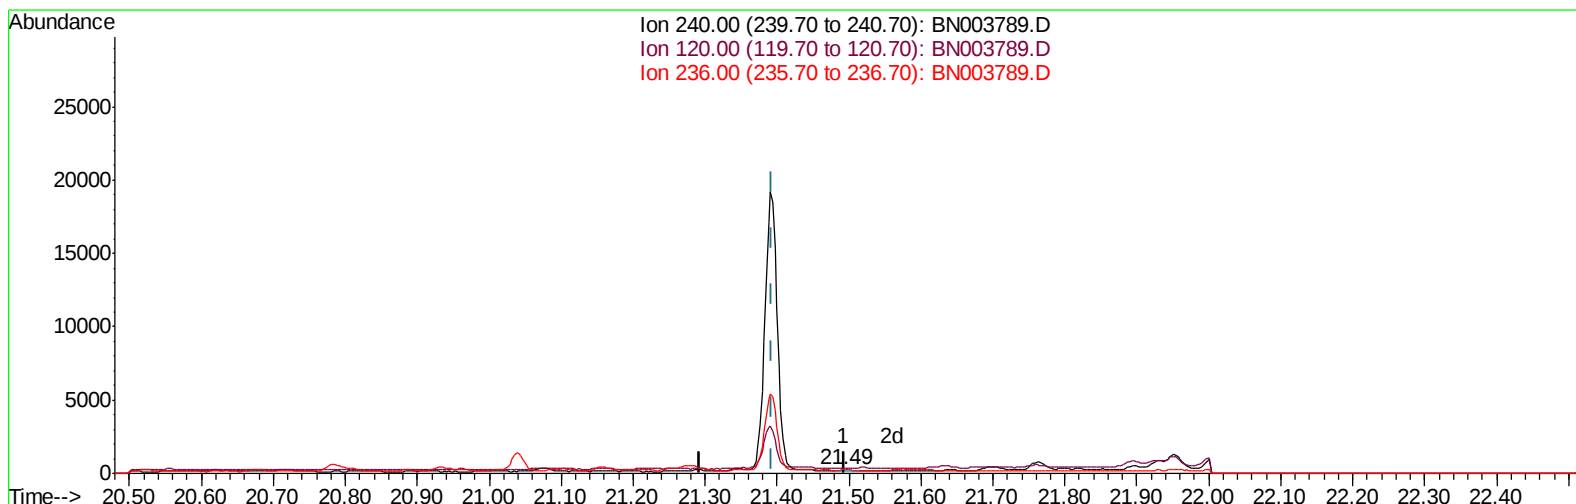

TIC: BN003789.D

(16) Chrysene-d12 (I)

21.493min (+0.099) 0.40ng/ul

response 16

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	190.10#
236.00	27.60	116.34#
0.00	0.00	0.00