
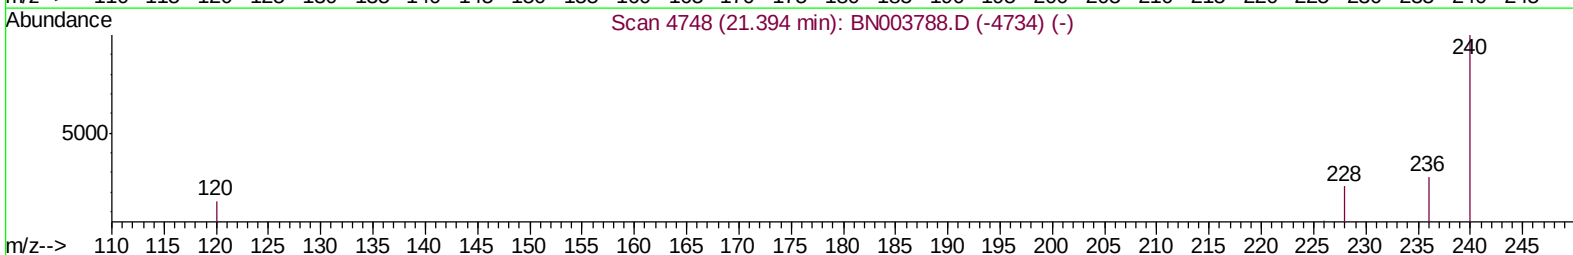
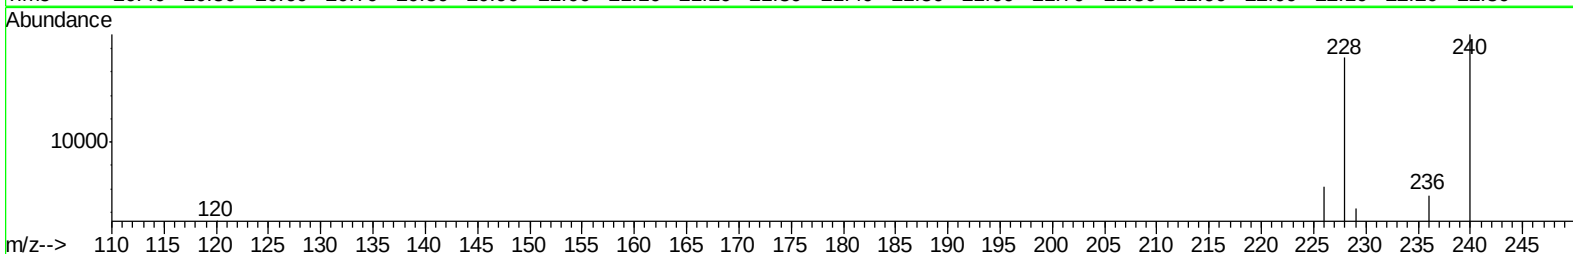


Data File : BN003789.D  
Acq On : 10 Dec 2018 21:49  
Operator : JU/SJ  
Sample : J6077-11  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 11 04:34:04 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 11 04:22:54 2018  
Response via : Initial Calibration

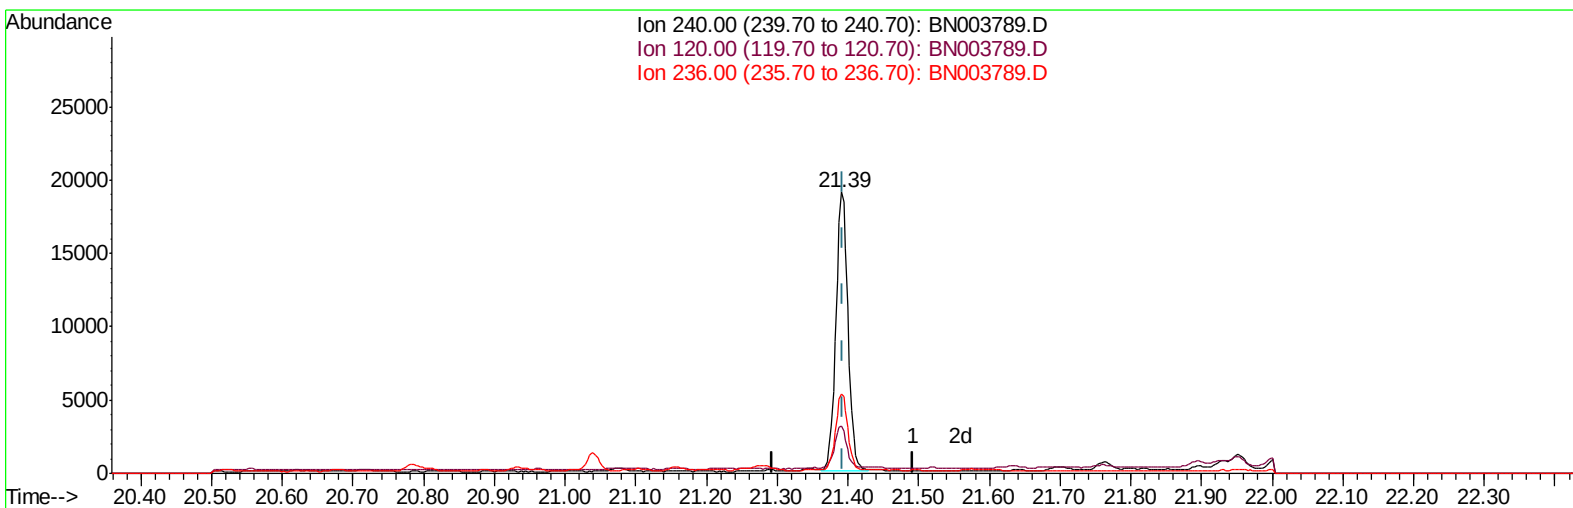

TIC: BN003789.D

(16) Chrysene-d12 (I)

21.391min (-0.003) 0.40ng/ul m

response 22513

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 240.00 | 100   | 100    |
| 120.00 | 14.00 | 16.88# |
| 236.00 | 27.60 | 28.36  |
| 0.00   | 0.00  | 0.00   |