
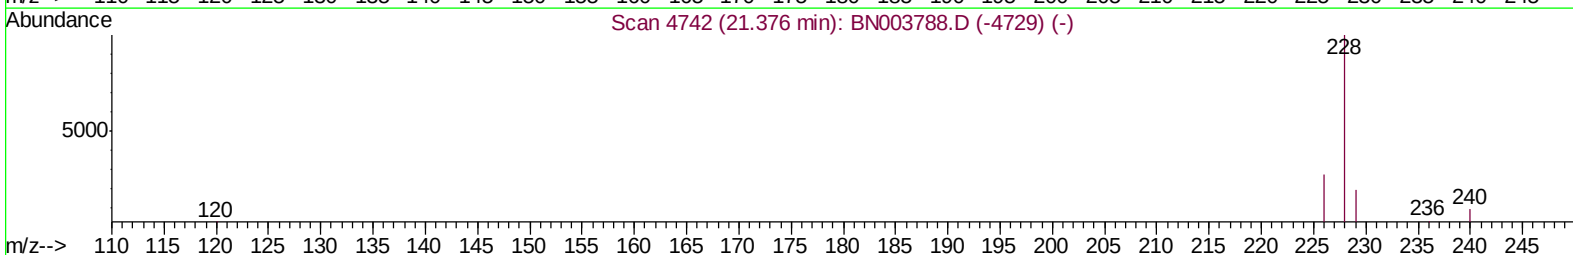
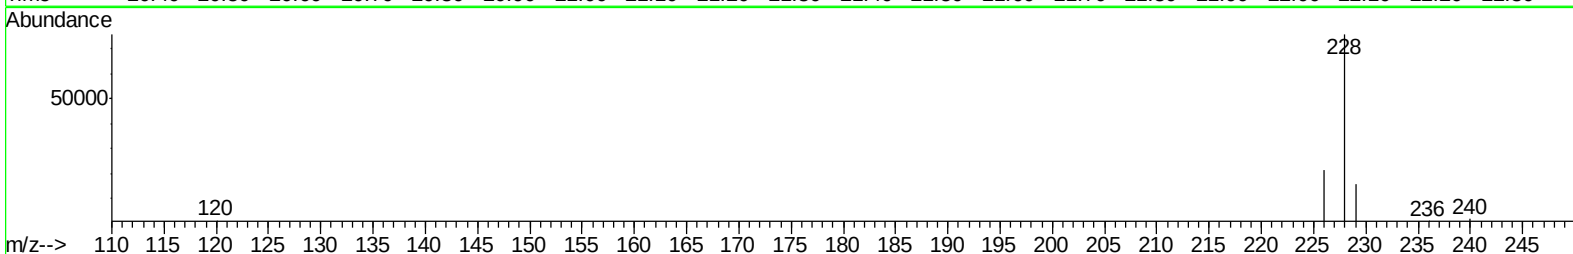


Data File : BN003789.D
Acq On : 10 Dec 2018 21:49
Operator : JU/SJ
Sample : J6077-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 11 04:35:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

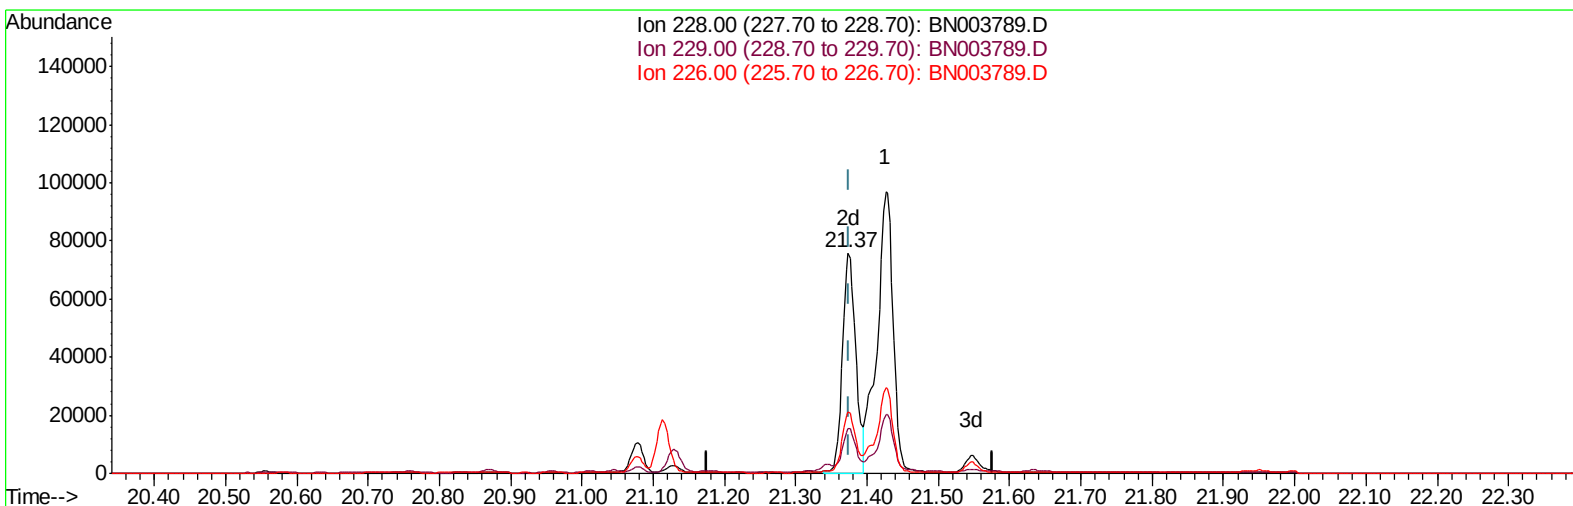

TIC: BN003789.D

(18) Benzo(a)anthracene
21.373min (-0.003) 1.38ng/ul m
response 98283

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	20.46
226.00	26.40	27.93
0.00	0.00	0.00