
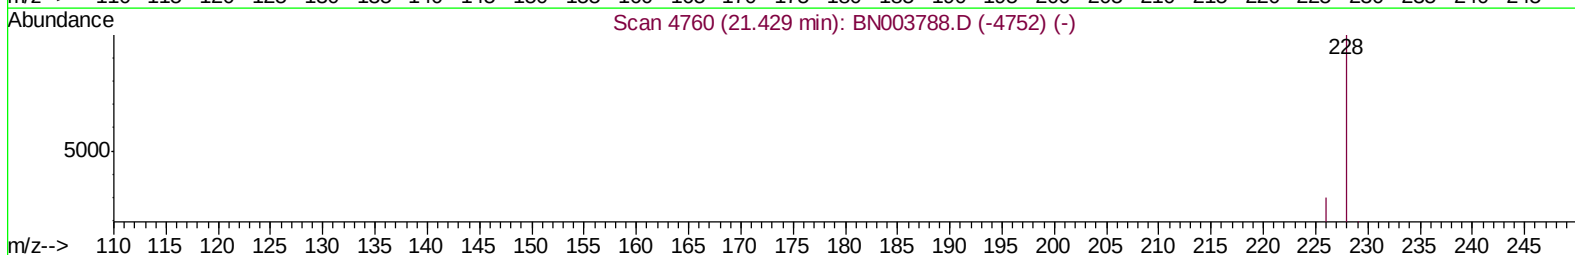
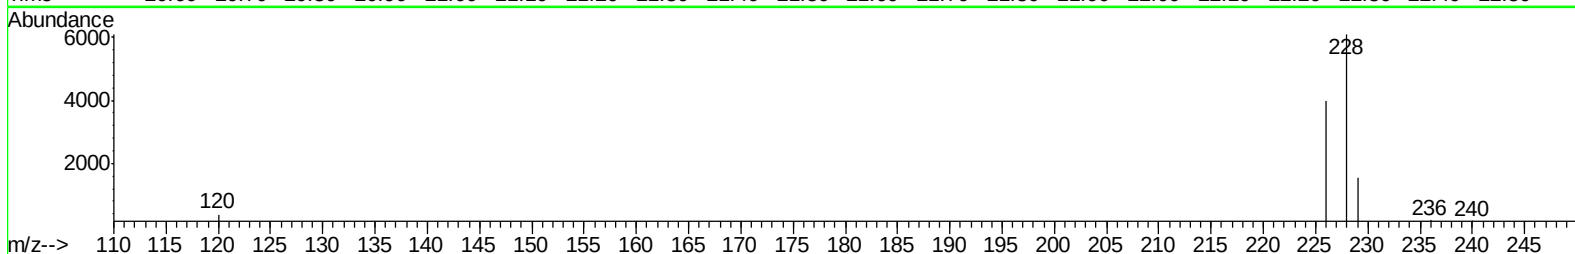


Data File : BN003789.D
Acq On : 10 Dec 2018 21:49
Operator : JU/SJ
Sample : J6077-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 11 04:35:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

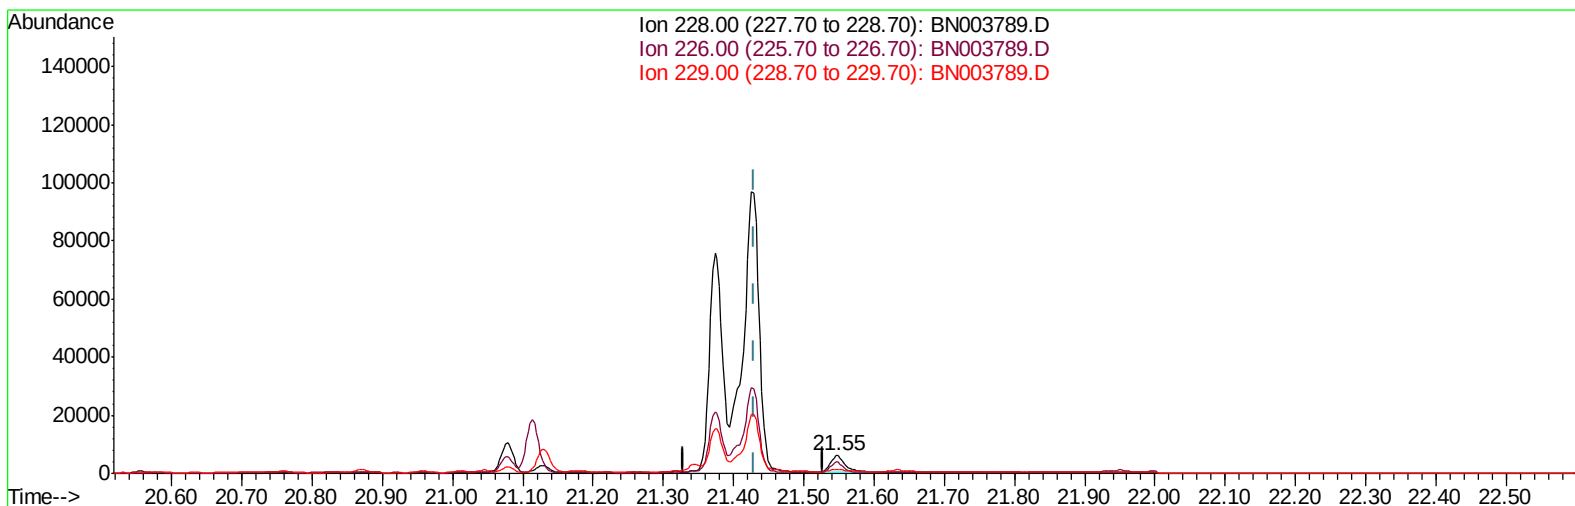

TIC: BN003789.D

(19) Chrysene

21.546min (+0.117) 0.10ng/ul

response 8118

Ion	Exp%	Act%
228.00	100	100
226.00	30.00	65.22#
229.00	19.60	25.11#
0.00	0.00	0.00