
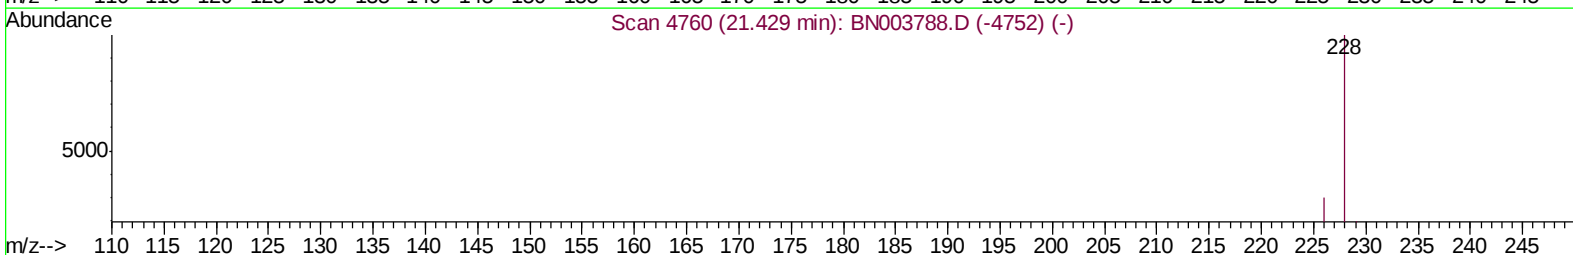
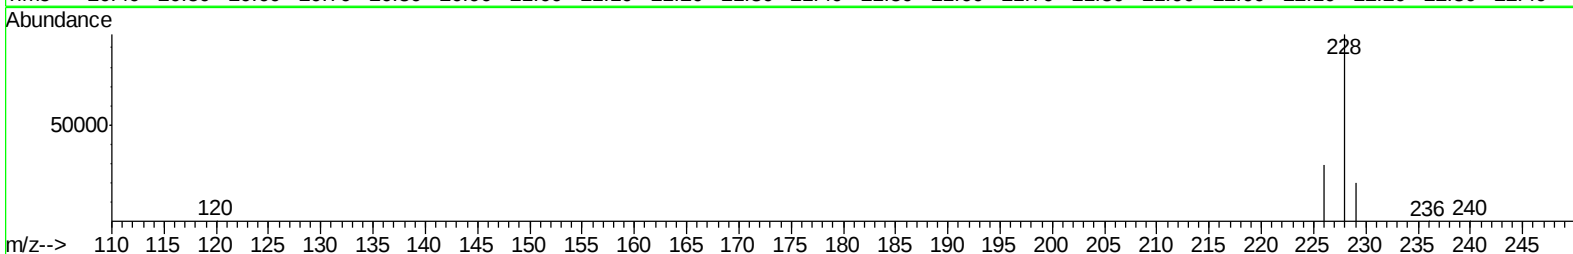


Data File : BN003789.D  
Acq On : 10 Dec 2018 21:49  
Operator : JU/SJ  
Sample : J6077-11  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 11 04:35:42 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 11 04:22:54 2018  
Response via : Initial Calibration

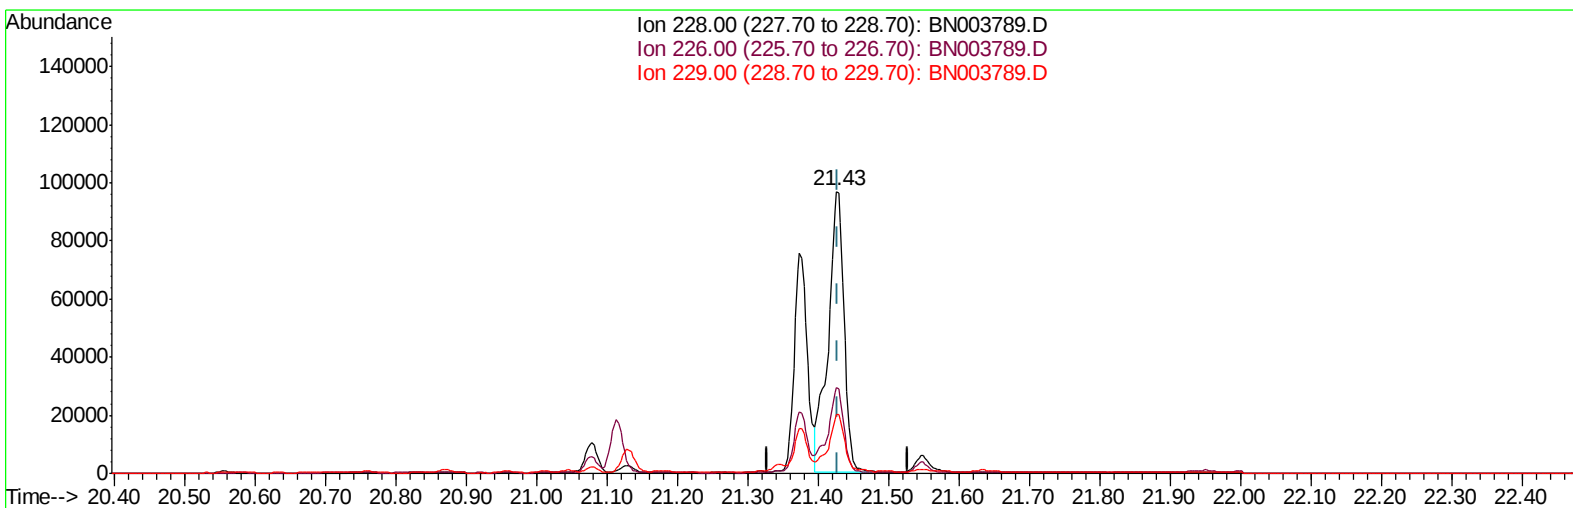

TIC: BN003789.D

(19) Chrysene

21.426min (-0.003) 1.88ng/ul m

response 153054

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 228.00 | 100   | 100   |
| 226.00 | 30.00 | 30.32 |
| 229.00 | 19.60 | 21.10 |
| 0.00   | 0.00  | 0.00  |