
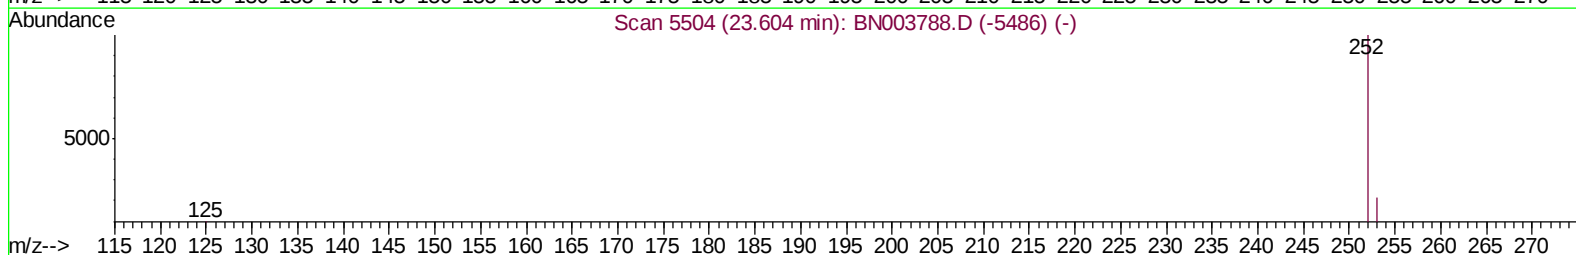
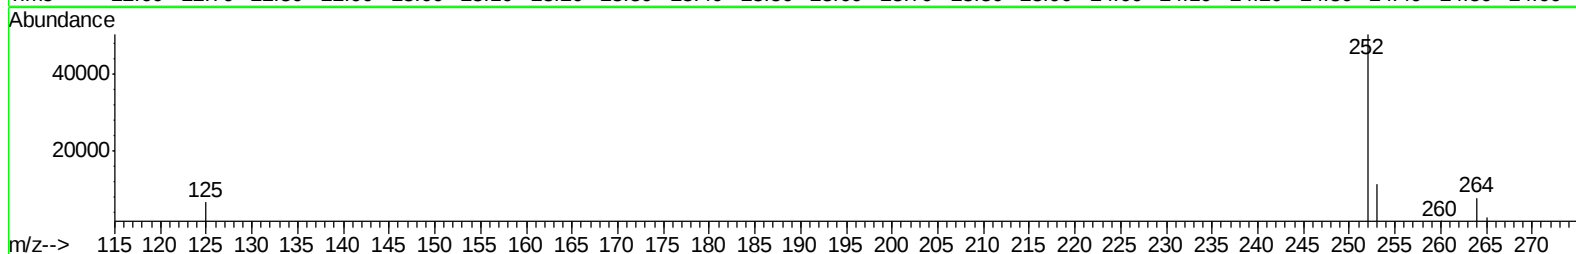


Data File : BN003789.D
Acq On : 10 Dec 2018 21:49
Operator : JU/SJ
Sample : J6077-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 11 04:36:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

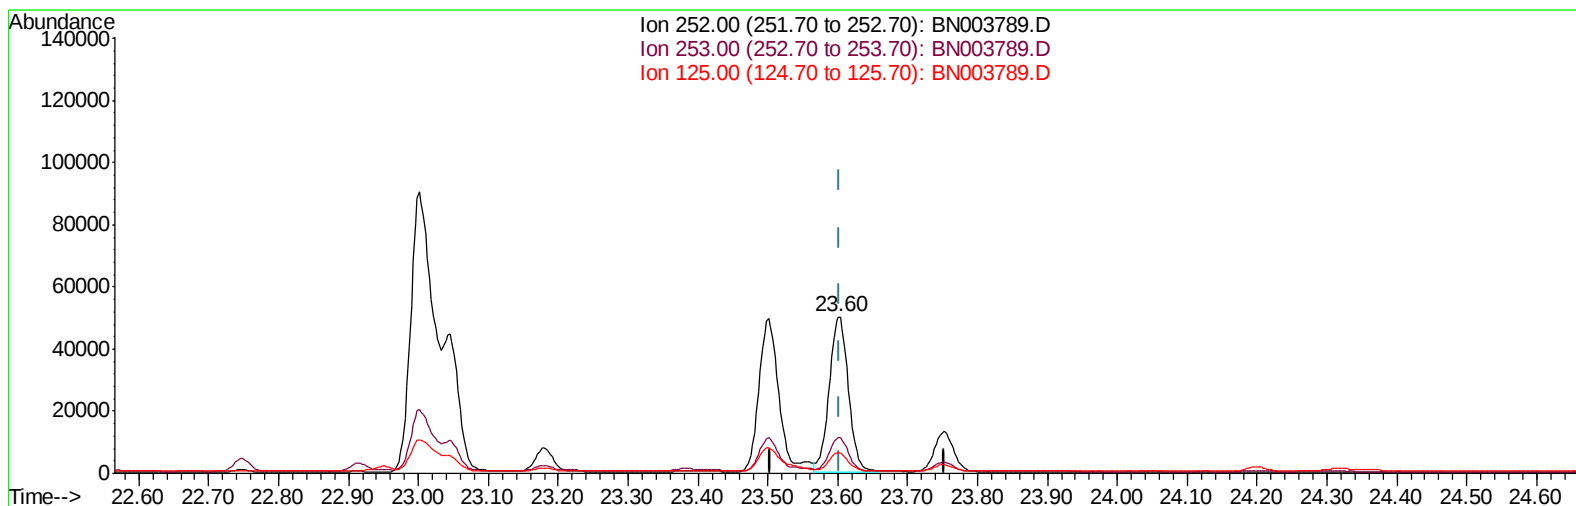

TIC: BN003789.D

(23) Benzo(a)pyrene (C)

23.601min (-0.003) 1.53ng/ul m

response 94404

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	23.00
125.00	12.80	13.35
0.00	0.00	0.00