
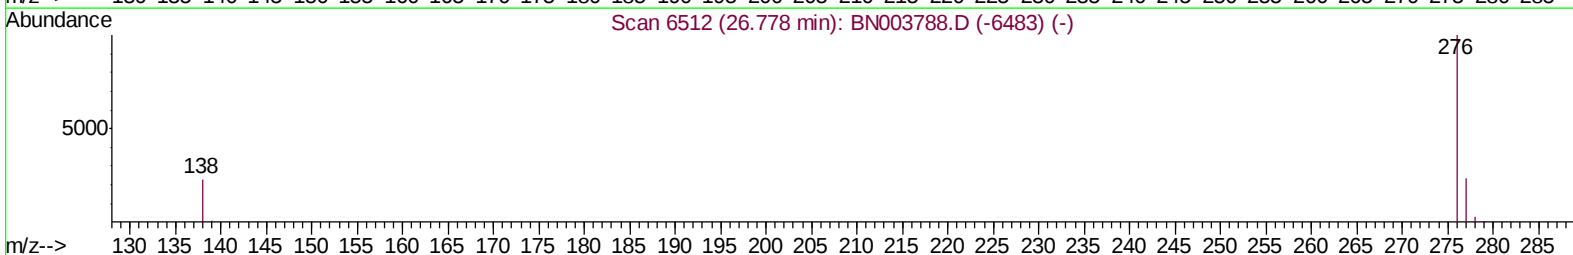
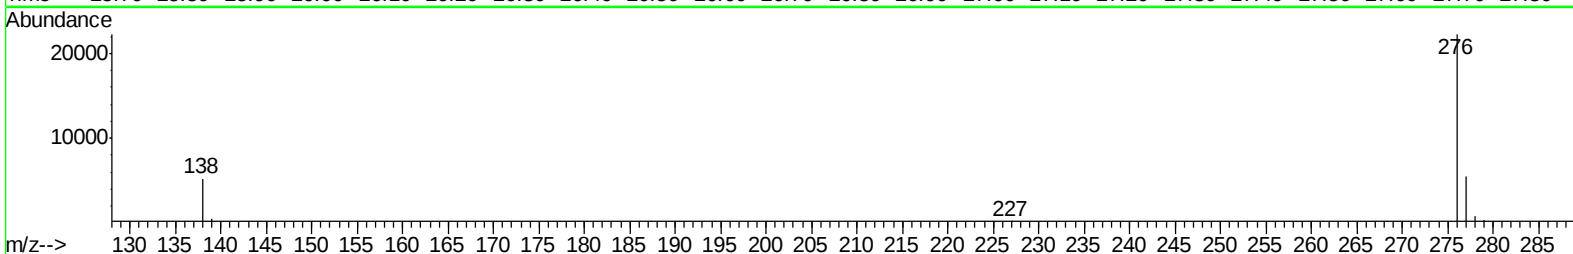


Data File : BN003789.D
Acq On : 10 Dec 2018 21:49
Operator : JU/SJ
Sample : J6077-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 11 04:36:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

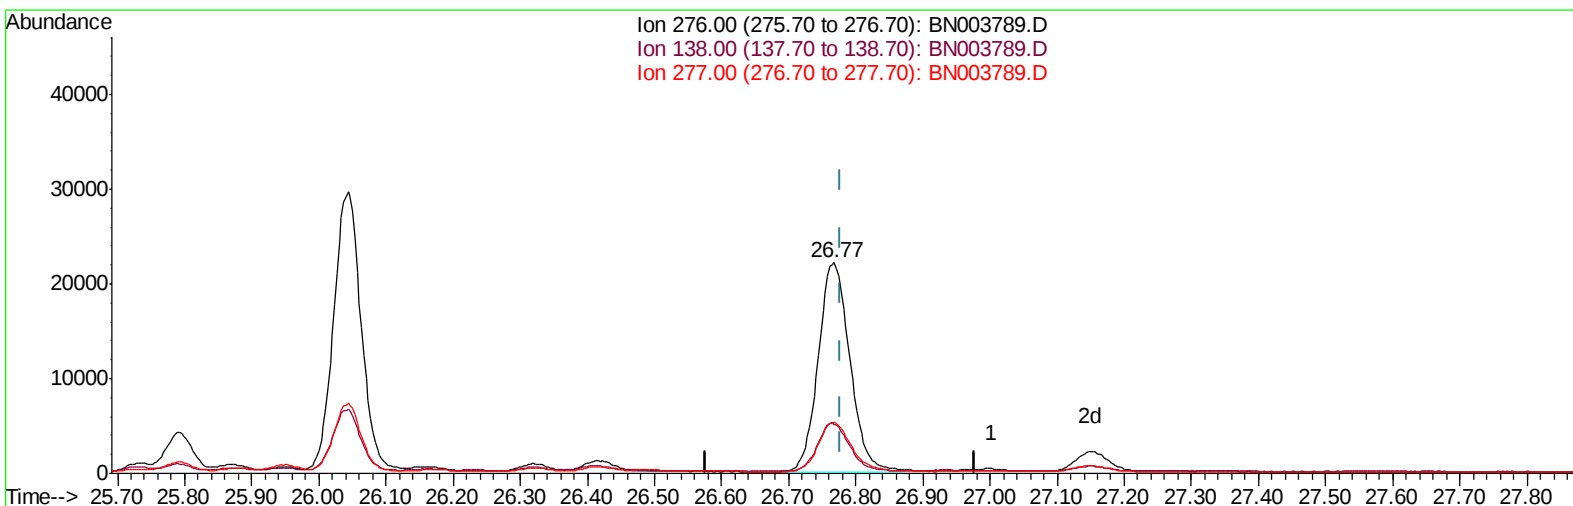

TIC: BN003789.D

(26) Benzo(g,h,i)perylene

26.768min (-0.010) 1.18ng/ul m

response 72422

Ion	Exp%	Act%
276.00	100	100
138.00	22.10	23.33
277.00	24.10	24.37
0.00	0.00	0.00