
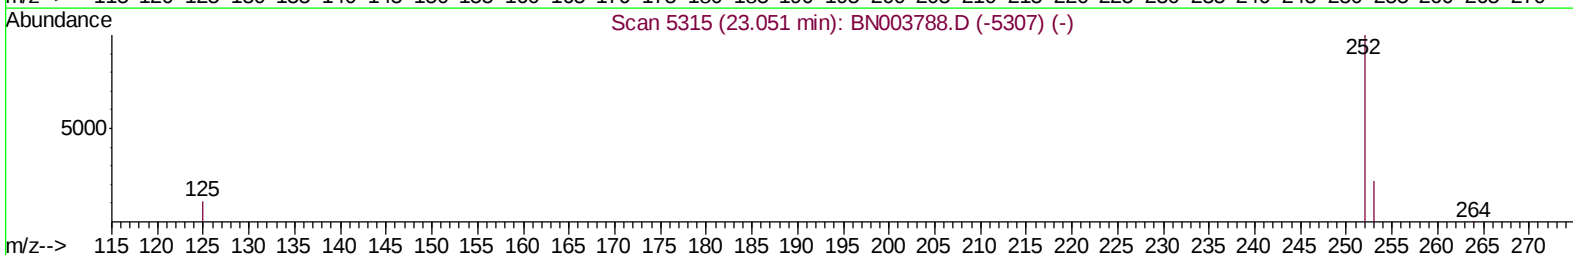
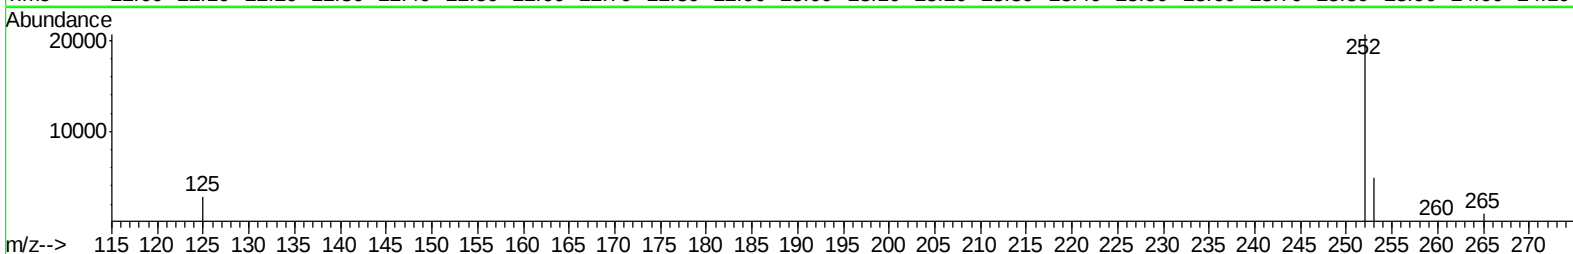


Data File : BN003790.D  
Acq On : 10 Dec 2018 22:24  
Operator : JU/SJ  
Sample : J6077-11DL 5X  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 11 04:26:28 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 11 04:22:54 2018  
Response via : Initial Calibration

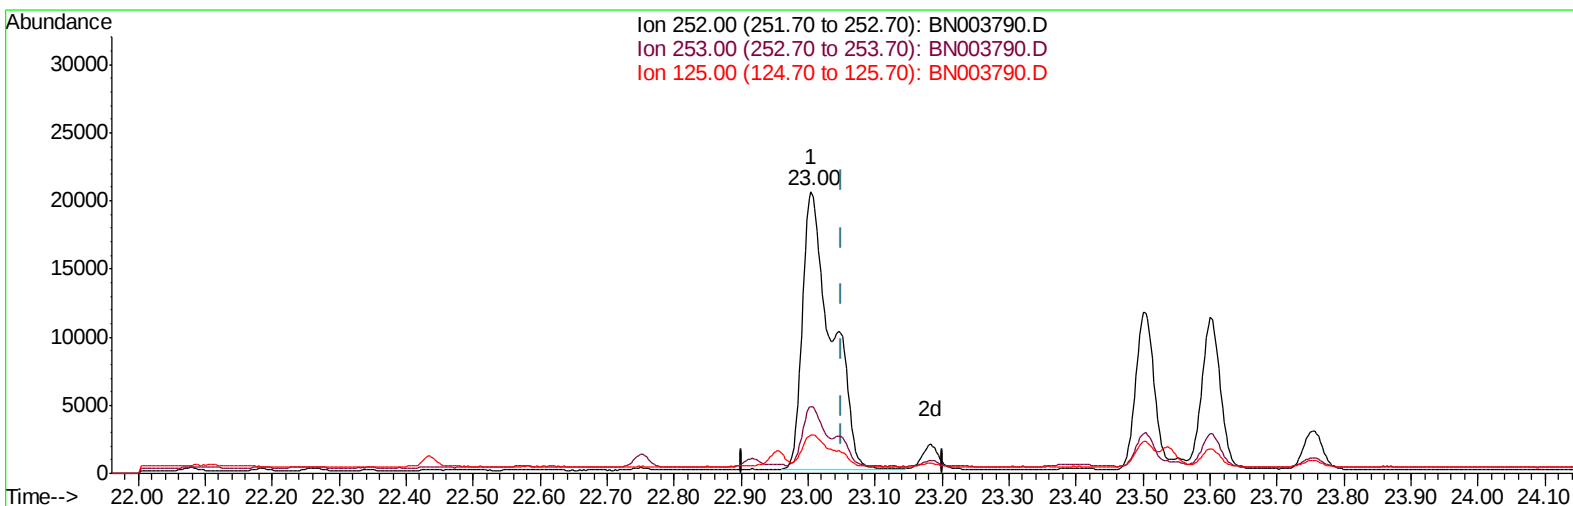

TIC: BN003790.D

(22) Benzo(k)fluoranthene  
23.004min (-0.047) 0.78ng/ul  
response 61559

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 23.10 | 23.69  |
| 125.00 | 11.30 | 13.65# |
| 0.00   | 0.00  | 0.00   |