
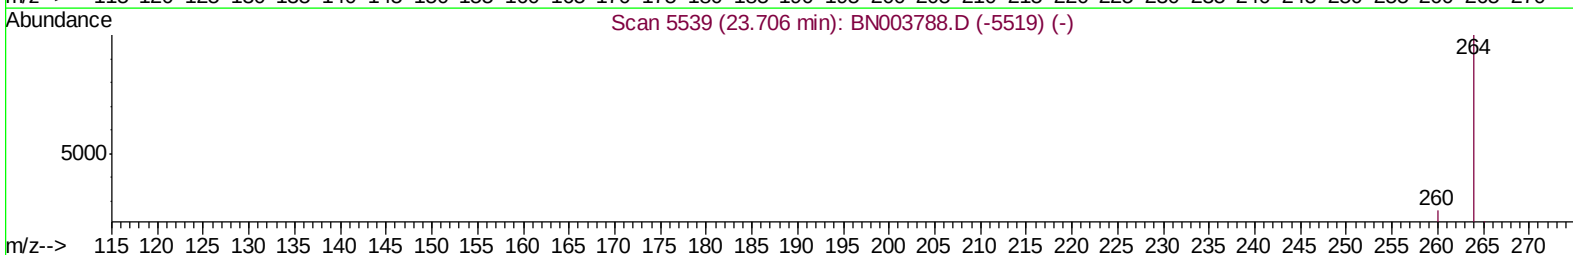
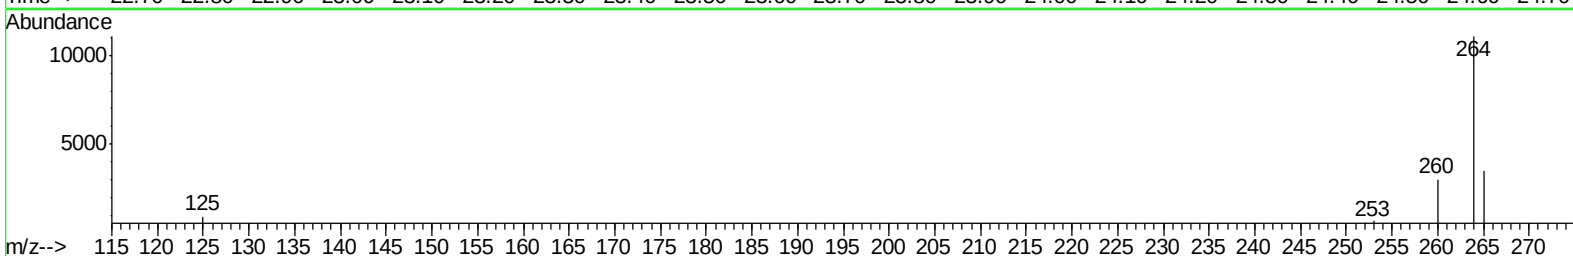


Data File : BN003791.D
Acq On : 10 Dec 2018 22:59
Operator : JU/SJ
Sample : J6077-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 11 04:43:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

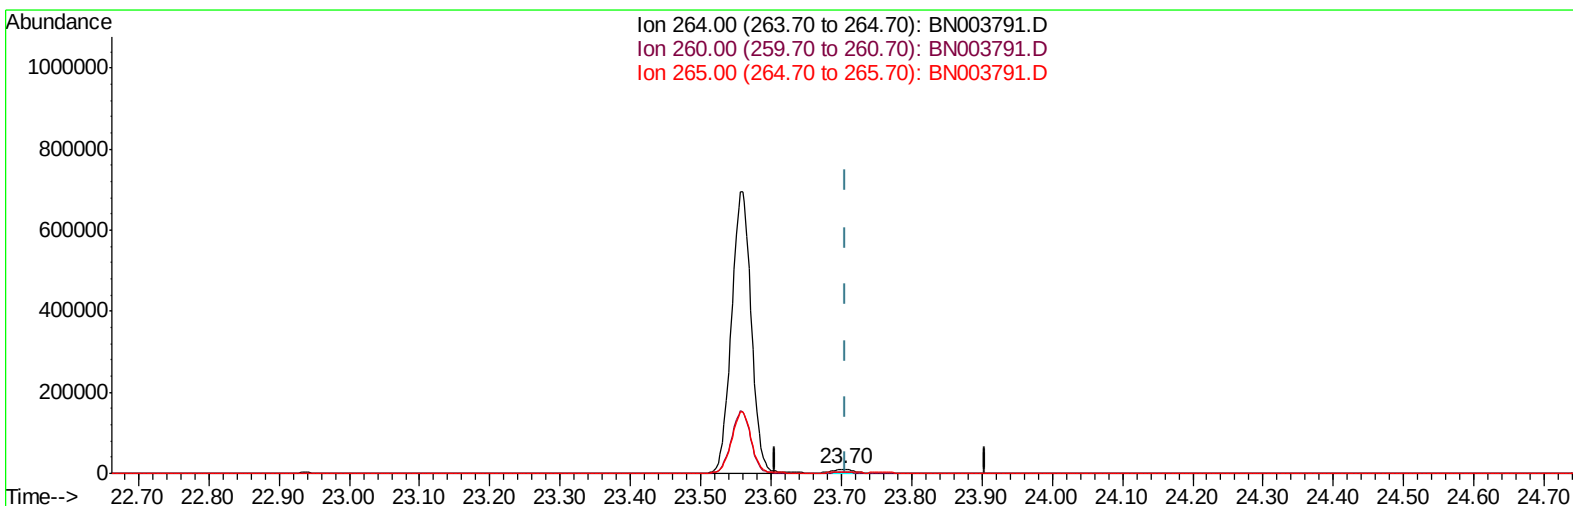

TIC: BN003791.D

(20) Perylene-d12 (I)

23.703min (-0.003) 0.40ng/ul m

response 19001

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	27.16
265.00	33.50	31.31
0.00	0.00	0.00